




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

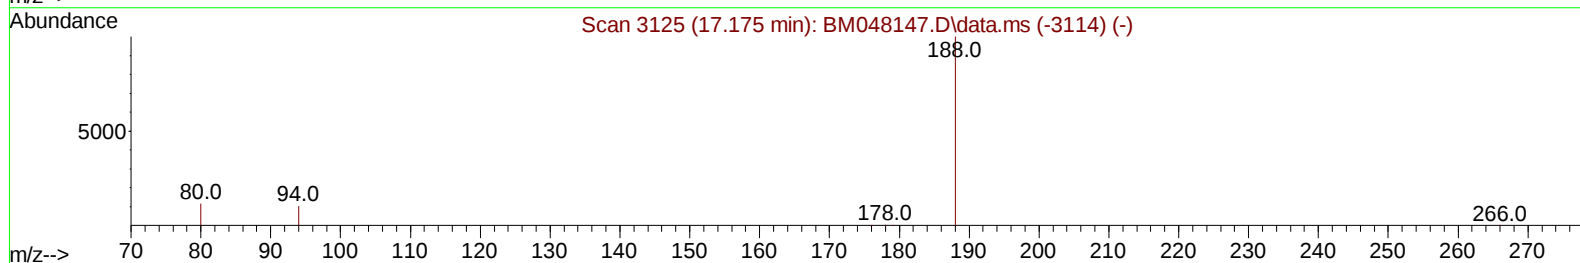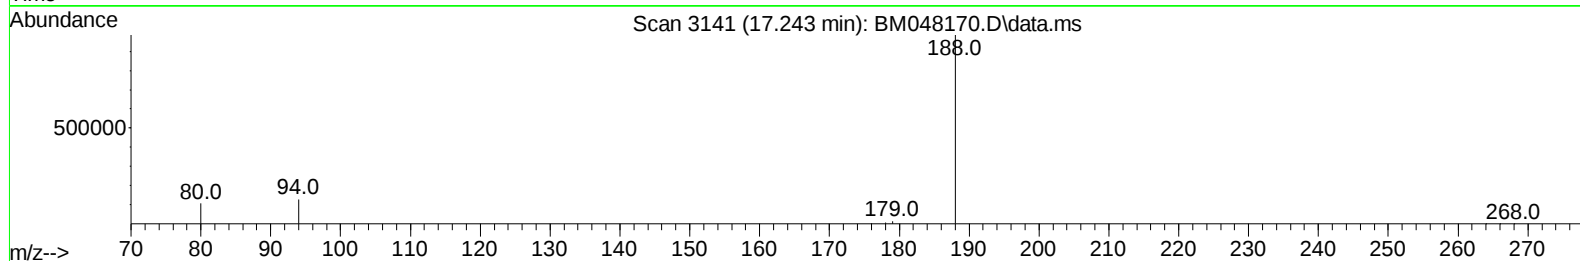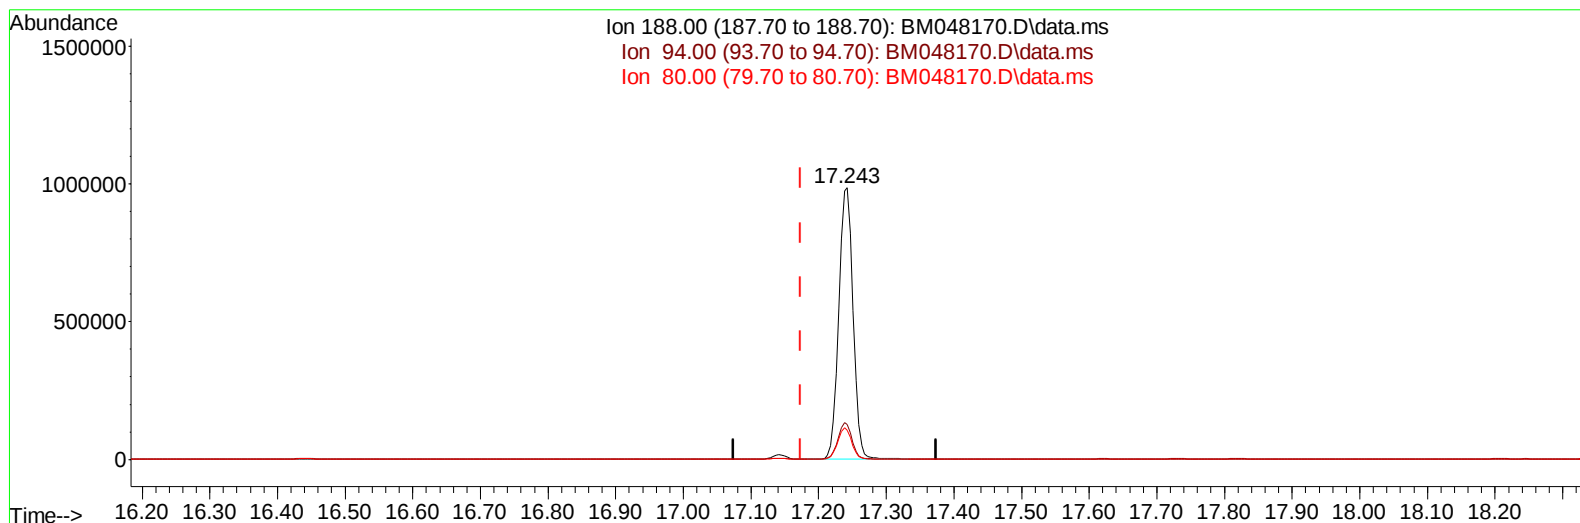

TIC: BM048170.D\data.ms

(13) Phenanthrene-d10 (I)

17.243min (+ 0.069) 0.40 ng/u1

response 1447718

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	12.90
80.00	12.40	10.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

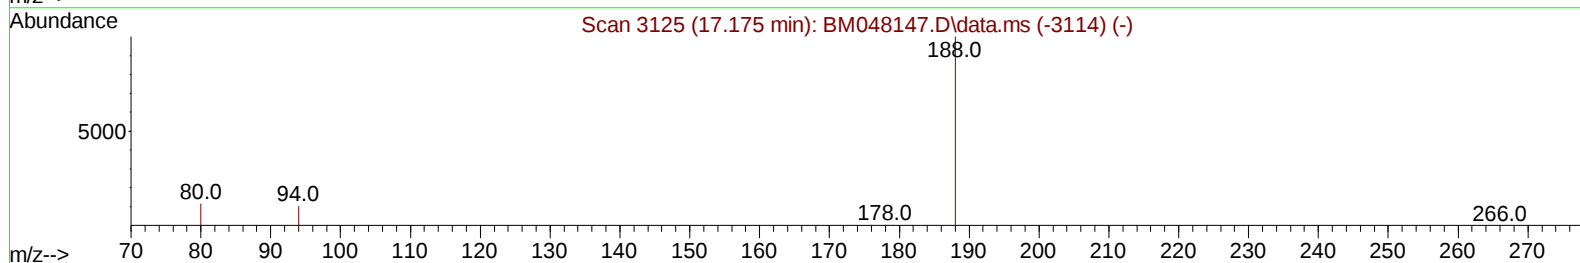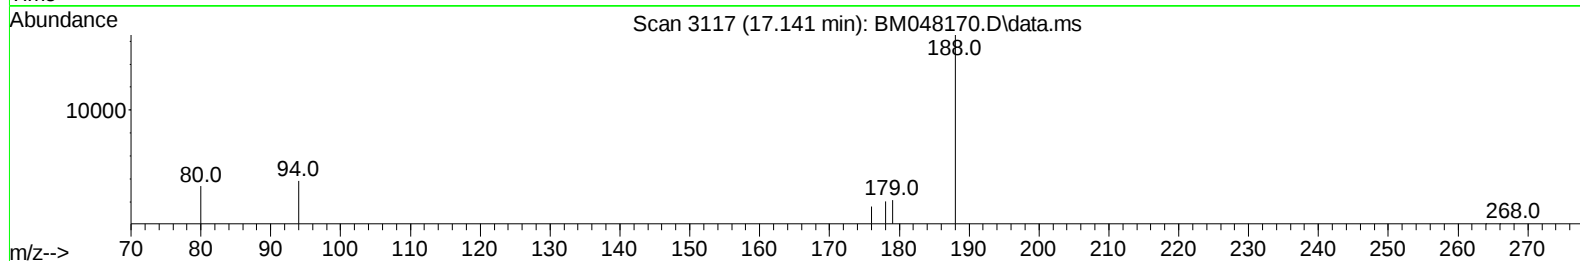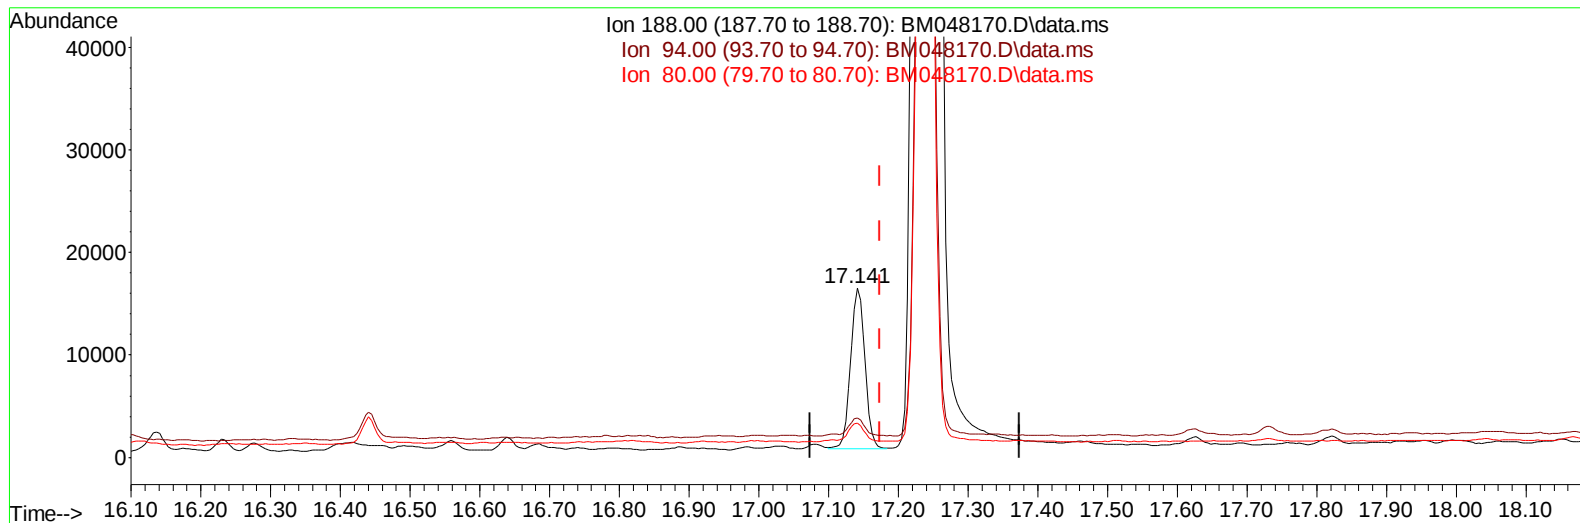

TIC: BM048170.D\data.ms

(13) Phenanthrene-d10 (I)

17.141min (-0.033) 0.40 ng/ul m

response 22384

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	23.19#
80.00	12.40	20.32#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

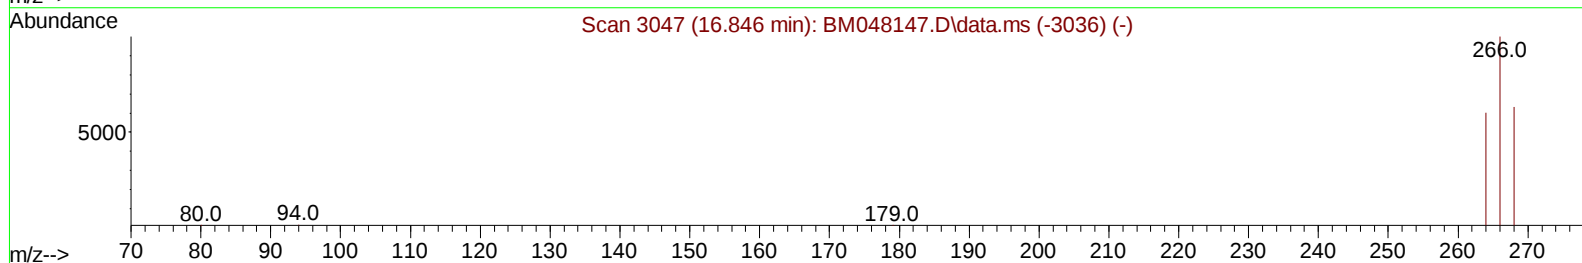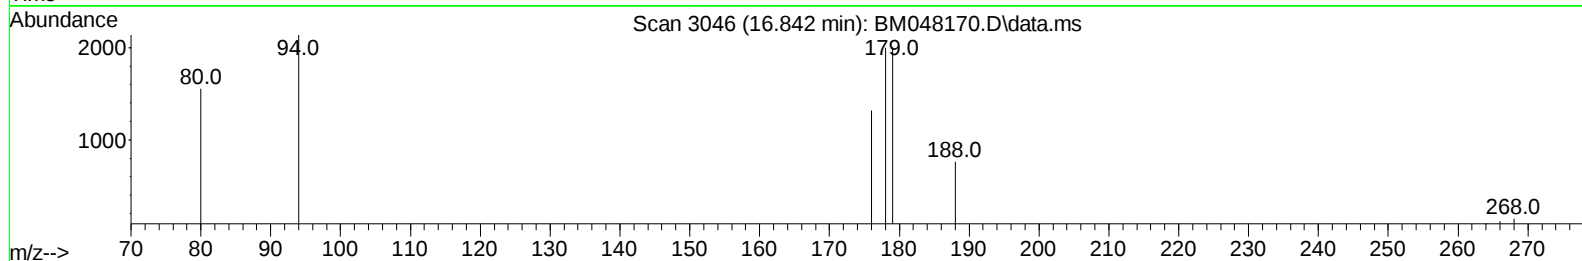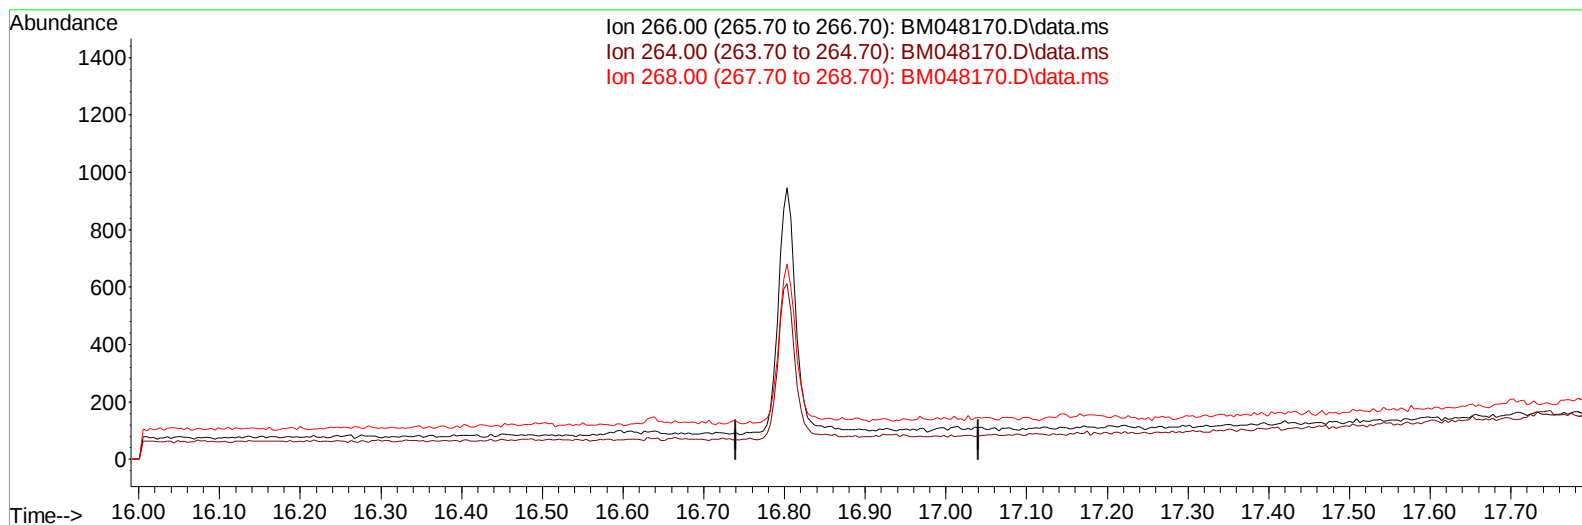

TIC: BM048170.D\data.ms

(14) Pentachlorophenol

16.840min (-16.840) 0.00 ng/u1

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048170.D
 Acq On : 22 Oct 2024 00:51
 Operator : RC/JU
 Sample : P4380-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 23:11:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

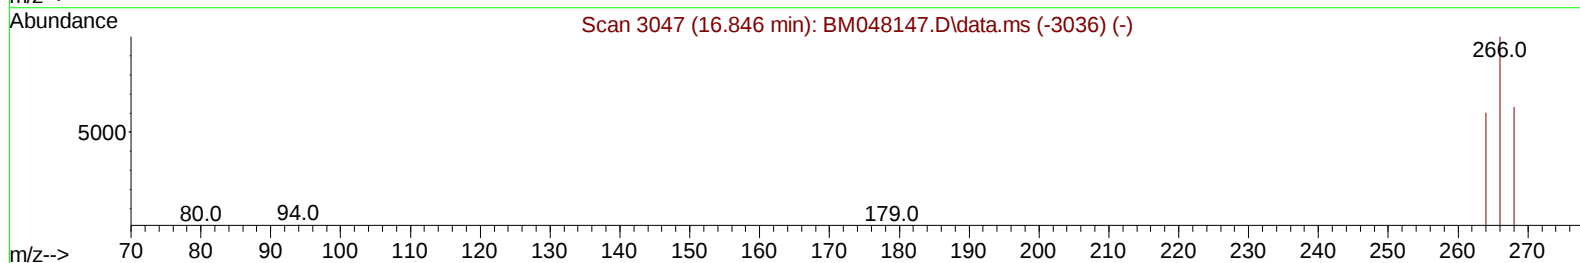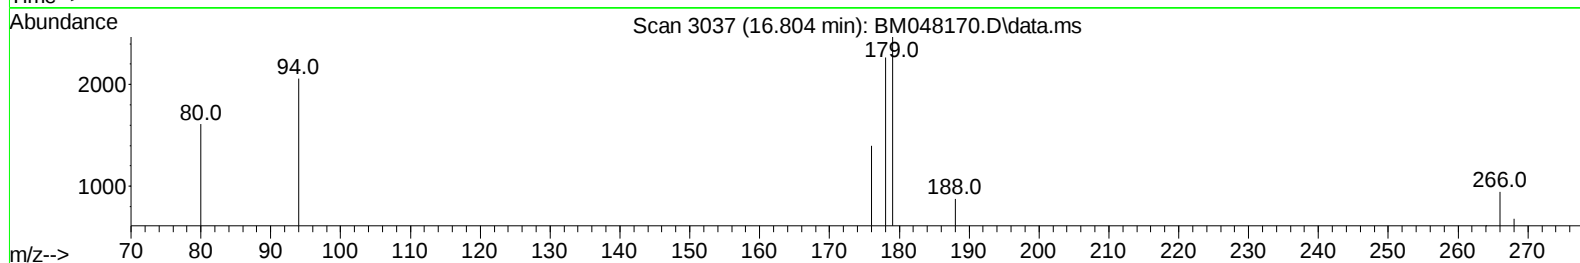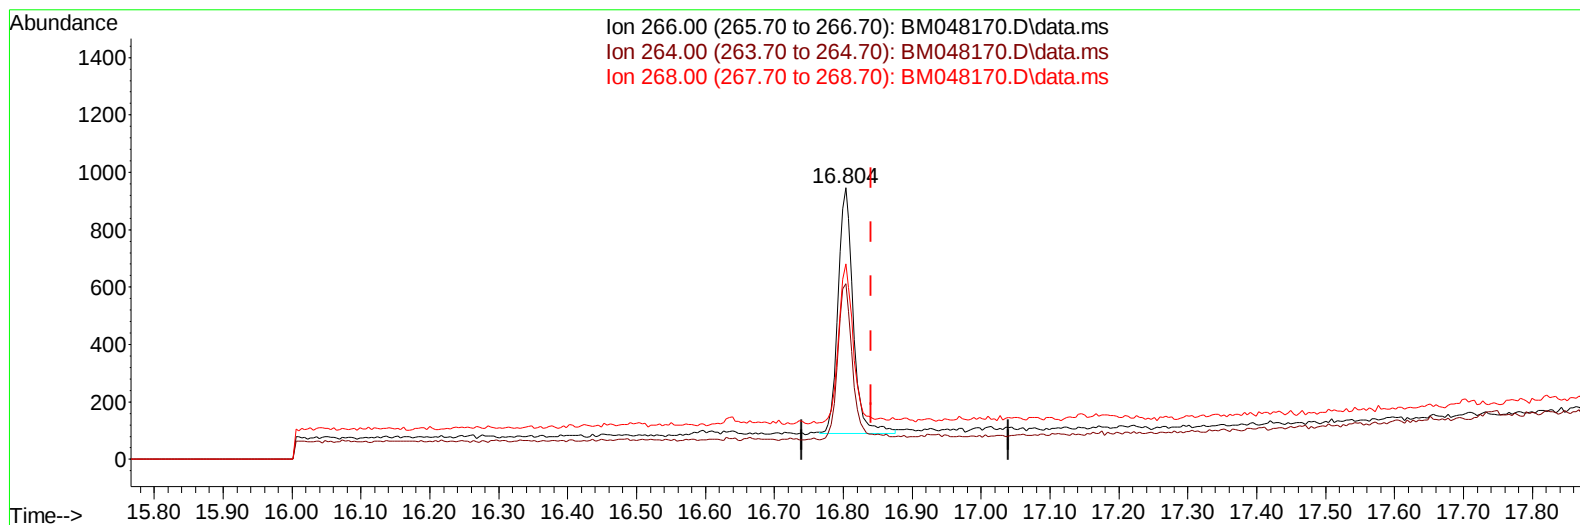

TIC: BM048170.D\data.ms

(14) Pentachlorophenol

16.804min (-0.037) 0.17 ng/ul m

response 1307

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

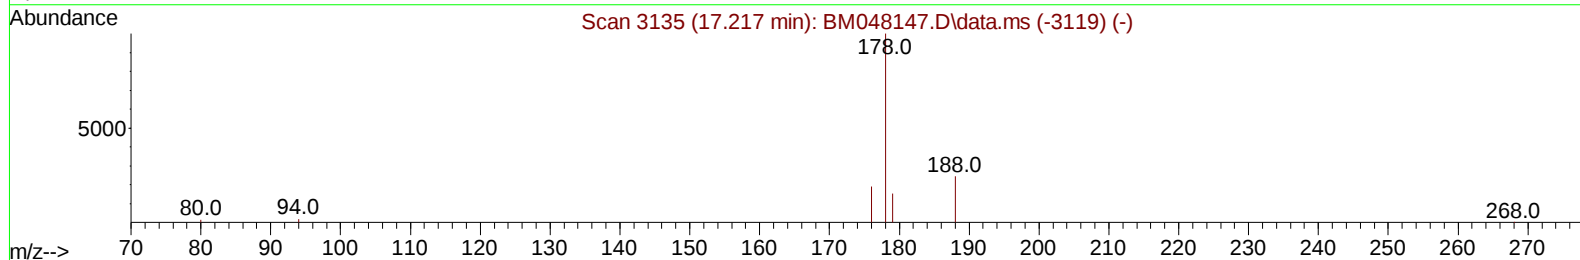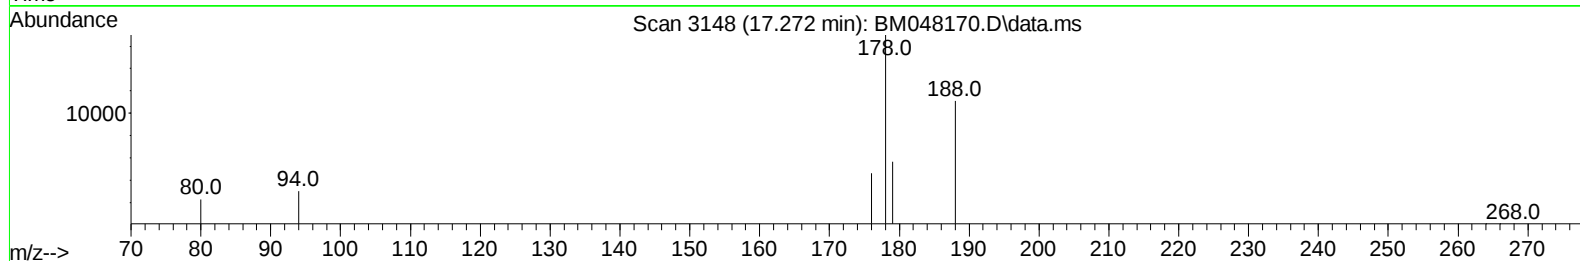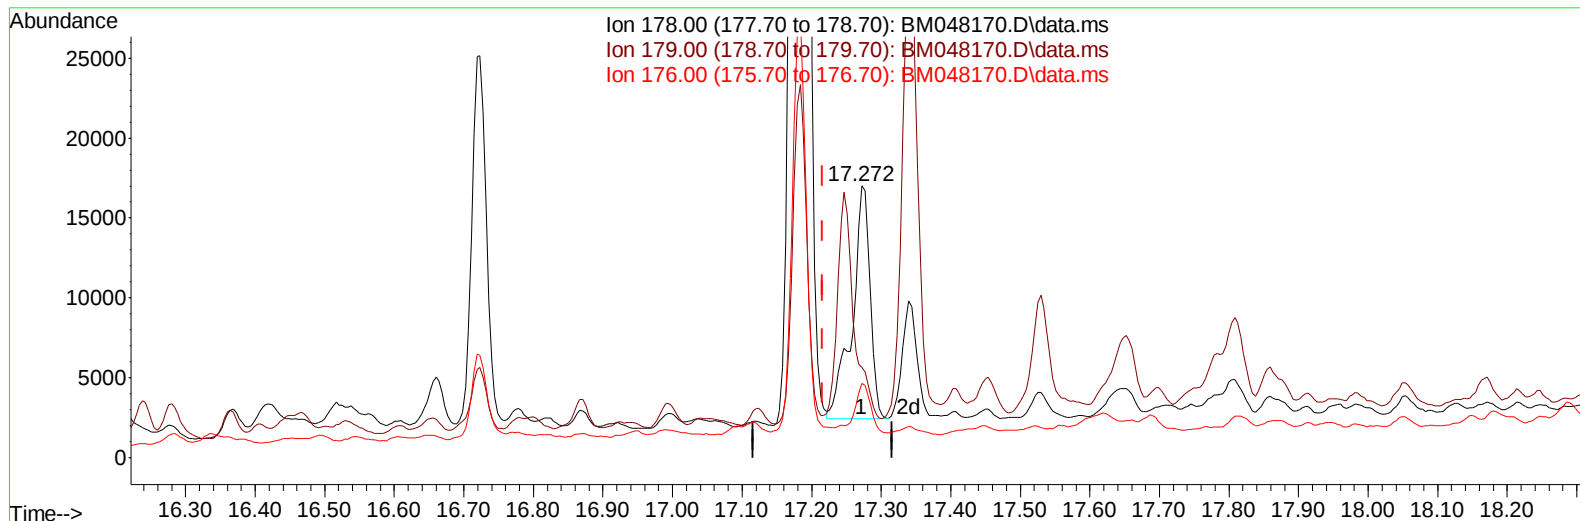

TIC: BM048170.D\data.ms

(15) Phenanthrene

17.272min (+ 0.056) 0.46 ng/u1

response 25892

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	33.24#
176.00	20.00	27.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

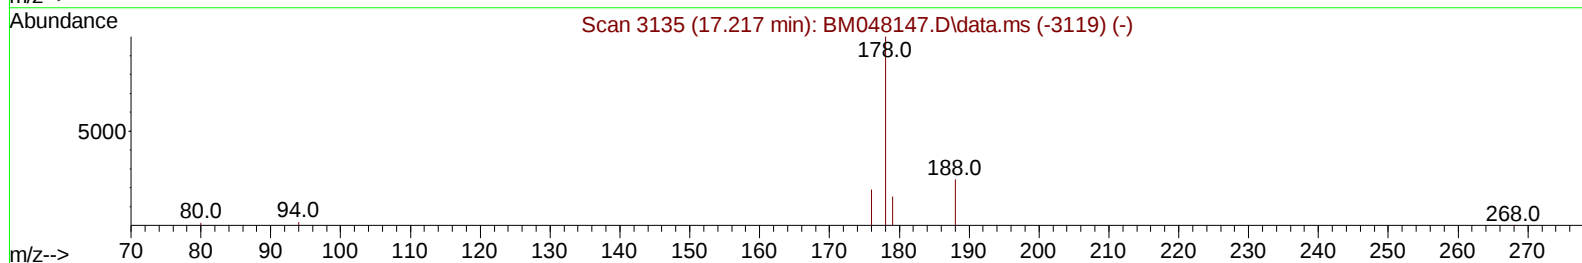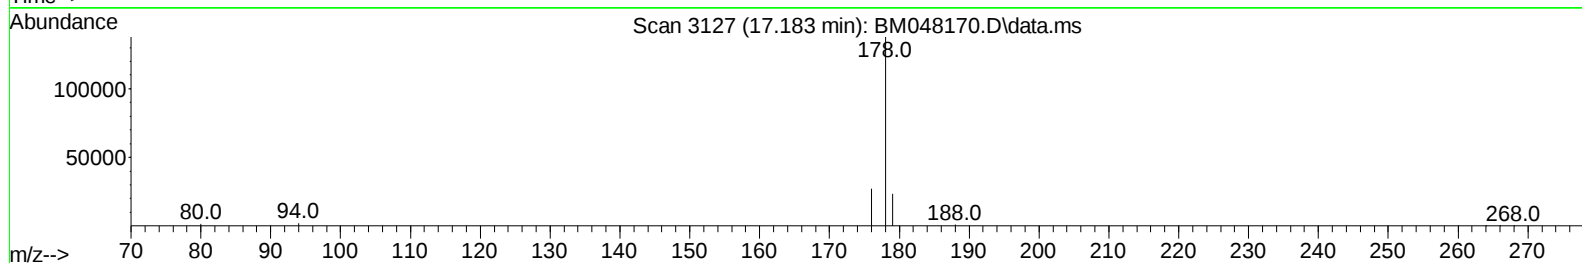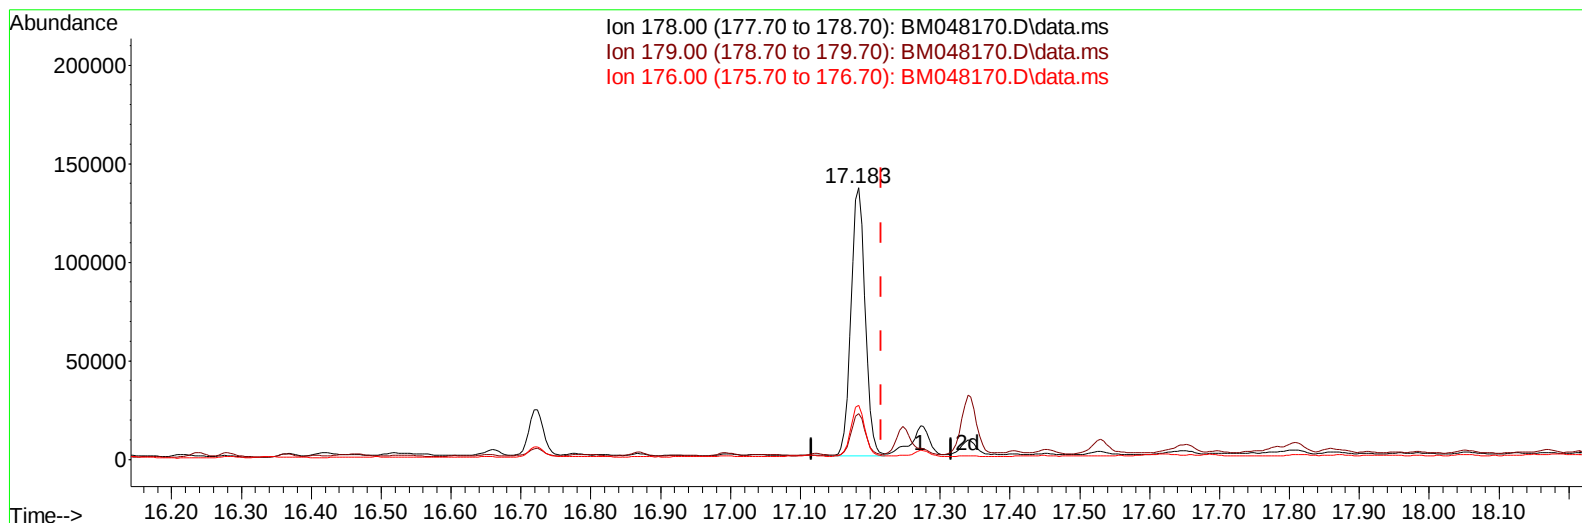

TIC: BM048170.D\data.ms

(15) Phenanthrene

17.183min (-0.033) 3.39 ng/u1 m

response 191678

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	16.96
176.00	20.00	19.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

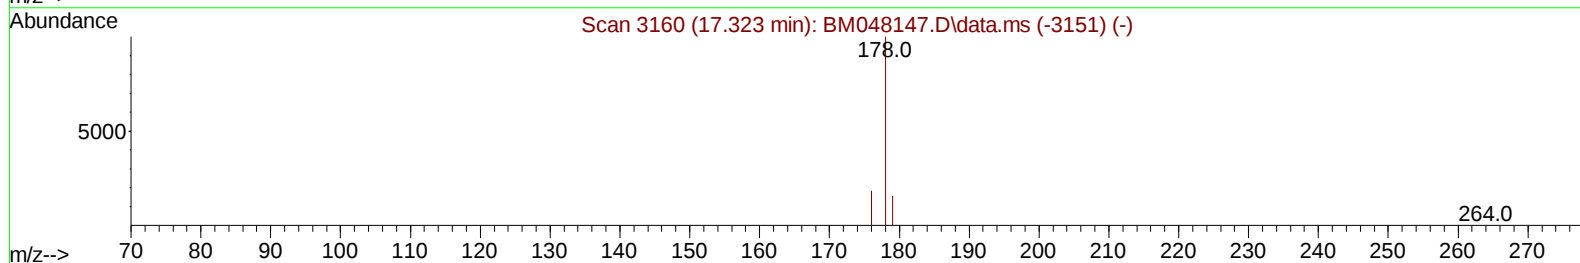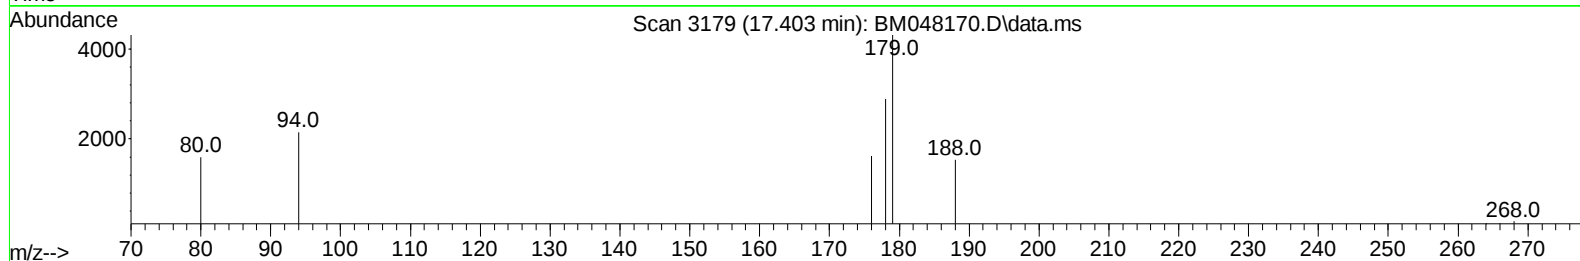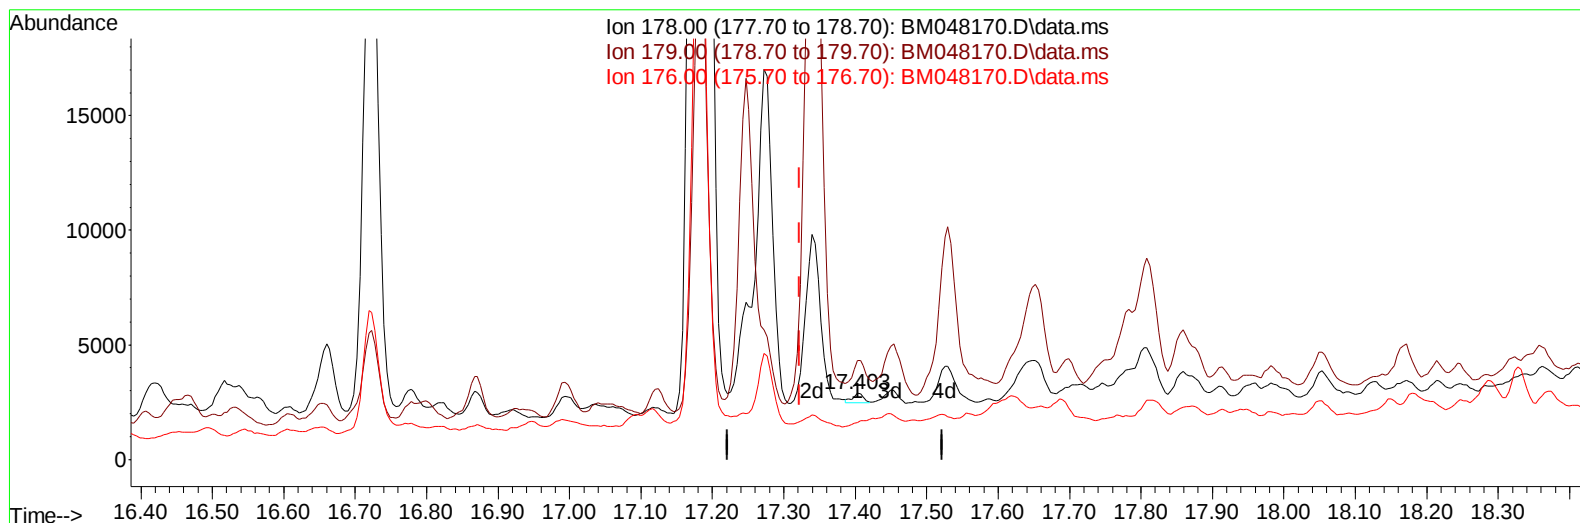

TIC: BM048170.D\data.ms

(16) Anthracene

17.403min (+ 0.081) 0.01 ng/u1

response 443

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	149.67#
176.00	20.00	56.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

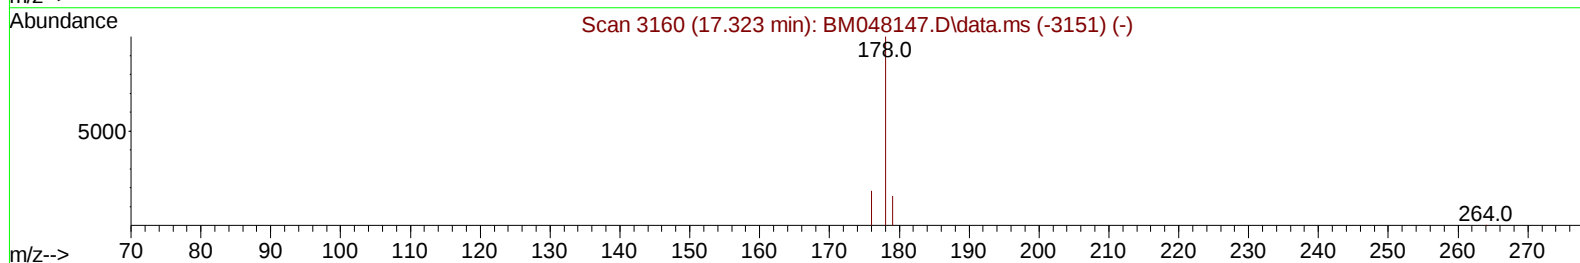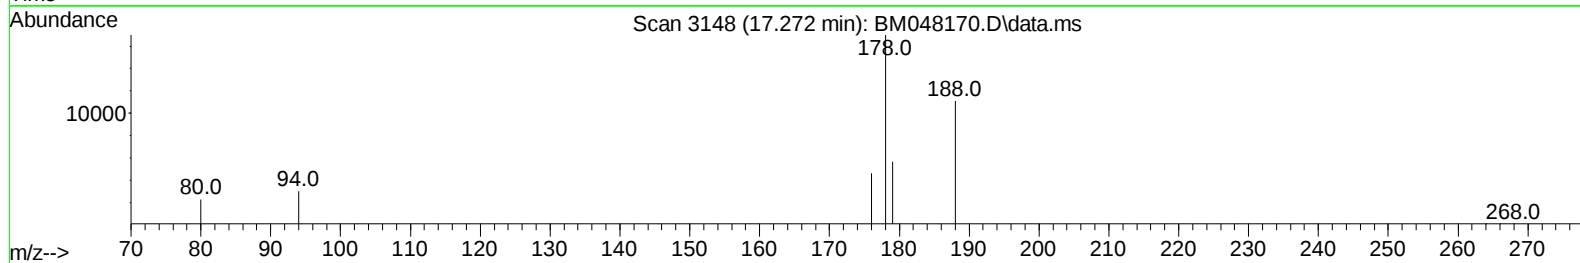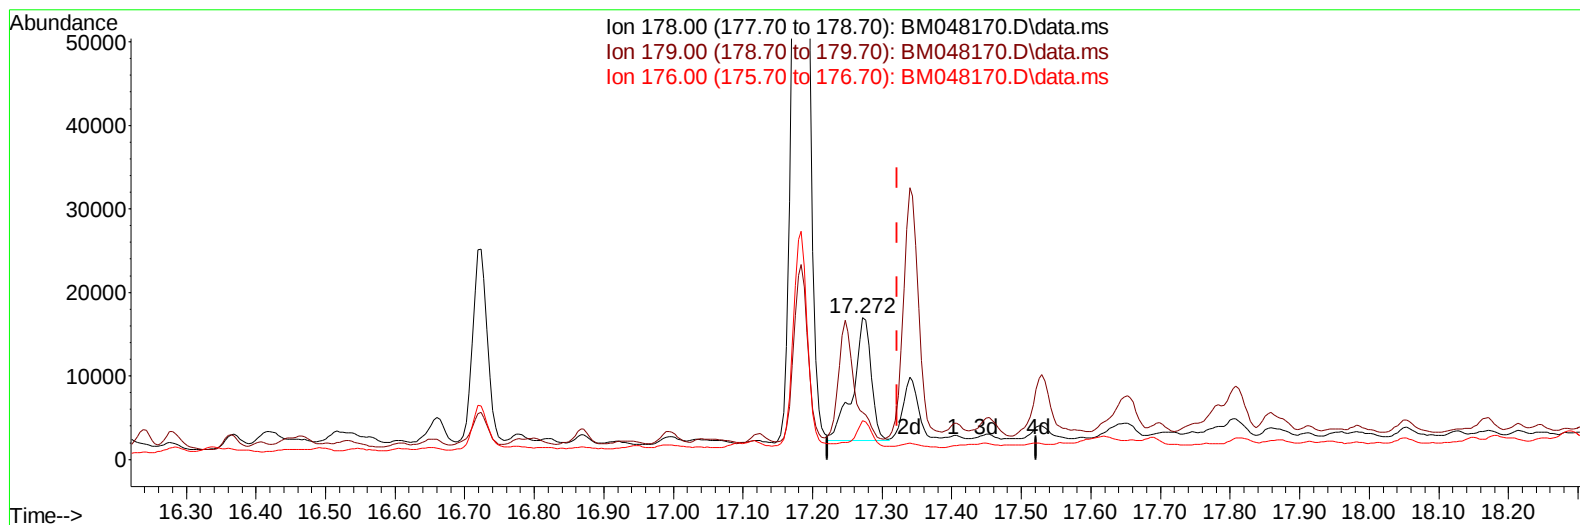

TIC: BM048170.D\data.ms

(16) Anthracene

17.272min (-0.049) 0.50 ng/u1 m

response 26939

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	33.24#
176.00	20.00	27.20#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

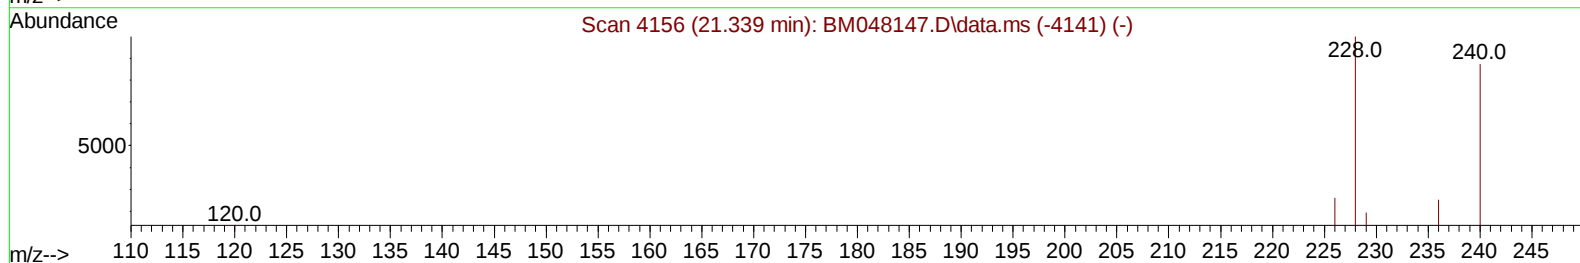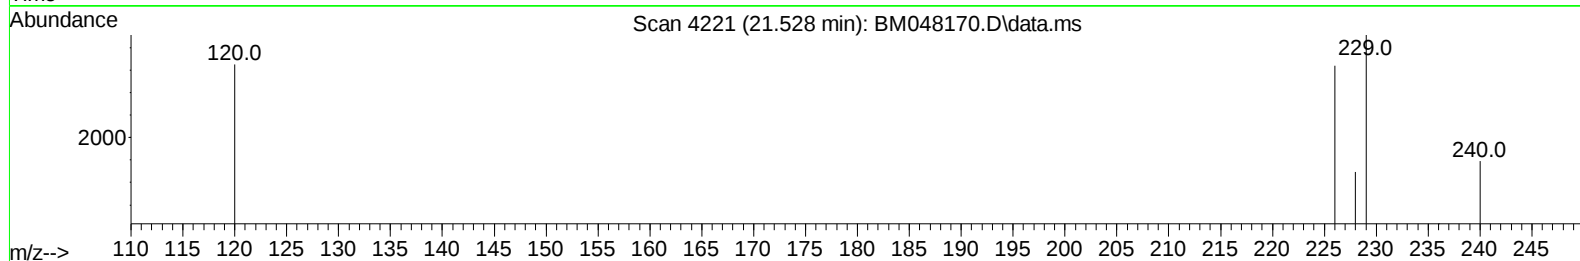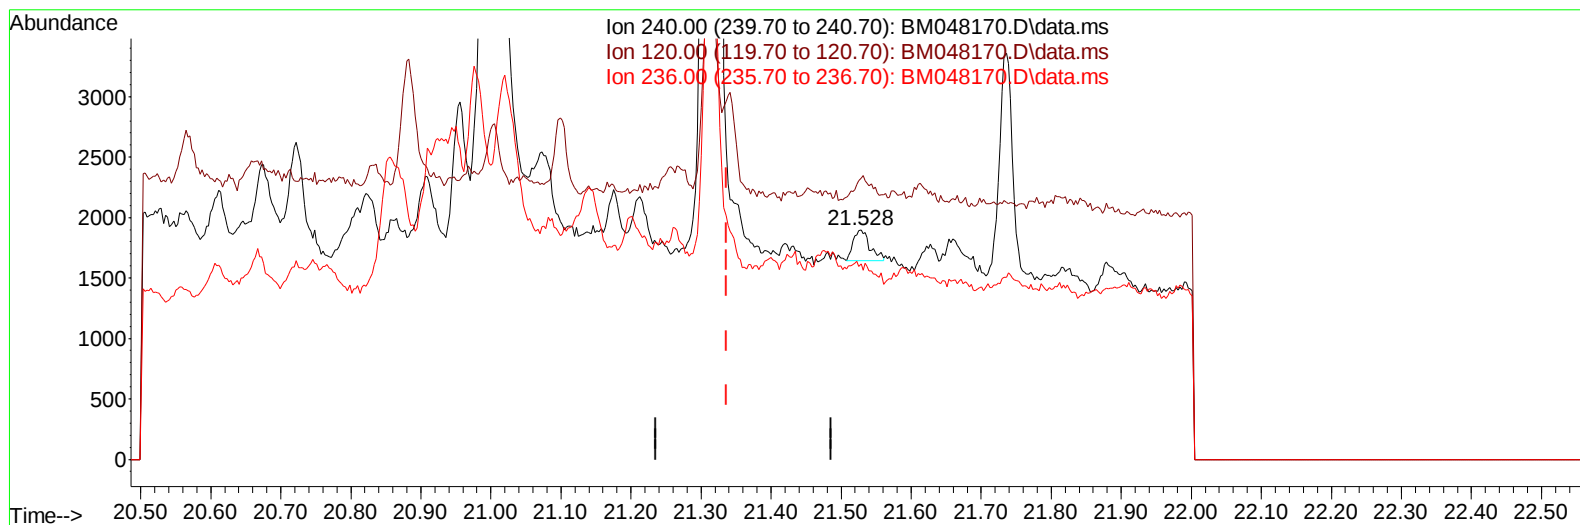

TIC: BM048170.D\data.ms

(17) Chrysene-d12

21.528min (+ 0.192) 0.40 ng/u1

response 419

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	122.64#
236.00	30.60	85.28#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

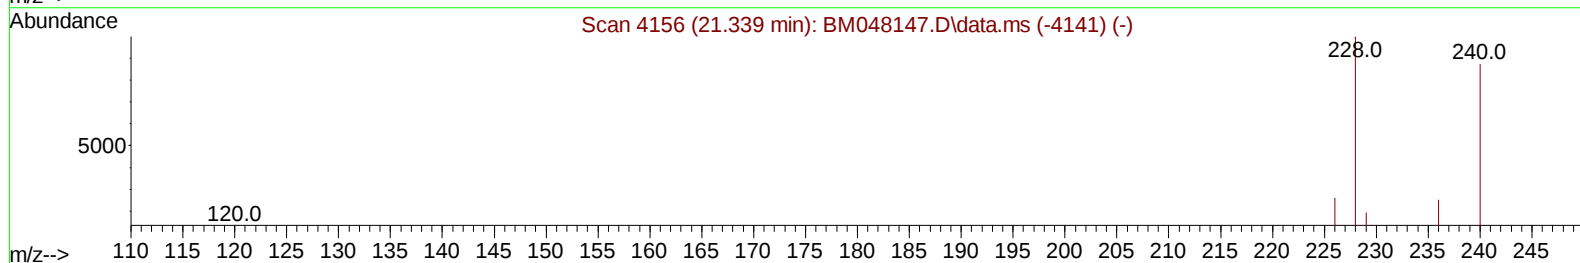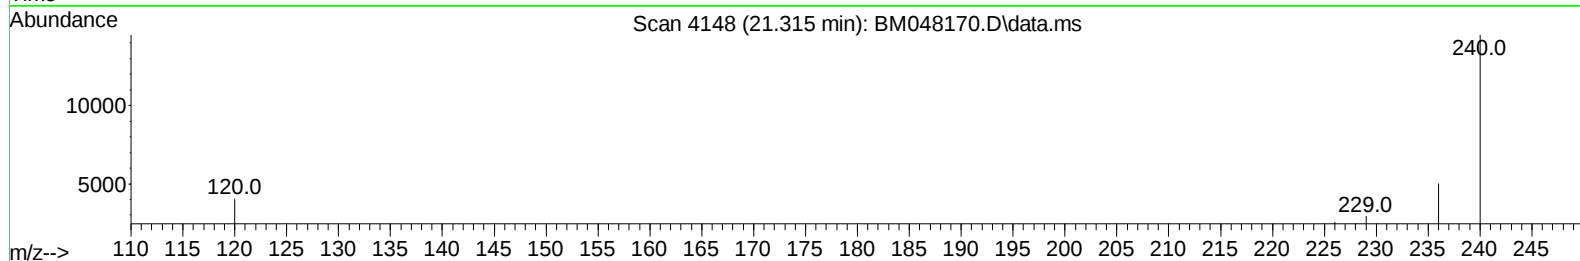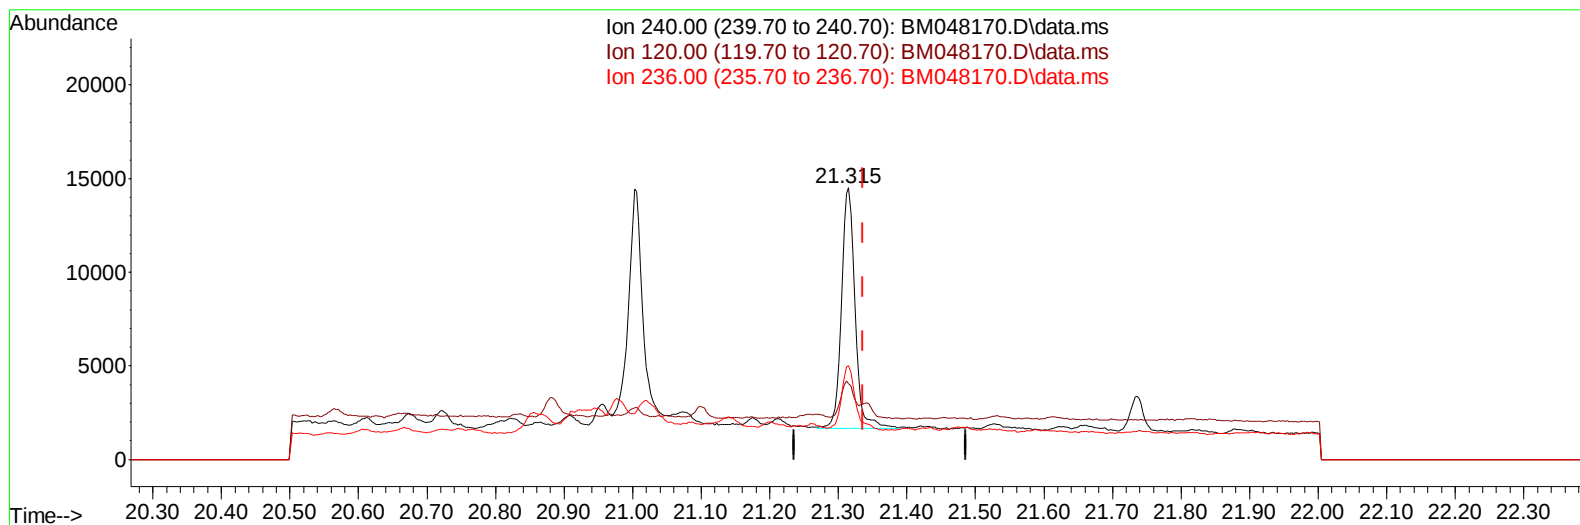

TIC: BM048170.D\data.ms

(17) Chrysene-d12

21.315min (-0.021) 0.40 ng/ul m

response 17682

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	27.93#
236.00	30.60	34.65
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

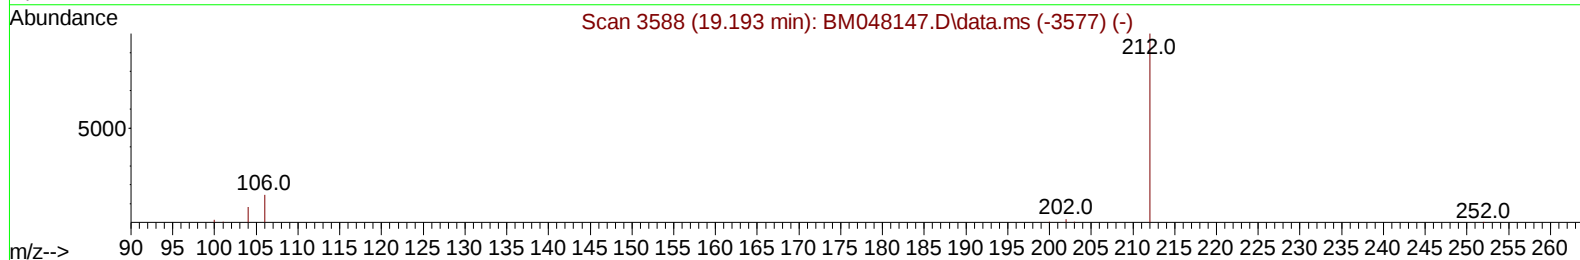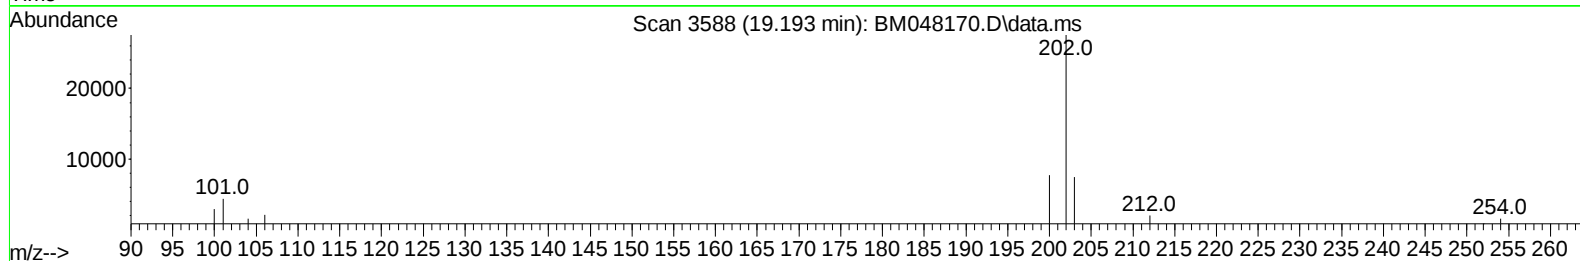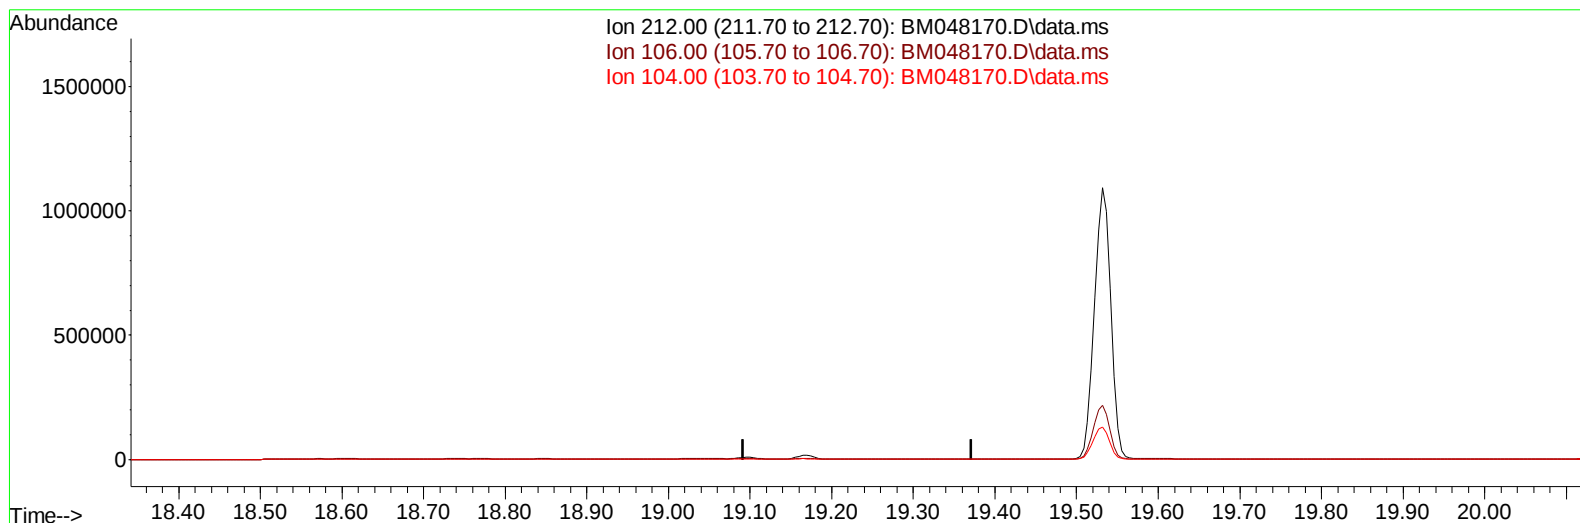

TIC: BM048170.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.191min (-19.191) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

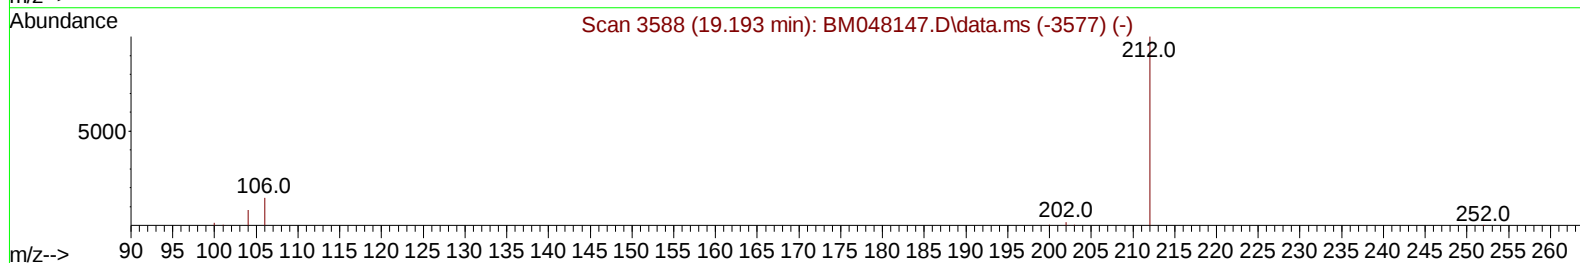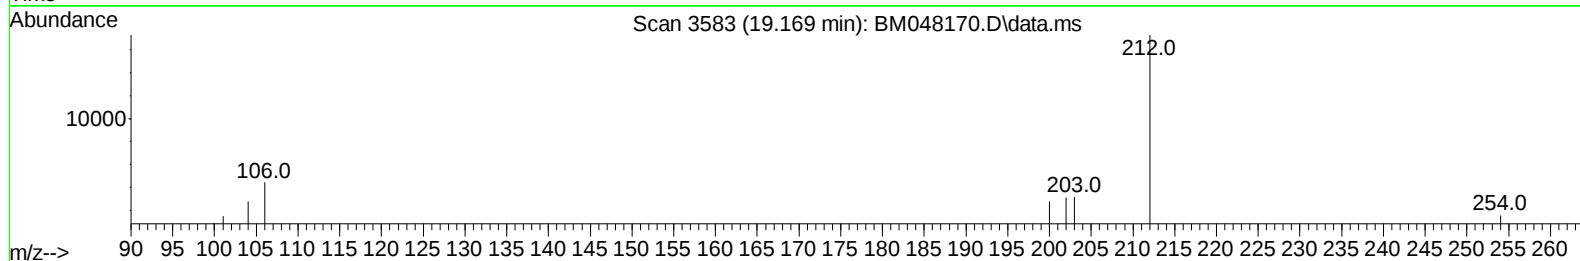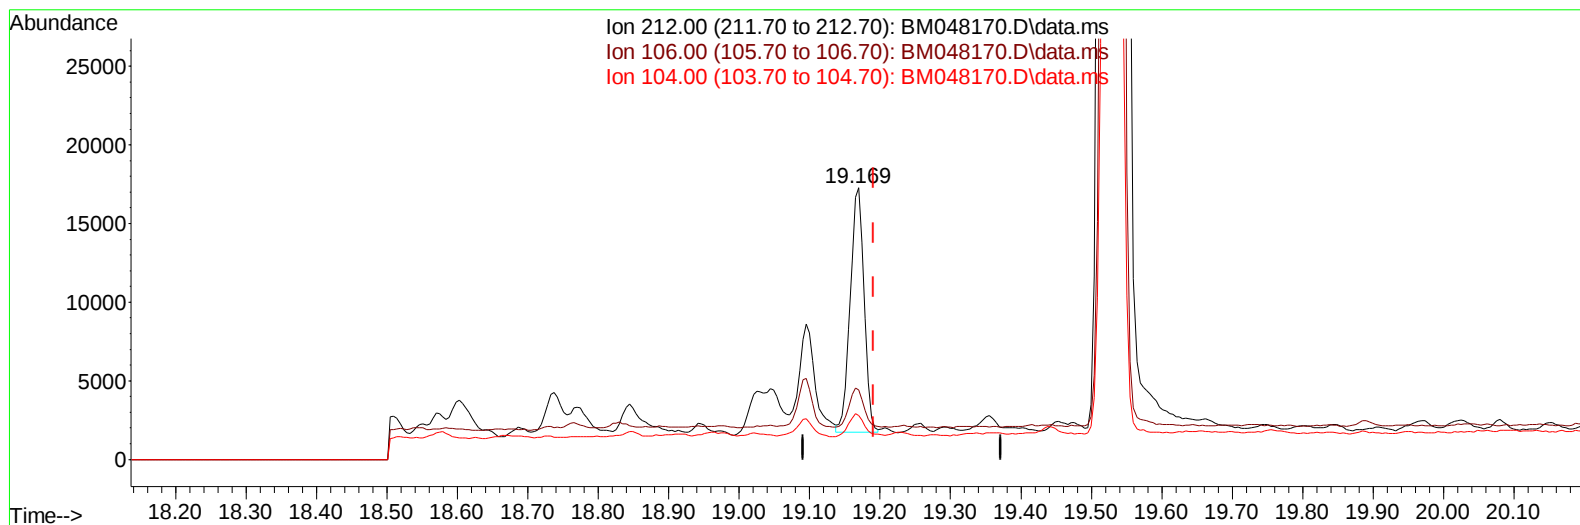

TIC: BM048170.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.169min (-0.022) 0.41 ng/u1 m

response 21202

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

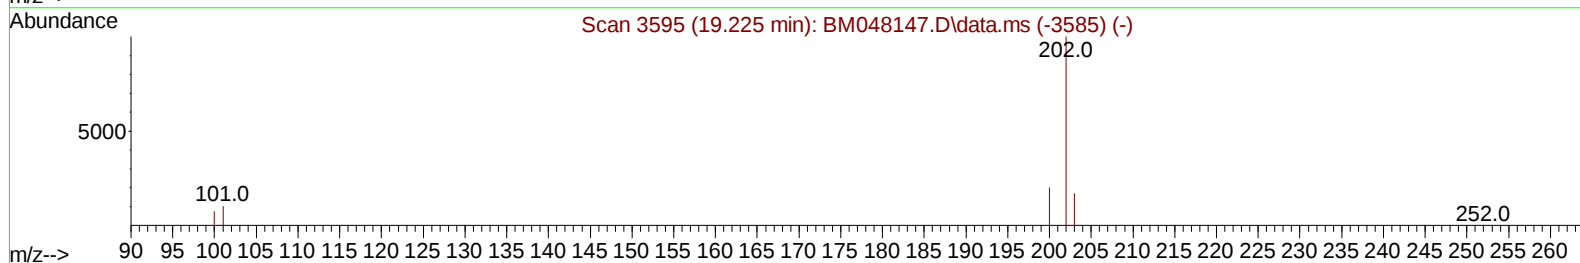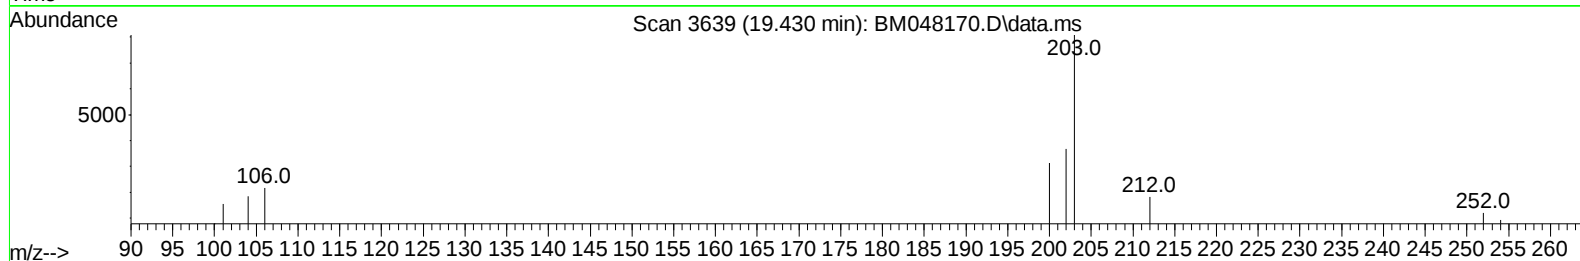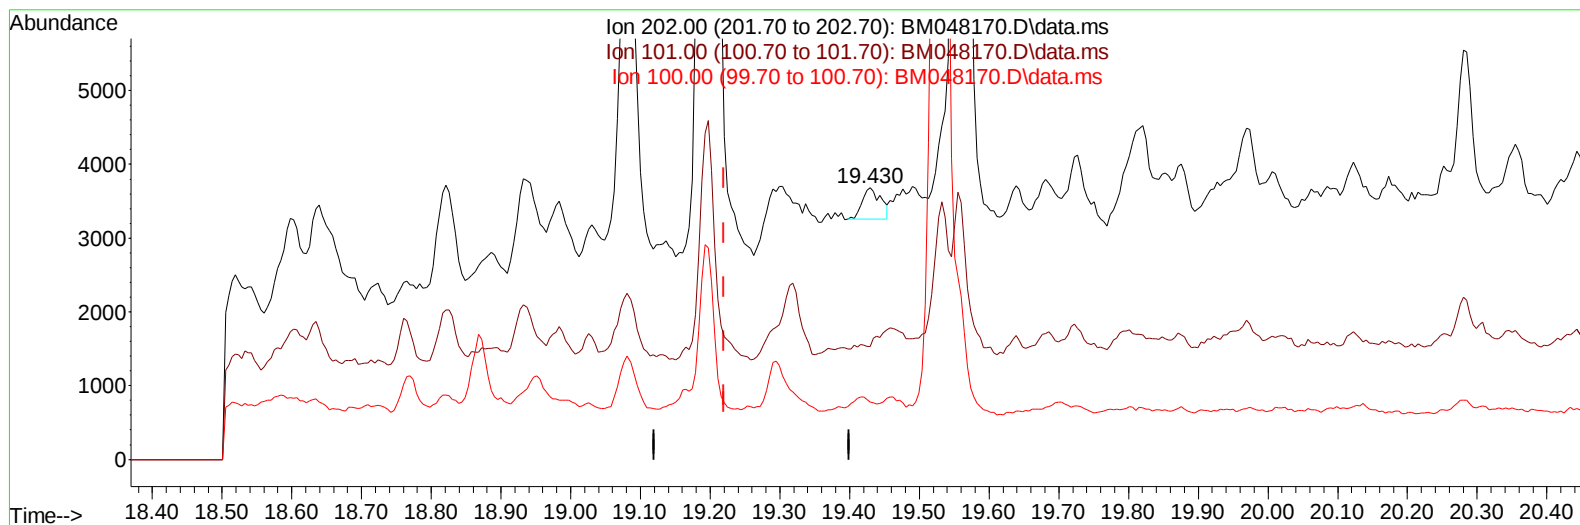

TIC: BM048170.D\data.ms

(19) Fluoranthene (C)

19.430min (+ 0.210) 0.01 ng/u1

response 778

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	41.74#
100.00	8.90	21.03#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

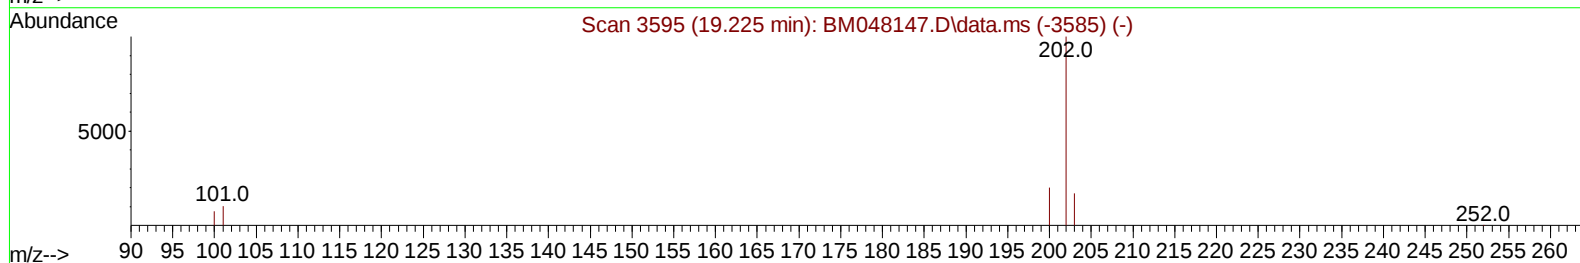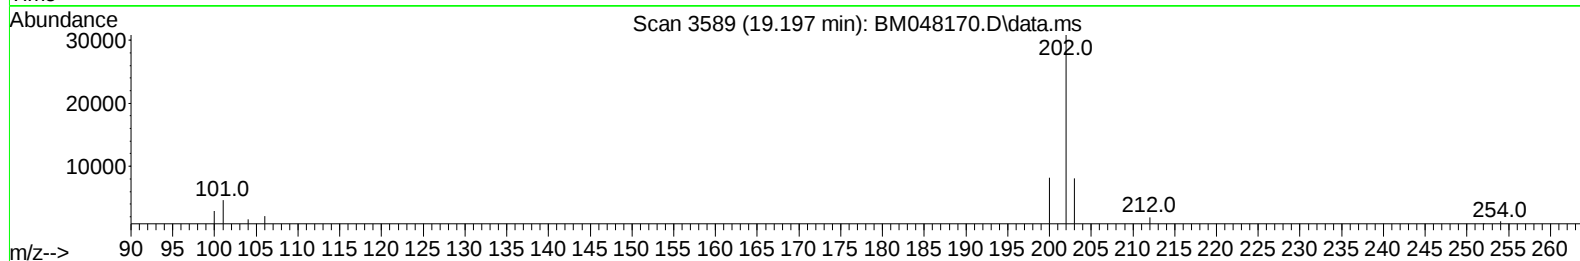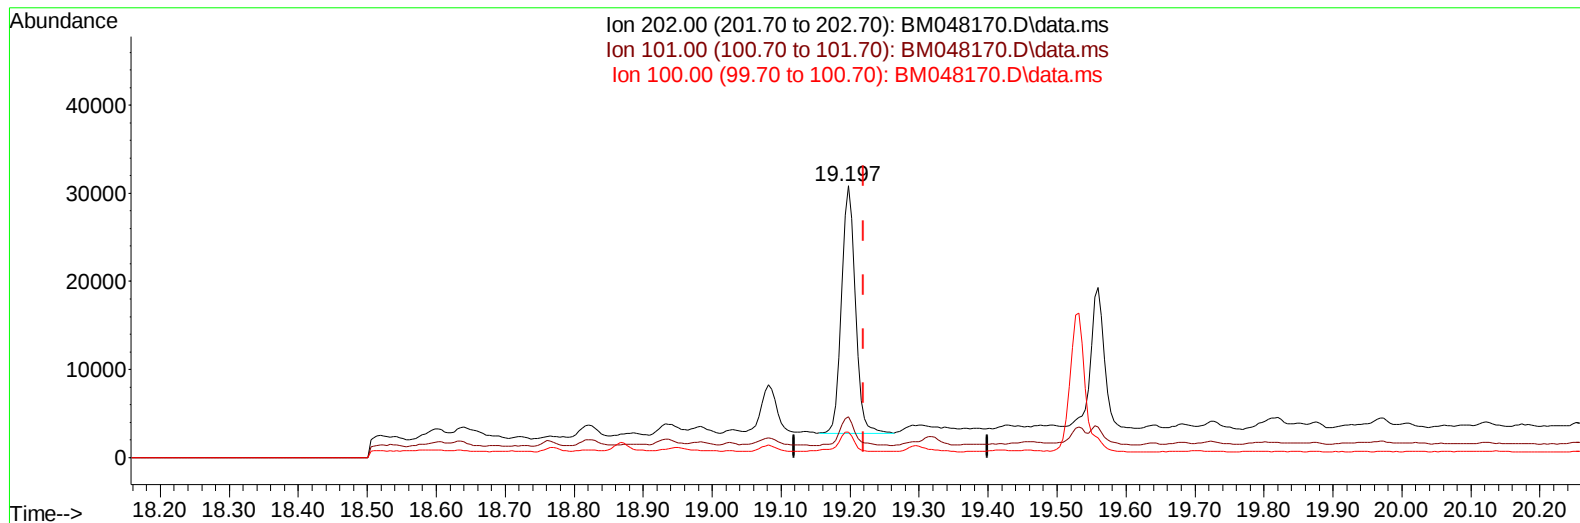

TIC: BM048170.D\data.ms

(19) Fluoranthene (C)

19.197min (-0.022) 0.57 ng/u1 m

response 39777

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	14.89#
100.00	8.90	9.30
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

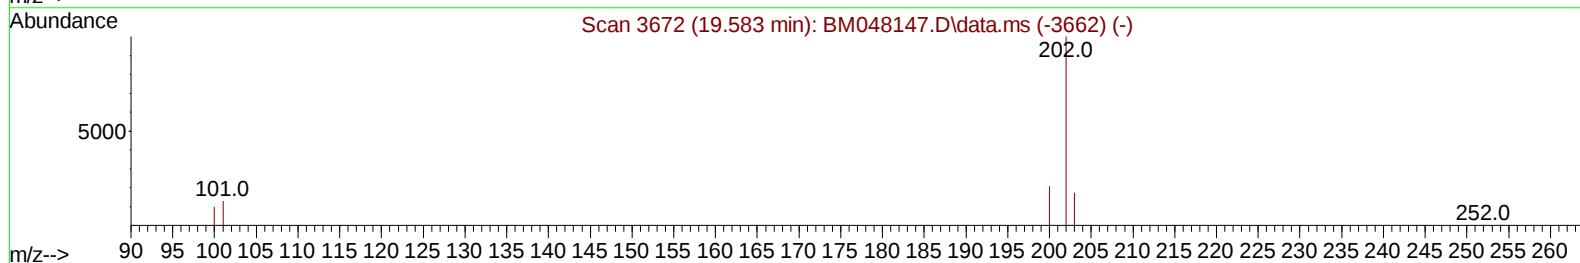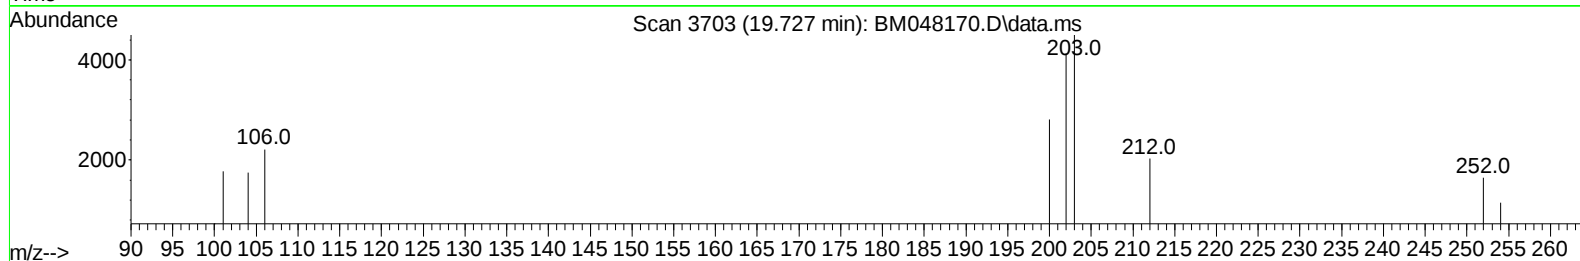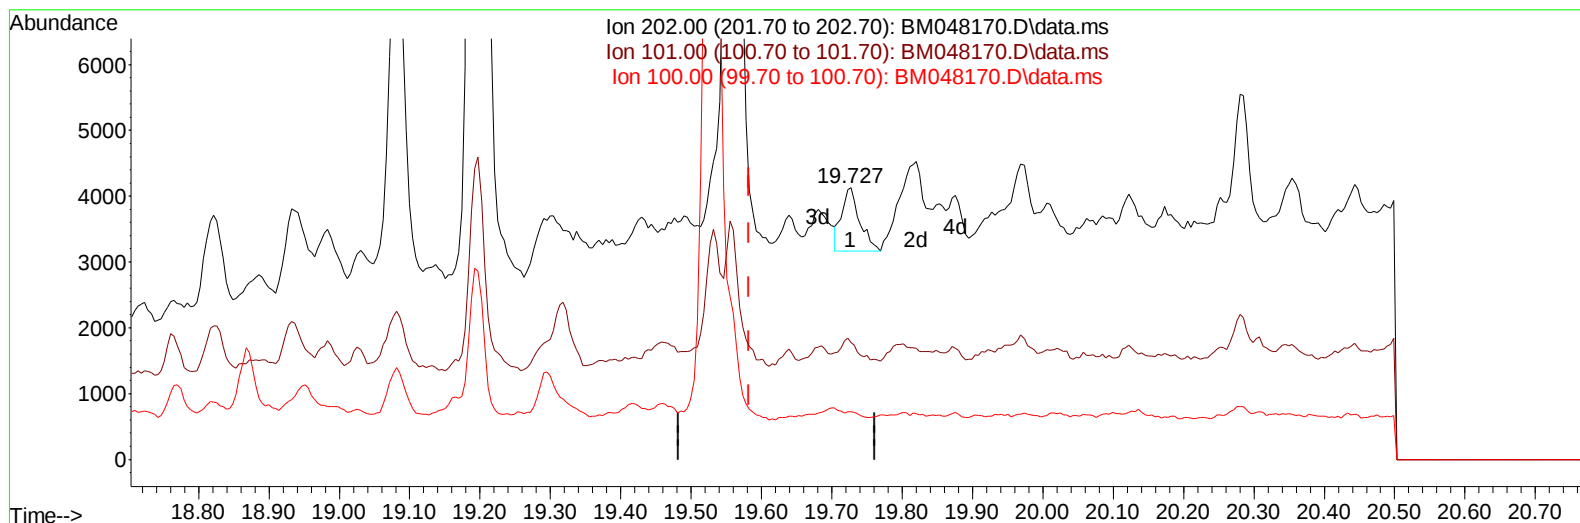

TIC: BM048170.D\data.ms

(20) Pyrene

19.727min (+ 0.145) 0.02 ng/u1

response 1730

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	43.13#
100.00	10.10	17.62#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

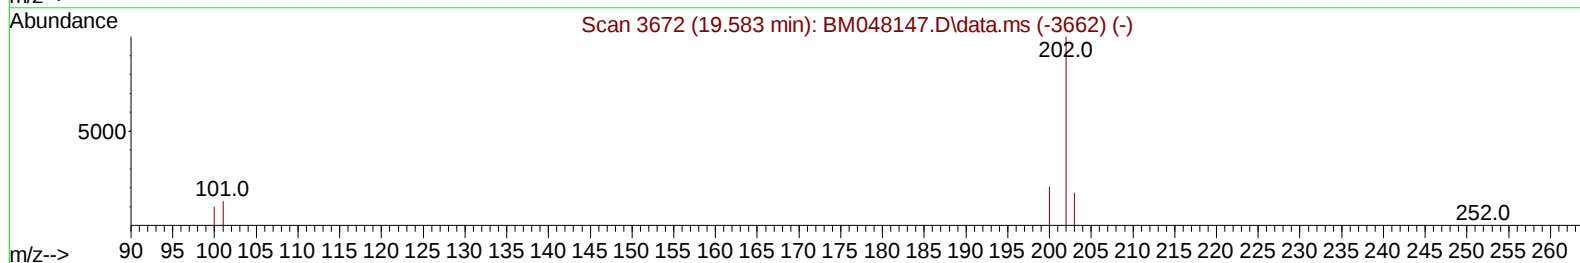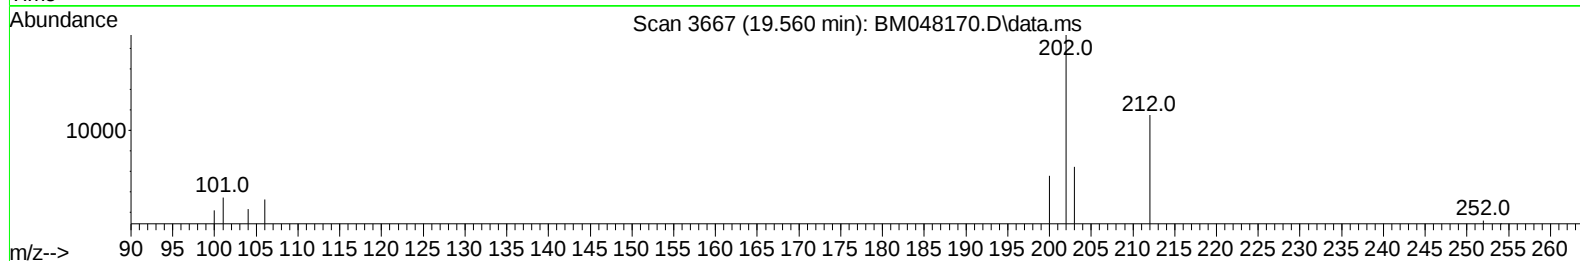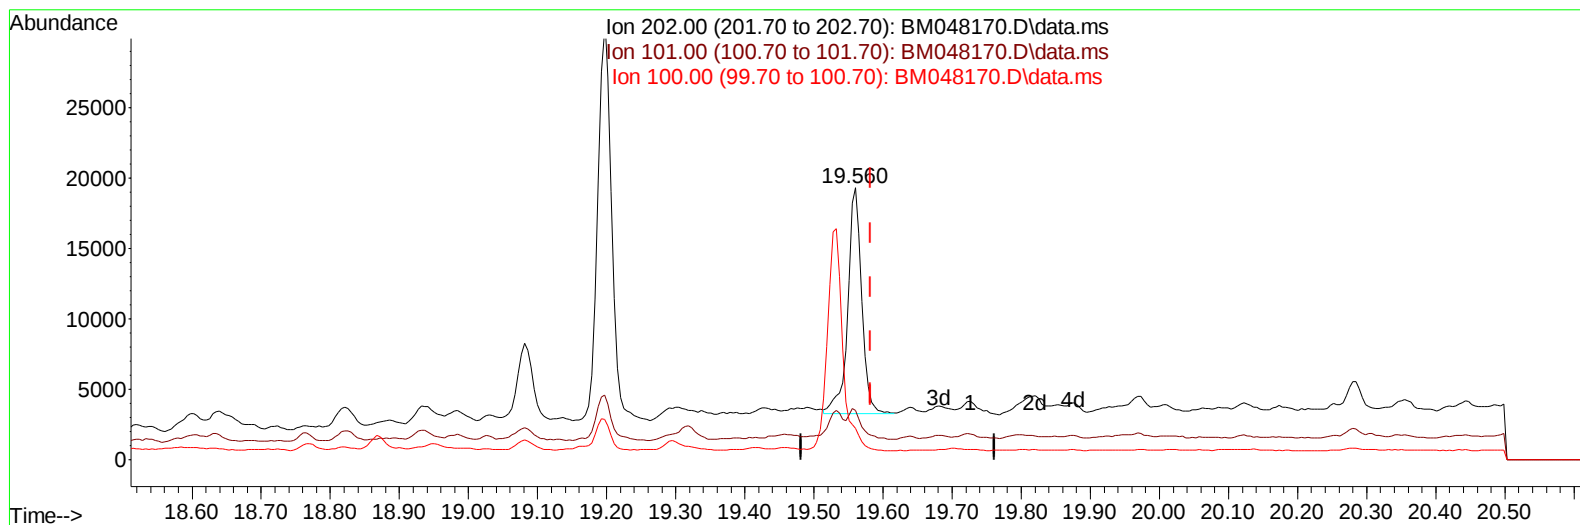

TIC: BM048170.D\data.ms

(20) Pyrene

19.560min (-0.022) 0.30 ng/ul m

response 22577

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	18.07#
100.00	10.10	11.51
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

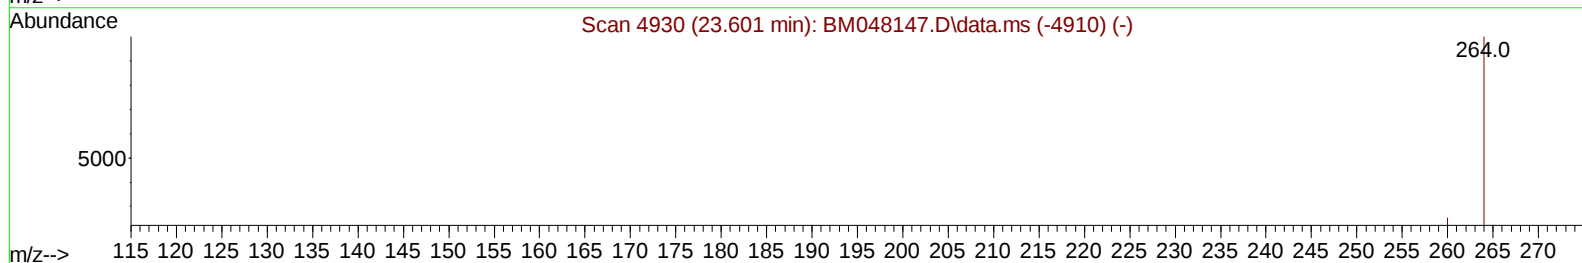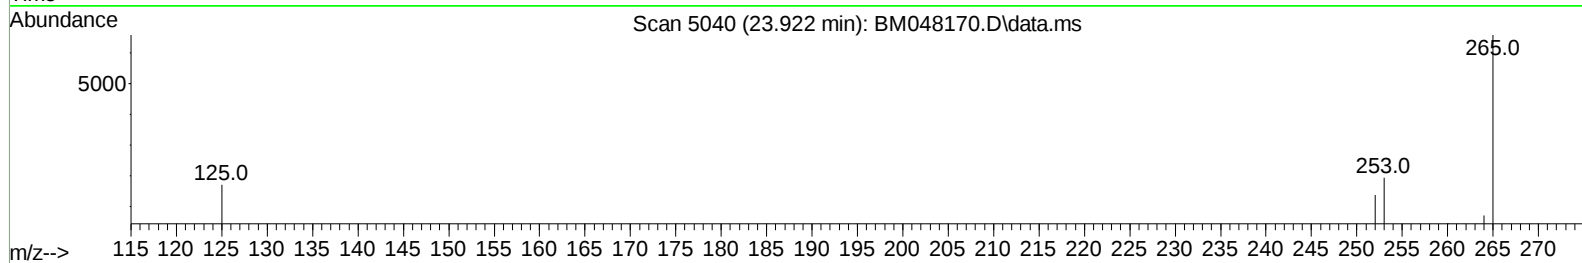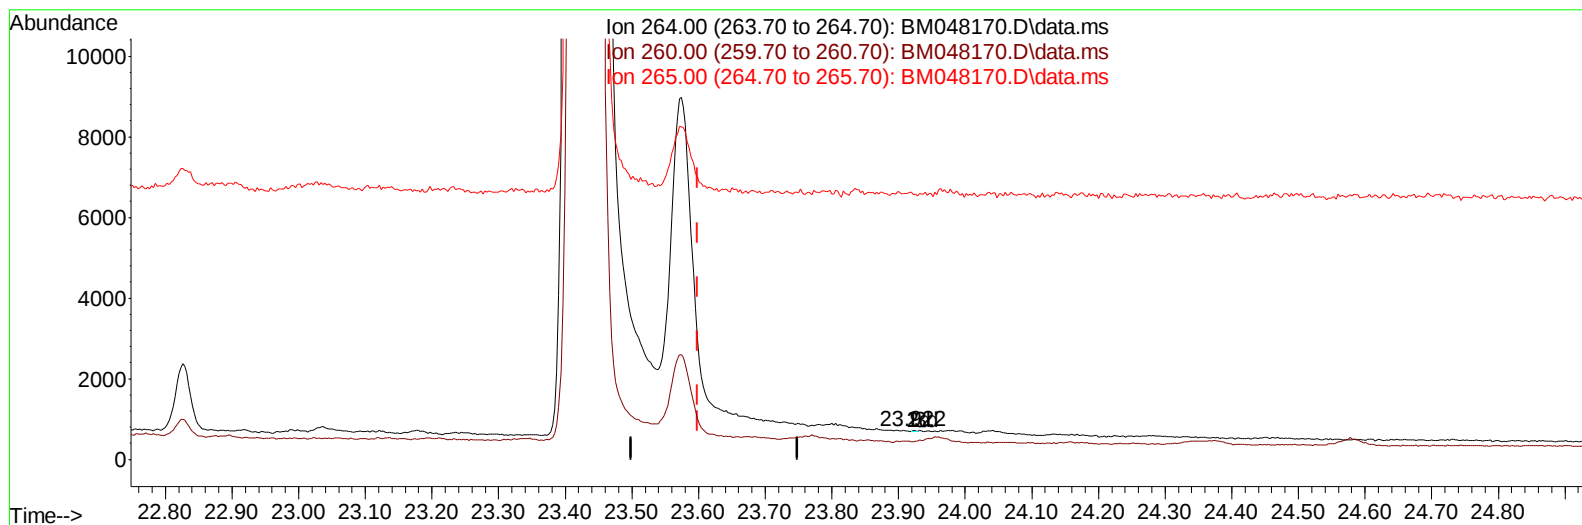

TIC: BM048170.D\data.ms

(23) Perylene-d12 (I)

23.922min (+ 0.324) 0.40 ng/u1

response 8

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	61.89#
265.00	128.10	913.91#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

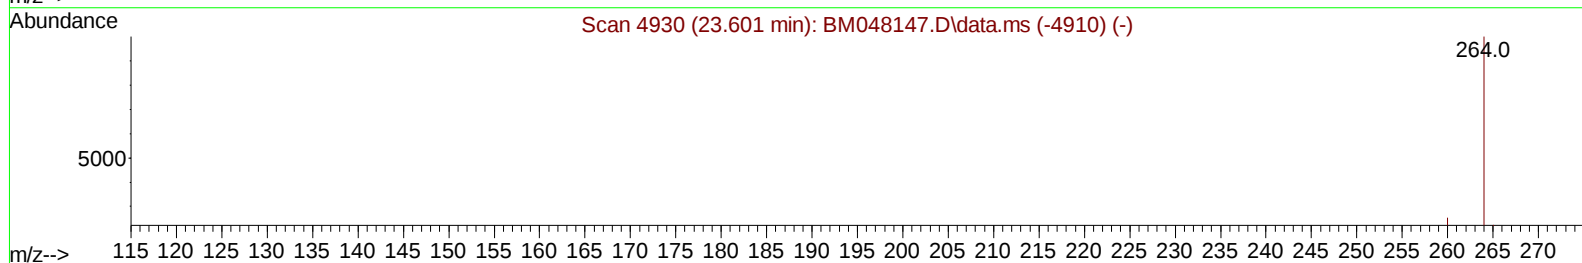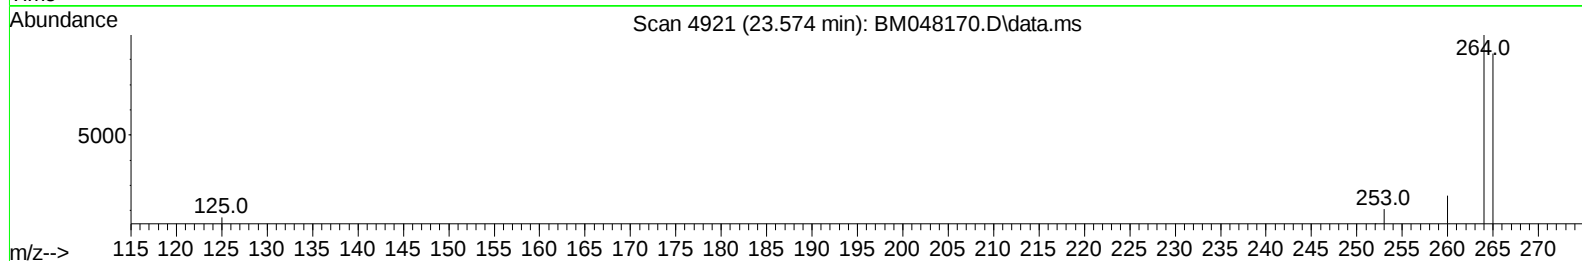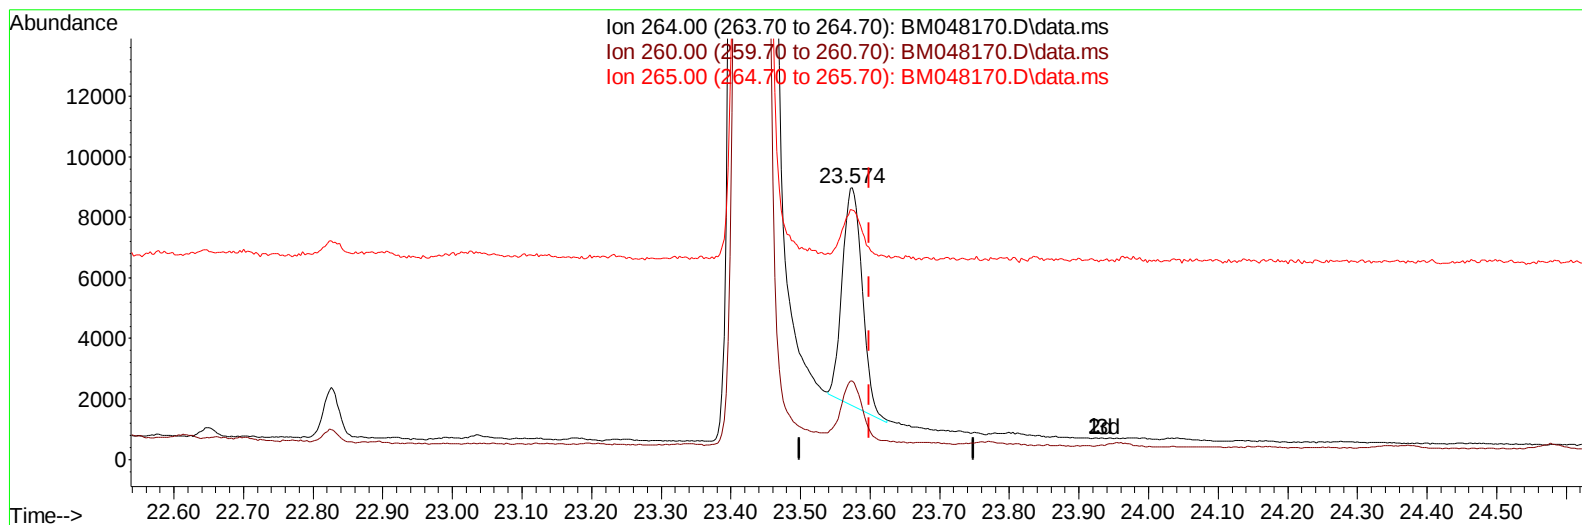

TIC: BM048170.D\data.ms

(23) Perylene-d12 (I)

23.574min (-0.024) 0.40 ng/ul m

response 14208

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	28.90
265.00	128.10	91.90#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048170.D
 Acq On : 22 Oct 2024 00:51
 Operator : RC/JU
 Sample : P4380-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27H3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 22 01:24:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 23:11:55 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.767	152		6537	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.552	136		20241	0.400	ng/ul	-0.04
9) Acenaphthene-d10	14.396	164		16753	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.141	188		22384m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.315	240		17682m	0.400	ng/ul	-0.02
23) Perylene-d12	23.574	264		14208m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.235	96		32870	3.699	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.146	152		11065	0.392	ng/ul	-0.05
18) Fluoranthene-d10	19.169	212		21202m	0.412	ng/ul	-0.02
Target Compounds							
							Qvalue
5) Naphthalene	10.601	128		1172257	21.310	ng/ul	96
7) 2-Methylnaphthalene	12.218	142		101007	3.209	ng/ul	98
8) 1-Methylnaphthalene	12.438	142		105370	2.909	ng/ul	98
10) Acenaphthylene	14.118	152		110917	1.433	ng/ul	99
11) Acenaphthene	14.465	153		74076	1.339	ng/ul	98
12) Fluorene	15.450	166		104339	1.761	ng/ul	98
14) Pentachlorophenol	16.804	266		1307m	0.174	ng/ul	
15) Phenanthrene	17.183	178		191678m	3.388	ng/ul	
16) Anthracene	17.272	178		26939m	0.503	ng/ul	
19) Fluoranthene	19.197	202		39777m	0.573	ng/ul	
20) Pyrene	19.560	202		22577m	0.303	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048170.D
Acq On : 22 Oct 2024 00:51
Operator : RC/JU
Sample : P4380-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27H3

Manual IntegrationsAPPROVED

Quant Time: Oct 22 01:24:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

