




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

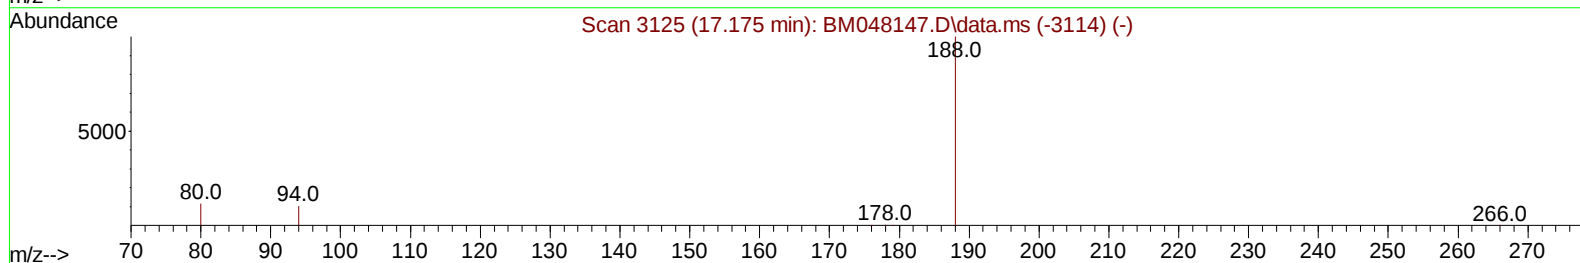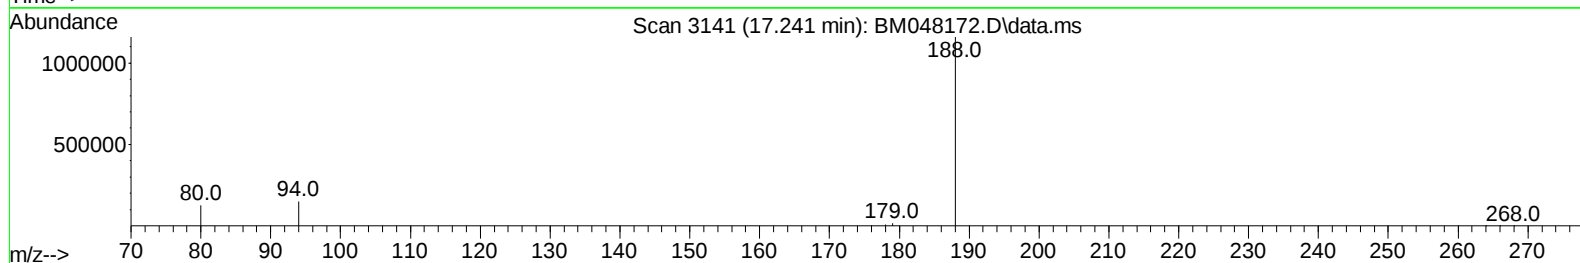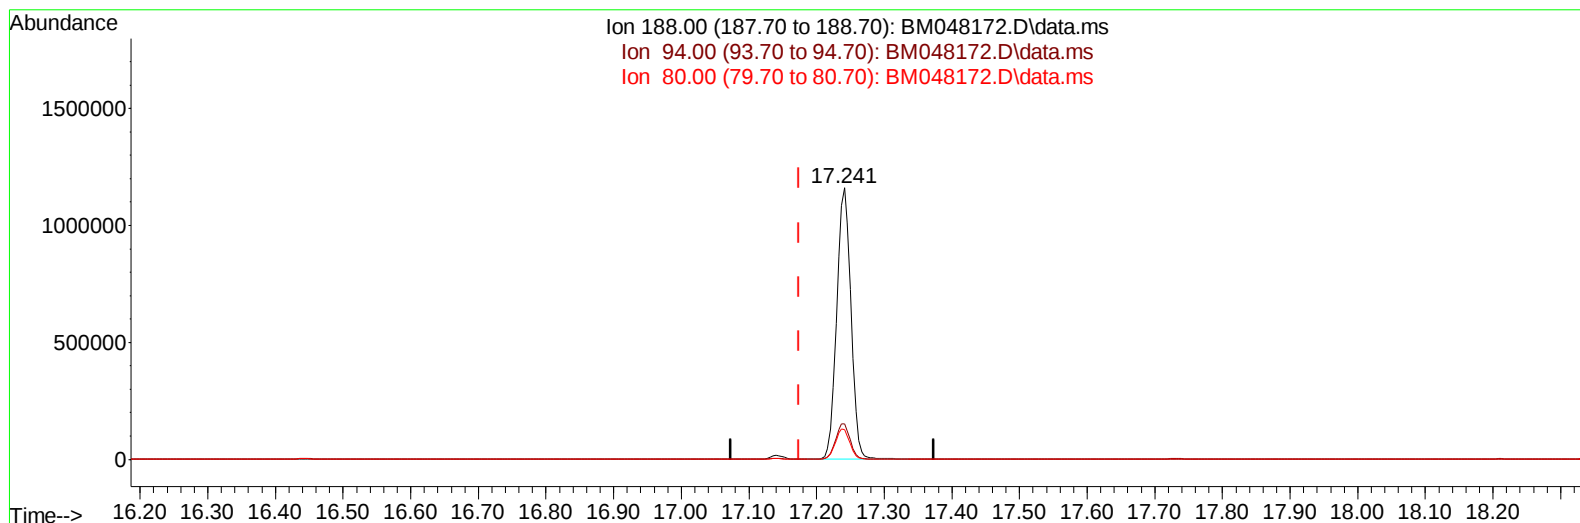

TIC: BM048172.D\data.ms

(13) Phenanthrene-d10 (I)

17.241min (+ 0.068) 0.40 ng/u1

response 1706432

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	13.07
80.00	12.40	10.88
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

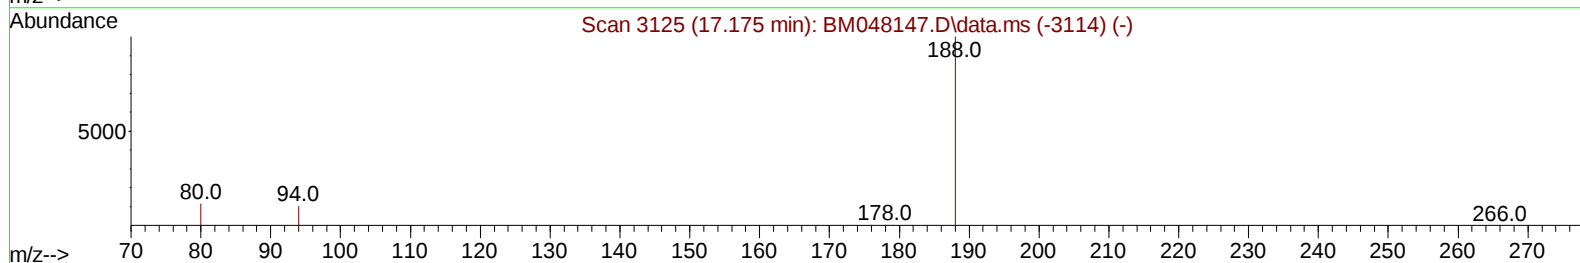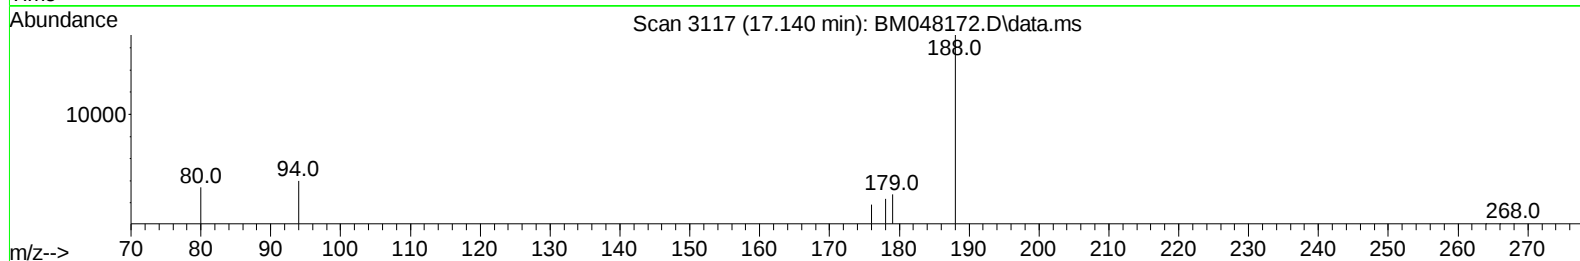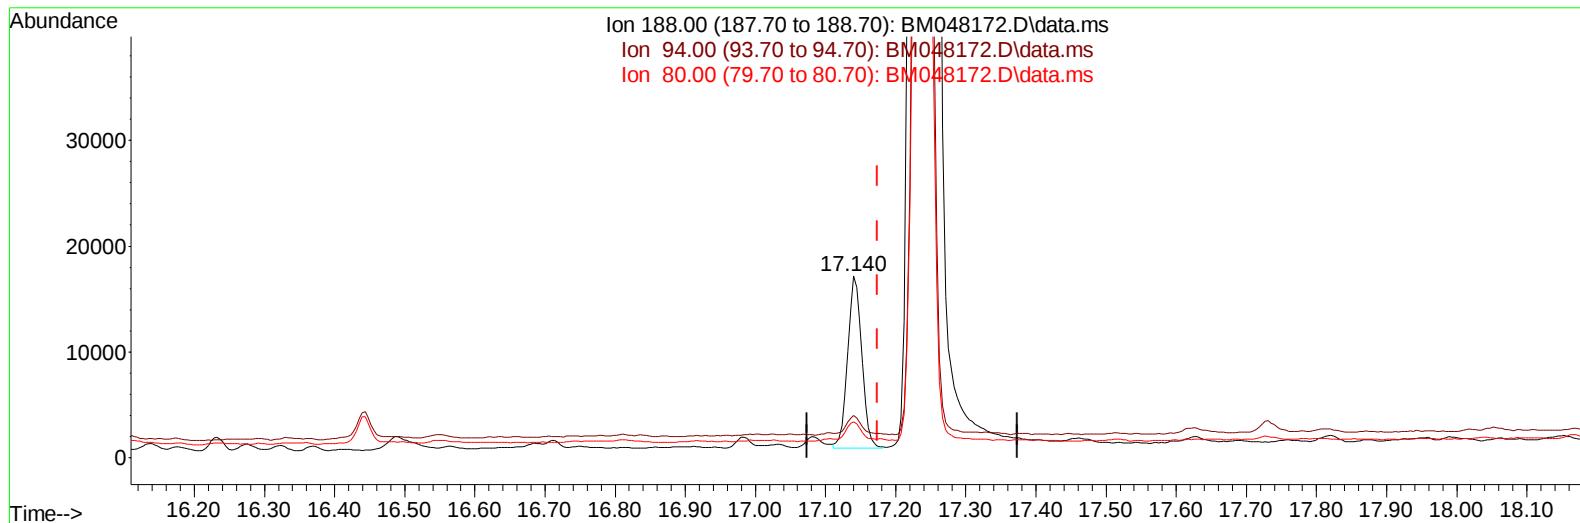

TIC: BM048172.D\data.ms

(13) Phenanthrene-d10 (I)

17.140min (-0.034) 0.40 ng/u1 m

response 22949

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	23.02#
80.00	12.40	19.63#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

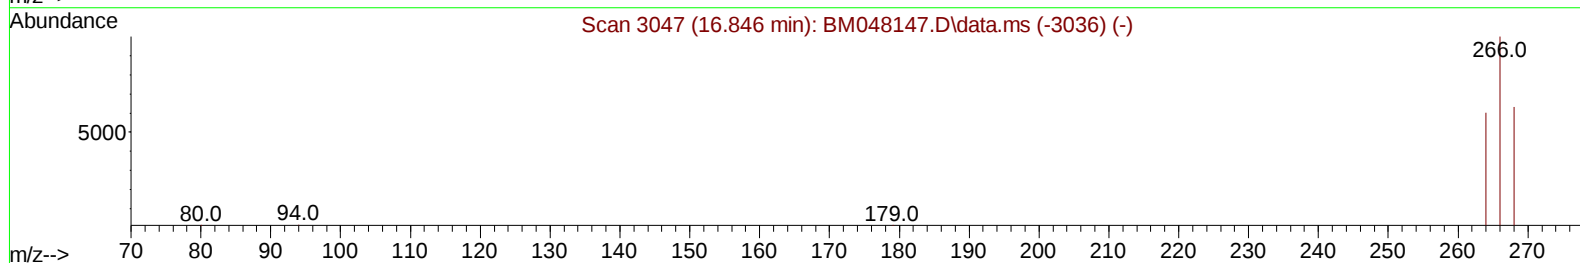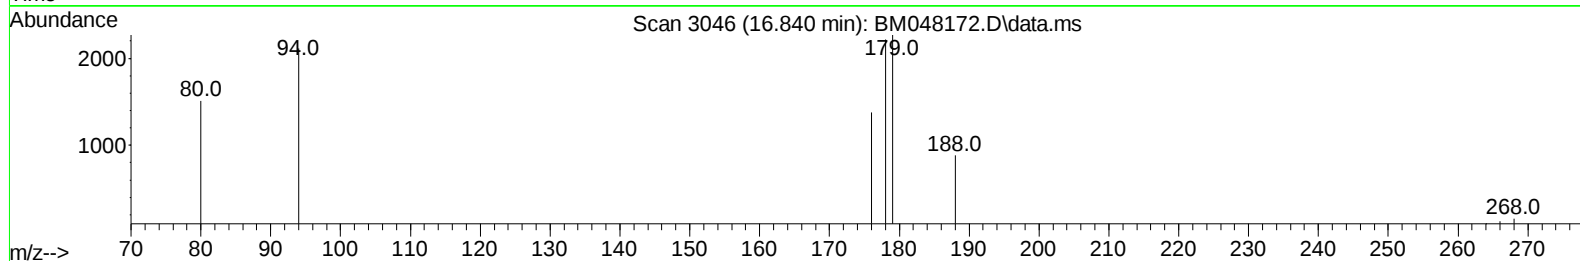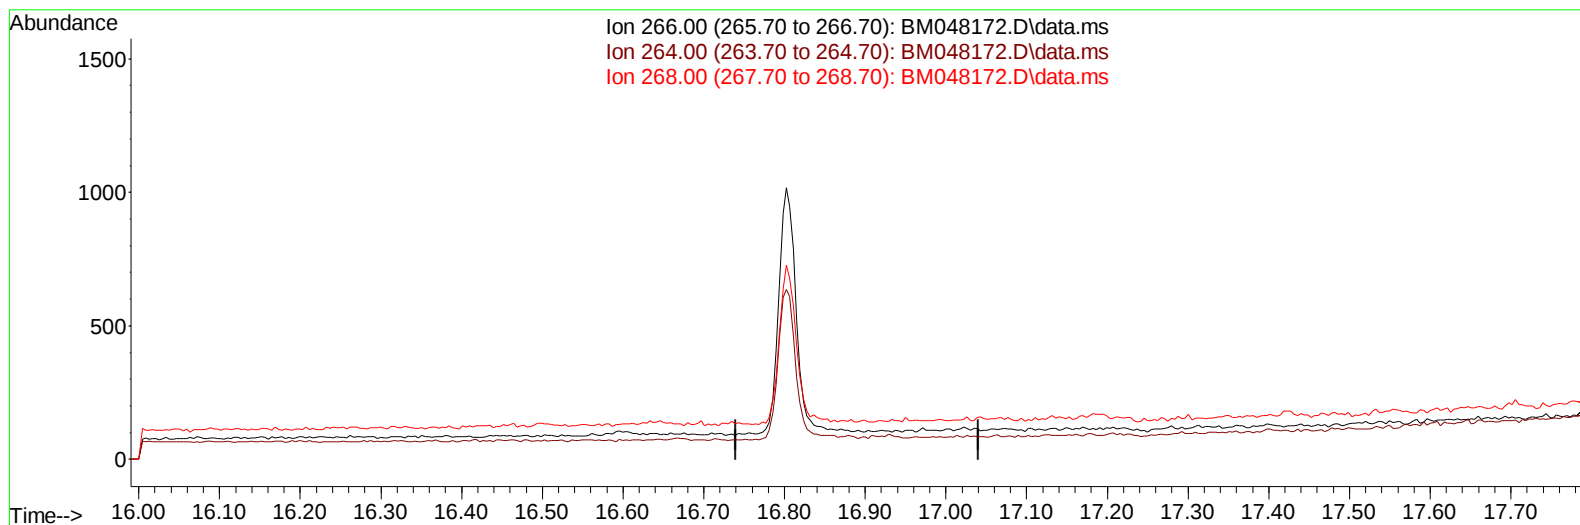

TIC: BM048172.D\data.ms

(14) Pentachlorophenol

16.840min (-16.840) 0.00 ng/ul

response 0

Ion	Exp%	Act%
266.00	100.00	0.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

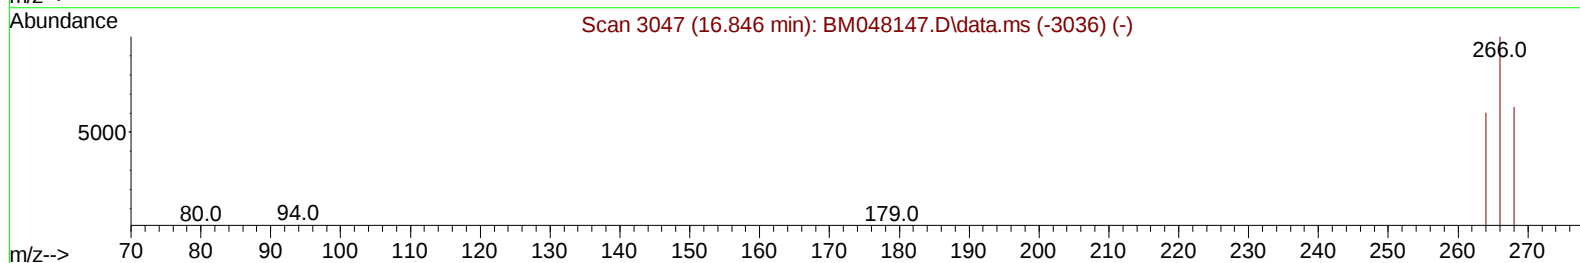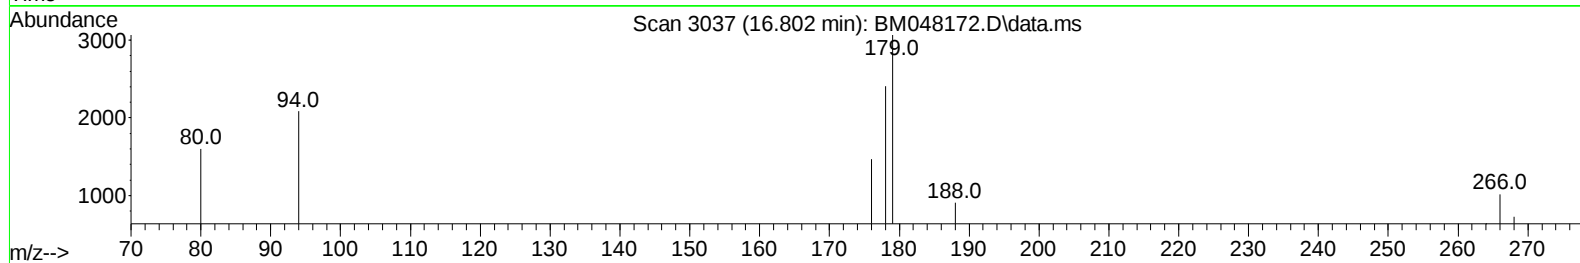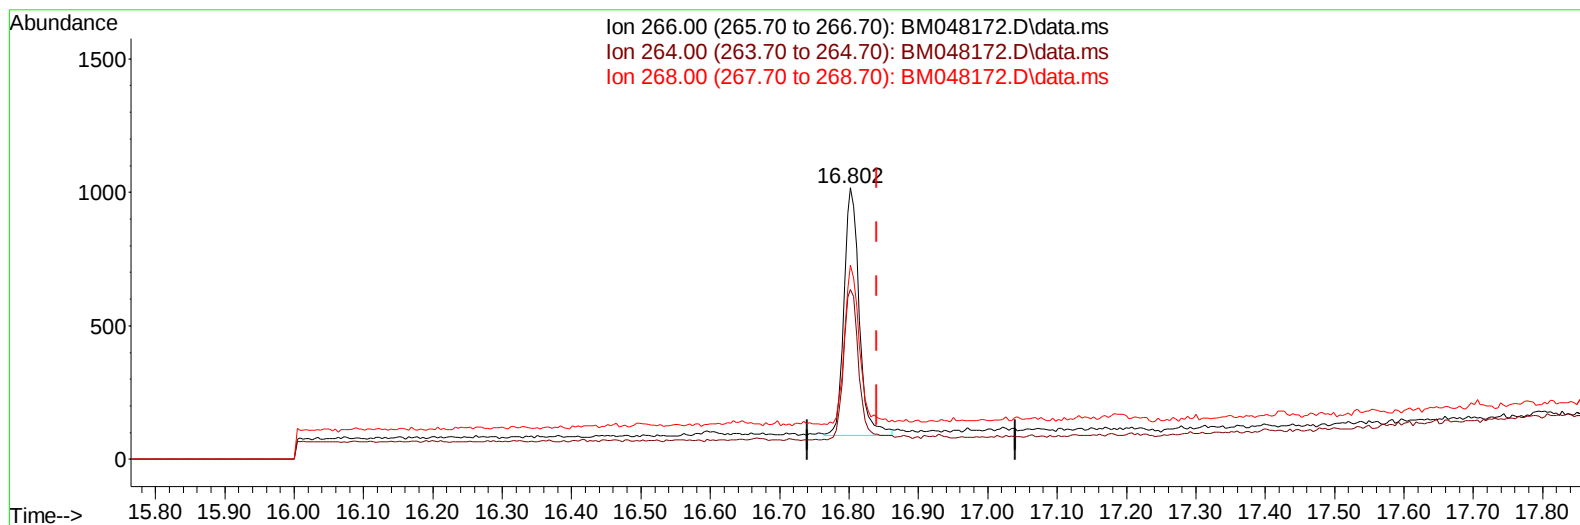

TIC: BM048172.D\data.ms

(14) Pentachlorophenol

16.802min (-0.038) 0.18 ng/u1 m

response 1401

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.70	0.00#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

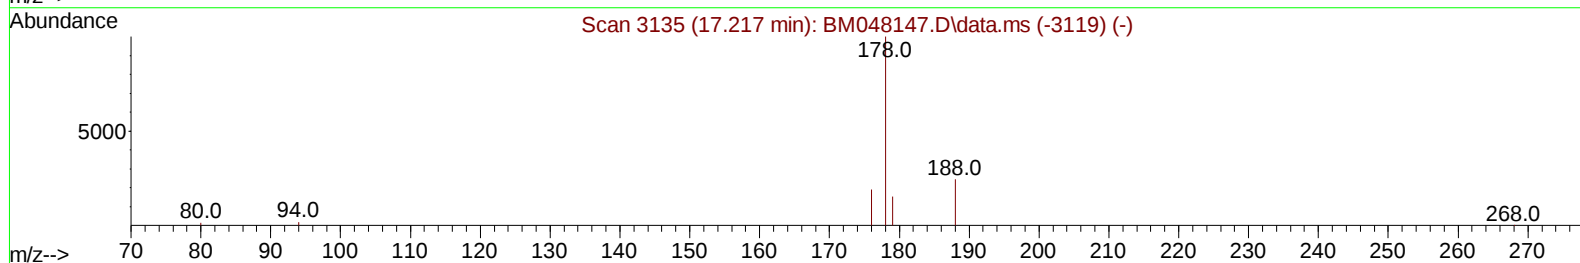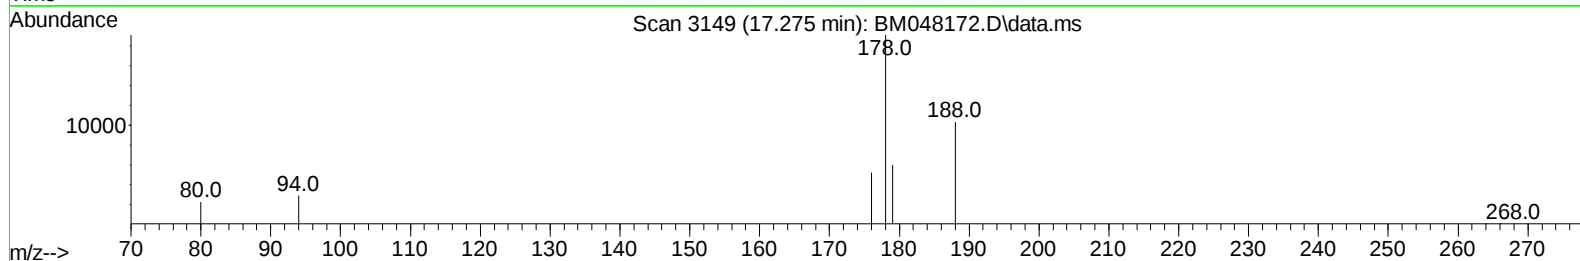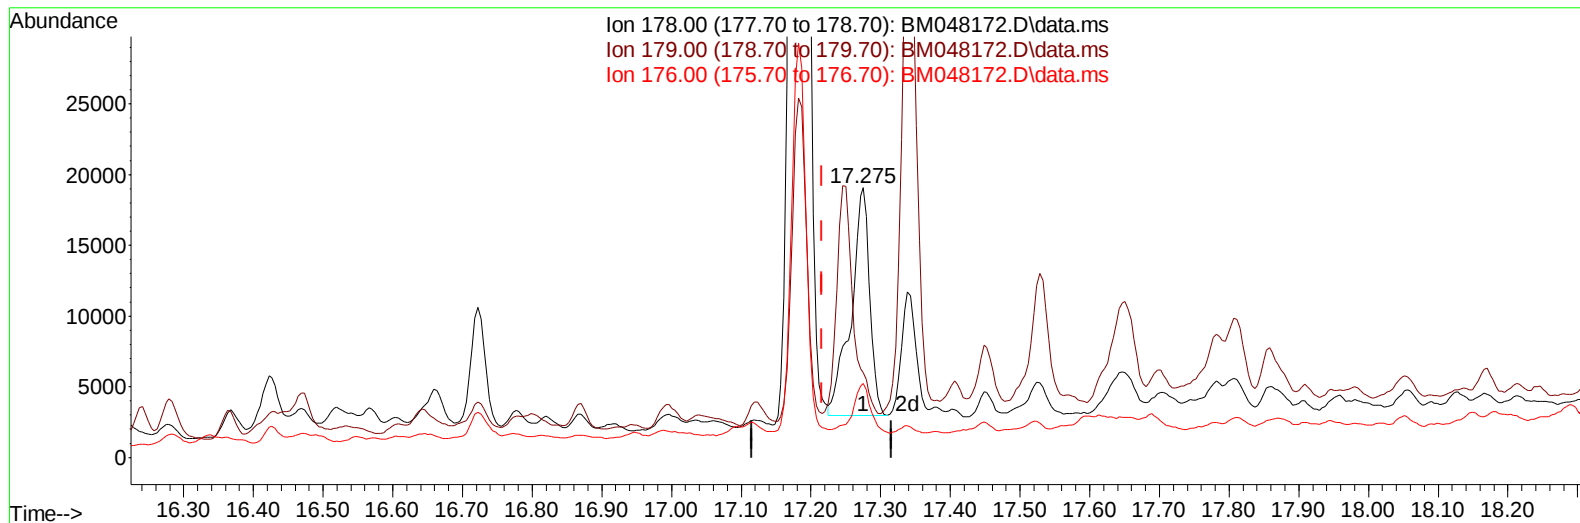

TIC: BM048172.D\data.ms

(15) Phenanthrene

17.275min (+ 0.059) 0.52 ng/u1

response 29934

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	31.40#
176.00	20.00	27.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048172.D
 Acq On : 22 Oct 2024 02:04
 Operator : RC/JU
 Sample : P4380-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 23:11:55 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

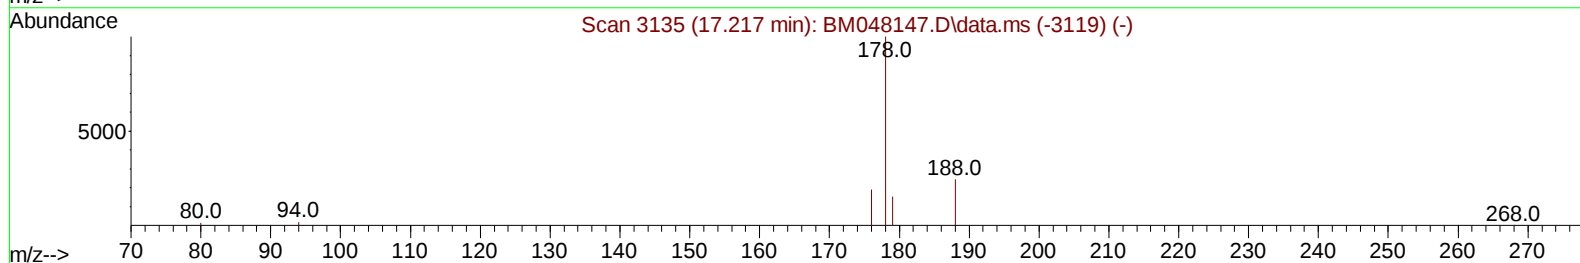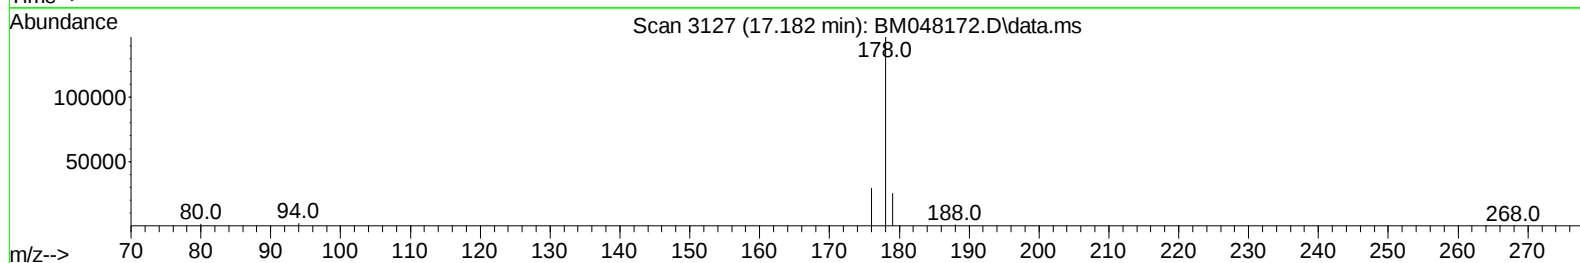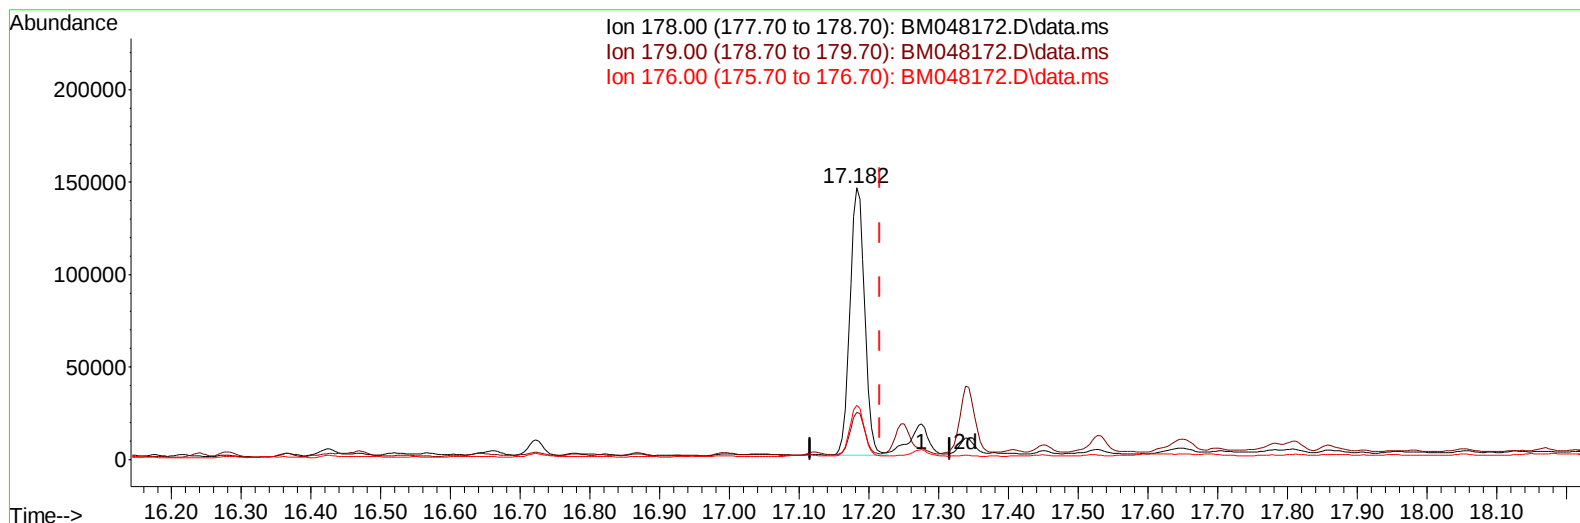

TIC: BM048172.D\data.ms

(15) Phenanthrene

17.182min (-0.034) 3.65 ng/u1 m

response 211774

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	17.31
176.00	20.00	19.95
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

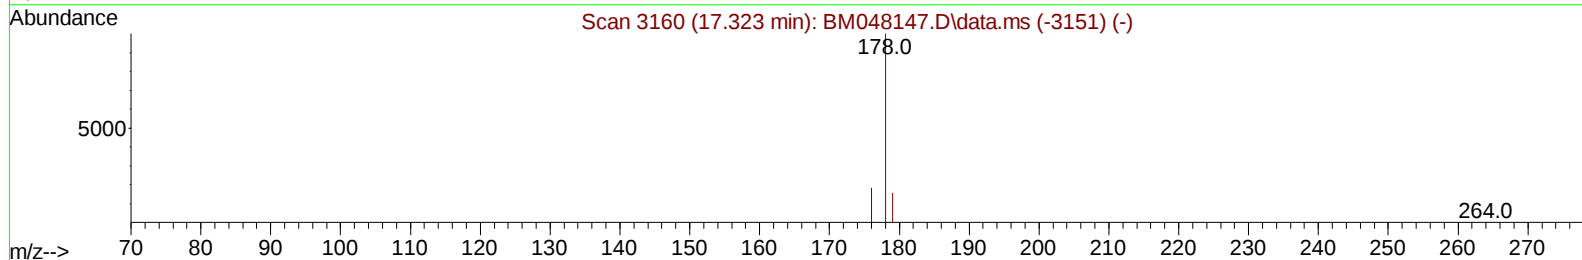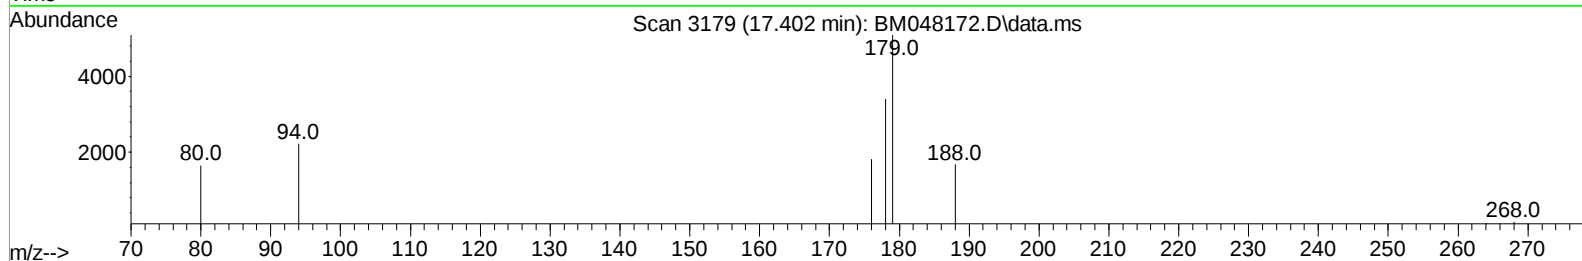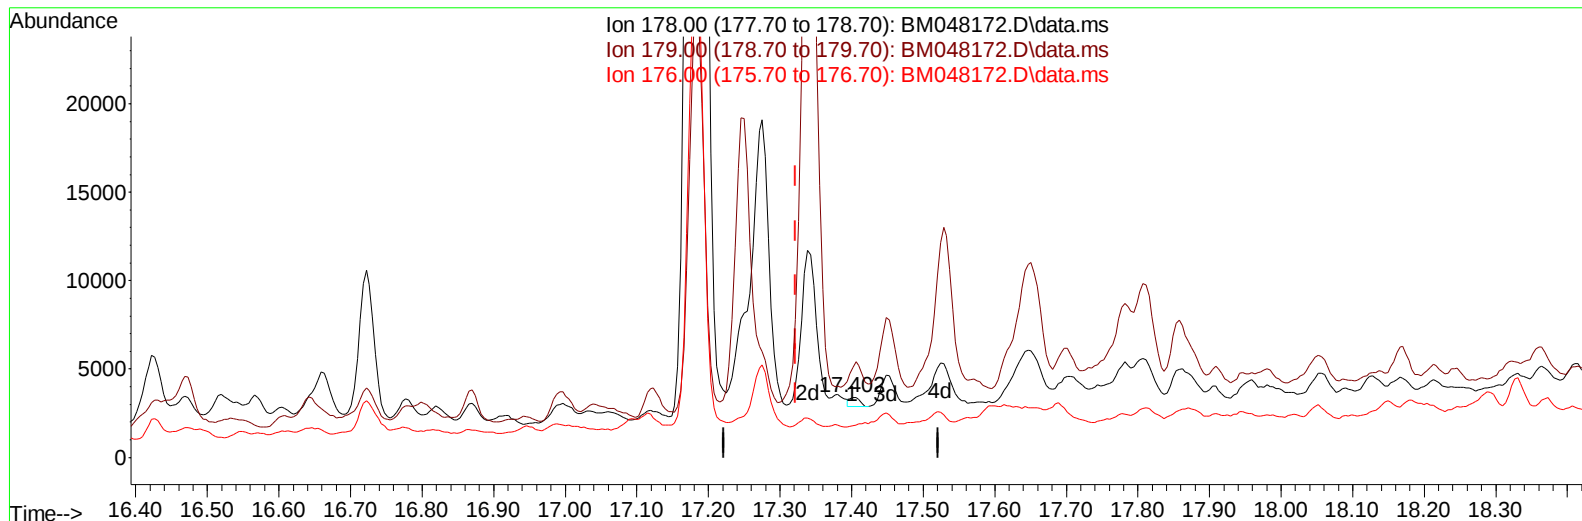

TIC: BM048172.D\data.ms

(16) Anthracene

17.402min (+ 0.080) 0.01 ng/u1

response 510

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	149.53#
176.00	20.00	53.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

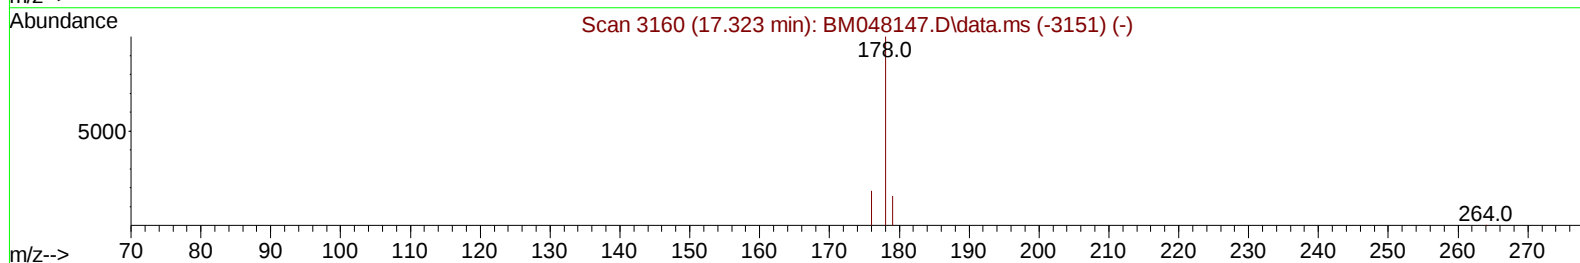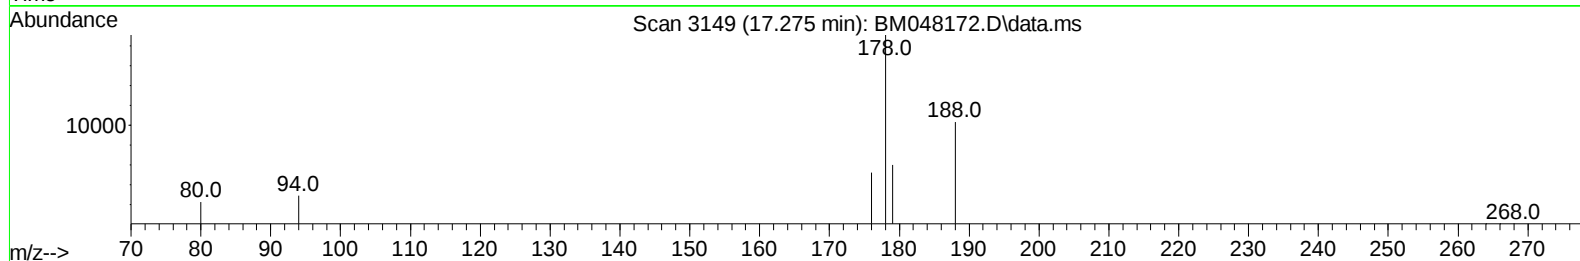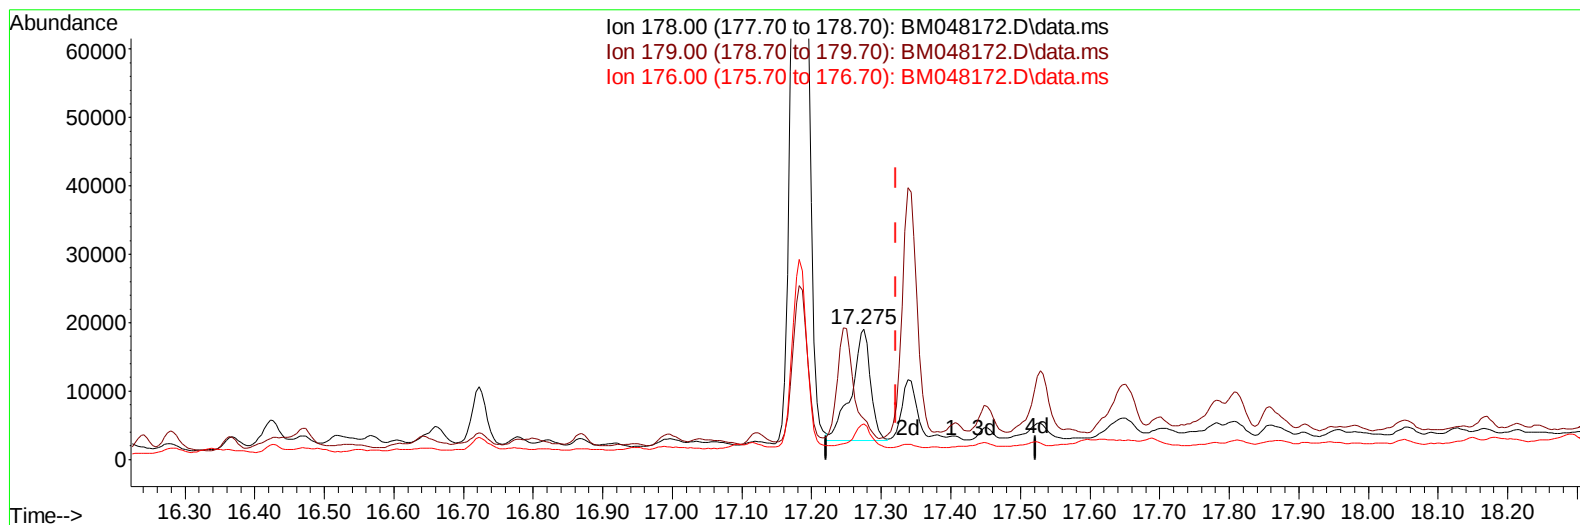

TIC: BM048172.D\data.ms

(16) Anthracene

17.275min (-0.046) 0.57 ng/ul m

response 31142

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	31.40#
176.00	20.00	27.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

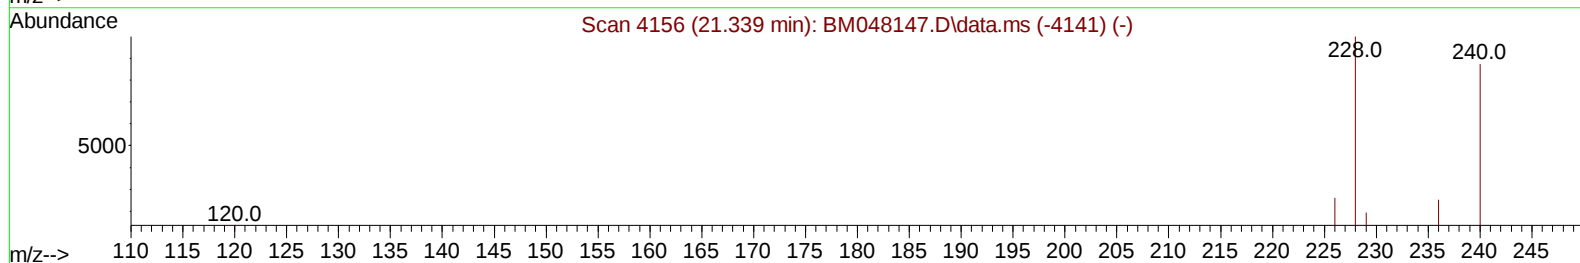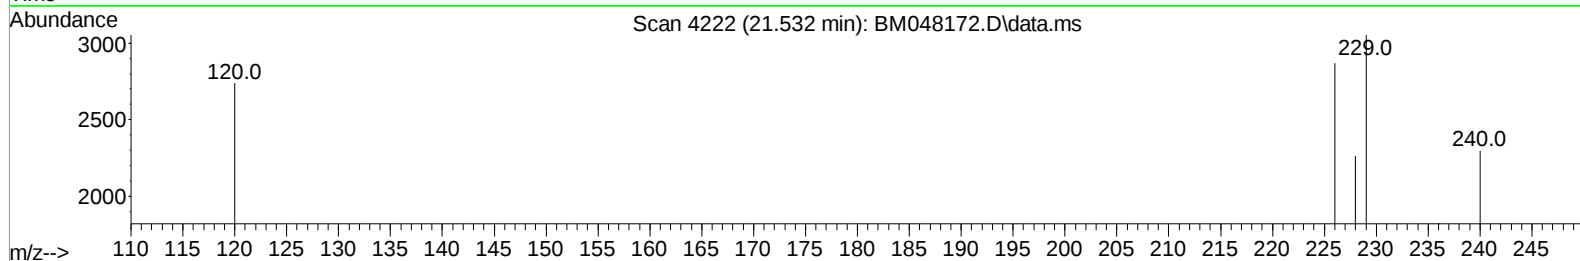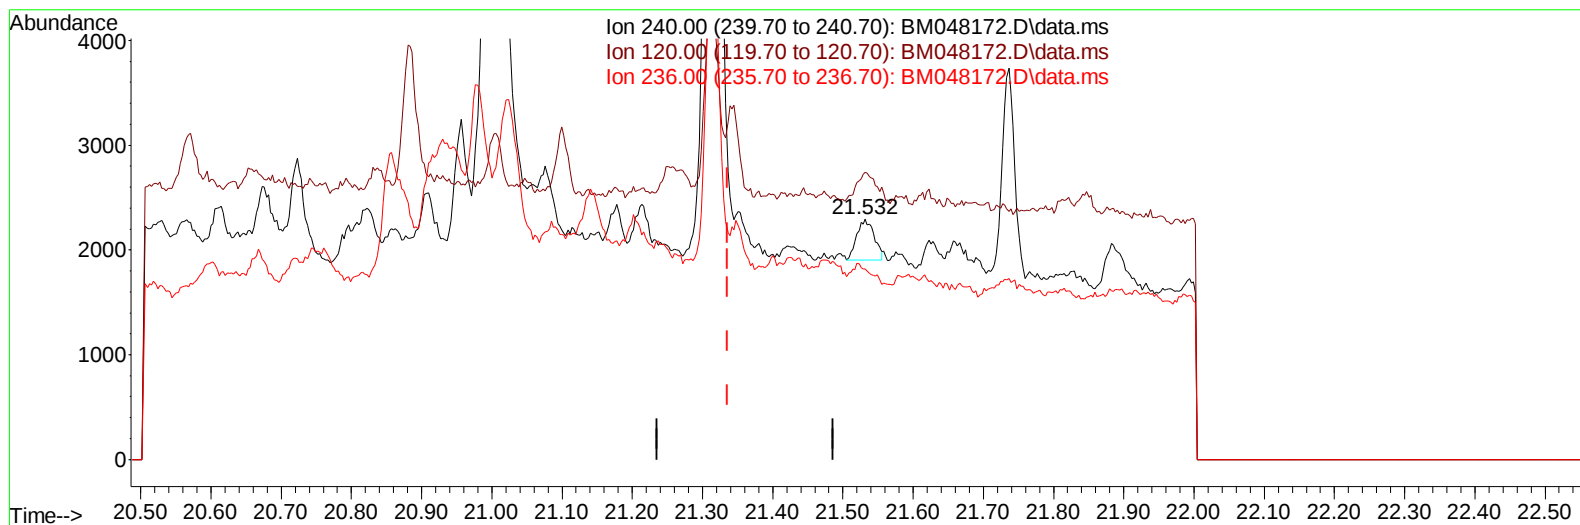

TIC: BM048172.D\data.ms

(17) Chrysene-d12

21.532min (+ 0.196) 0.40 ng/u1

response 664

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	119.24#
236.00	30.60	79.19#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

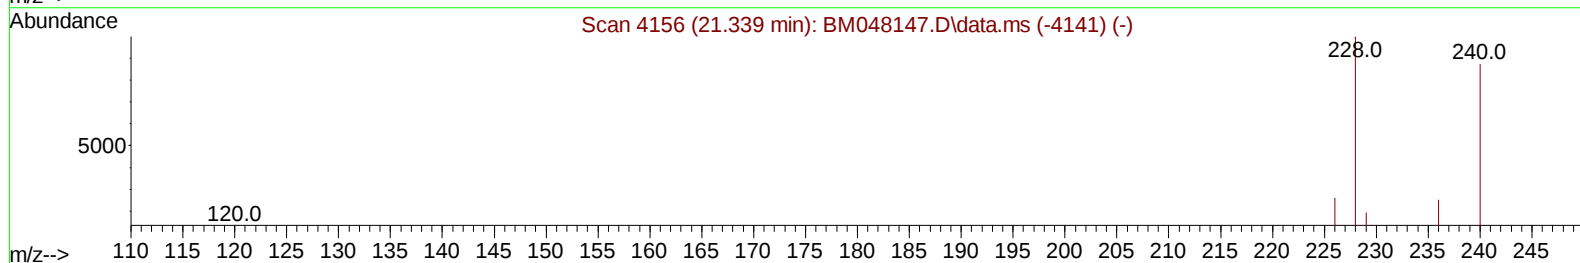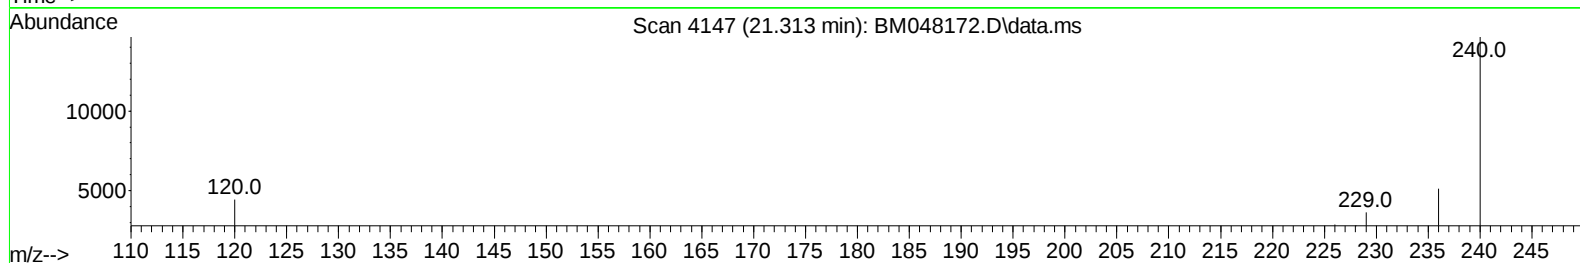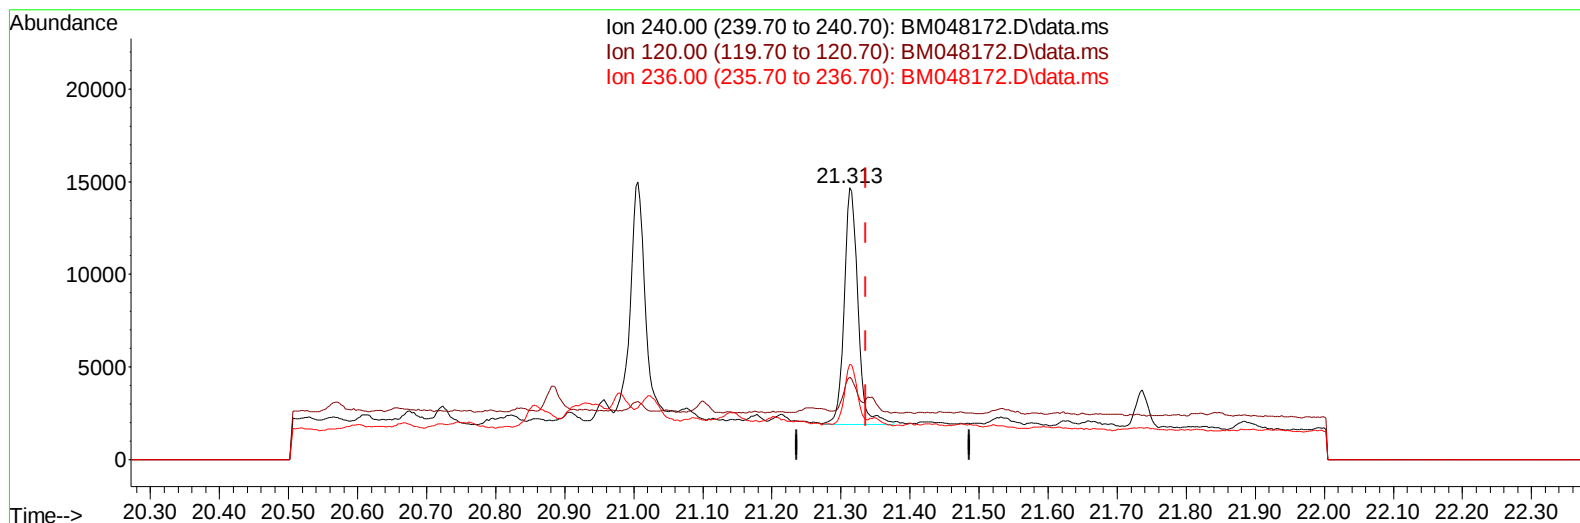

TIC: BM048172.D\data.ms

(17) Chrysene-d12

21.313min (-0.023) 0.40 ng/u1 m

response 17737

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	30.25#
236.00	30.60	34.91
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

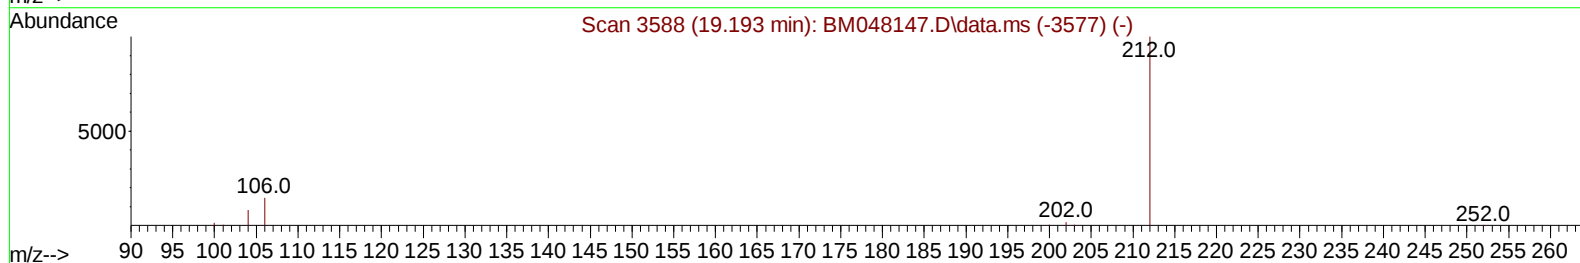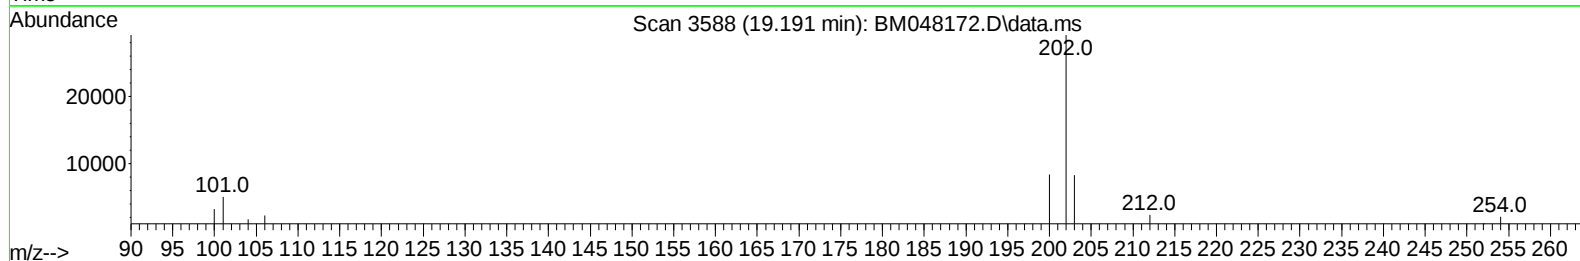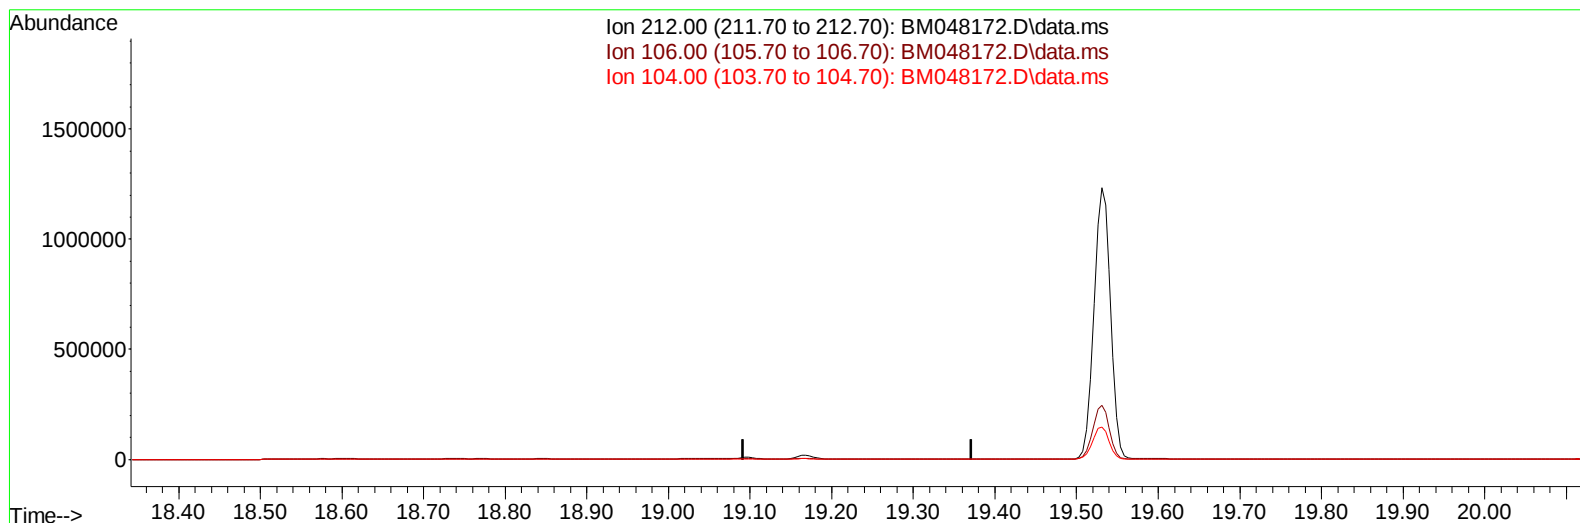

TIC: BM048172.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.191min (-19.191) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

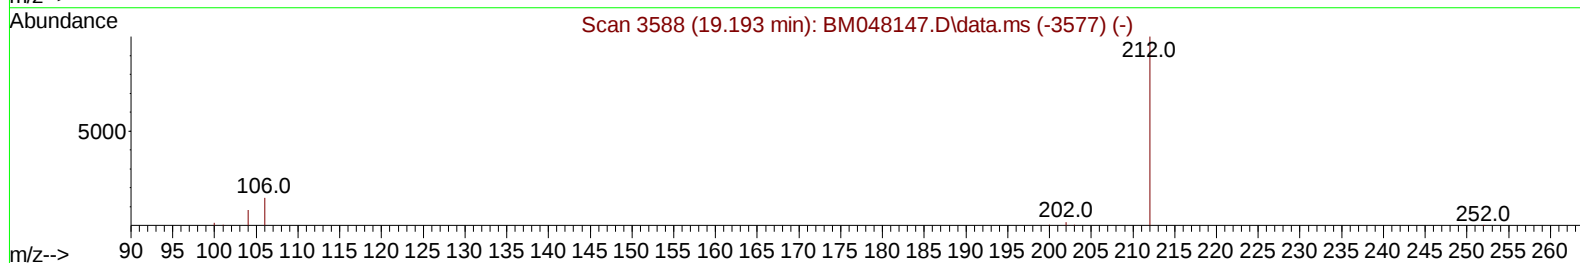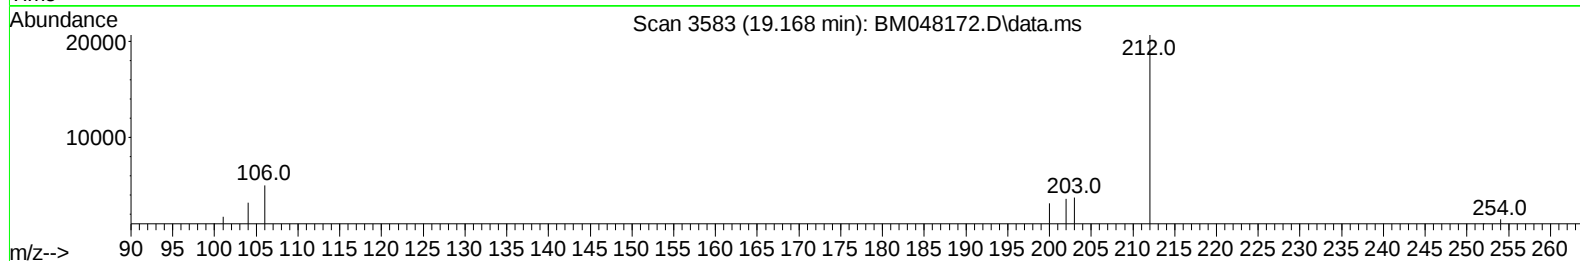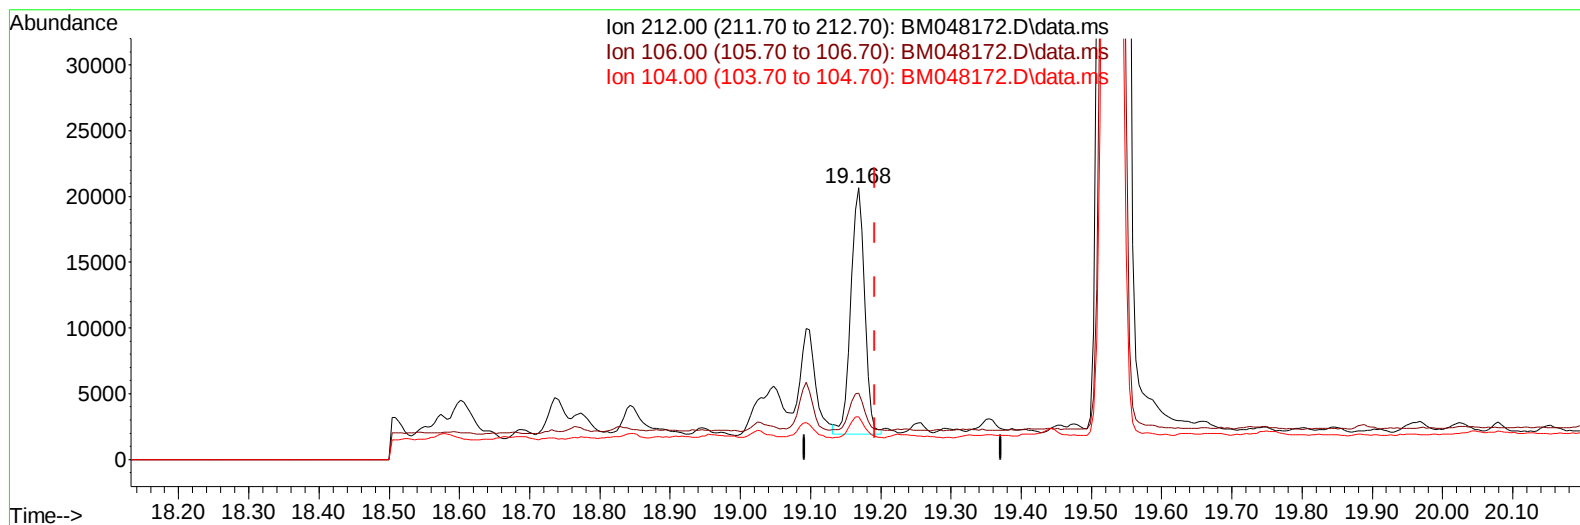

TIC: BM048172.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.168min (-0.023) 0.49 ng/u1 m

response 25268

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

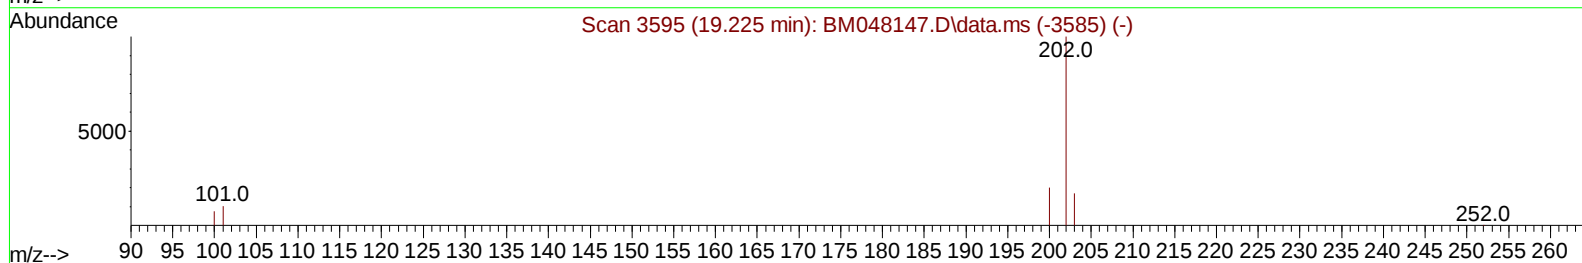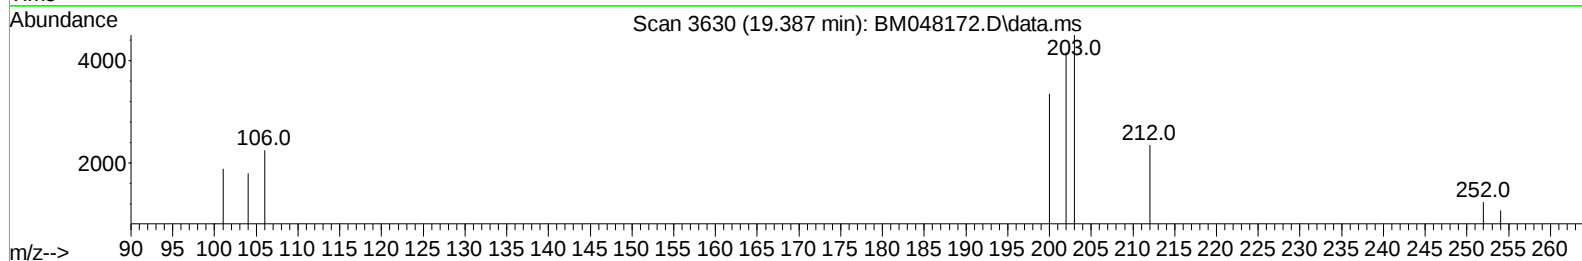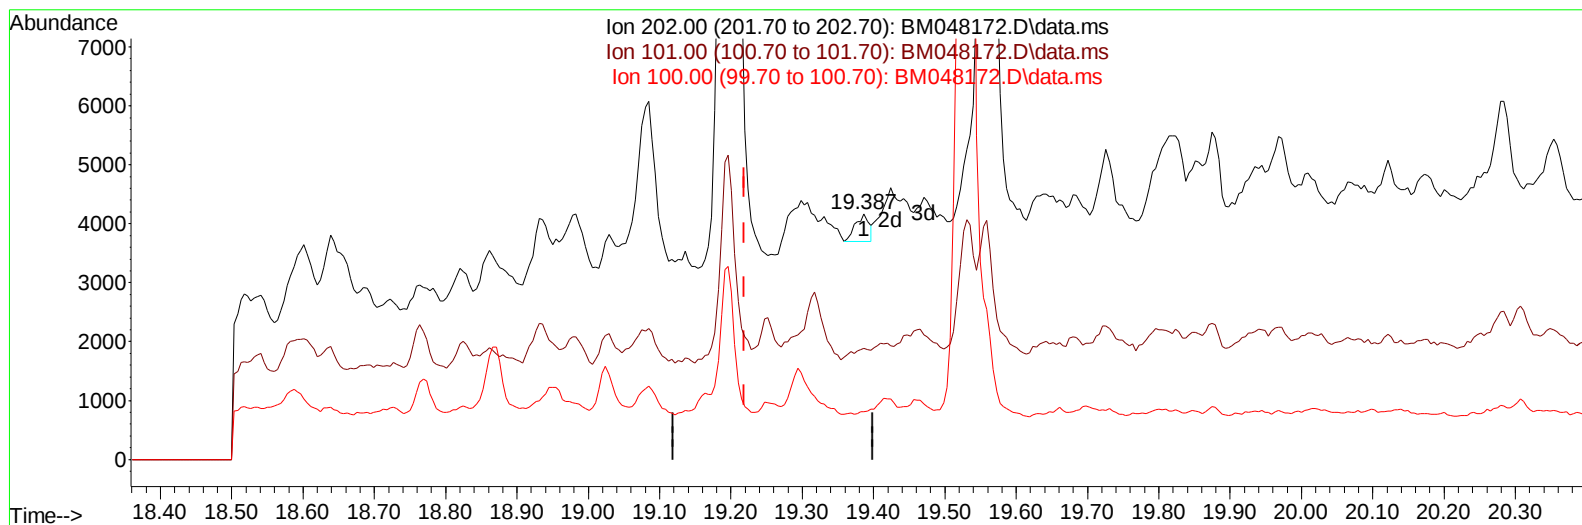

TIC: BM048172.D\data.ms

(19) Fluoranthene (C)

19.387min (+ 0.167) 0.01 ng/u1

response 610

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	45.25#
100.00	8.90	19.49#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

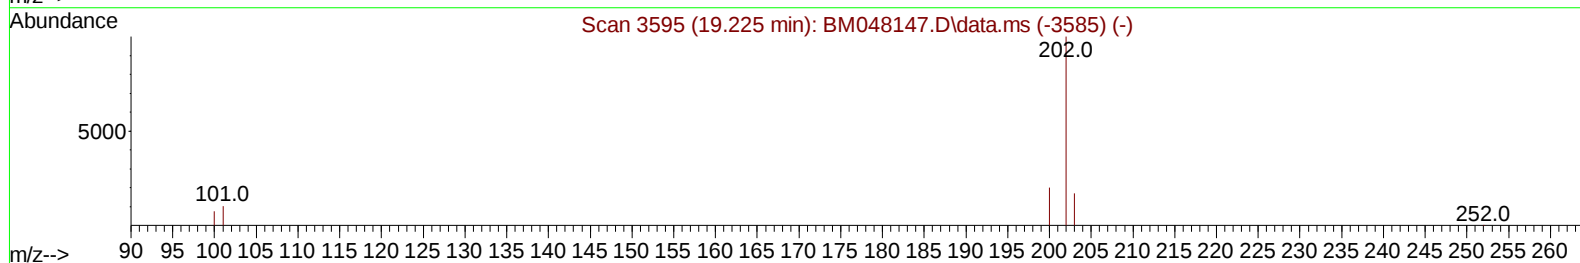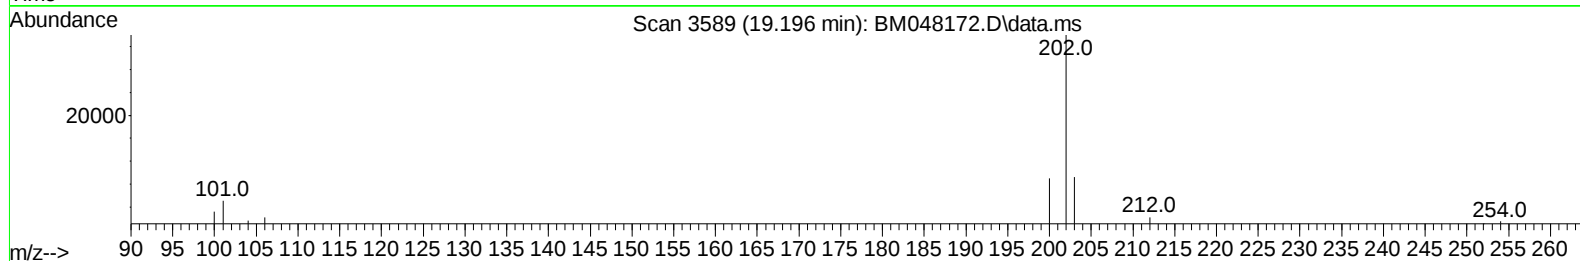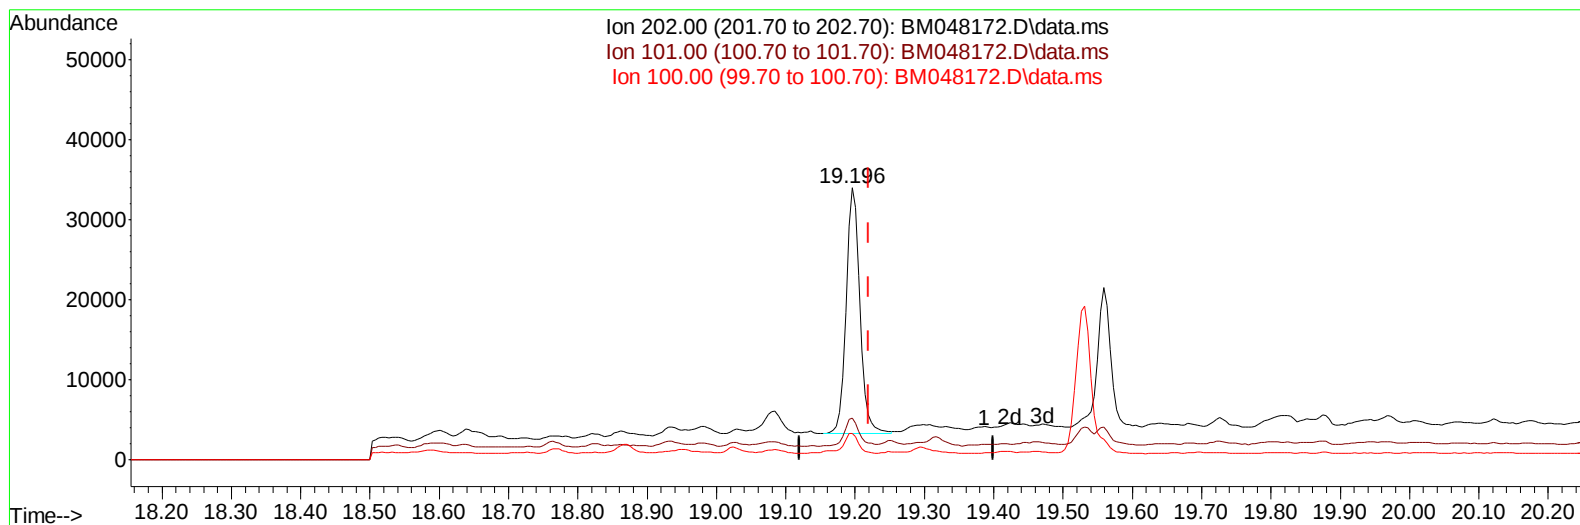

TIC: BM048172.D\data.ms

(19) Fluoranthene (C)

19.196min (-0.023) 0.61 ng/ul m

response 42714

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	15.20#
100.00	8.90	9.63
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

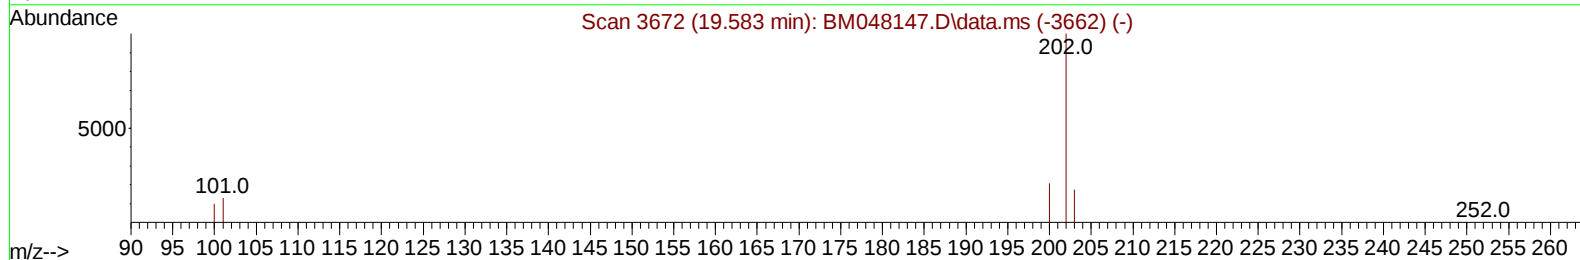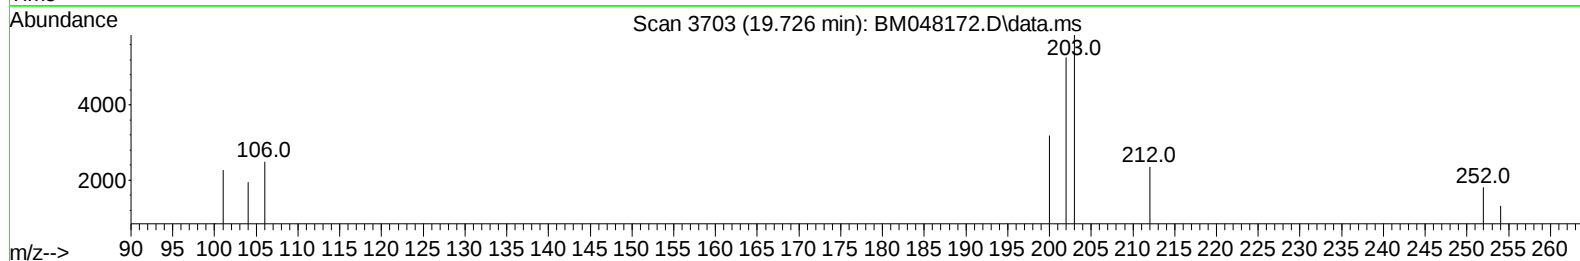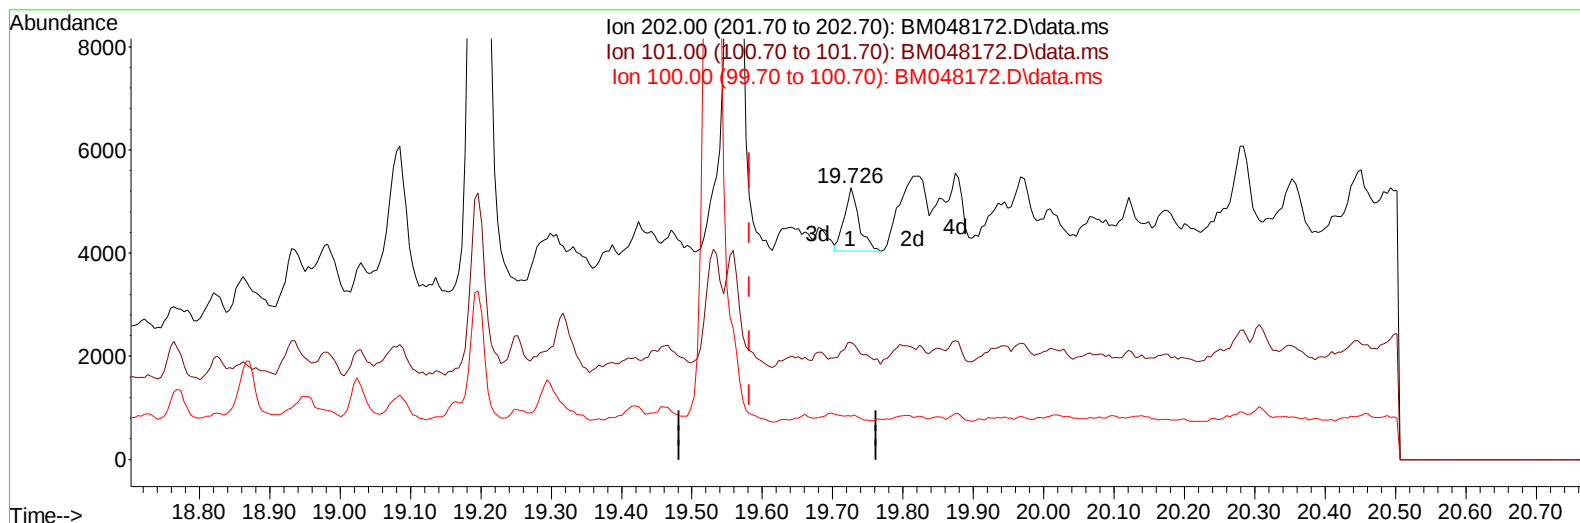

TIC: BM048172.D\data.ms

(20) Pyrene

19.726min (+ 0.144) 0.02 ng/u1

response 1759

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	42.94#
100.00	10.10	15.88#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

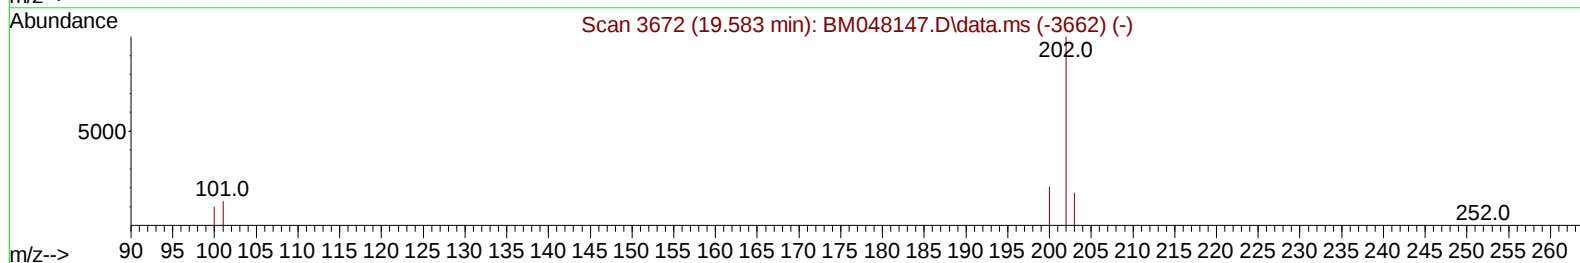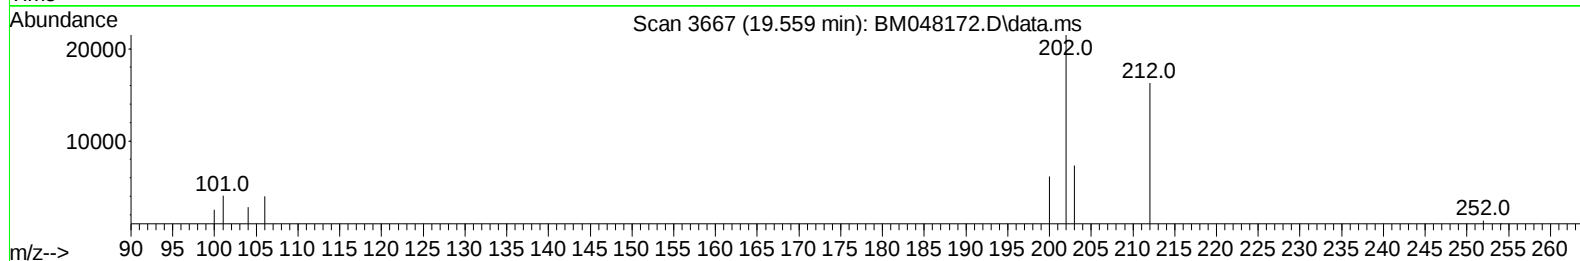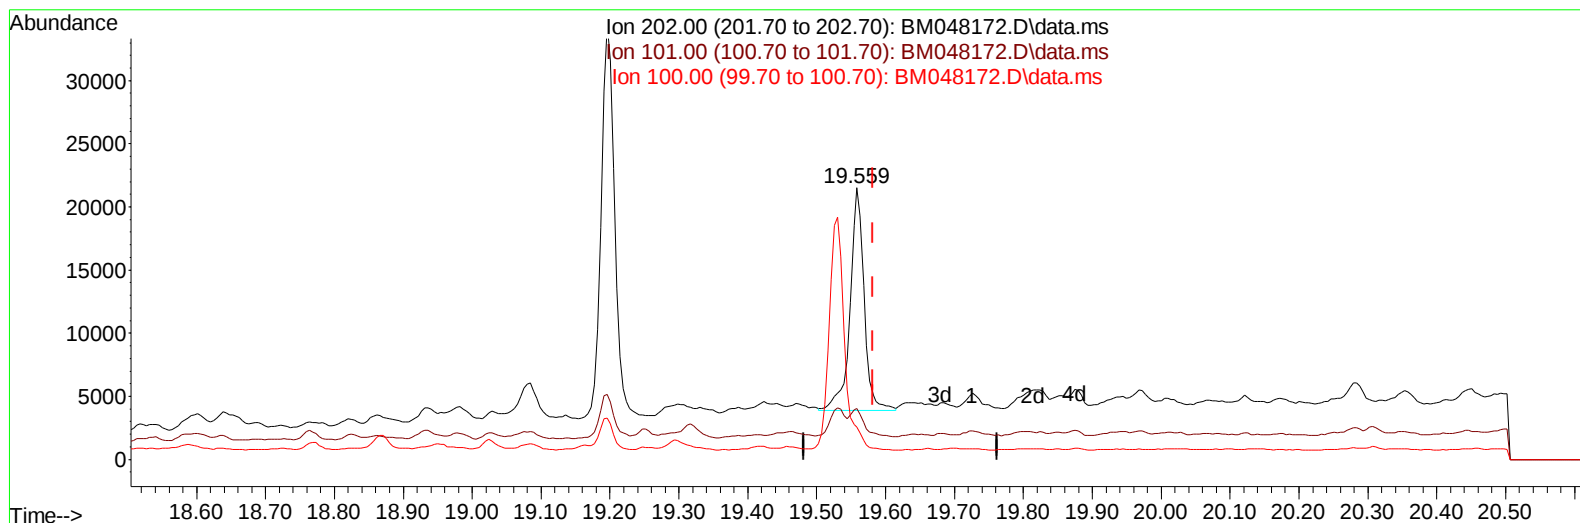

TIC: BM048172.D\data.ms

(20) Pyrene

19.559min (-0.023) 0.33 ng/u1 m

response 24775

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	18.86#
100.00	10.10	11.83
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

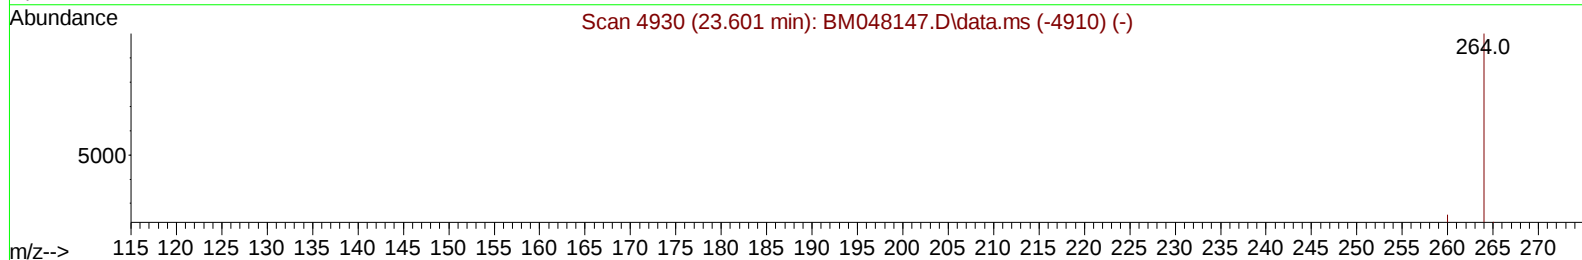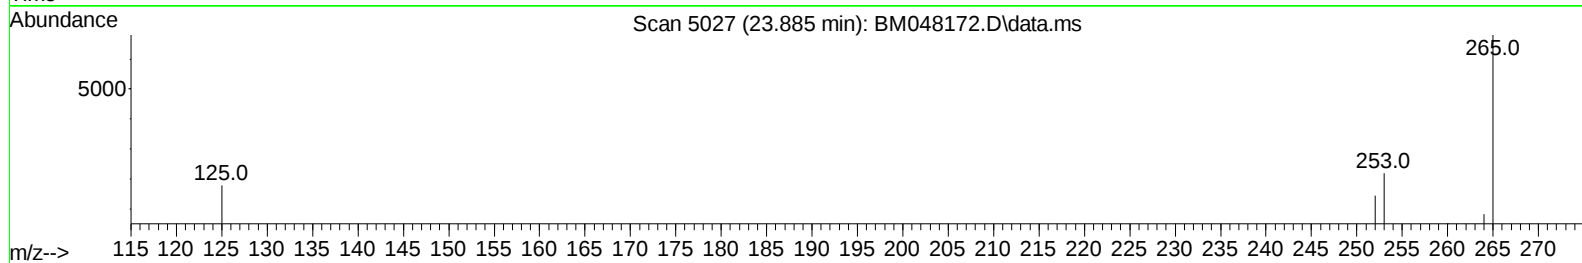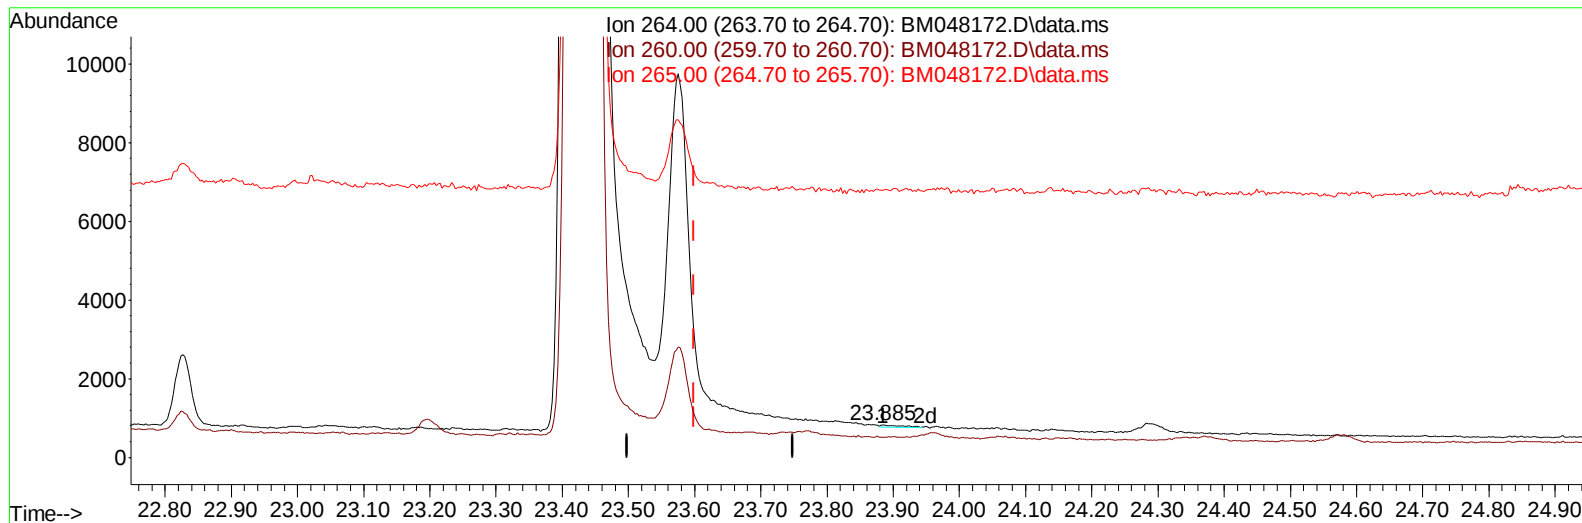

TIC: BM048172.D\data.ms

(23) Perylene-d12 (I)

23.885min (+ 0.286) 0.40 ng/u1

response 137

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	62.24#
265.00	128.10	820.02#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

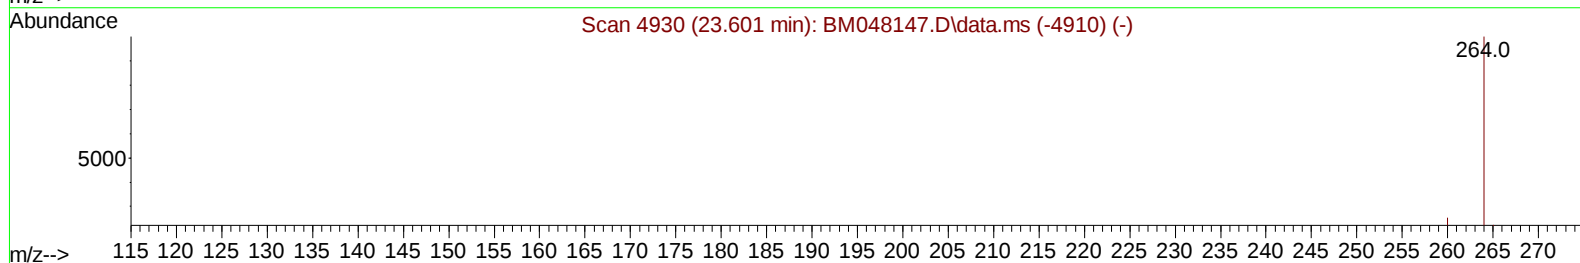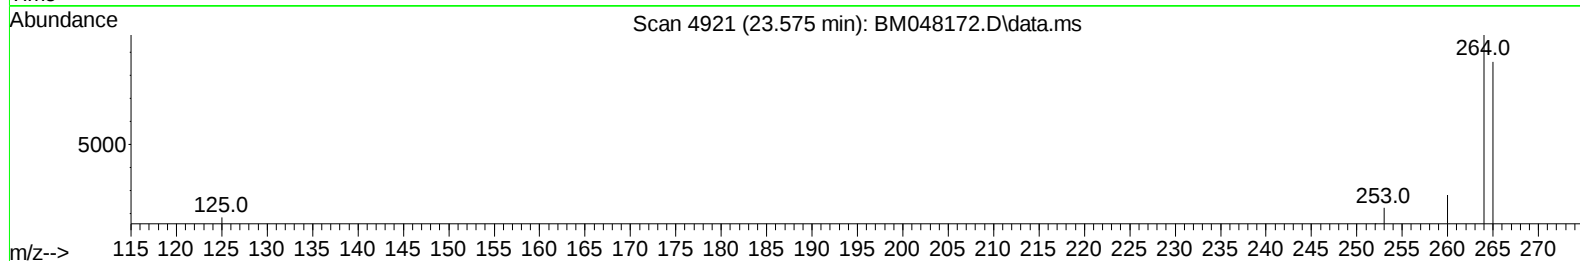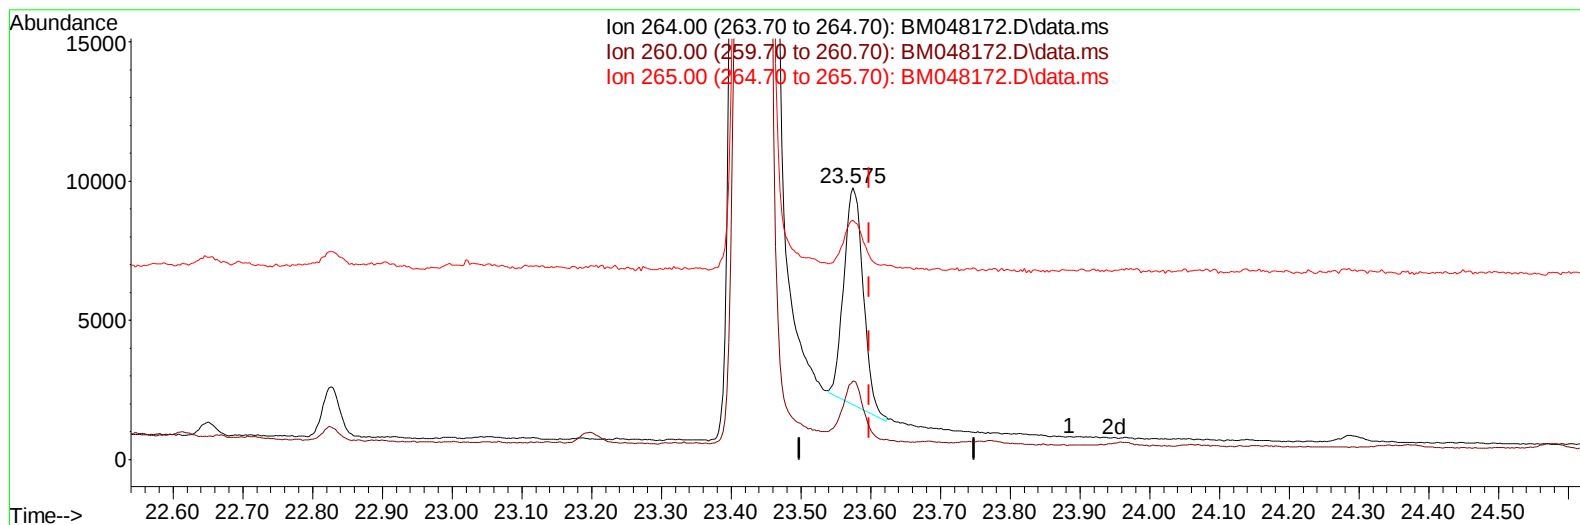

TIC: BM048172.D\data.ms

(23) Perylene-d12 (I)

23.575min (-0.023) 0.40 ng/ul m

response 15076

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	28.78
265.00	128.10	87.96#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048172.D
 Acq On : 22 Oct 2024 02:04
 Operator : RC/JU
 Sample : P4380-16
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J1

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 22 02:34:09 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 21 23:11:55 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.767	152		6490	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.556	136		19782	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.399	164		17912	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.140	188		22949m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.313	240		17737m	0.400	ng/ul	-0.02
23) Perylene-d12	23.575	264		15076m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.235	96		39047	4.426	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.145	152		13305	0.483	ng/ul	-0.06
18) Fluoranthene-d10	19.168	212		25268m	0.490	ng/ul	-0.02
Target Compounds							
							Qvalue
5) Naphthalene	10.605	128		1453875	27.043	ng/ul	95
7) 2-Methylnaphthalene	12.222	142		119223	3.876	ng/ul	98
8) 1-Methylnaphthalene	12.442	142		121942	3.445	ng/ul	98
10) Acenaphthylene	14.121	152		133156	1.609	ng/ul	99
11) Acenaphthene	14.464	153		84144	1.423	ng/ul	98
12) Fluorene	15.449	166		113288	1.788	ng/ul	98
14) Pentachlorophenol	16.802	266		1401m	0.182	ng/ul	
15) Phenanthrene	17.182	178		211774m	3.651	ng/ul	
16) Anthracene	17.275	178		31142m	0.568	ng/ul	
19) Fluoranthene	19.196	202		42714m	0.614	ng/ul	
20) Pyrene	19.559	202		24775m	0.331	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048172.D
Acq On : 22 Oct 2024 02:04
Operator : RC/JU
Sample : P4380-16
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J1

Manual IntegrationsAPPROVED

Quant Time: Oct 22 02:34:09 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 21 23:11:55 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

