




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

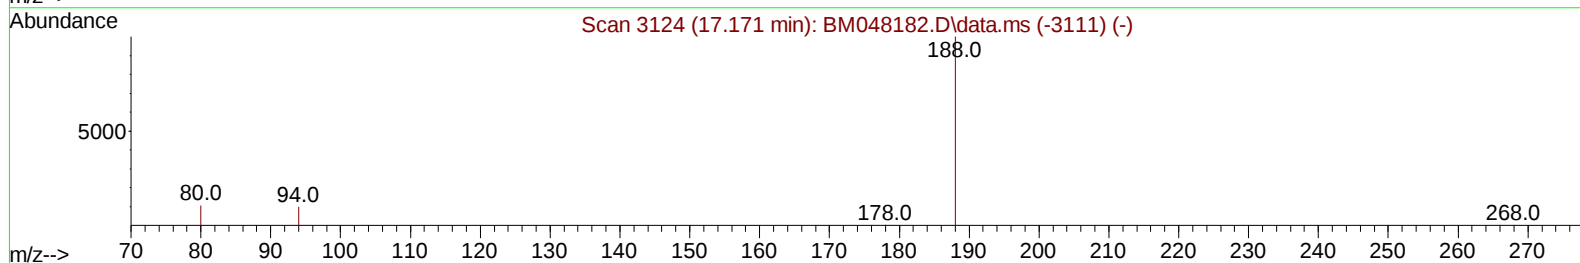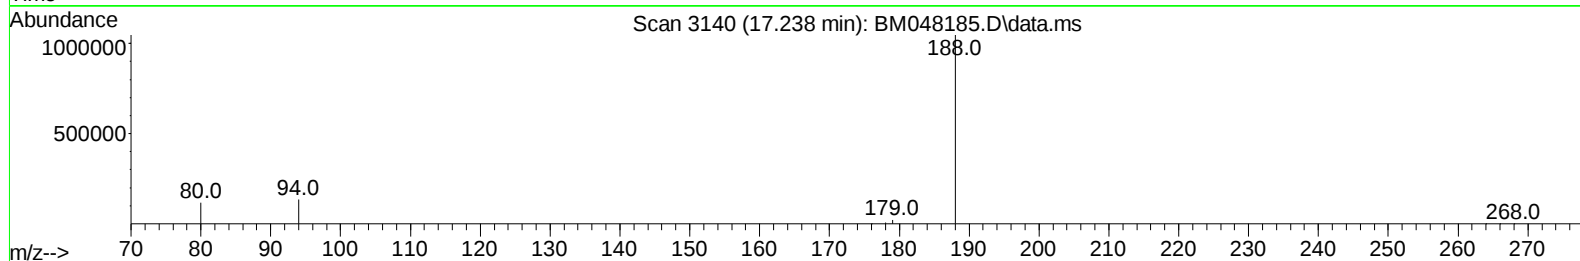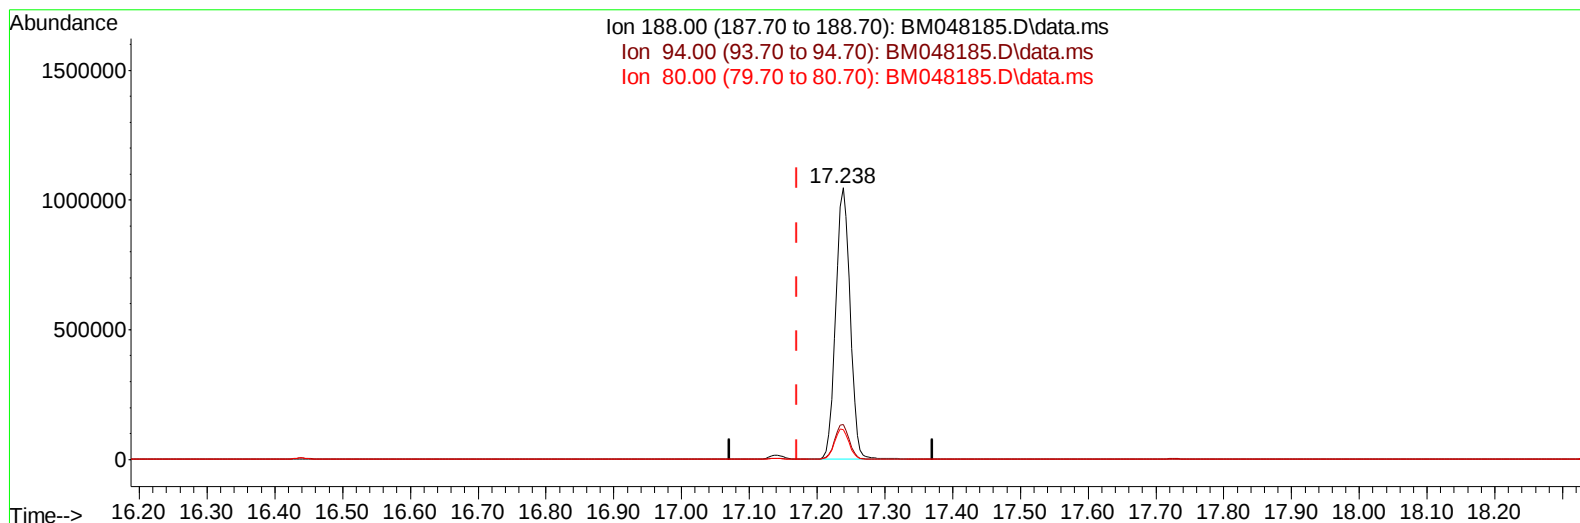

TIC: BM048185.D\data.ms

(13) Phenanthrene-d10 (I)

17.238min (+ 0.068) 0.40 ng/u1

response 1538018

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	12.88
80.00	12.40	11.06
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

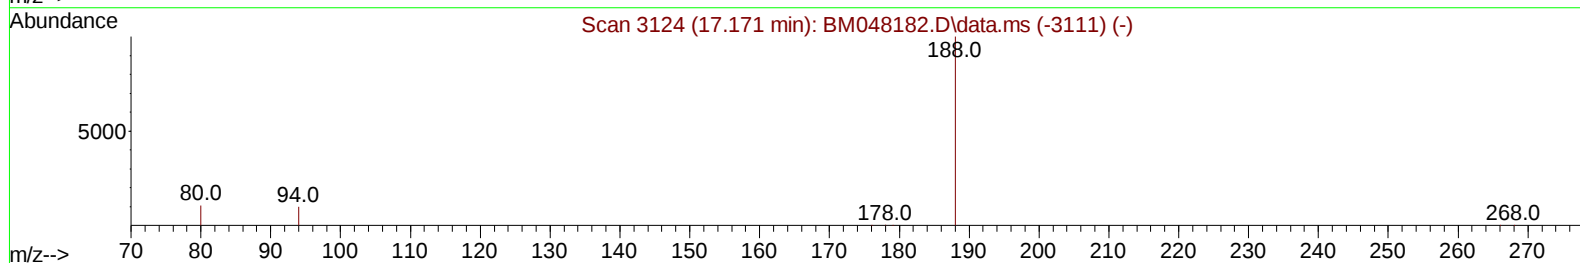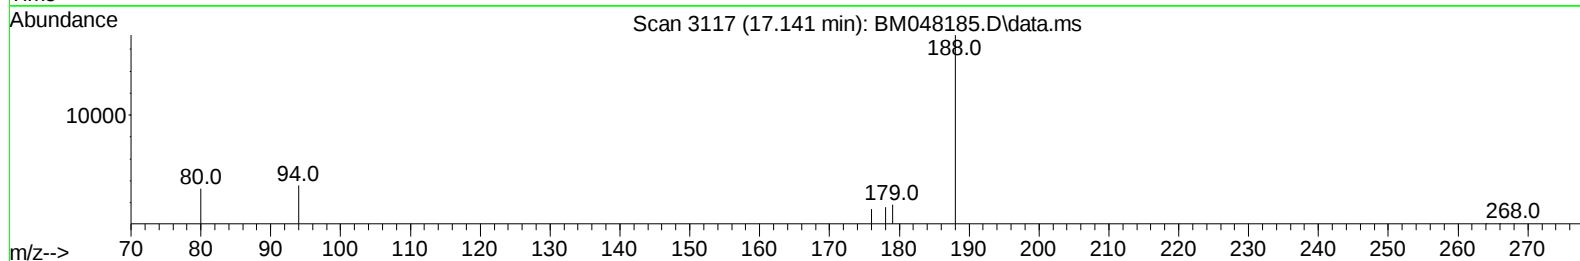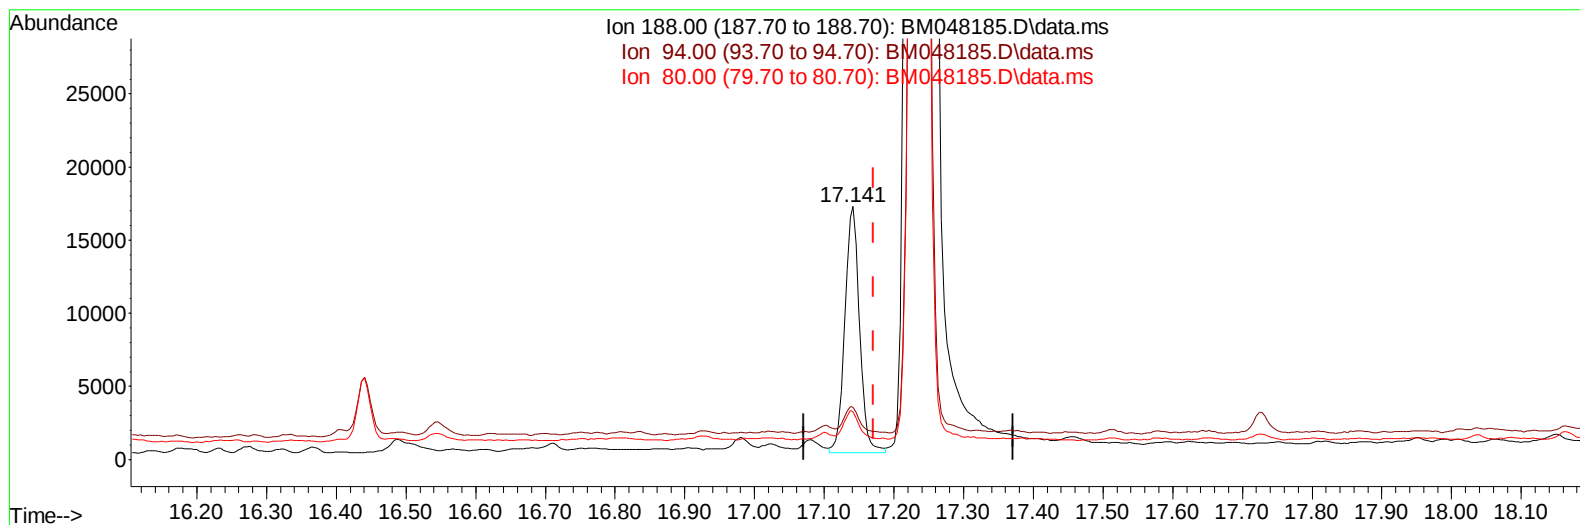

TIC: BM048185.D\data.ms

(13) Phenanthrene-d10 (I)

17.141min (-0.029) 0.40 ng/ul m

response 24679

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	11.80	20.61#
80.00	12.40	18.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

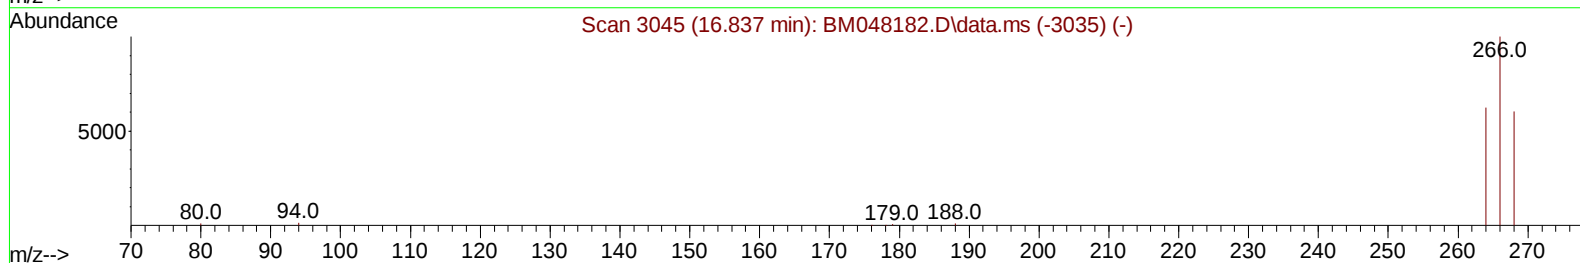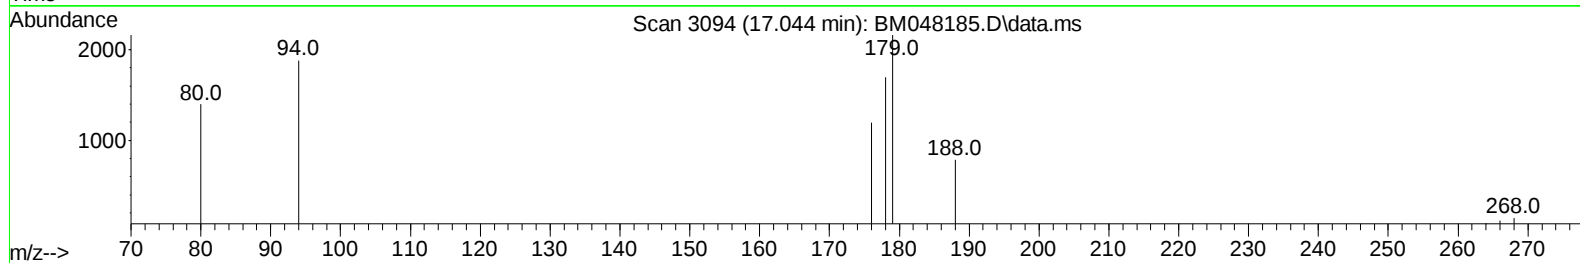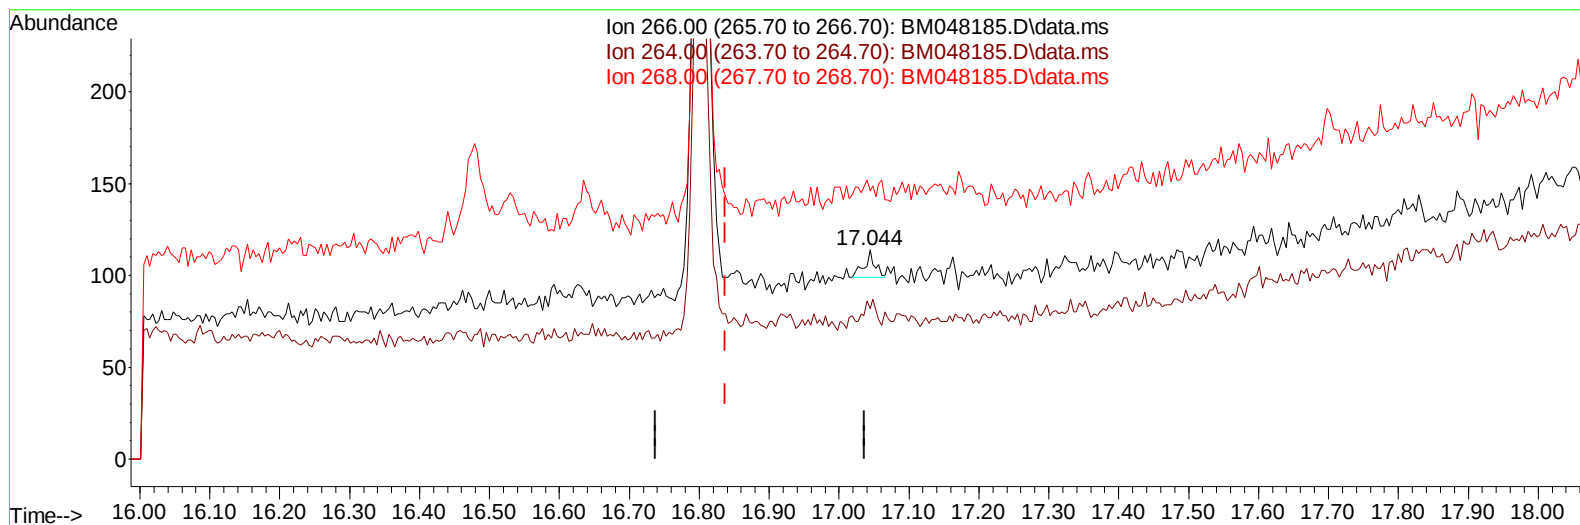

TIC: BM048185.D\data.ms

(14) Pentachloropheno1

17.044min (+ 0.207) 0.00 ng/u1

response

15

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.70	113.33#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

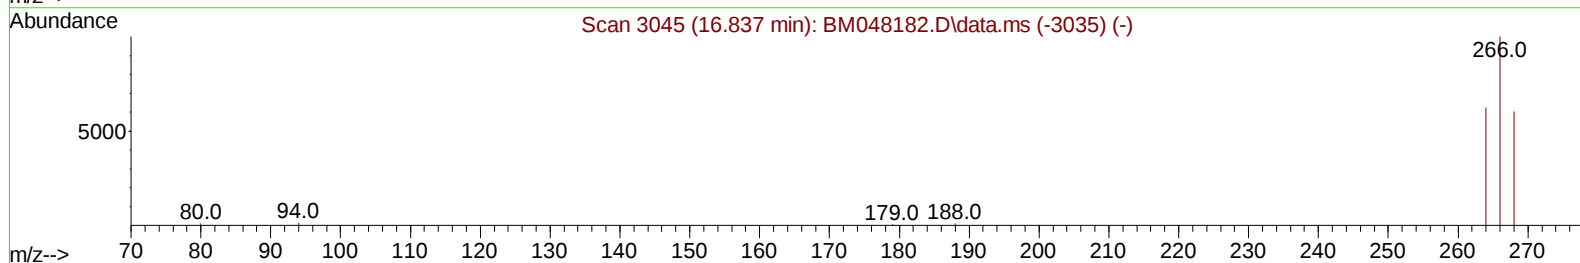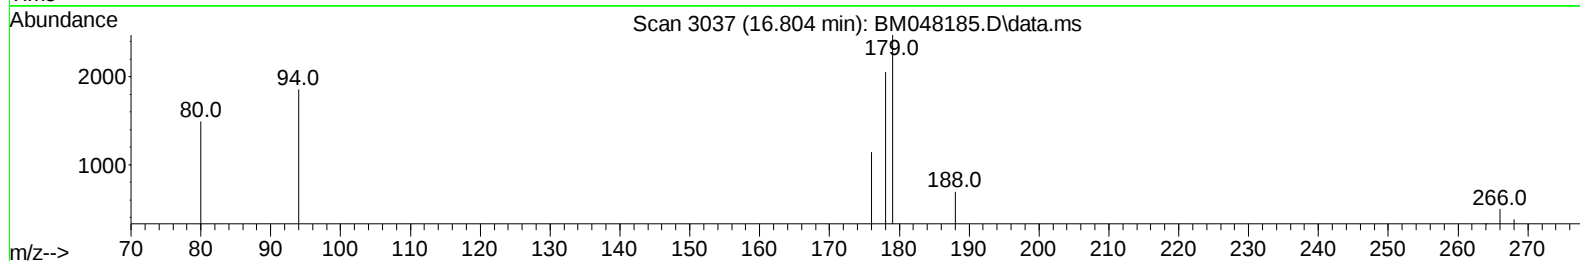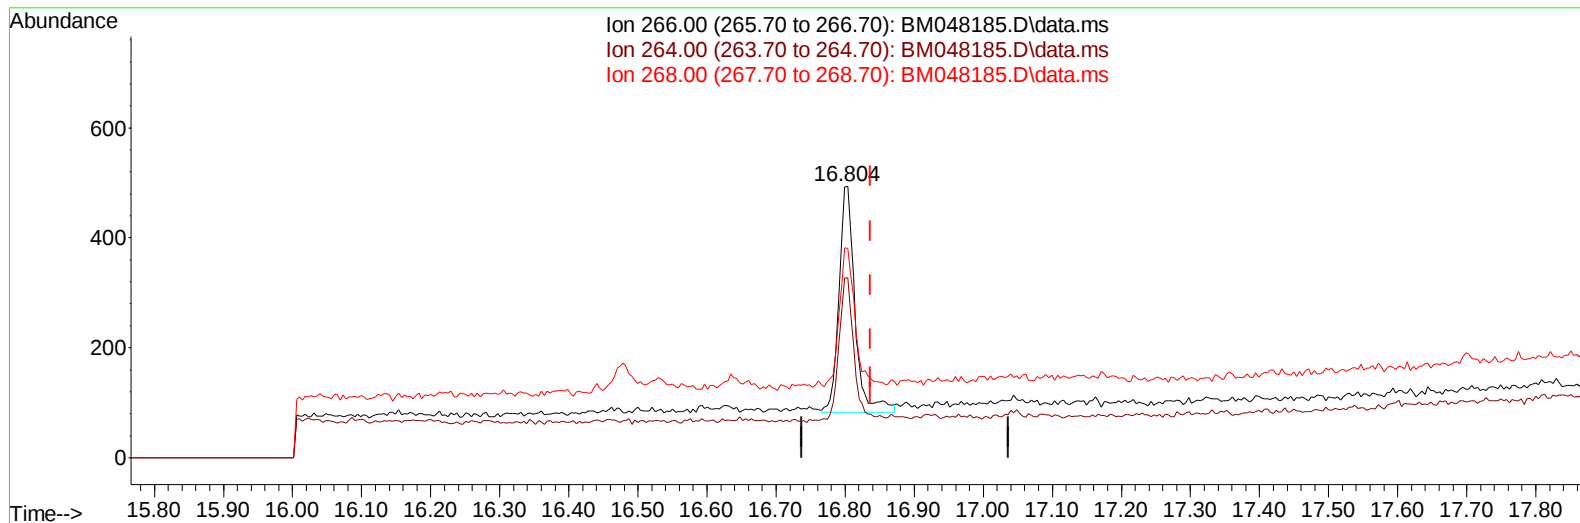

TIC: BM048185.D\data.ms

(14) Pentachlorophenol

16.804min (-0.034) 0.08 ng/u1 m

response 661

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	62.70	2.57#
268.00	64.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

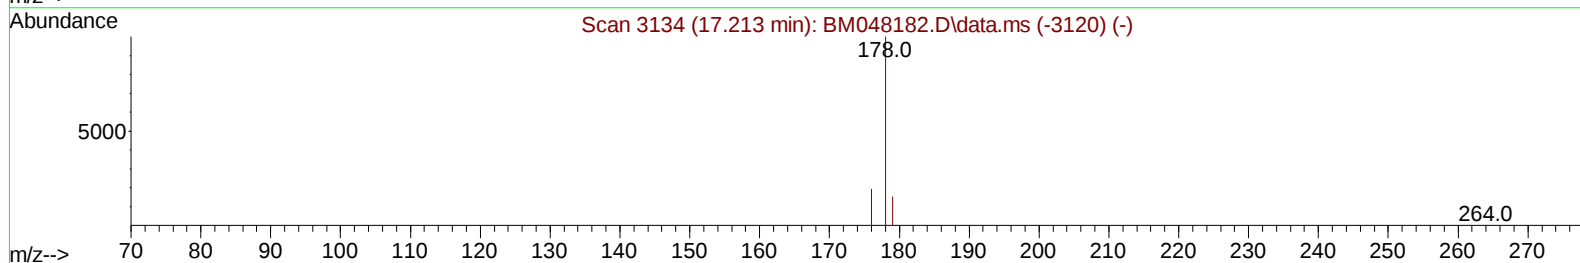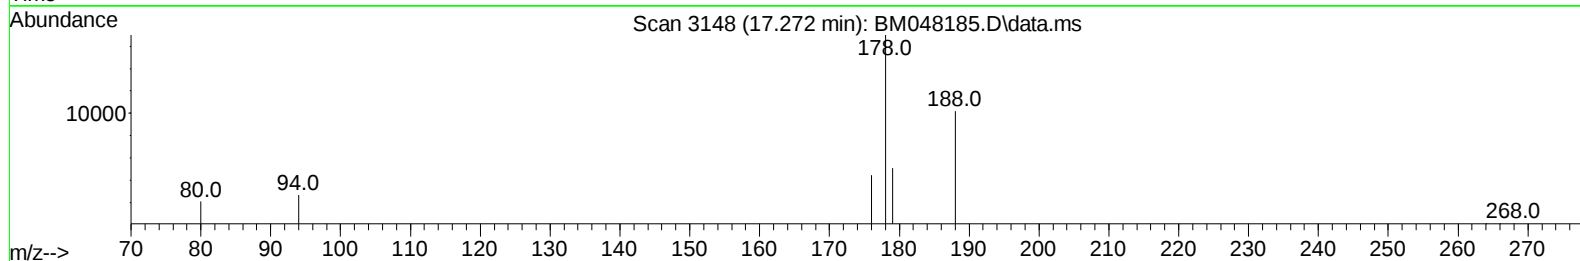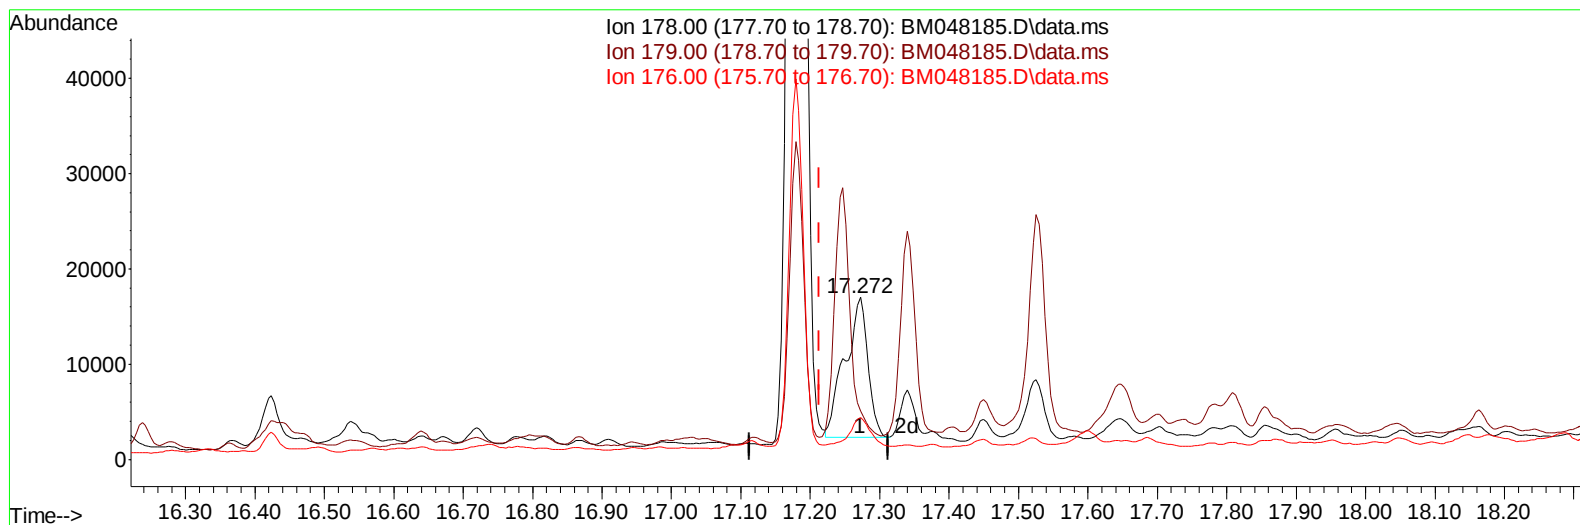

TIC: BM048185.D\data.ms

(15) Phenanthrene

17.272min (+ 0.059) 0.54 ng/u1

response 33691

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	29.72#
176.00	20.00	26.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

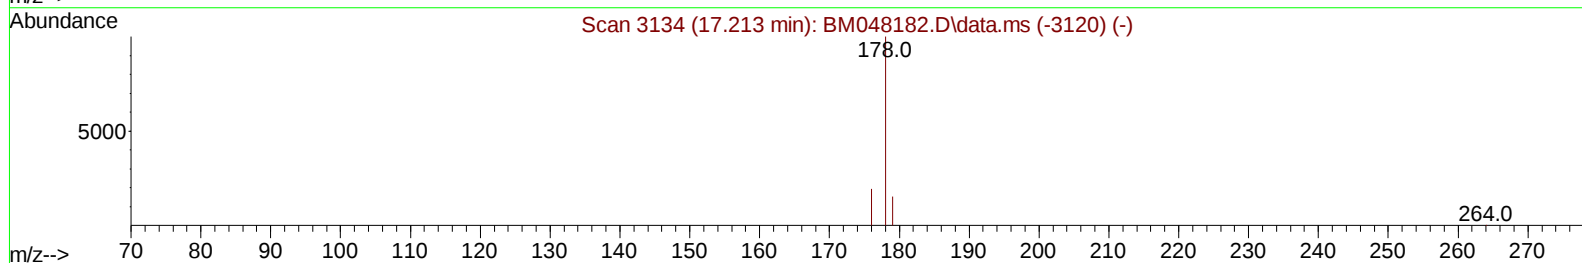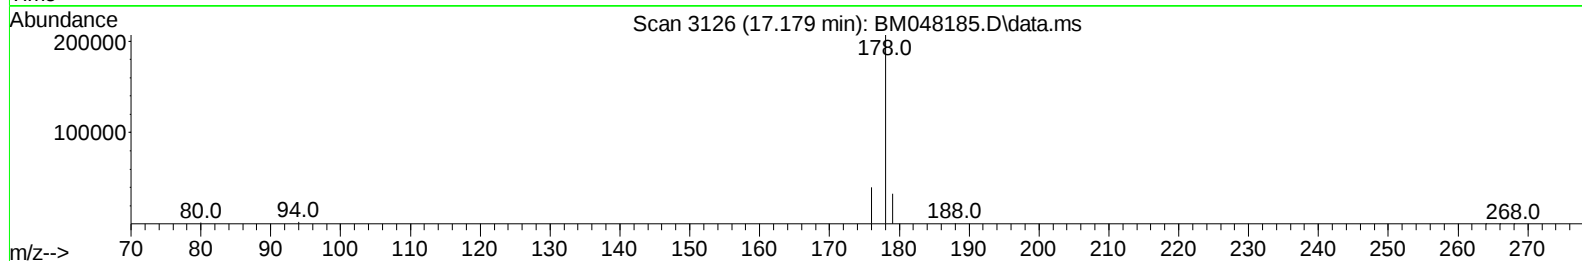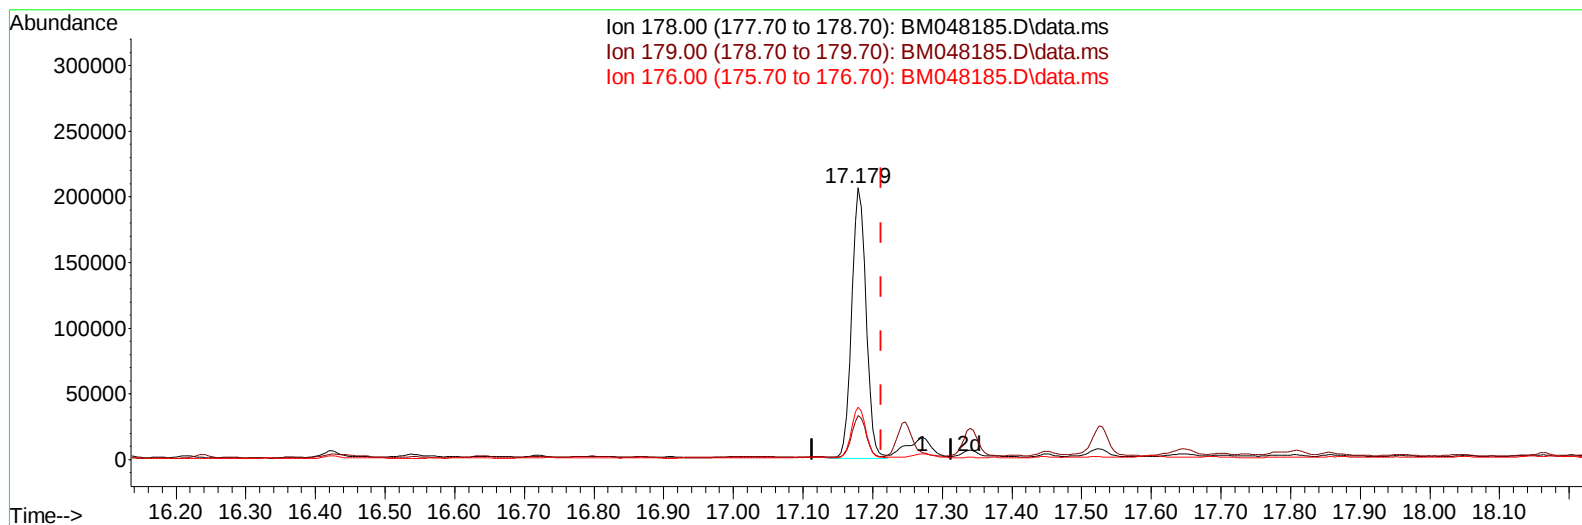

TIC: BM048185.D\data.ms

(15) Phenanthrene

17.179min (-0.034) 4.72 ng/ul m

response 294386

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	16.50	16.14
176.00	20.00	19.32
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

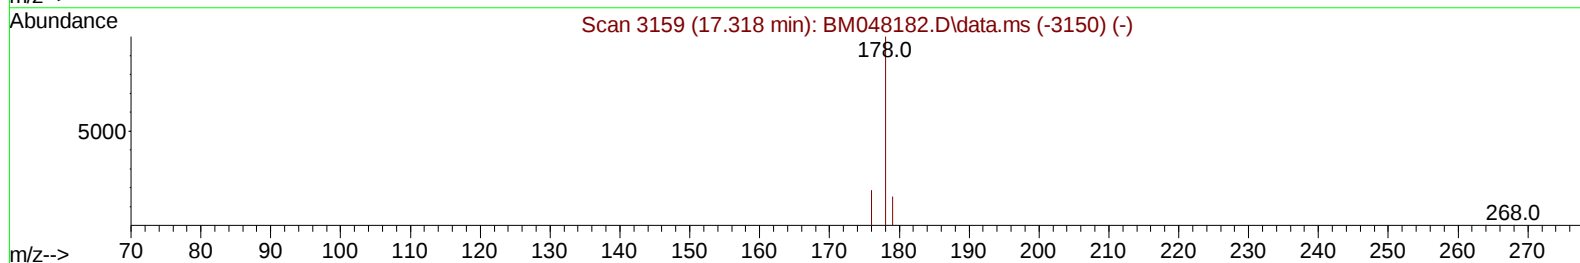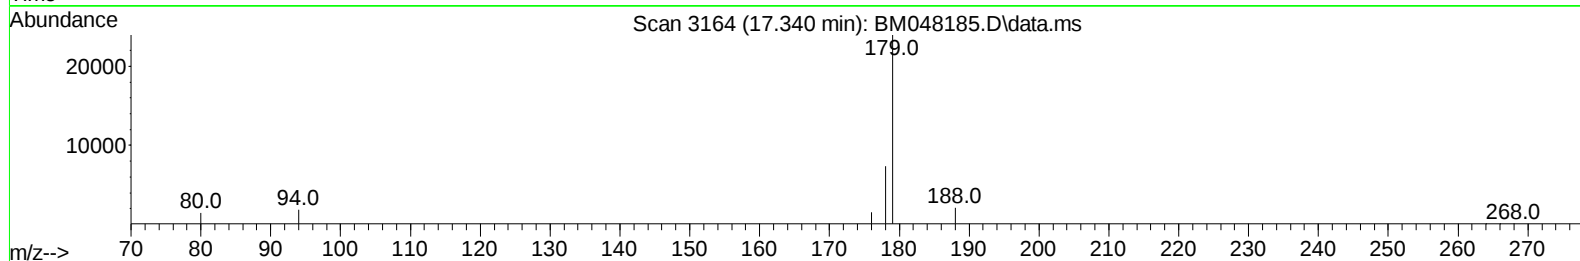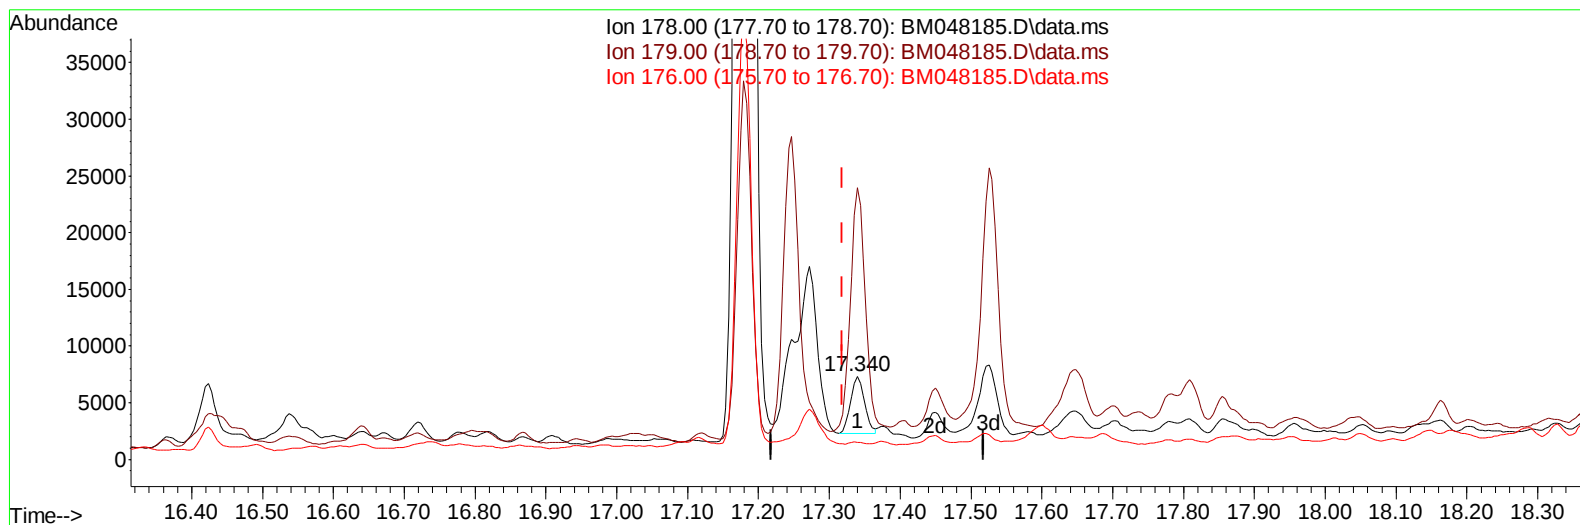

TIC: BM048185.D\data.ms

(16) Anthracene

17.340min (+ 0.021) 0.12 ng/u1

response 6831

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	326.79#
176.00	20.00	20.84
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

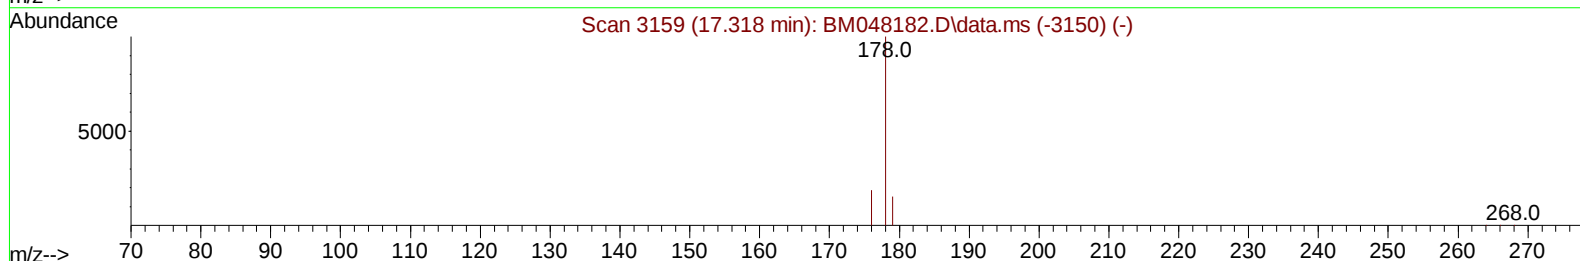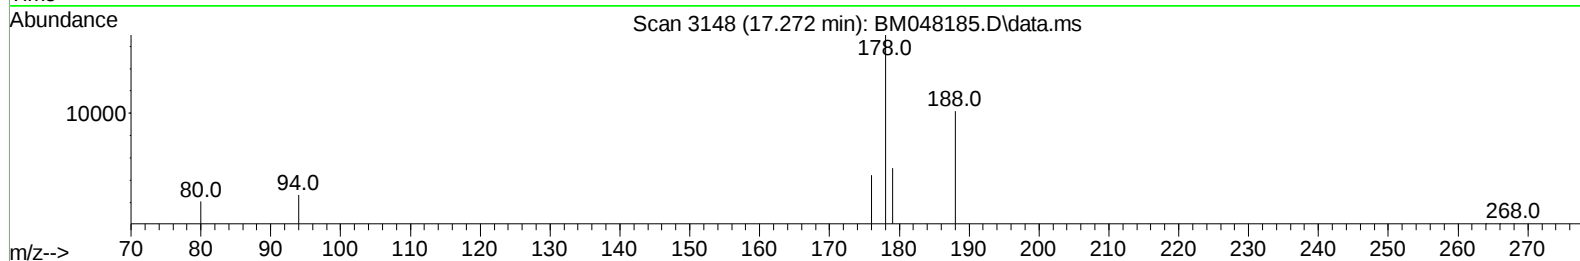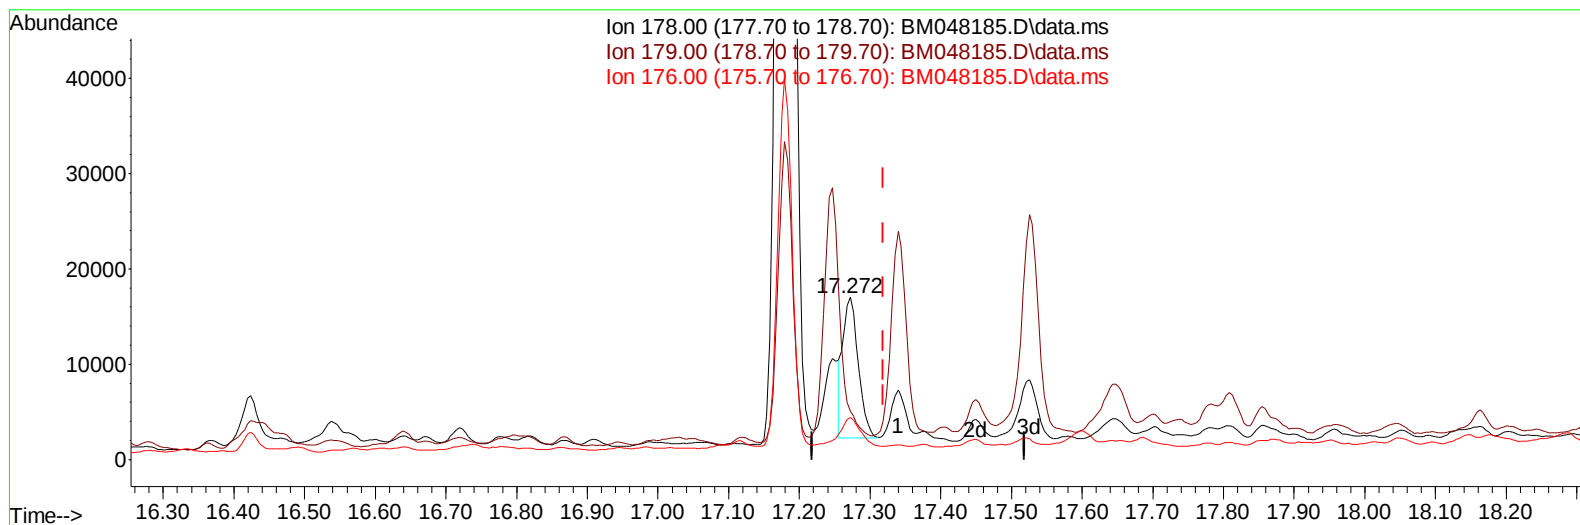

TIC: BM048185.D\data.ms

(16) Anthracene

17.272min (-0.046) 0.38 ng/u1 m

response 22261

Ion	Exp%	Act%
178.00	100.00	100.00
179.00	18.10	29.72#
176.00	20.00	26.05#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

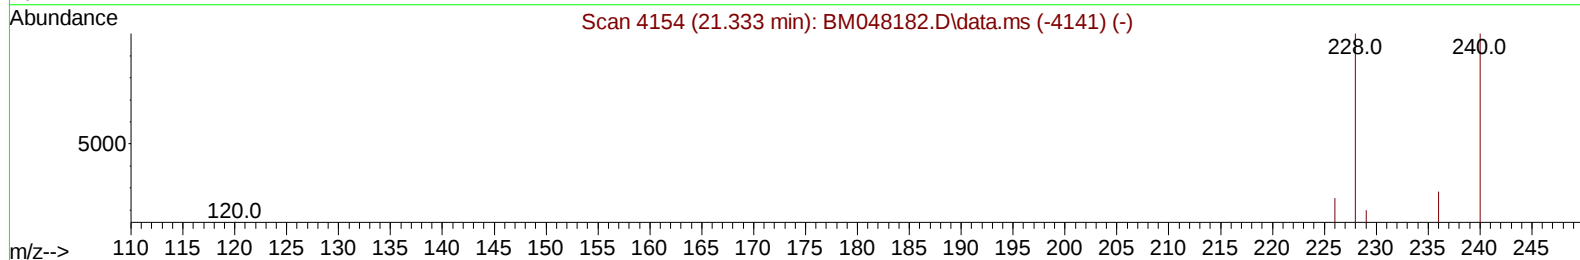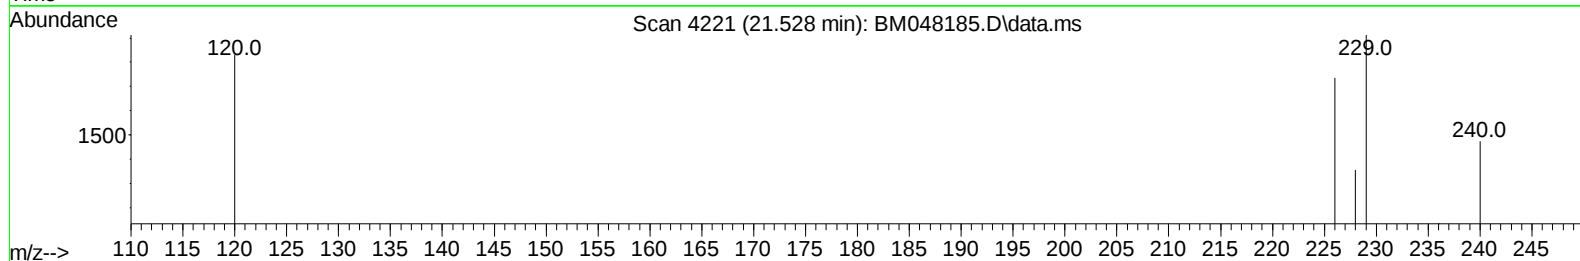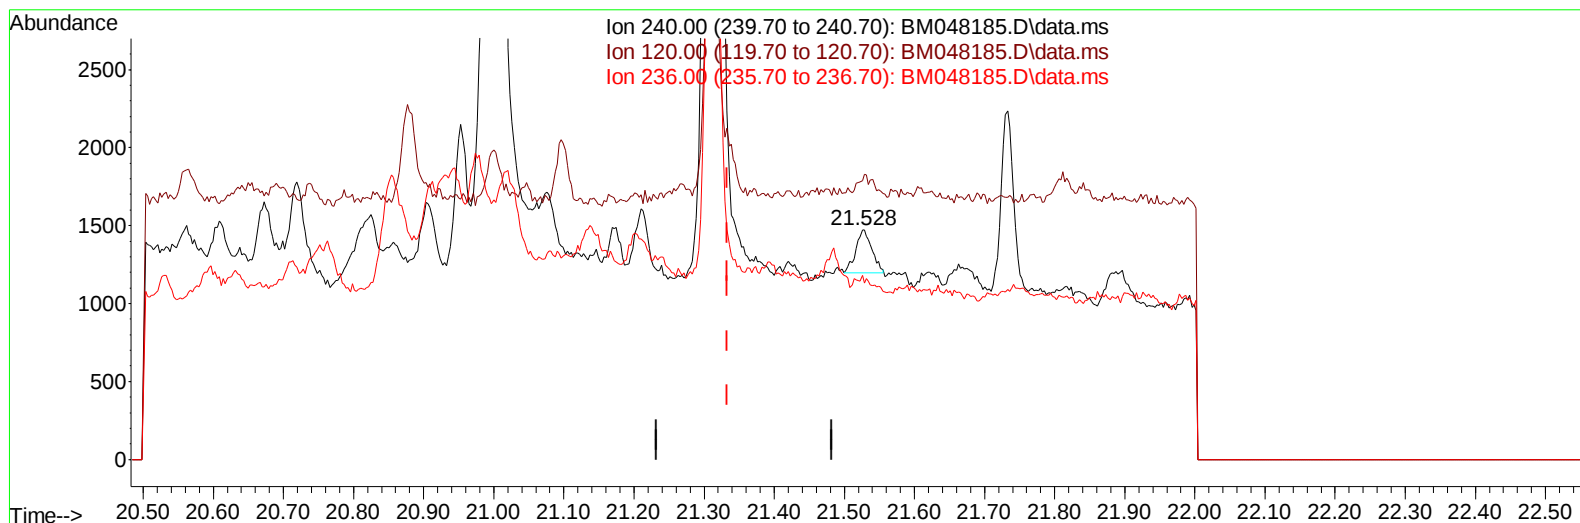

TIC: BM048185.D\data.ms

(17) Chrysene-d12

21.528min (+ 0.196) 0.40 ng/u1

response 440

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	124.24#
236.00	30.60	76.92#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

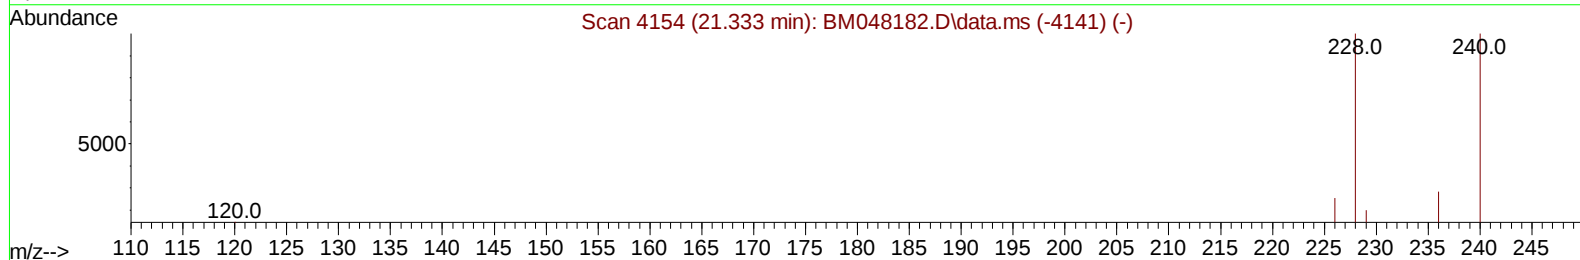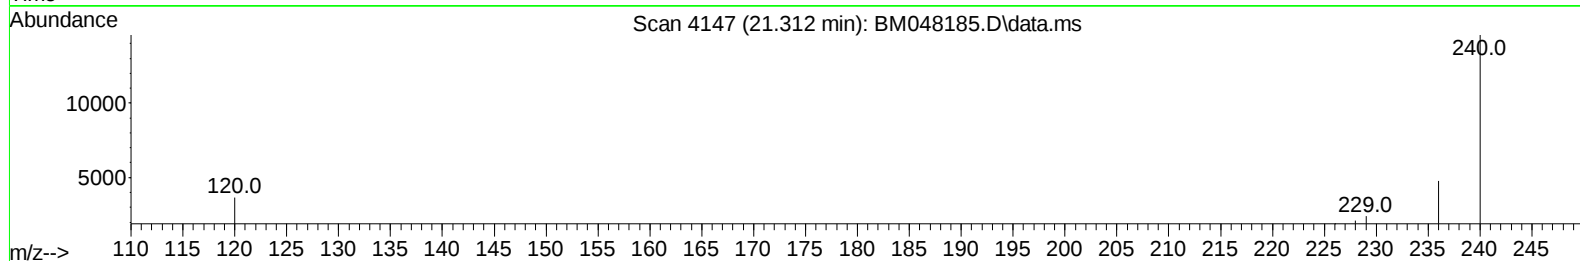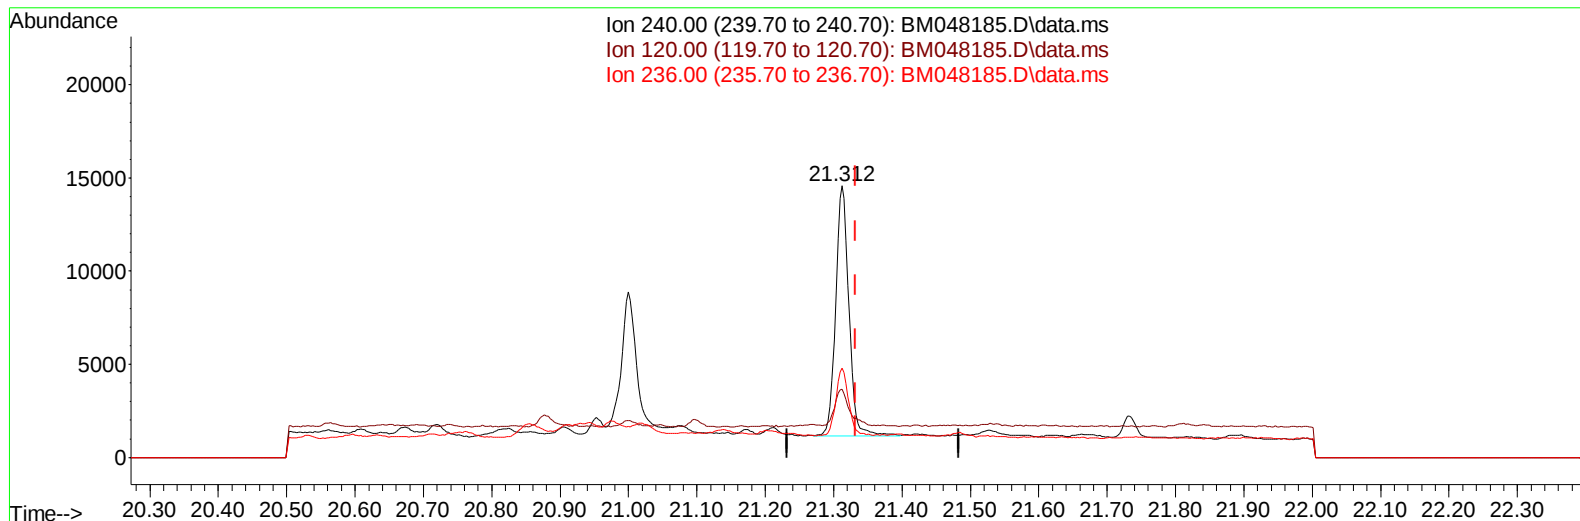

TIC: BM048185.D\data.ms

(17) Chrysene-d12

21.312min (-0.020) 0.40 ng/ul m

response 18132

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	22.80	25.07
236.00	30.60	32.85
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

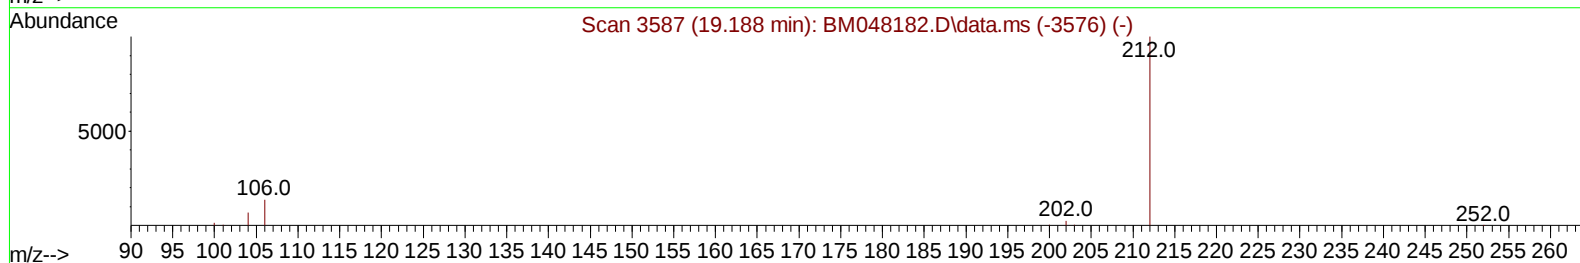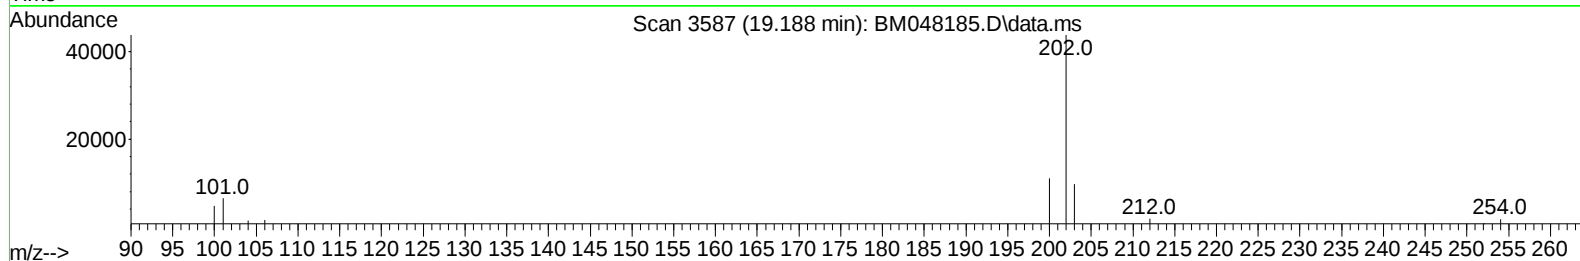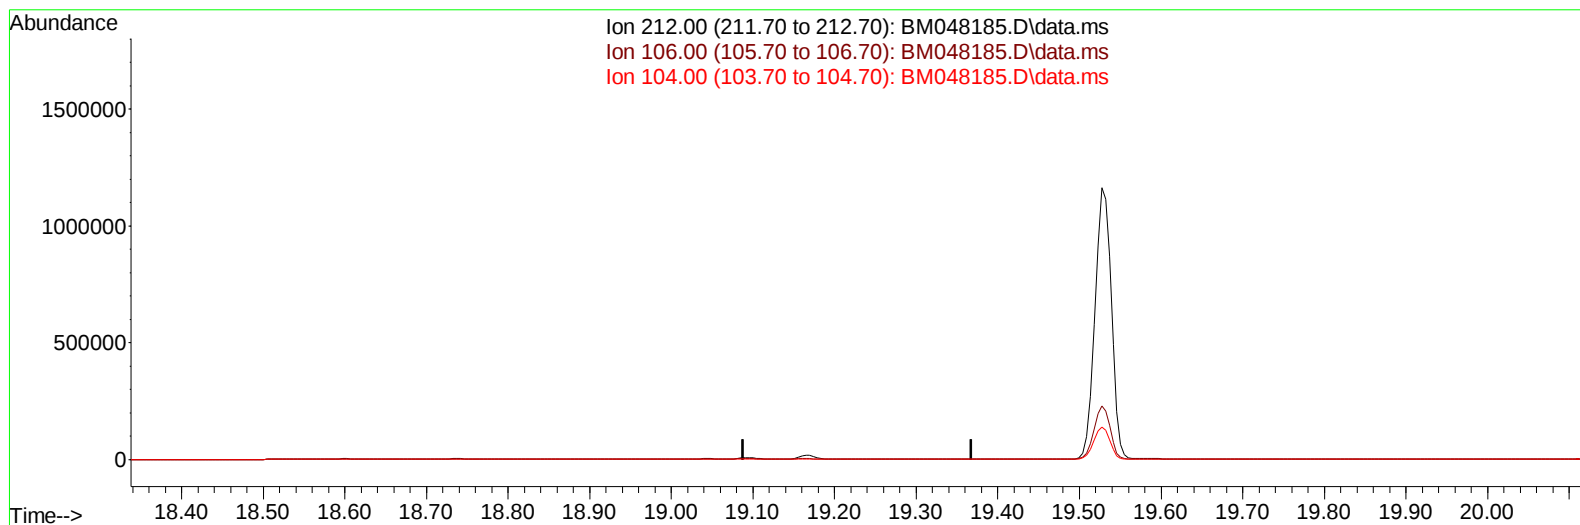

TIC: BM048185.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.188min (-19.188) 0.00 ng/u1

response 0

Ion	Exp%	Act%
212.00	100.00	0.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

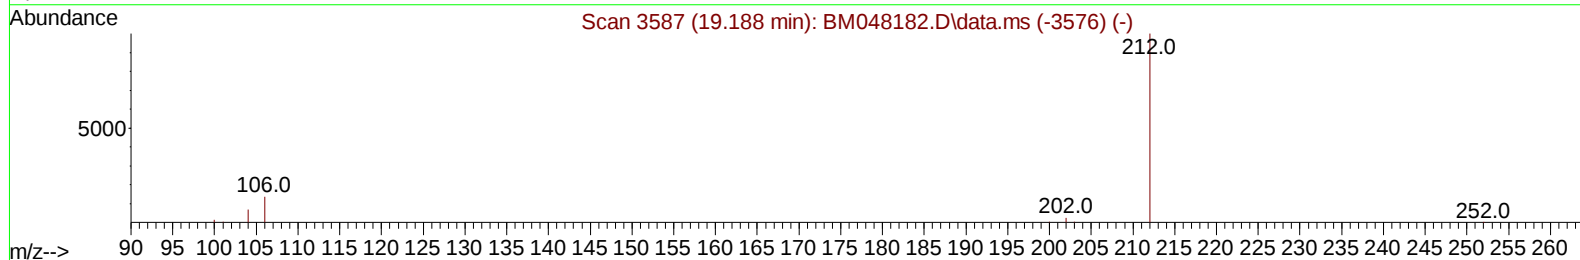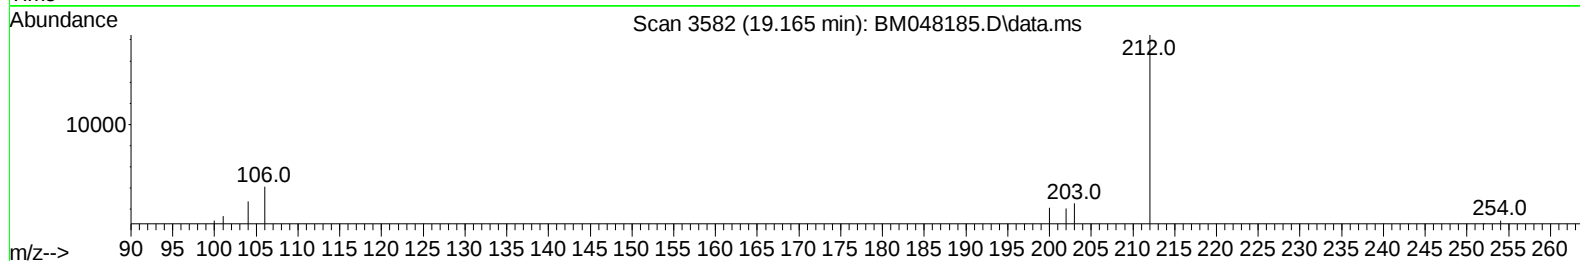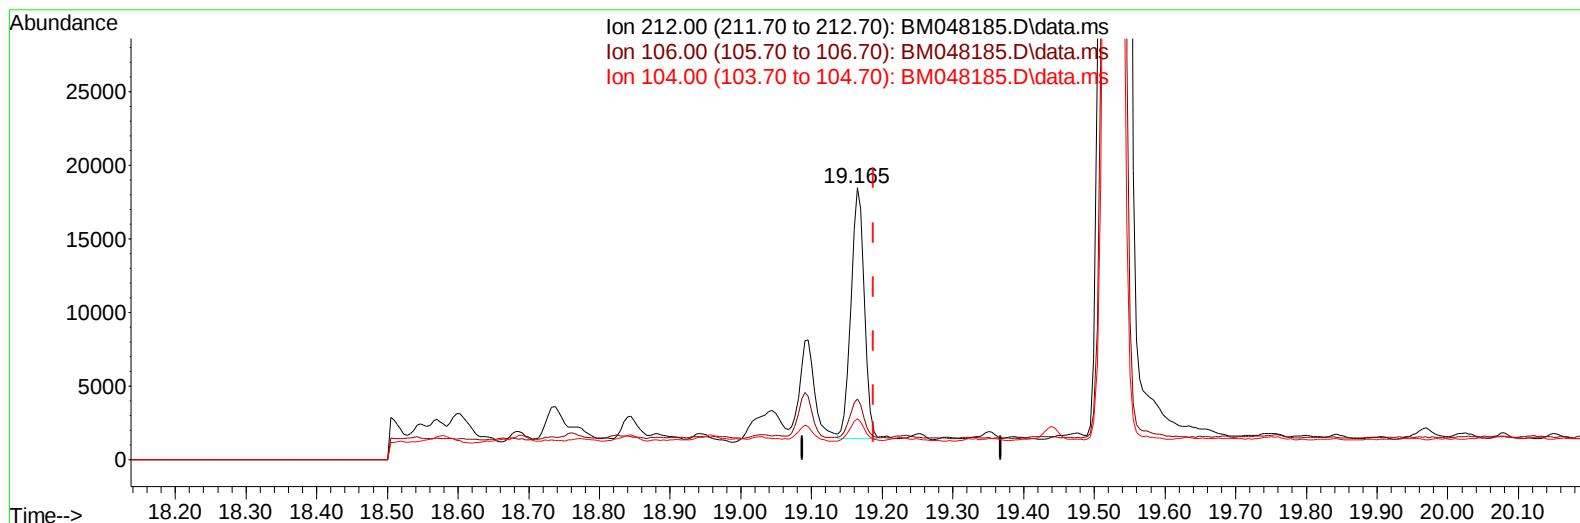

TIC: BM048185.D\data.ms

(18) Fluoranthene-d10 (SURR)

19.165min (-0.023) 0.42 ng/u1 m

response 22363

Ion	Exp%	Act%
212.00	100.00	100.00
106.00	15.00	0.00#
104.00	8.80	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

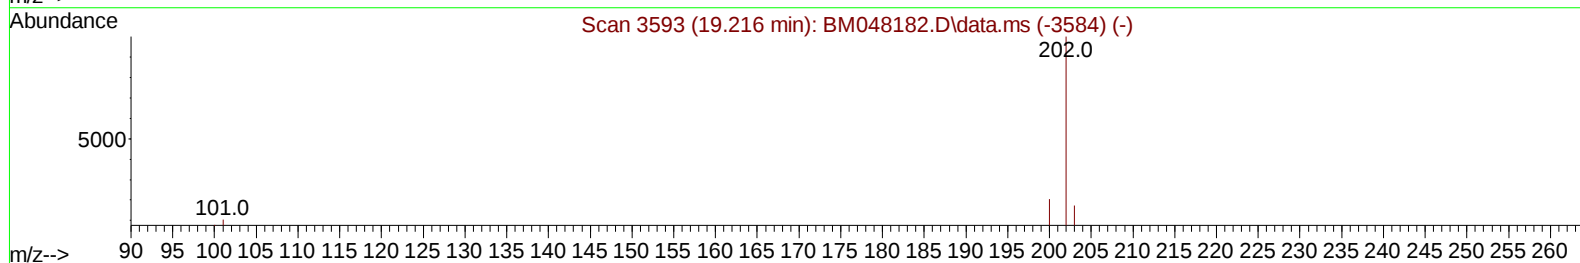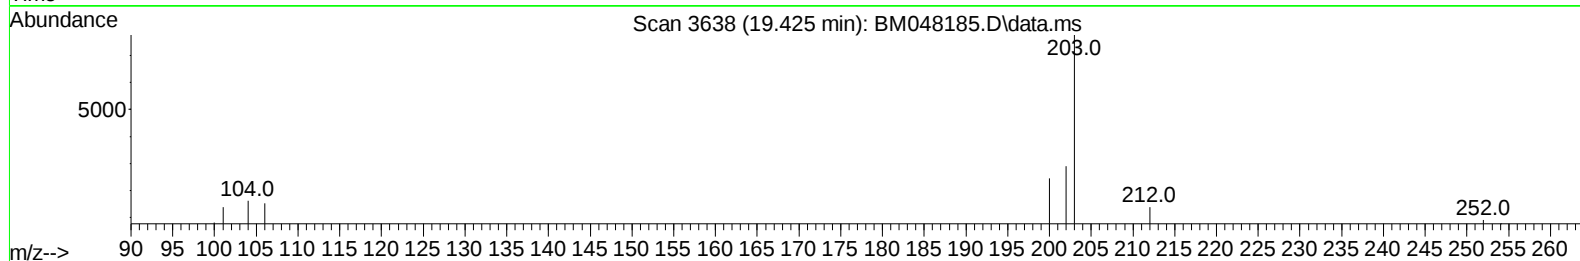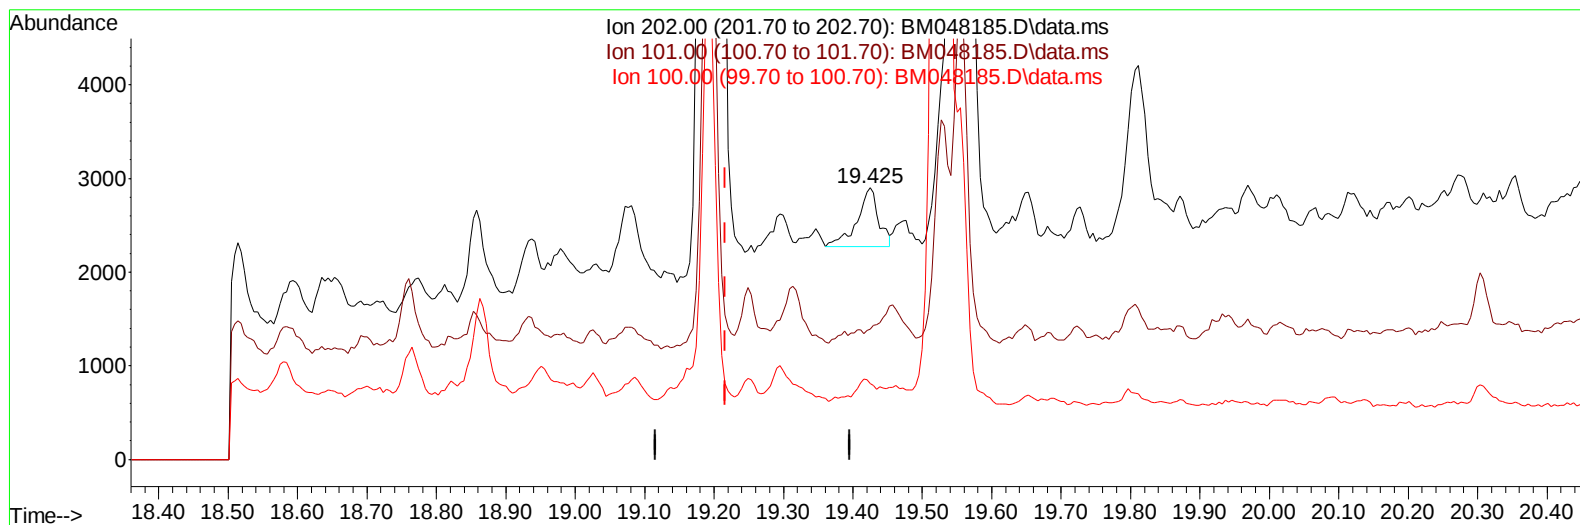

TIC: BM048185.D\data.ms

(19) Fluoranthene (C)

19.425min (+ 0.209) 0.02 ng/u1

response 1343

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	47.88#
100.00	8.90	27.84#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

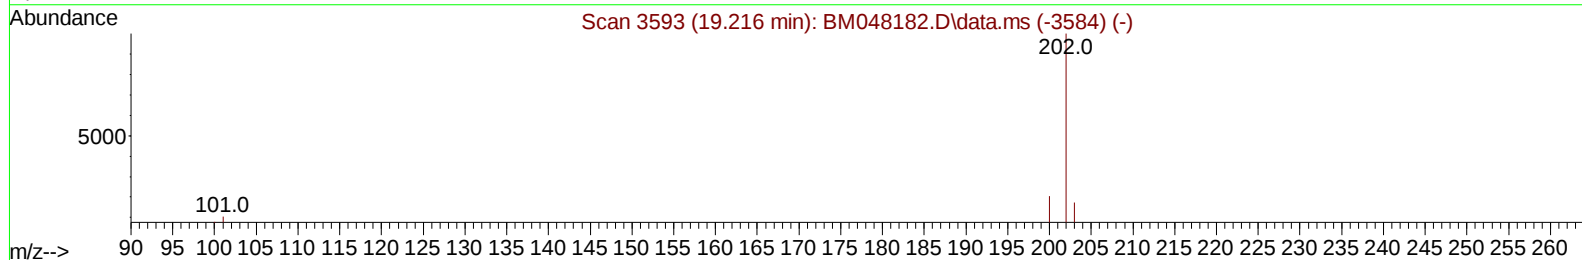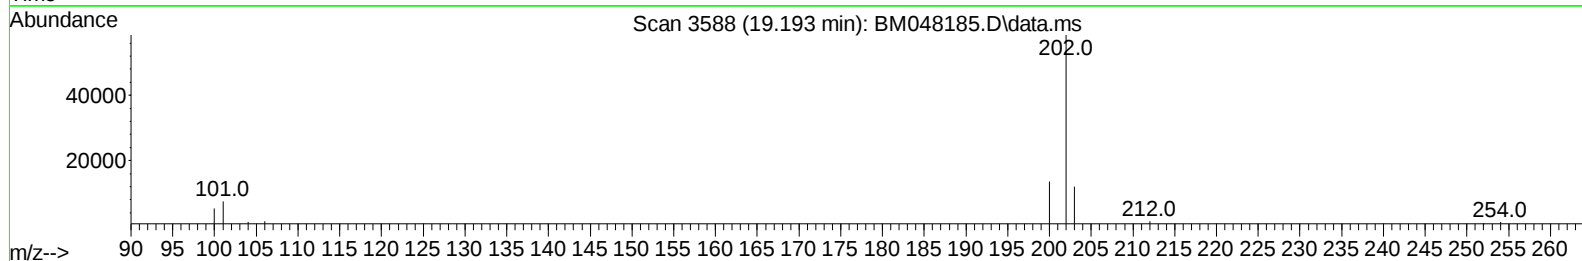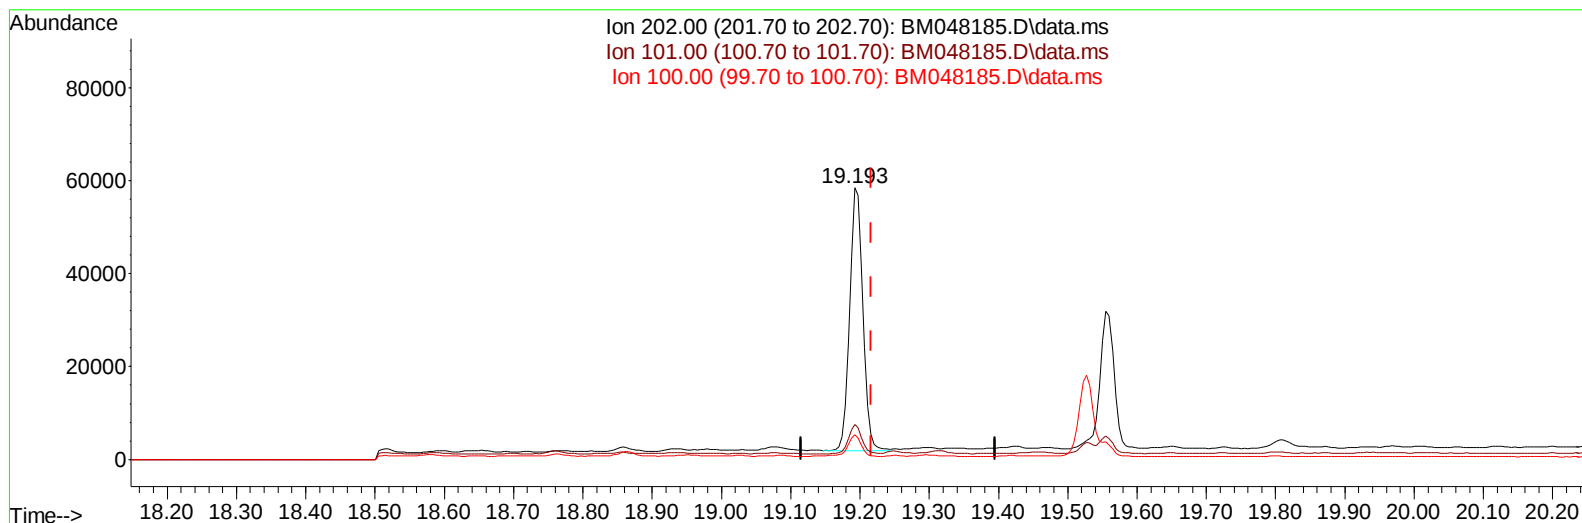

TIC: BM048185.D\data.ms

(19) Fluoranthene (C)

19.193min (-0.023) 1.06 ng/ul m

response 75306

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	11.60	12.89
100.00	8.90	9.14
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

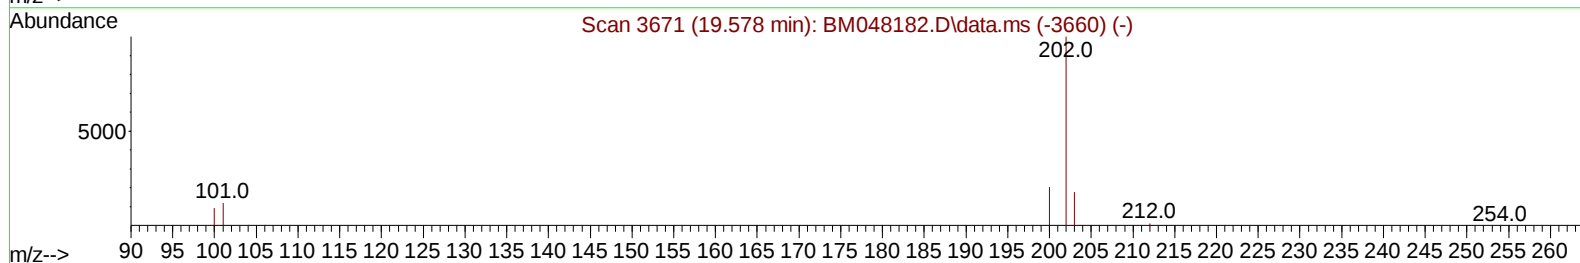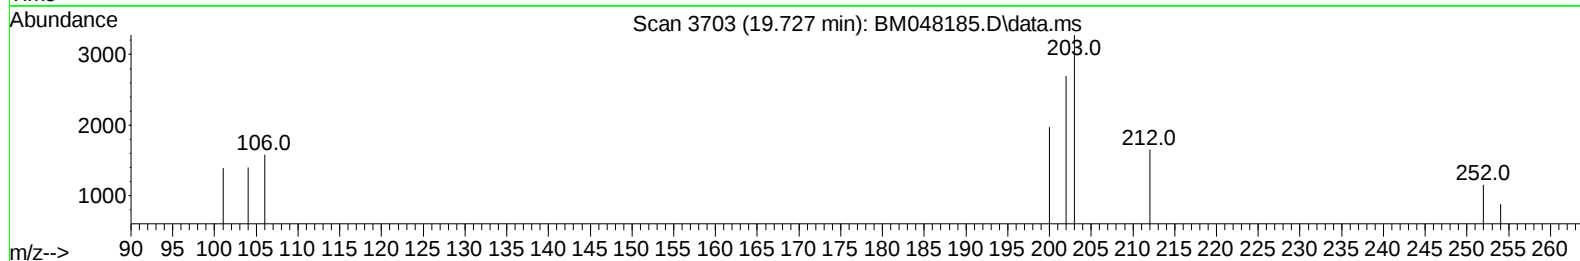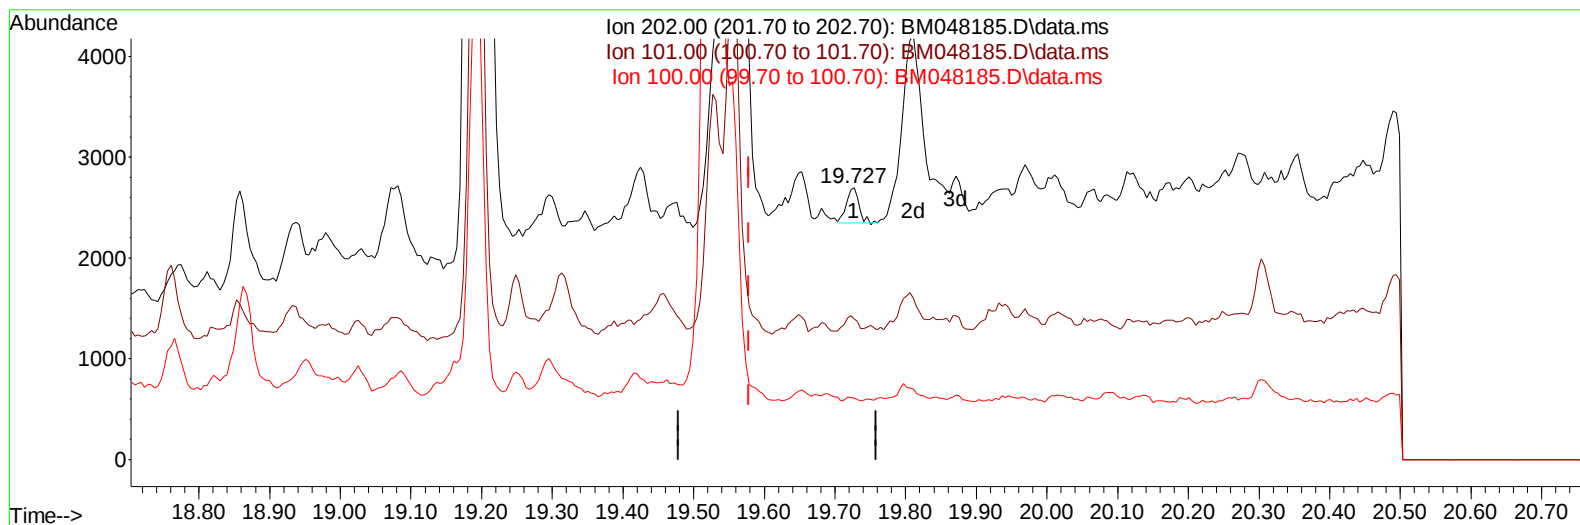

TIC: BM048185.D\data.ms

(20) Pyrene

19.727min (+ 0.149) 0.01 ng/u1

response 423

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	51.80#
100.00	10.10	22.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

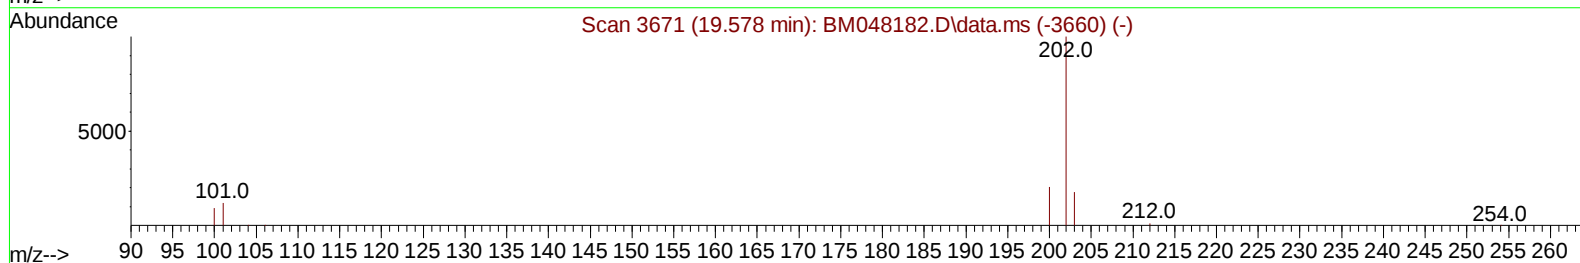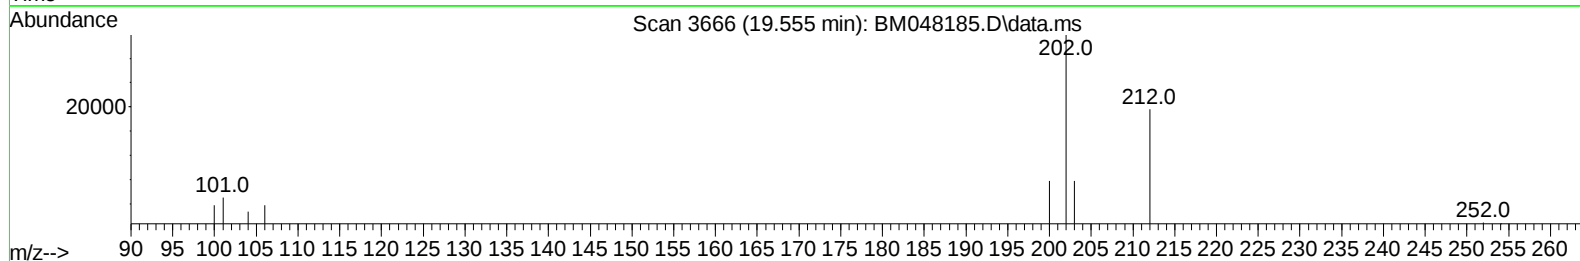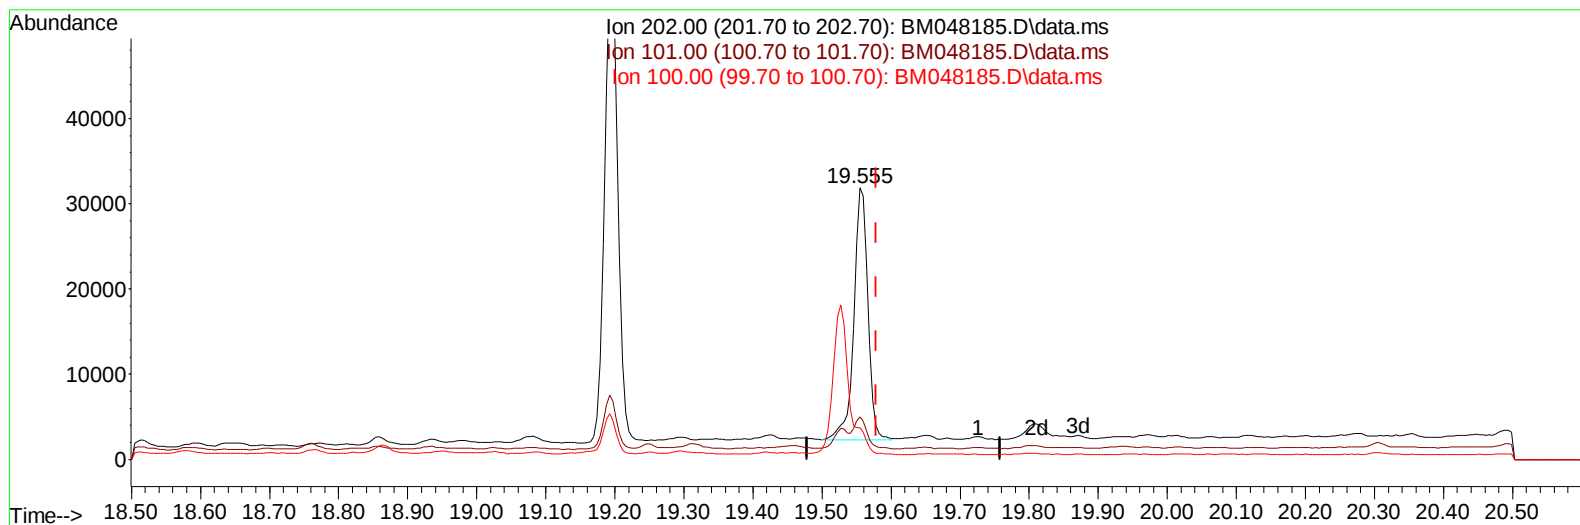

TIC: BM048185.D\data.ms

(20) Pyrene

19.555min (-0.023) 0.55 ng/ul m

response 41999

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	13.30	15.80
100.00	10.10	11.78
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

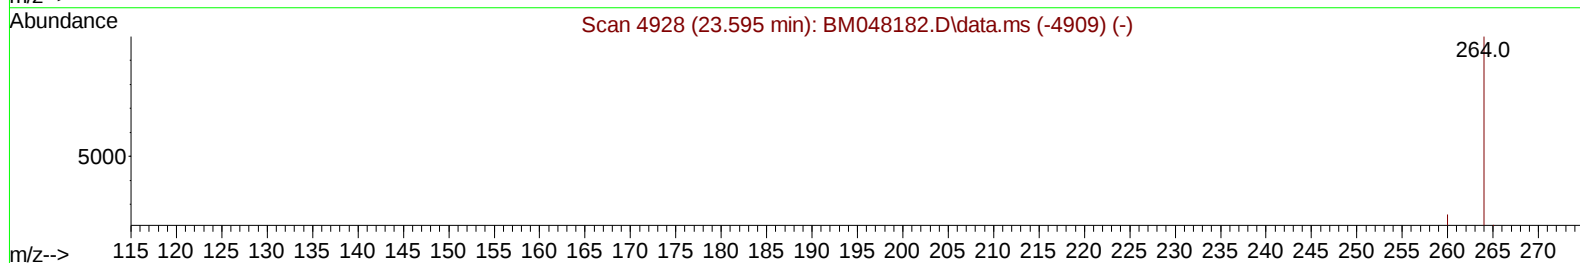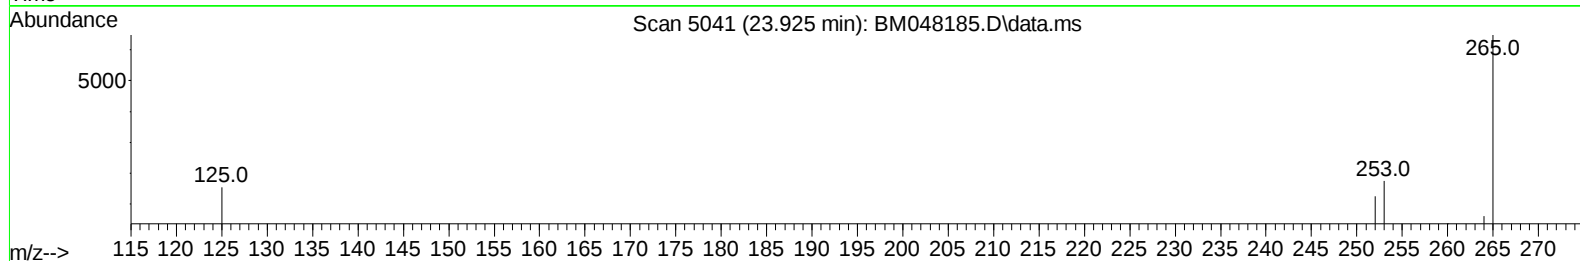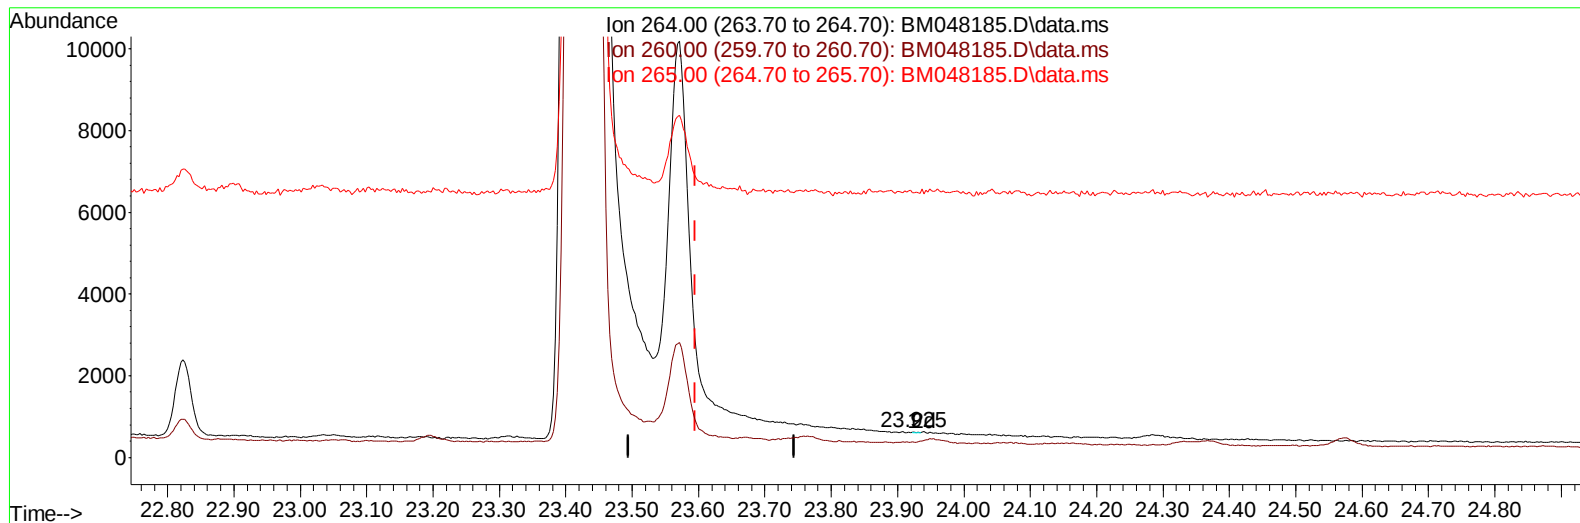

TIC: BM048185.D\data.ms

(23) Perylene-d12 (I)

23.925min (+ 0.330) 0.40 ng/u1

response 9

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	58.94#
265.00	128.10	1042.67#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

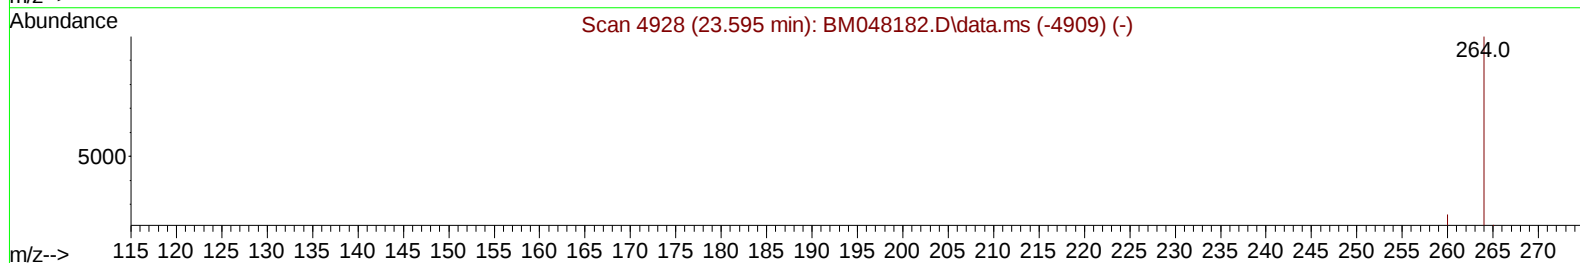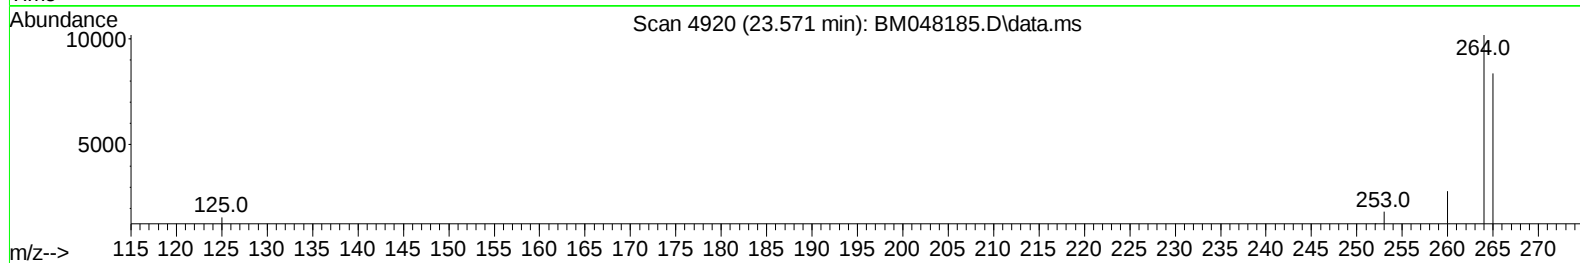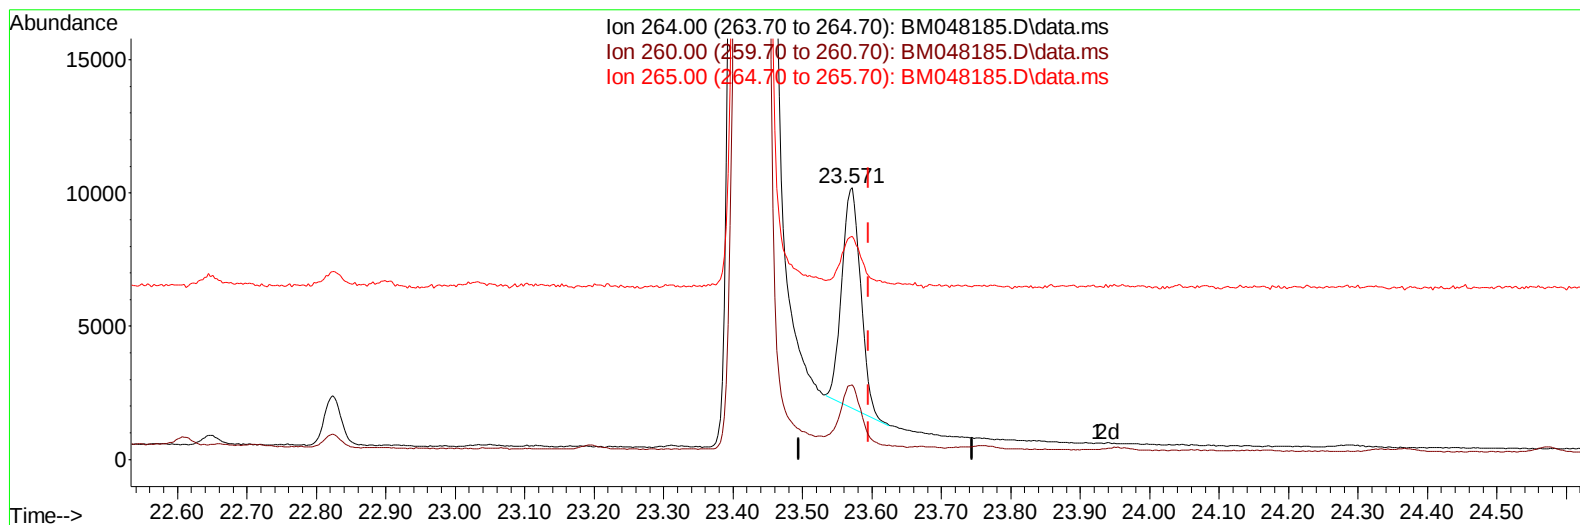

TIC: BM048185.D\data.ms

(23) Perylene-d12 (I)

23.571min (-0.023) 0.40 ng/ul m

response 15505

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.80	27.59
265.00	128.10	82.08#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048185.D
 Acq On : 22 Oct 2024 10:31
 Operator : RC/JU
 Sample : P4380-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 10/23/2024
 Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 22 11:01:13 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 22 10:58:11 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.767	152		6375	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.552	136		19992	0.400	ng/ul	#-0.03
9) Acenaphthene-d10	14.396	164		17786	0.400	ng/ul	#-0.02
13) Phenanthrene-d10	17.141	188		24679m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.312	240		18132m	0.400	ng/ul	-0.02
23) Perylene-d12	23.571	264		15505m	0.400	ng/ul	-0.02
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.235	96		35821	4.134	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.146	152		10402	0.373	ng/ul	-0.05
18) Fluoranthene-d10	19.165	212		22363m	0.424	ng/ul	-0.02
Target Compounds							Qvalue
5) Naphthalene	10.601	128		389050	7.161	ng/ul	96
7) 2-Methylnaphthalene	12.218	142		84928	2.732	ng/ul	98
8) 1-Methylnaphthalene	12.438	142		109091	3.049	ng/ul	97
10) Acenaphthylene	14.118	152		28359	0.345	ng/ul#	94
11) Acenaphthene	14.460	153		130779	2.227	ng/ul	98
12) Fluorene	15.446	166		62950	1.001	ng/ul	99
14) Pentachlorophenol	16.804	266		661m	0.080	ng/ul	
15) Phenanthrene	17.179	178		294386m	4.720	ng/ul	
16) Anthracene	17.272	178		22261m	0.377	ng/ul	
19) Fluoranthene	19.193	202		75306m	1.058	ng/ul	
20) Pyrene	19.555	202		41999m	0.549	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048185.D
Acq On : 22 Oct 2024 10:31
Operator : RC/JU
Sample : P4380-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E27J0

Manual IntegrationsAPPROVED

Quant Time: Oct 22 11:01:13 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 22 10:58:11 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 10/23/2024
Supervised By :mohammad ahmed 10/23/2024

