

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
 Data File : BM048152.D
 Acq On : 21 Oct 2024 13:23
 Operator : RC/JU
 Sample : P4389-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E27J8

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 10/22/2024
 Supervised By :mohammad ahmed 10/23/2024

Quant Time: Oct 21 14:08:07 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 19 00:48:23 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.771	152	6138	0.400	ng/ul	-0.03
4) Naphthalene-d8	10.556	136	18936	0.400	ng/ul	-0.03
9) Acenaphthene-d10	14.404	164	9835	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.144	188	19118m	0.400	ng/ul	-0.03
17) Chrysene-d12	21.345	240	12924m	0.400	ng/ul	0.00
23) Perylene-d12	23.589	264	9187m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.235	96	34466	4.131	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.178	152	9697	0.367	ng/ul	-0.02
18) Fluoranthene-d10	19.173	212	19344	0.514	ng/ul	-0.02
Target Compounds						Qvalue
5) Naphthalene	10.605	128	3664	0.071	ng/ul#	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102124\
Data File : BM048152.D
Acq On : 21 Oct 2024 13:23
Operator : RC/JU
Sample : P4389-04
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
E27J8

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024


Quant Time: Oct 21 14:08:07 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-SIM-BM101824.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 19 00:48:23 2024
Response via : Initial Calibration

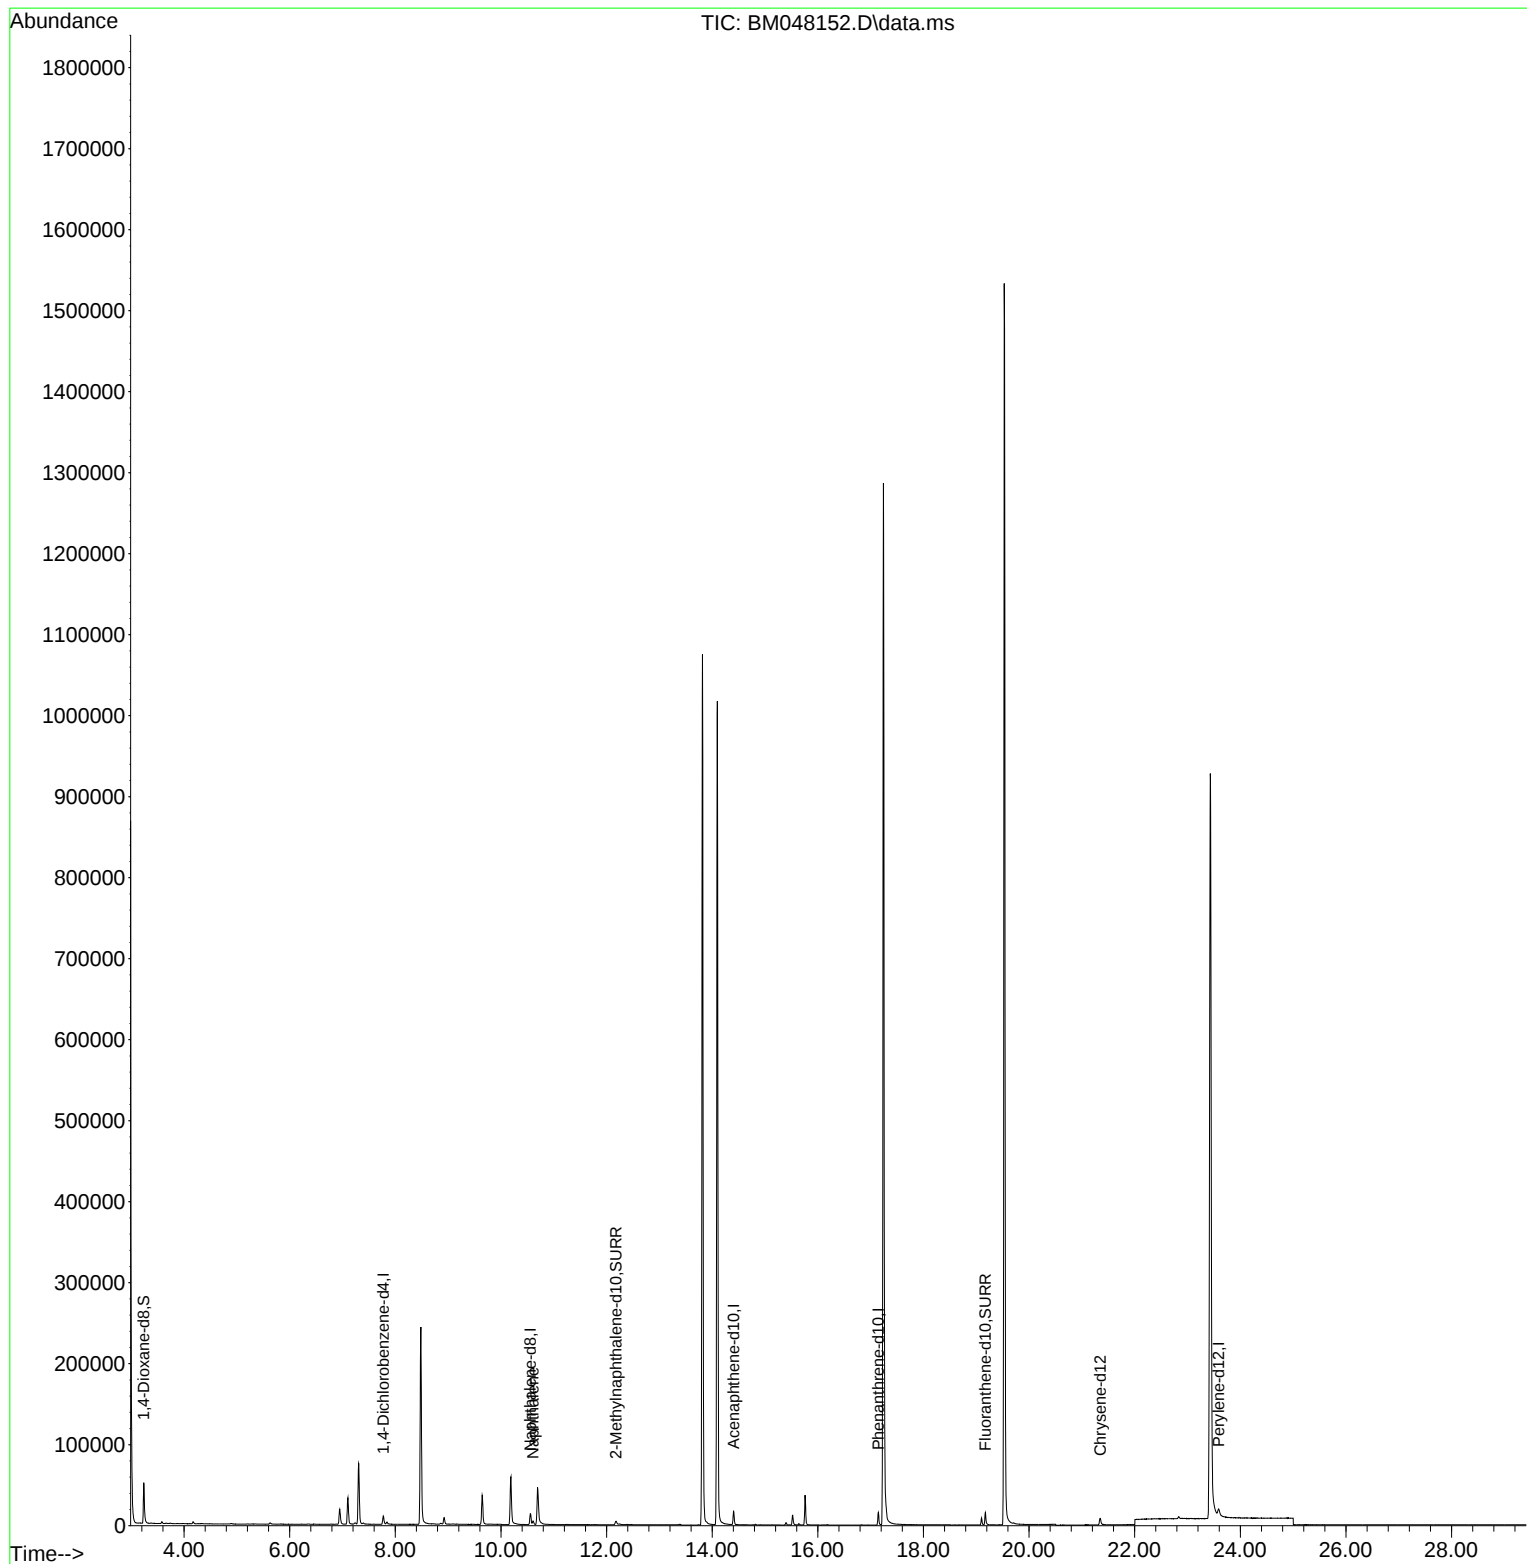

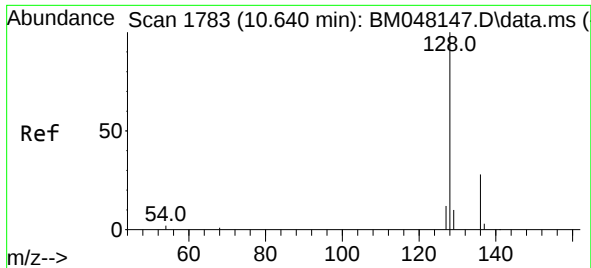

#5
Naphthalene
Concen: 0.071 ng/ul
RT: 10.605 min Scan# 11
Delta R.T. -0.033 min
Lab File: BM048152.D
Acq: 21 Oct 2024 13:23

Instrument :
BNA_M
ClientSampleId :
E27J8

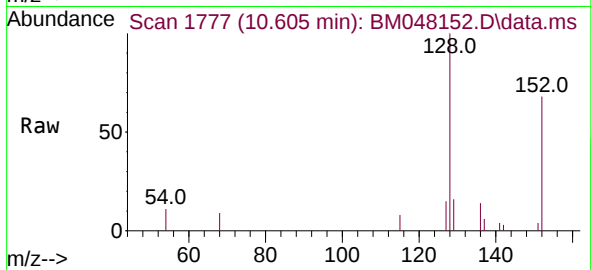

Tgt Ion:128 Resp: 3664
Ion Ratio Lower Upper
128 100
129 16.1 10.6 15.8
127 15.2 11.3 16.9

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 10/22/2024
Supervised By :mohammad ahmed 10/23/2024

