


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102215\
Data File : BM002966.D
Acq On : 22 Oct 2015 02:26
Operator : UM/IZ
Sample : G4075-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JG9J0

Quant Time: Oct 22 13:34:15 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 16:23:48 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMdadoda
10/22/2015 4:57:01 PM

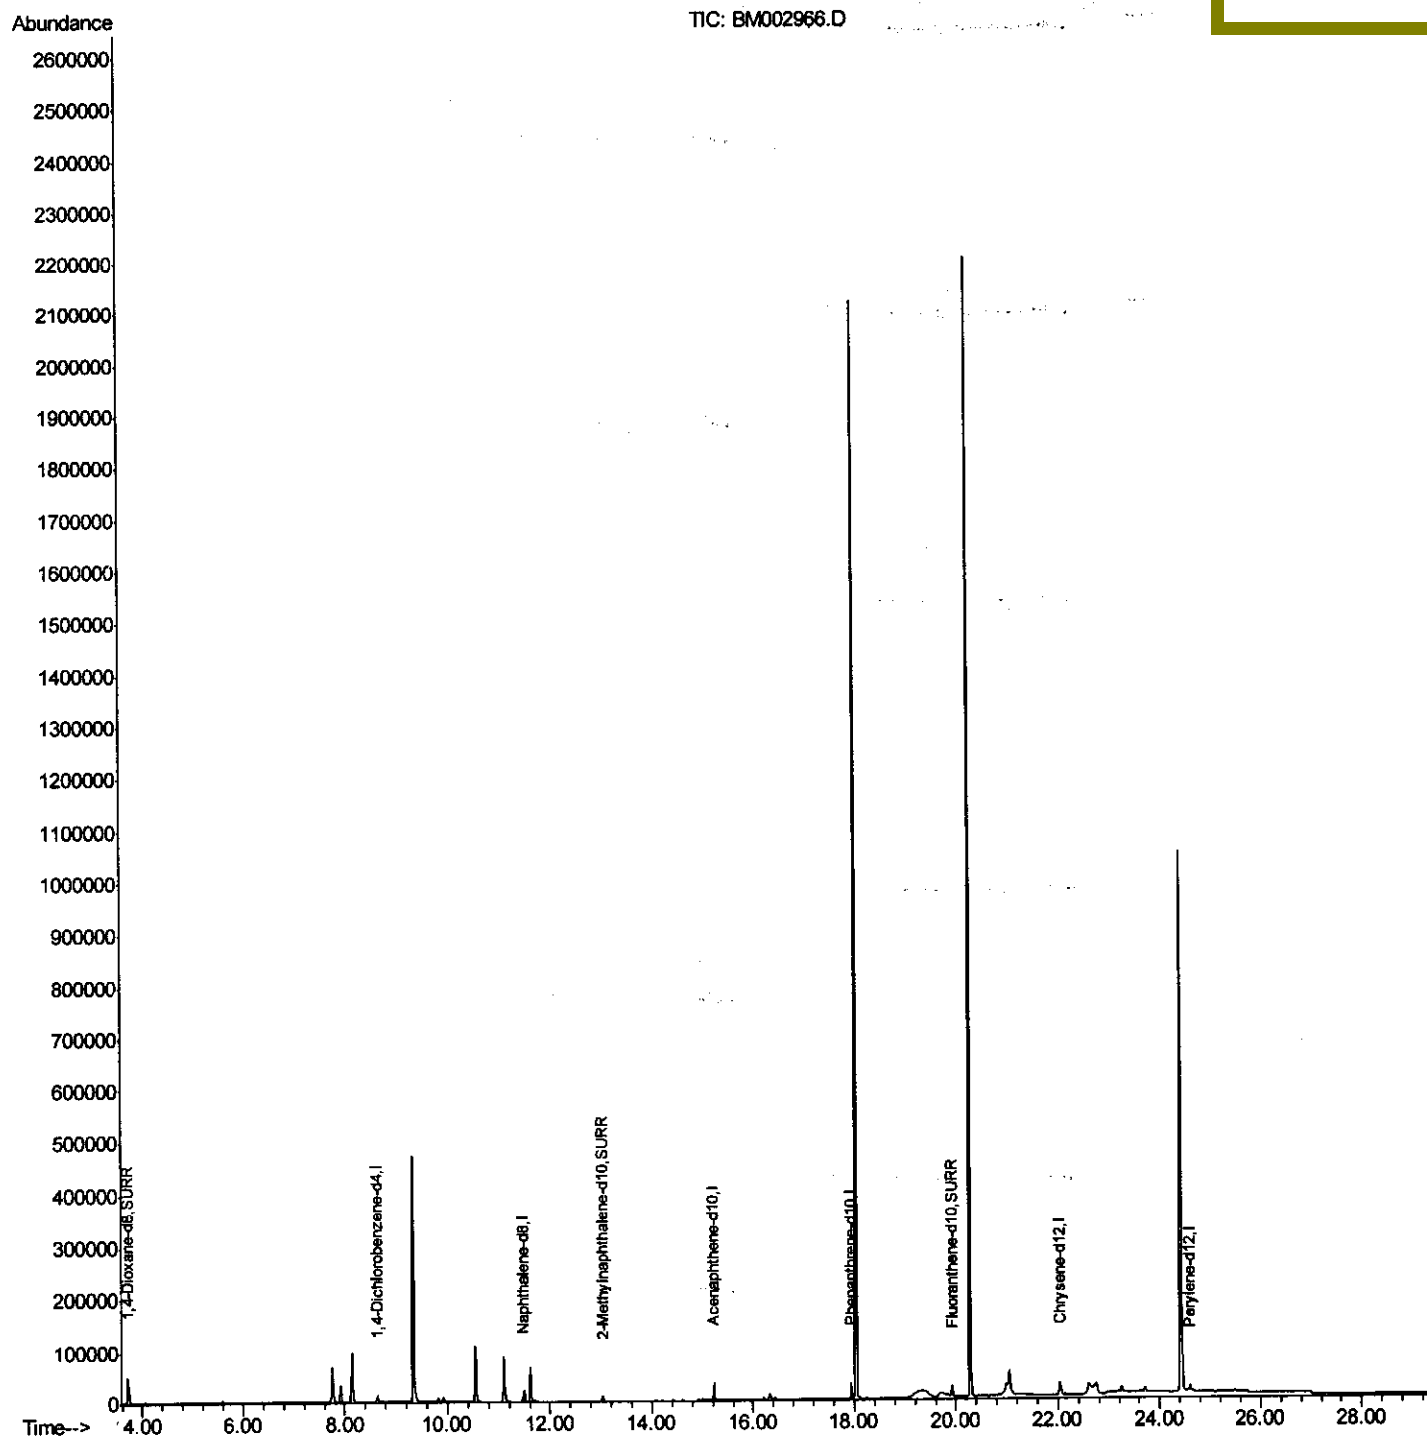

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102215\
 Data File : BM002966.D
 Acq On : 22 Oct 2015 02:26
 Operator : UM/IZ
 Sample : G4075-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JG9J0

Manual Integrations
 APPROVED

MMdadoda
 10/22/2015 4:57:01 PM

Quant Time: Oct 22 12:05:40 2015
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 21 16:23:48 2015
 Response via : Initial Calibration

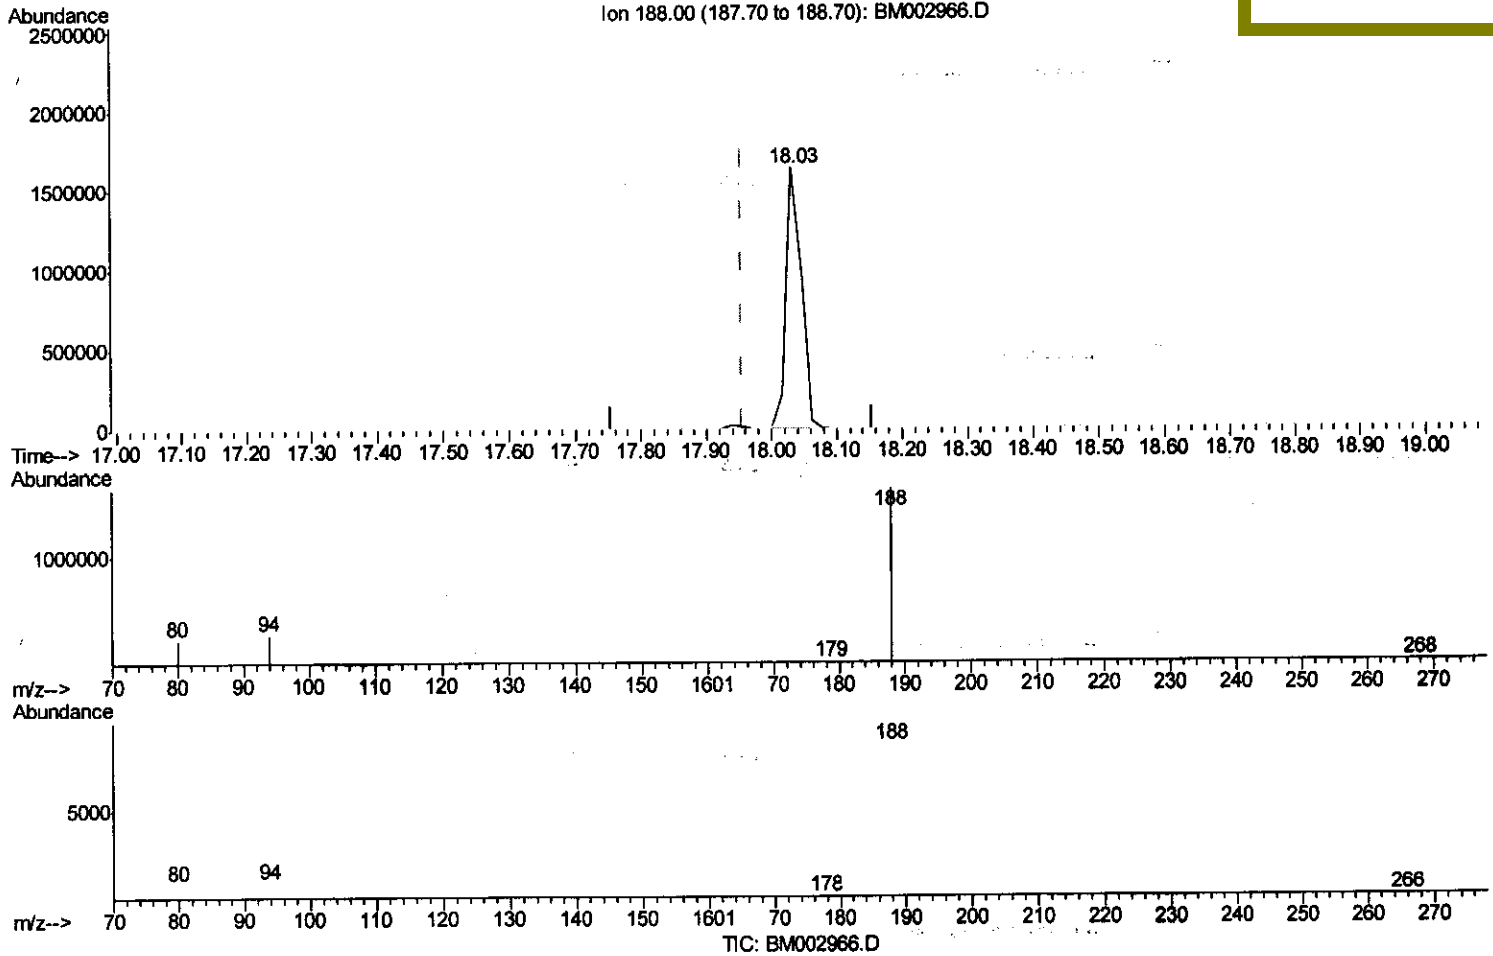

(12) Phenanthrene-d10 (I)

18.031min (+0.077) 0.40ng/ul

response 2650691

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	16.03#
80.00	8.90	13.33#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102215\
Data File : BM002966.D
Acq On : 22 Oct 2015 02:26
Operator : UM/IZ
Sample : G4075-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JG9J0

Quant Time: Oct 22 12:05:40 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 16:23:48 2015
Response via : Initial Calibration

Manual Integrations
APPROVED

MMdadoda
10/22/2015 4:57:01 PM

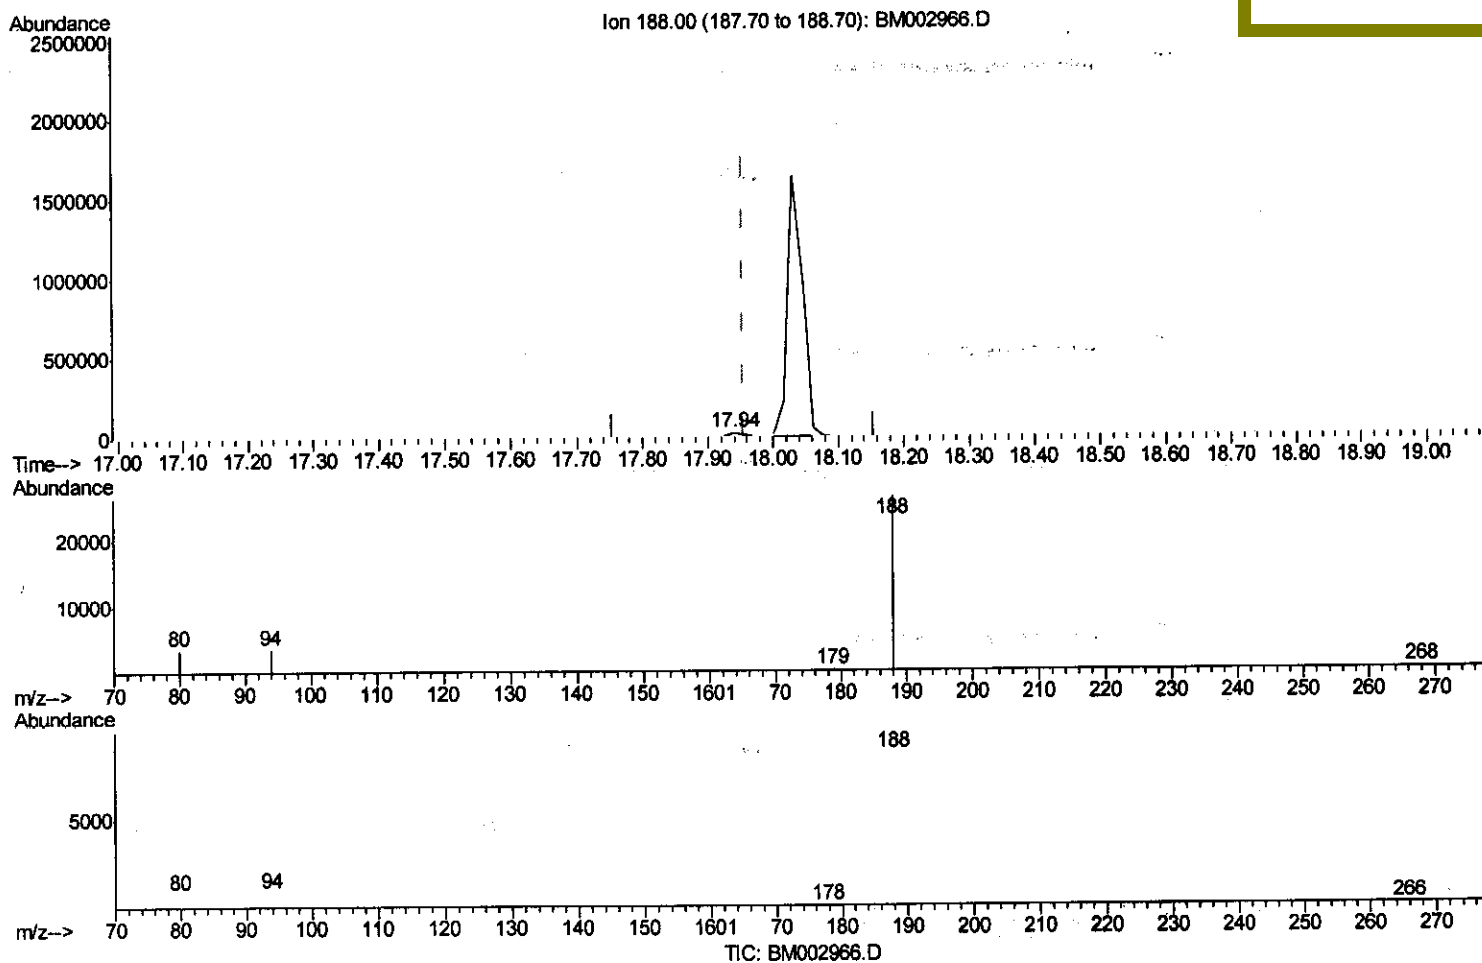

(12) Phenanthrene-d10 (I)

17.938min (-0.016) 0.40ng/ul m

response 40573

Ion	Exp%	Act%
188.00	100	100
94.00	9.00	13.56#
80.00	8.90	13.33#
0.00	0.00	0.00

U.M.
10/23/15

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102215\
Data File : BM002966.D
Acq On : 22 Oct 2015 02:26
Operator : UM/IZ
Sample : G4075-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Oct 22 13:34:15 2015
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 16:23:48 2015
Response via : Initial Calibration

Instrument :
BNA_M
ClientSampleId :
JG9J0

Manual Integrations
APPROVED

MMdadoda
10/22/2015 4:57:01 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.64	152	8952	0.40	ng/ul	-0.02
4) Naphthalene-d8	11.48	136	38075	0.40	ng/ul	-0.02
8) Acenaphthene-d10	15.23	164	20337	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.94	188	40573m	0.40	ng/ul	-0.02
18) Chrysene-d12	22.03	240	25615	0.40	ng/ul	-0.01
22) Perylene-d12	24.60	264	22917	0.40	ng/ul	-0.02

> U.M.
10/23/15

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
2) 1,4-Dioxane-d8	3.71	96	41030	4.29	ng/uL	0.00
6) 2-Methylnaphthalene-d10	13.04	152	17063	0.27	ng/ul	-0.01
16) Fluoranthene-d10	19.93	212	30433	0.28	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed