

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102215\
 Data File : BM002957.D
 Acq On : 21 Oct 2015 21:01
 Operator : UM/IZ
 Sample : G4075-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JG9H9

Manual Integrations
 APPROVED

MMdadoda
 10/22/2015 4:56:53 PM

Quant Time: Oct 22 14:28:17 2015
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM102215.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 21 16:23:48 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.66	152	4795	0.40	ng/ul	0.00
4) Naphthalene-d8	11.49	136	22673	0.40	ng/ul	-0.01
8) Acenaphthene-d10	15.23	164	14078	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.95	188	30373m	0.40	ng/ul	0.00
18) Chrysene-d12	22.04	240	30551	0.40	ng/ul	0.00
22) Perylene-d12	24.61	264	26116m	0.40	ng/ul	-0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.71	96	25264	4.93	ng/uL	0.00
6) 2-Methylnaphthalene-d10	13.05	152	11837	0.31	ng/ul	0.00
16) Fluoranthene-d10	19.93	212	28883	0.36	ng/ul	0.00
Target Compounds						
17) Fluoranthene	19.96	202	3017	0.03	ng/ul	Ovalue 80
21) Chrysene	22.08	228	1811	0.02	ng/ul#	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM102215\
Data File : BM002957.D
Acq On : 21 Oct 2015 21:01
Operator : UM/IZ
Sample : G4075-11
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
JG9H9

Manual Integrations
APPROVED

MMdadoda
10/22/2015 4:56:53 PM

Quant Time: Oct 22 14:28:17 2015
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-SIM-BM102215.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 21 16:23:48 2015
Response via : Initial Calibration

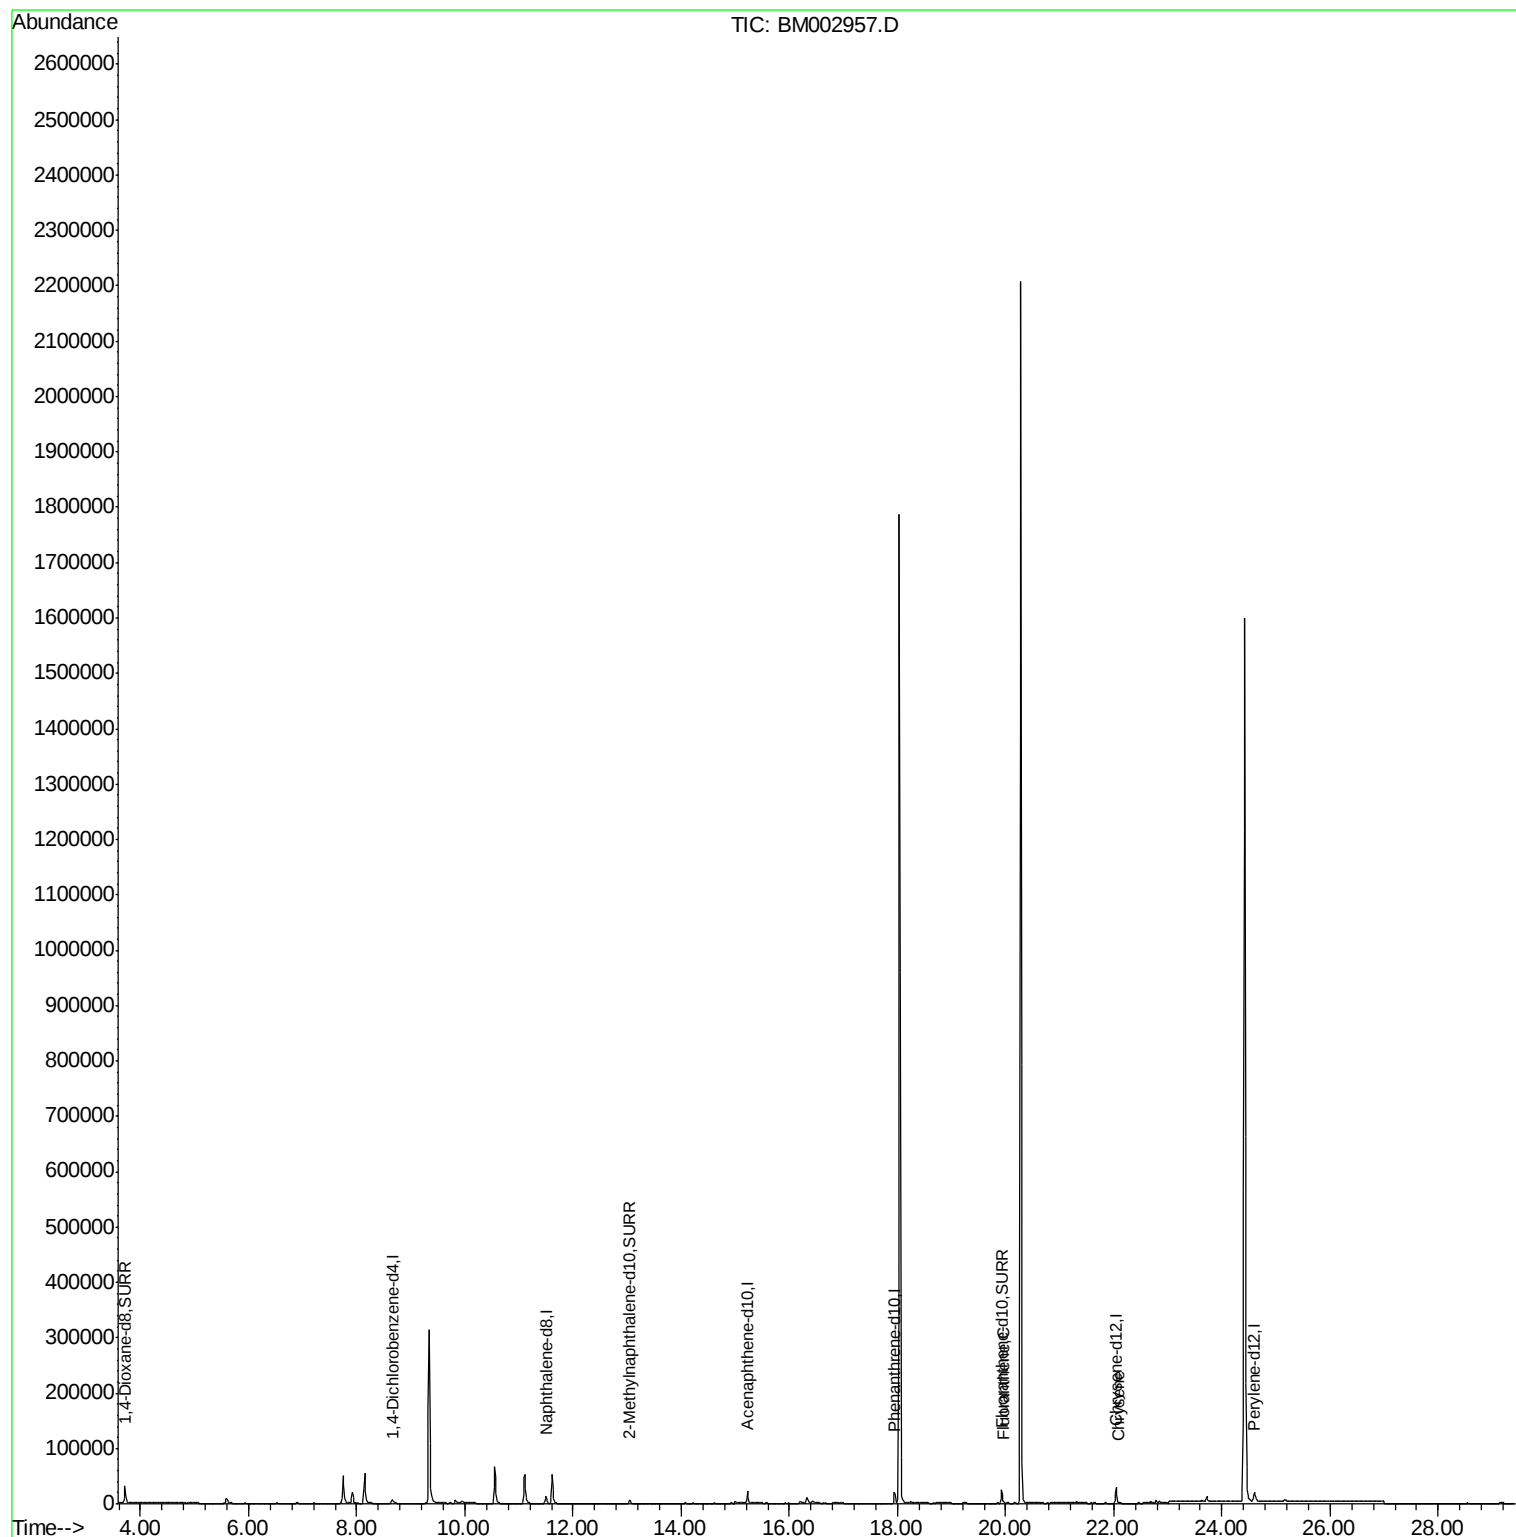

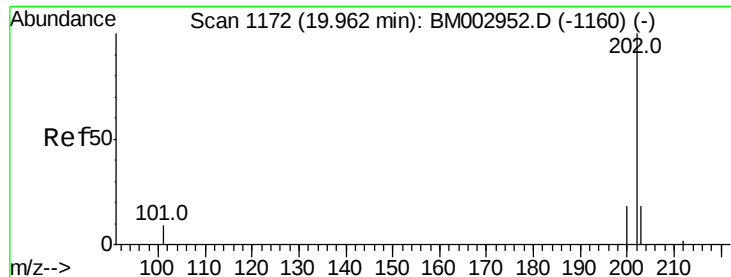

#17

Fluoranthene

Concen: 0.03 ng/ul

RT: 19.96 min Scan# 1172

Delta R.T. -0.00 min

Lab File: BM002957.D

Acq: 21 Oct 2015 21:01

Instrument :

BNA_M





ClientSampleId :

JG9H9

Tot Ion:	202	Resp:	3017
Ion Ratio	Lower	Upper	
202	100		
101	19.9	0.0	33.1
203	26.7	0.0	37.2

Manual Integrations
APPROVED

MMdadoda
10/22/2015 4:56:53 PM

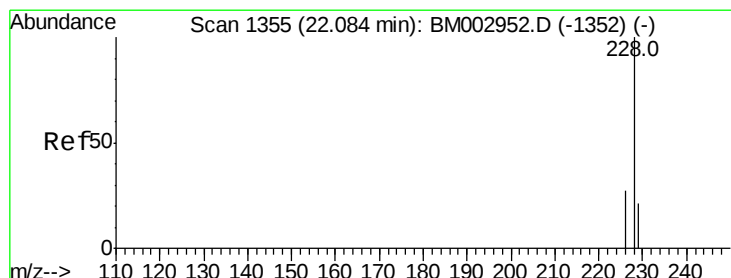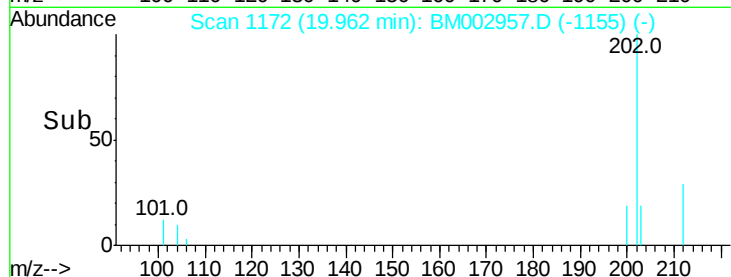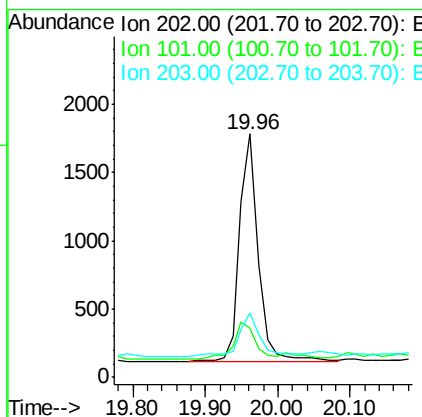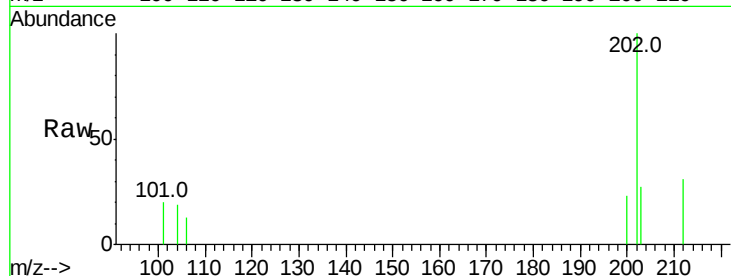

#21

Chrysene

Concen: 0.02 ng/ul

RT: 22.08 min Scan# 1355

Delta R.T. -0.00 min

Lab File: BM002957.D

Acq: 21 Oct 2015 21:01

Tgt Ion:	228	Resp:	1811
Ion Ratio	Lower	Upper	
228	100		
226	38.6	25.7	38.5#
229	34.1	15.2	22.8#

