


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102215\
Data File : BM002945.D
Acq On : 21 Oct 2015 11:31
Operator : UM/IZ
Sample : DFTPP35
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP35

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 21 16:23:48 2015

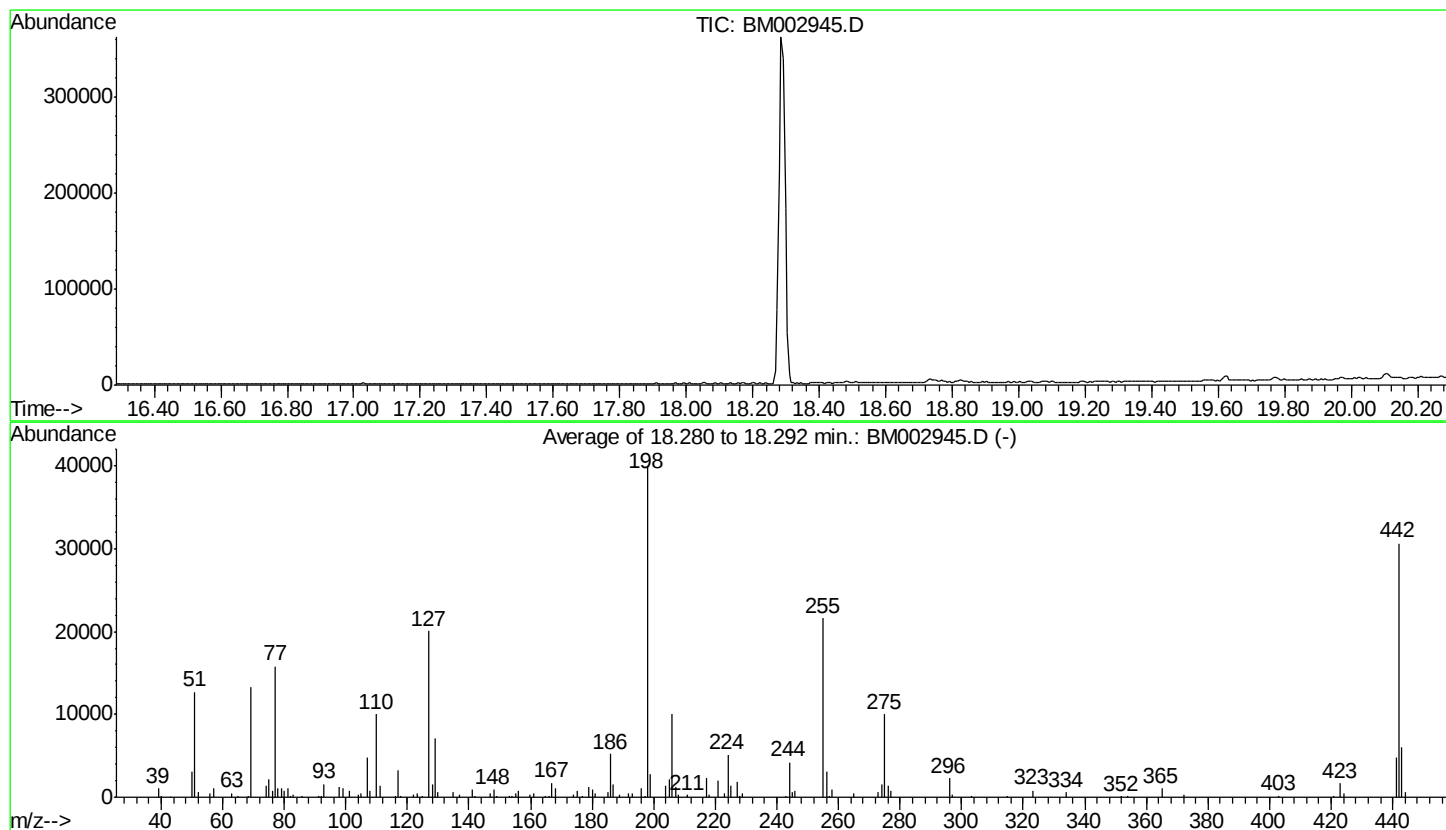

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2578

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.8	12715	PASS
68	69	0.00	2	0.8	105	PASS
69	198	0.00	100	33.3	13339	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.1	20039	PASS
197	198	0.00	1	0.3	102	PASS
198	198	100	100	100.0	40032	PASS
199	198	5	9	7.0	2813	PASS
275	198	10	60	25.1	10037	PASS
365	198	1	100	2.6	1037	PASS
441	443	0.01	100	80.4	4801	PASS
442	198	50	100	76.6	30666	PASS
443	442	15	24	19.5	5968	PASS

m/z	Abundance
39.00	993.0
39.90	305.0
43.00	501.0
44.00	1063.0
50.00	2749.0
51.10	10826.0
52.00	566.0
56.00	409.0
57.00	898.0
63.00	441.0
69.00	11495.0
73.90	1069.0
75.00	1910.0
76.00	591.0
77.00	13530.0
78.00	956.0
79.00	852.0
79.90	673.0
81.00	994.0
93.00	1250.0
98.00	970.0
99.00	1051.0
100.90	553.0
103.90	310.0
105.00	352.0
107.00	3957.0
108.00	742.0
110.00	7873.0
111.00	1135.0
117.00	2635.0
122.00	302.0
123.00	418.0
127.00	15693.0
128.00	1144.0
129.00	5649.0
129.90	512.0
135.00	566.0
136.90	306.0
141.10	770.0
147.00	403.0
148.00	779.0
155.00	429.0
156.00	570.0
160.90	344.0
167.00	1316.0
168.00	1074.0
174.90	510.0
179.00	912.0
180.00	589.0
181.00	353.0
184.90	481.0
186.00	3831.0
186.90	1146.0
192.00	330.0
192.90	387.0
196.00	876.0
198.00	29560.0
198.90	2203.0
204.00	944.0
205.00	1482.0
206.00	7005.0
207.00	1339.0
217.00	1649.0
221.00	1376.0
222.90	338.0
224.00	3673.0
225.00	961.0
227.00	1492.0
228.90	433.0
244.00	3032.0
245.00	493.0
246.00	482.0
255.00	15014.0
256.00	2287.0
257.90	635.0
264.90	326.0
273.00	440.0
274.00	1018.0
275.00	6864.0
276.00	919.0
276.90	477.0
296.00	1576.0
323.00	517.0
334.00	393.0
364.90	587.0
423.00	925.0
424.10	366.0
441.00	2866.0
442.00	17128.0
443.00	3492.0
443.90	389.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
39.00	1171.0
43.00	538.0
44.00	1021.0
50.00	3715.0
51.00	15236.0
52.00	849.0
56.00	568.0
57.00	1300.0
63.00	630.0
65.00	321.0
68.10	315.0
69.00	15655.0
74.00	1663.0
75.00	2371.0
76.00	891.0
77.10	18568.0
78.00	1363.0
79.00	1233.0
79.90	938.0
81.00	1368.0
82.00	338.0
83.00	387.0
85.90	369.0
91.00	330.0
92.00	341.0
93.00	1894.0
98.00	1480.0
99.00	1268.0
101.00	863.0
104.00	466.0
104.90	554.0
107.00	5668.0
108.00	950.0
110.00	11949.0
111.00	1772.0
116.00	342.0
117.00	3953.0
121.90	323.0
123.00	686.0
127.00	23800.0
128.00	1835.0
129.00	8251.0
130.00	741.0
135.00	865.0
136.90	413.0
141.00	993.0
141.90	376.0
146.90	607.0
148.00	1075.0
149.00	309.0
153.00	335.0
154.00	324.0
155.00	605.0
156.00	856.0
160.00	329.0
161.00	476.0
164.90	364.0
167.00	2020.0
168.00	1211.0
174.00	487.0
175.00	895.0
176.90	366.0
179.00	1541.0
180.00	1165.0
181.00	481.0
185.00	727.0
186.00	6165.0
187.00	1809.0
189.00	402.0
191.90	506.0
192.90	541.0
195.90	1378.0
197.10	307.0
198.00	46696.0
199.00	3237.0
204.00	1563.0
205.00	2591.0
206.00	11741.0
207.00	1906.0
207.90	449.0
211.10	391.0
217.00	2840.0
217.90	460.0
221.00	2221.0
223.00	584.0
224.00	5970.0
225.00	1545.0
227.00	2151.0
228.00	391.0
228.90	507.0
243.00	322.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

244.00	4969.0
245.00	658.0
246.00	825.0
255.00	25240.0
256.00	3636.0
257.00	316.0
258.00	1221.0
265.00	446.0
273.00	715.0
274.00	1955.0
275.00	11463.0
276.00	1594.0
277.00	851.0
296.00	2704.0
297.00	350.0
303.00	301.0
323.00	920.0
334.00	598.0
353.90	331.0
364.90	1338.0
372.00	538.0
402.90	323.0
423.00	1932.0
424.00	620.0
441.00	5332.0
442.00	33880.0
443.00	6740.0
444.00	695.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

m/z	Abundance
39.00	986.0
43.00	548.0
44.00	1088.0
50.00	2997.0
51.00	12083.0
52.00	612.0
56.00	456.0
57.00	1091.0
63.00	486.0
65.00	332.0
69.00	12869.0
74.00	1385.0
75.00	2044.0
76.00	701.0
77.10	15276.0
78.00	1062.0
79.00	945.0
80.00	734.0
81.00	1061.0
83.00	345.0
85.90	339.0
93.00	1609.0
98.00	1355.0
99.00	1088.0
101.00	740.0
104.00	393.0
104.90	399.0
107.00	4689.0
108.00	747.0
110.00	10140.0
111.00	1427.0
115.90	354.0
117.00	3309.0
117.90	309.0
121.90	333.0
123.00	438.0
125.00	314.0
127.00	20624.0
128.00	1556.0
129.00	7340.0
130.00	584.0
135.00	608.0
137.00	378.0
141.00	860.0
147.00	489.0
147.90	880.0
153.00	308.0
155.00	469.0
156.00	796.0
159.90	386.0
160.90	441.0
165.00	301.0
165.90	321.0
167.00	1809.0
168.00	1069.0
174.00	432.0
175.00	705.0
176.90	331.0
178.90	1407.0
180.00	1067.0
181.00	411.0
185.00	715.0
186.00	5684.0
187.00	1699.0
188.90	320.0
191.90	404.0
193.00	543.0
196.10	1220.0
198.00	43840.0
199.00	3001.0
204.00	1525.0
205.00	2565.0
206.00	11214.0
207.00	1639.0
207.90	420.0
210.70	373.0
211.00	363.0
216.90	2643.0
217.90	370.0
221.00	2328.0
223.00	570.0
224.00	5845.0
225.00	1489.0
226.90	2122.0
229.00	574.0
243.00	379.0
244.00	4744.0
245.00	616.0
246.00	804.0
255.00	24464.0
256.00	3487.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

258.00	1107.0
265.00	587.0
273.00	761.0
274.00	1850.0
275.00	11786.0
276.00	1490.0
277.00	904.0
296.00	2478.0
296.90	389.0
303.00	342.0
314.90	320.0
323.00	1051.0
334.00	664.0
352.00	337.0
365.00	1186.0
372.10	467.0
403.00	321.0
421.00	315.0
423.00	2087.0
424.00	640.0
441.00	6207.0
442.00	40992.0
443.00	7673.0
444.00	781.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35

Scan 2578 (18.251 min): BM002945.D
DFTPP35

m/z	Abundance
43.00	517.0
44.00	1165.0
207.00	321.0

Instrument :
BNA_M
ClientSampleId :
DFTPP35