

Scan 2577 (18.245 min): BM002970.D
DFTPP36

m/z	Abundance
41.00	313.0
44.00	1005.0
55.00	320.0
207.00	593.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
39.00	913.0
40.00	308.0
41.00	326.0
44.00	883.0
50.00	2630.0
51.10	10737.0
52.00	564.0
55.00	329.0
56.00	485.0
57.00	997.0
63.00	474.0
69.00	11540.0
74.00	1094.0
75.00	1791.0
76.10	571.0
77.00	12800.0
78.00	1110.0
79.00	898.0
79.90	570.0
81.00	994.0
82.00	346.0
83.00	435.0
90.90	316.0
93.00	1503.0
98.00	1016.0
99.00	871.0
100.90	470.0
104.00	343.0
105.00	415.0
107.00	4064.0
107.90	615.0
110.00	8116.0
111.00	1260.0
117.00	2671.0
123.00	493.0
127.00	15899.0
128.00	1247.0
129.00	5690.0
129.90	543.0
135.00	502.0
141.00	620.0
146.90	448.0
147.90	705.0
155.00	374.0
156.00	597.0
161.00	405.0
165.00	303.0
167.00	1508.0
168.00	805.0
174.00	307.0
175.00	660.0
177.00	311.0
179.00	872.0
180.00	731.0
181.00	359.0
185.00	526.0
186.00	3962.0
187.00	1131.0
192.00	334.0
193.00	474.0
196.00	953.0
198.00	29632.0
198.90	1949.0
204.00	990.0
205.00	1638.0
206.00	7229.0
207.00	1646.0
208.00	359.0
217.00	1817.0
221.00	1315.0
222.90	374.0
224.00	4000.0
225.00	1035.0
227.00	1323.0
244.00	2860.0
245.00	358.0
245.90	627.0
255.00	14487.0
256.00	2114.0
257.90	684.0
273.00	472.0
274.00	1180.0
275.00	6566.0
276.00	880.0
277.00	429.0
296.00	1404.0
323.00	537.0
334.00	325.0
364.90	503.0
372.00	311.0
423.00	892.0
441.00	2361.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

442.0015814.0

443.003411.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
39.00	1309.0
40.00	354.0
41.00	320.0
43.00	307.0
44.00	969.0
50.00	3706.0
51.00	15611.0
52.00	759.0
55.10	449.0
56.00	562.0
57.00	1262.0
63.00	597.0
65.00	325.0
68.00	356.0
69.00	16164.0
73.00	353.0
74.00	1613.0
75.00	2696.0
76.00	902.0
77.10	19312.0
78.00	1388.0
79.00	1289.0
80.00	1006.0
81.00	1440.0
82.00	434.0
83.00	441.0
85.00	318.0
86.00	357.0
91.00	350.0
92.00	328.0
93.00	1991.0
98.00	1493.0
99.00	1274.0
100.90	818.0
103.90	497.0
104.90	470.0
107.00	6004.0
108.00	1079.0
110.00	11945.0
111.00	1886.0
116.00	325.0
117.00	3976.0
117.90	341.0
122.00	446.0
123.00	587.0
124.00	311.0
125.00	320.0
127.00	23968.0
128.00	1911.0
129.00	8541.0
130.00	808.0
135.00	853.0
137.00	431.0
140.90	1168.0
141.90	400.0
147.00	637.0
148.00	1100.0
149.00	331.0
152.90	370.0
155.00	691.0
156.00	931.0
160.00	341.0
161.00	623.0
165.00	432.0
166.00	320.0
167.00	2049.0
167.90	1190.0
173.90	513.0
175.00	800.0
176.90	457.0
179.00	1351.0
180.00	1227.0
181.00	612.0
185.00	795.0
186.00	6324.0
187.00	1817.0
188.90	340.0
191.90	524.0
193.00	707.0
196.00	1546.0
198.00	48312.0
198.90	3489.0
203.00	352.0
204.00	1476.0
205.00	2677.0
206.00	12096.0
207.00	2151.0
208.00	509.0
210.90	489.0
216.90	2700.0
218.00	428.0
221.00	2149.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

222.90	616.0
224.00	6173.0
225.00	1699.0
227.00	2262.0
229.00	538.0
242.00	367.0
243.00	354.0
244.00	4949.0
245.00	640.0
246.00	803.0
255.00	25912.0
256.00	3897.0
258.00	1191.0
265.00	550.0
273.00	715.0
274.00	2049.0
275.00	11954.0
276.00	1658.0
277.00	862.0
296.00	2732.0
297.00	353.0
303.00	308.0
323.00	959.0
334.00	601.0
354.00	355.0
365.00	1145.0
372.10	444.0
403.00	317.0
423.00	2048.0
424.00	479.0
441.00	5315.0
442.10	33992.0
443.10	6900.0
444.00	547.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

m/z	Abundance
39.00	1088.0
41.00	363.0
44.00	867.0
50.00	3299.0
51.10	12685.0
52.00	681.0
55.00	474.0
56.00	533.0
57.00	1187.0
63.00	553.0
65.00	307.0
68.00	317.0
69.00	13925.0
73.10	357.0
74.00	1367.0
75.00	2306.0
76.10	745.0
77.00	16221.0
78.10	1160.0
79.00	1019.0
80.00	845.0
81.00	1344.0
82.00	412.0
83.00	495.0
85.00	324.0
91.00	451.0
91.90	313.0
93.00	1828.0
98.00	1230.0
98.90	1145.0
101.00	649.0
104.00	348.0
104.90	509.0
107.00	5271.0
108.00	912.0
110.00	10822.0
110.90	1566.0
117.00	3557.0
121.90	351.0
123.00	657.0
125.00	306.0
127.00	21744.0
128.00	1610.0
129.00	8084.0
130.00	704.0
135.00	707.0
135.90	321.0
137.00	364.0
141.00	1061.0
141.90	333.0
142.90	300.0
147.00	715.0
148.00	1098.0
149.00	342.0
153.00	324.0
154.90	571.0
156.00	851.0
160.00	323.0
161.00	537.0
165.00	477.0
166.00	329.0
167.00	2080.0
167.90	931.0
174.00	494.0
175.00	918.0
176.90	477.0
178.90	1540.0
179.90	978.0
180.90	545.0
185.00	677.0
186.00	5942.0
187.00	1792.0
189.00	454.0
191.90	510.0
193.00	637.0
196.00	1489.0
198.00	47104.0
199.00	3162.0
204.00	1593.0
205.00	2609.0
206.00	11427.0
207.00	2057.0
208.10	466.0
210.80	377.0
217.00	2738.0
217.90	393.0
221.00	2303.0
221.80	457.0
223.00	644.0
224.00	6172.0
225.00	1515.0
227.00	2341.0

Instrument :
BNA_M
ClientSampleId :
DFTPP36

229.00	602.0
242.00	393.0
243.00	318.0
244.00	5164.0
245.00	643.0
246.00	793.0
255.00	25472.0
256.00	3602.0
257.00	332.0
258.00	1224.0
264.90	542.0
273.00	748.0
274.00	2031.0
275.00	12436.0
276.00	1613.0
277.00	887.0
296.00	2698.0
297.00	371.0
303.00	336.0
315.00	332.0
323.00	910.0
334.10	636.0
354.00	363.0
365.00	1293.0
372.10	499.0
422.00	329.0
423.00	2269.0
424.00	446.0
441.00	6556.0
442.10	42976.0
443.00	7856.0
444.00	659.0


Instrument :
BNA_M
ClientSampleId :
DFTPP36

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102315\
 Data File : BM002970.D
 Acq On : 22 Oct 2015 10:04
 Operator : UM/IZ
 Sample : DFTPP36
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP36

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM102215.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 23 15:47:05 2015

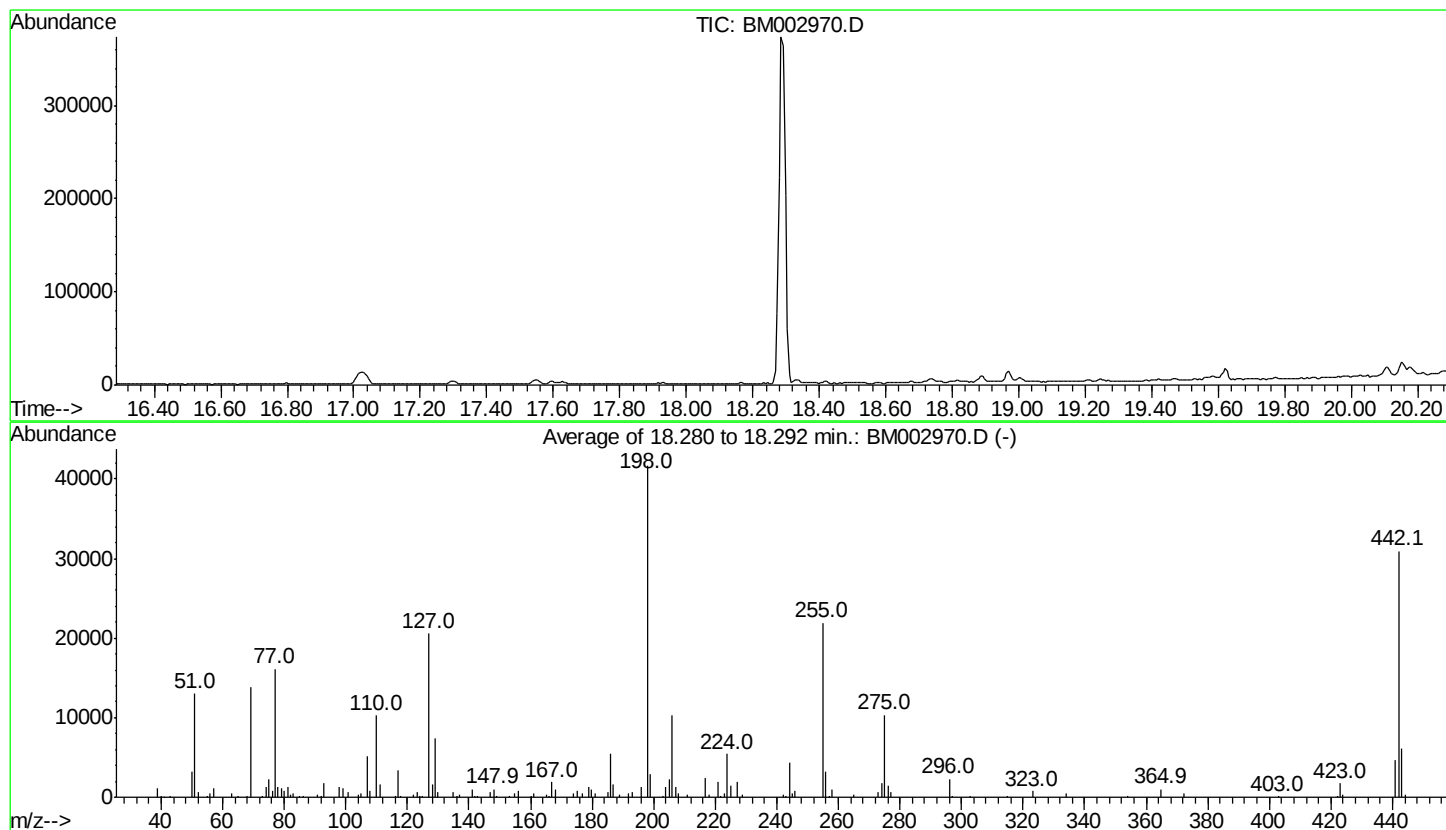

AutoFind: Scans 2583, 2584, 2585; Background Corrected with Scan 2577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	13011	PASS
68	69	0.00	2	1.6	224	PASS
69	198	0.00	100	33.3	13876	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.3	20537	PASS
197	198	0.00	1	0.0	0	PASS
198	198	100	100	100.0	41682	PASS
199	198	5	9	6.9	2866	PASS
275	198	10	60	24.8	10318	PASS
365	198	1	100	2.4	980	PASS
441	443	0.01	100	78.3	4744	PASS
442	198	50	100	74.2	30927	PASS
443	442	15	24	19.6	6055	PASS