
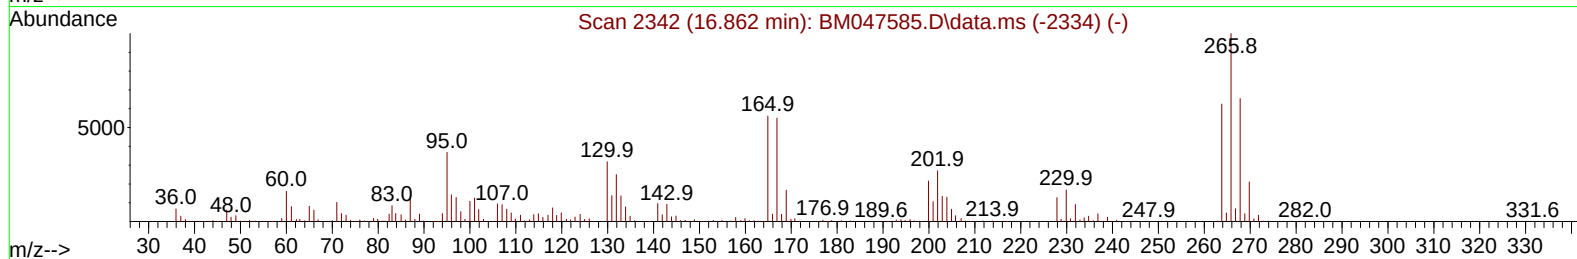
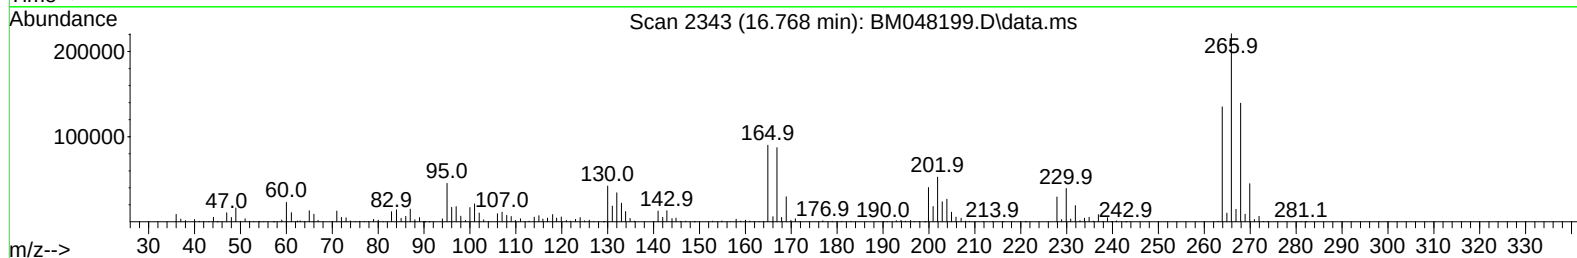


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102324\
Data File : BM048199.D
Acq On : 23 Oct 2024 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 14:47:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 13:43:53 2024
Response via : Initial Calibration

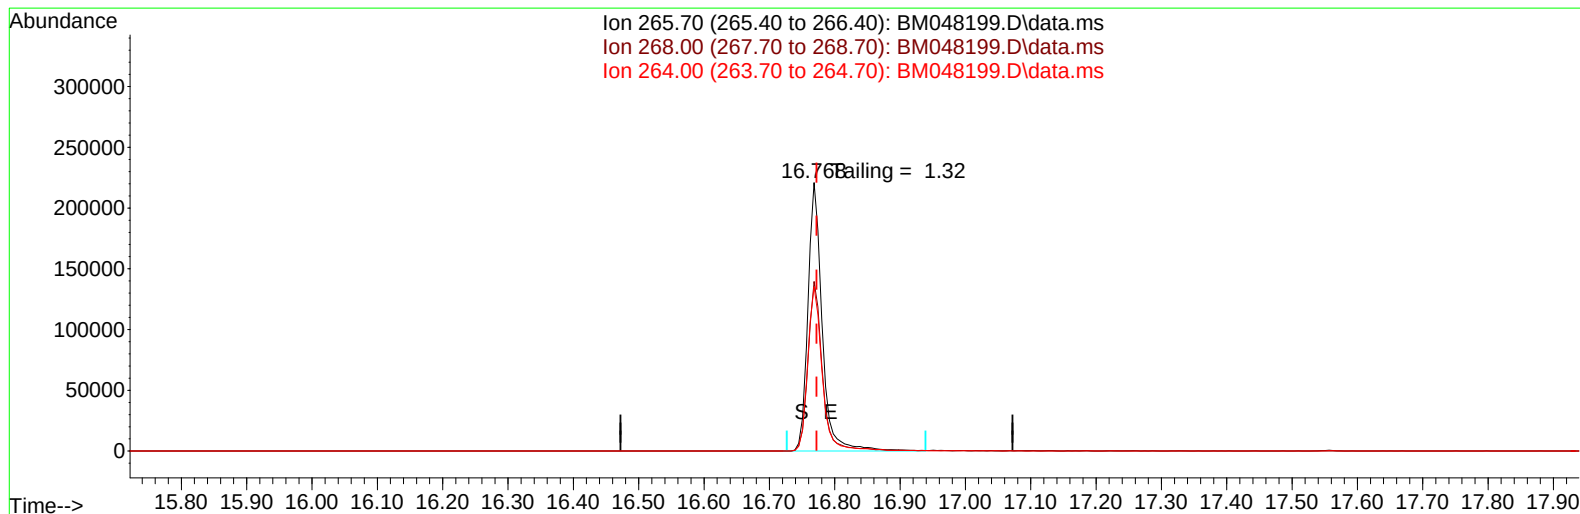

TIC: BM048199.D\data.ms

(70) Pentachlorophenol (C)




16.768min (-0.004) 0.00 ng

response 336927

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.30	63.12
264.00	62.50	61.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102324\
Data File : BM048199.D
Acq On : 23 Oct 2024 11:47
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 23 14:47:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 13:43:53 2024
Response via : Initial Calibration

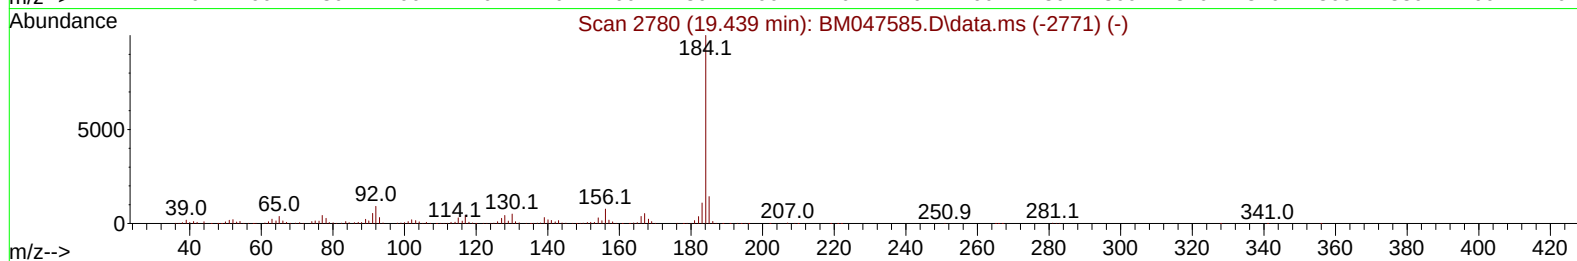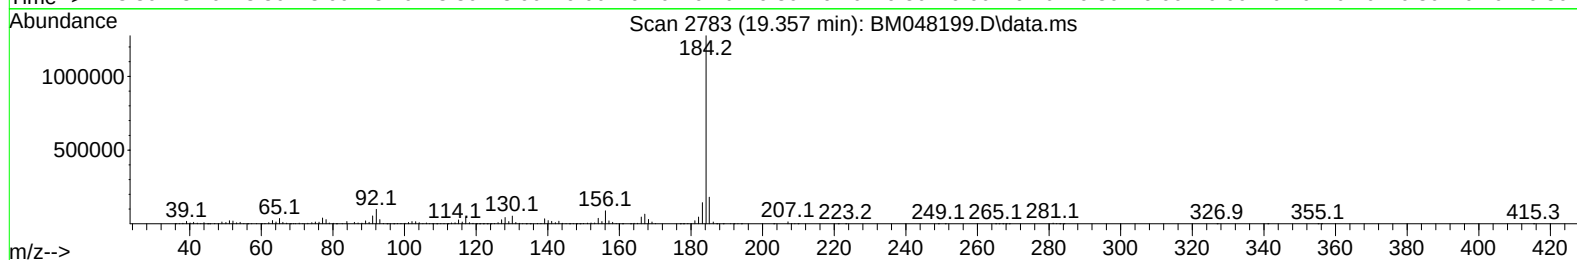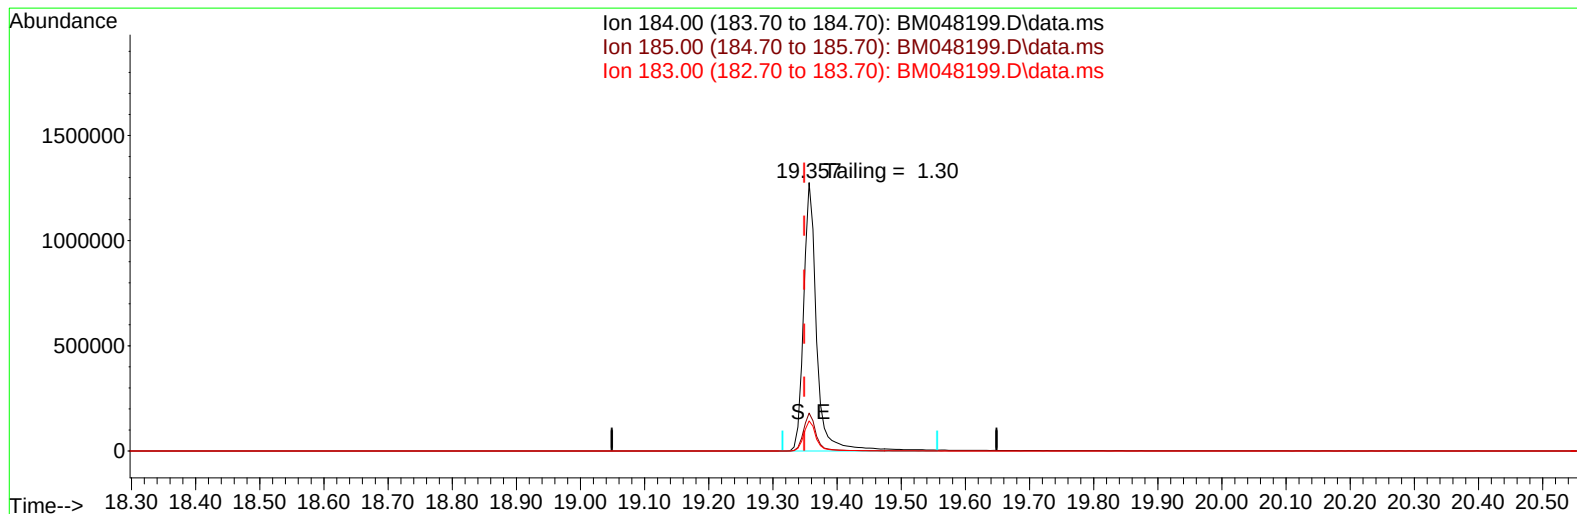

TIC: BM048199.D\data.ms

(77) Benzidine

19.357min (+ 0.008) 0.00 ng

response 1816071

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.15
183.00	10.90	11.22
0.00	0.00	0.00