

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102422\
 Data File : BM037208.D
 Acq On : 24 Oct 2022 17:51
 Operator : CG/JU
 Sample : N5103-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0B93

Quant Time: Oct 25 02:35:08 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:34:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.900	152	4512	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	14138	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.529	164	8582	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.271	188	19802	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.447	240	18235	0.400	ng/ul	# 0.00
23) Perylene-d12	23.821	264	17142	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.314	96	8065	1.466	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	6008	0.299	ng/ul	0.00
18) Fluoranthene-d10	19.294	212	19421	0.352	ng/ul	0.00
Target Compounds						
					Qvalue	
10) Acenaphthylene	14.251	152	931	0.025	ng/ul#	50


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102422\
Data File : BM037208.D
Acq On : 24 Oct 2022 17:51
Operator : CG/JU
Sample : N5103-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0B93


Quant Time: Oct 25 02:35:08 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 22 03:34:37 2022
Response via : Initial Calibration

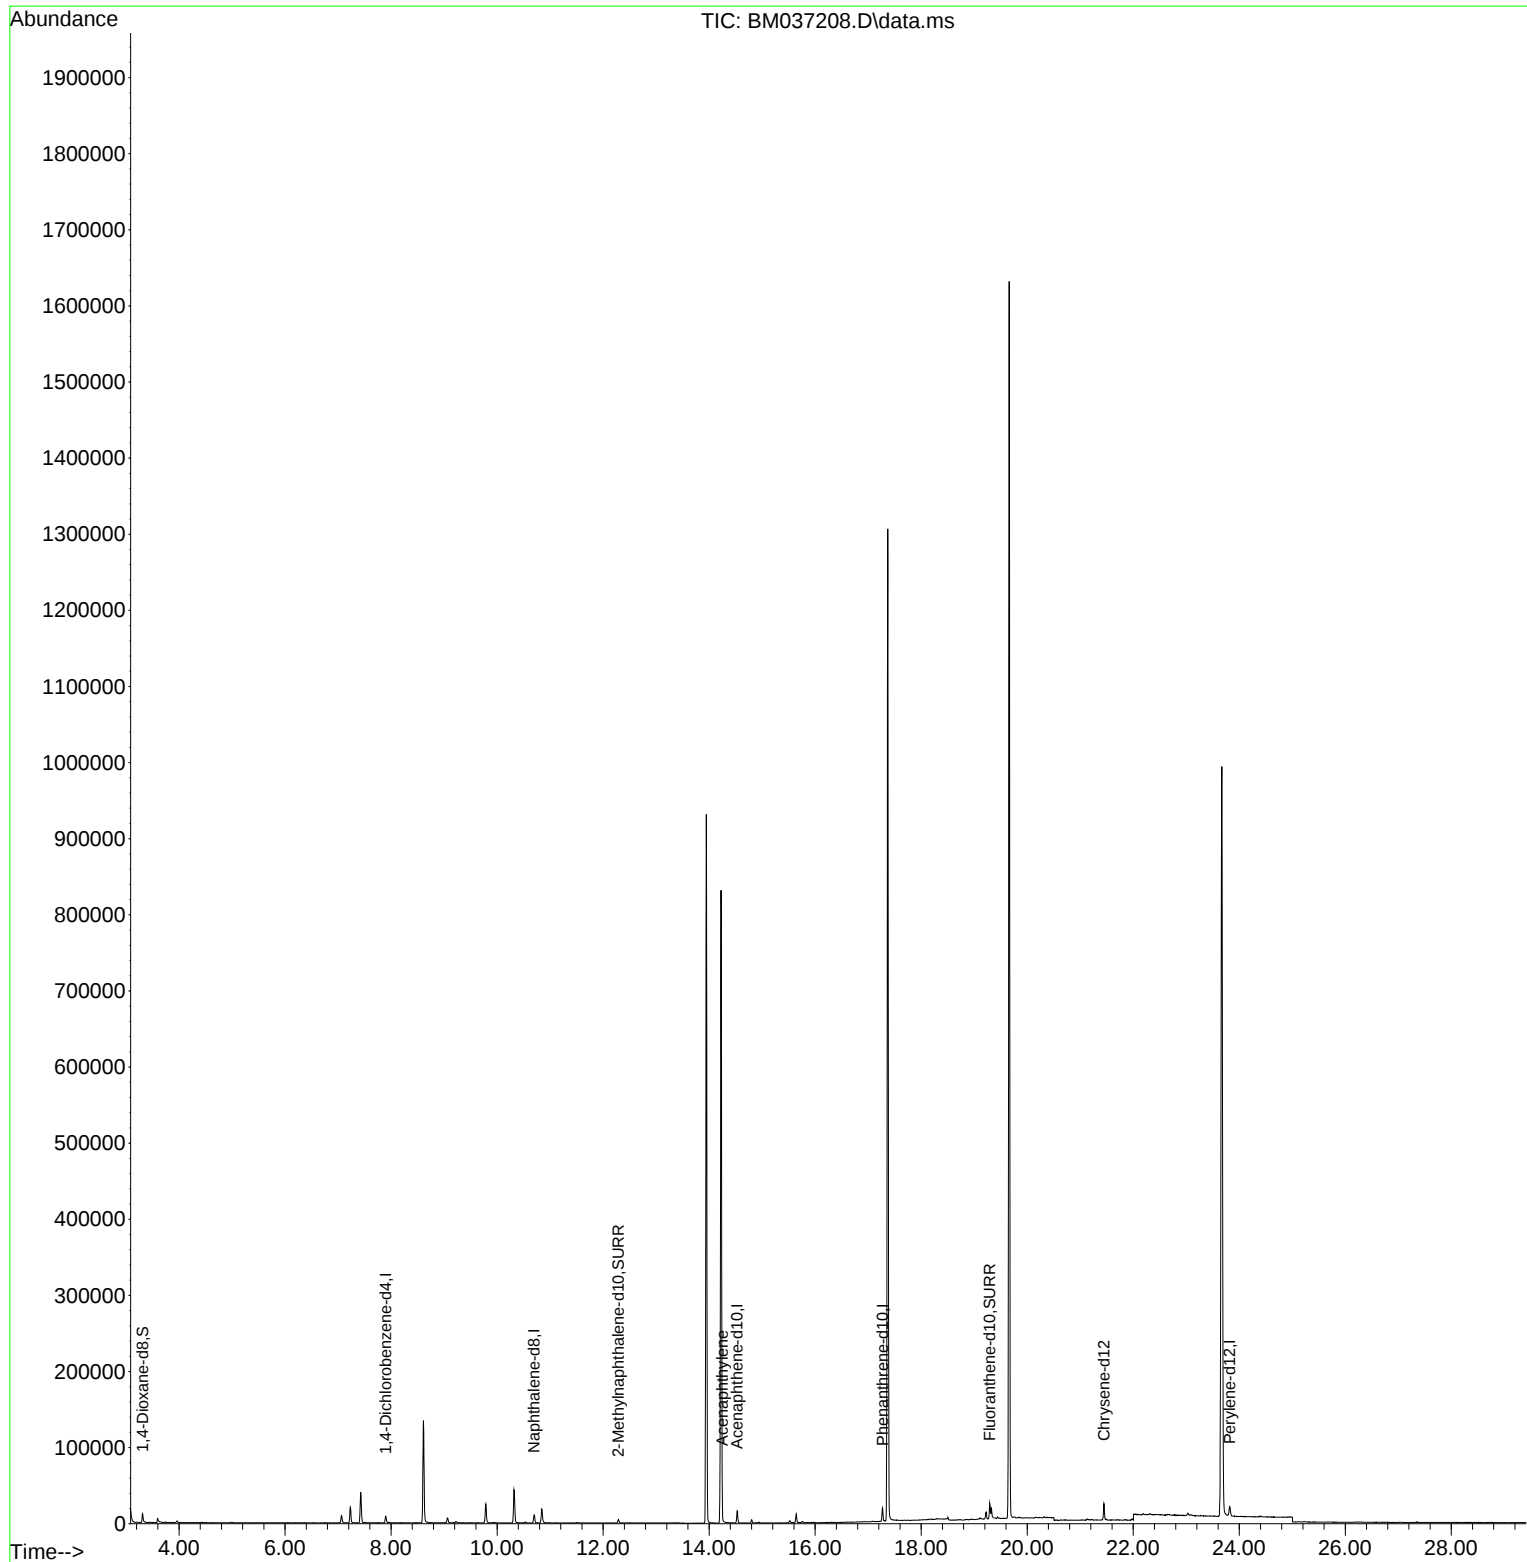

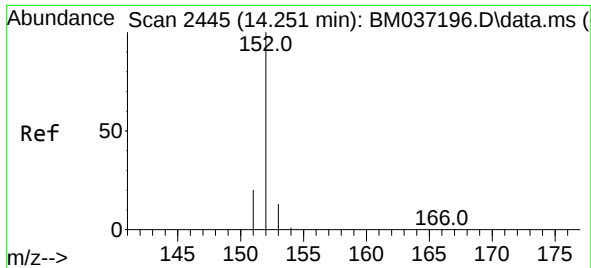

#10
 Acenaphthylene
 Concen: 0.025 ng/ul
 RT: 14.251 min Scan# 2445
 Delta R.T. -0.001 min
 Lab File: BM037208.D
 Acq: 24 Oct 2022 17:51

Instrument :
 BNA_M
 ClientSampleId :
 C0B93

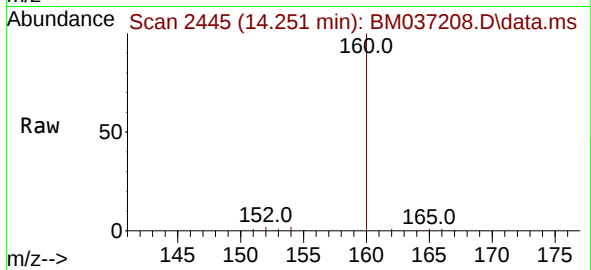

Tgt Ion:	152	Resp:	931
Ion	Ratio	Lower	Upper
152	100		
151	38.7	16.2	24.2#
153	39.7	10.8	16.2#

