
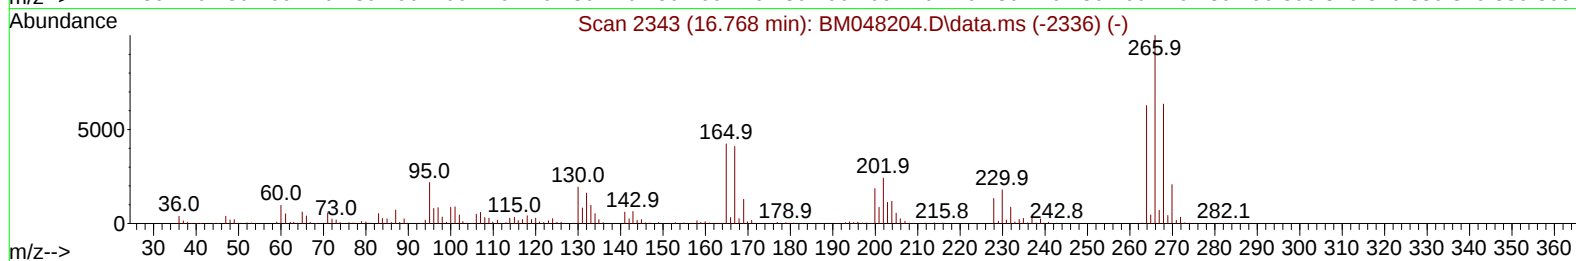
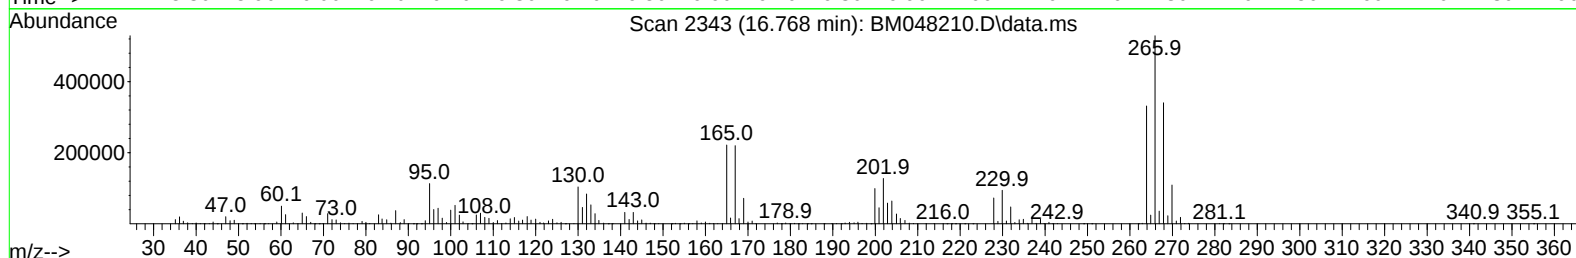


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048210.D
Acq On : 24 Oct 2024 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 12:20:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

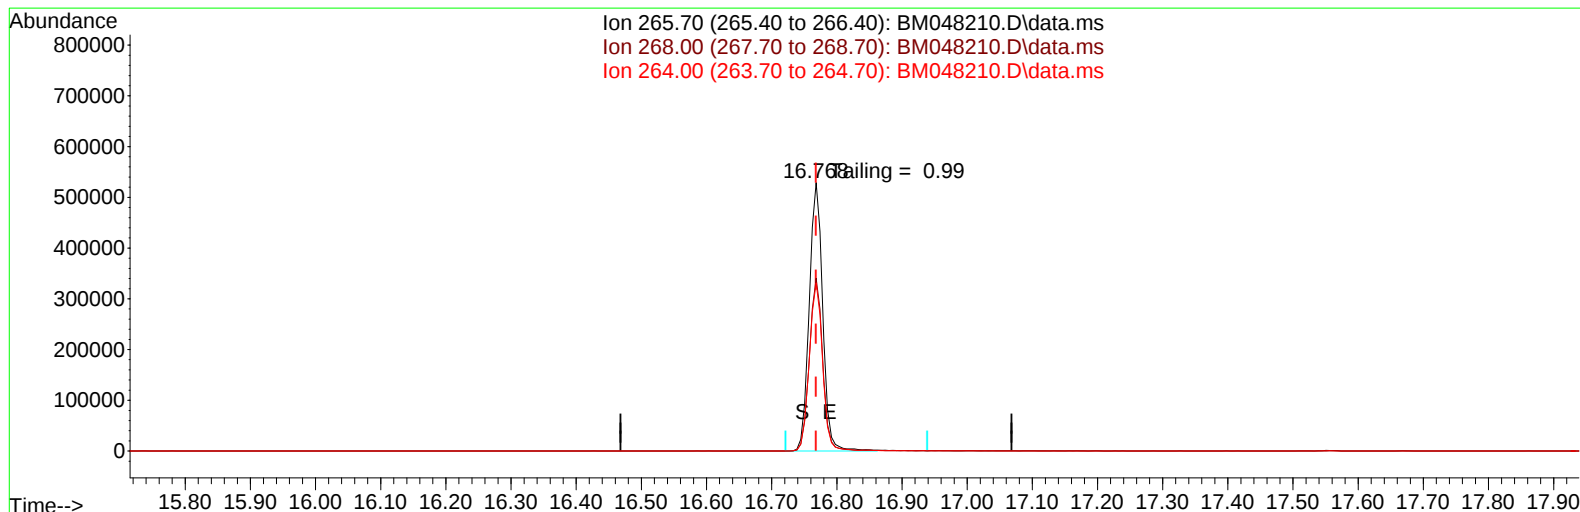

TIC: BM048210.D\data.ms

(70) Pentachlorophenol (C)




16.768min (-0.000) 92717.46 ng

response 764974

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	64.34
264.00	62.70	62.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048210.D
Acq On : 24 Oct 2024 10:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 12:20:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

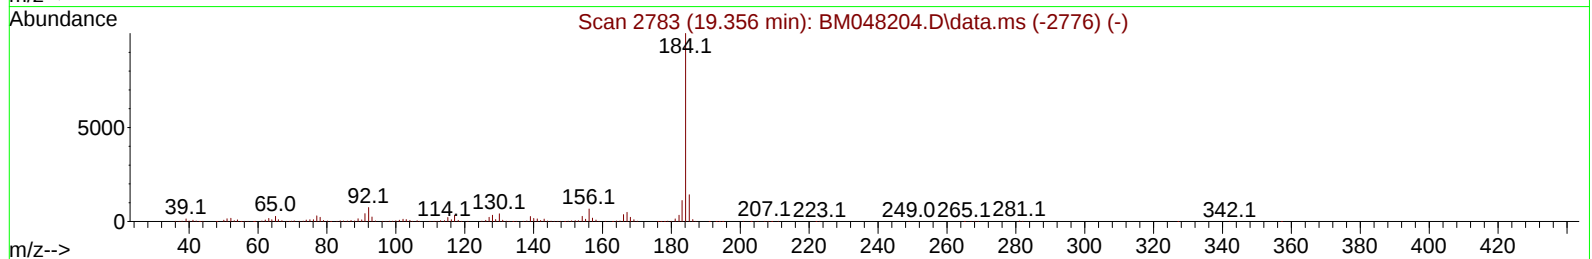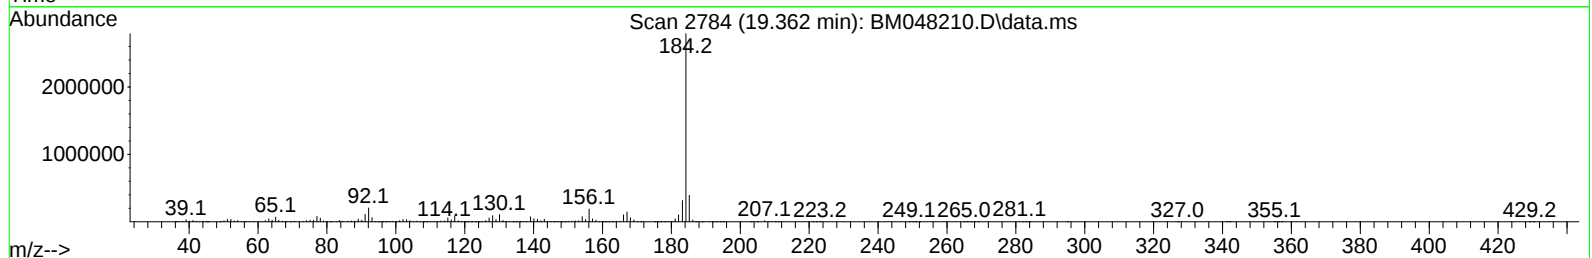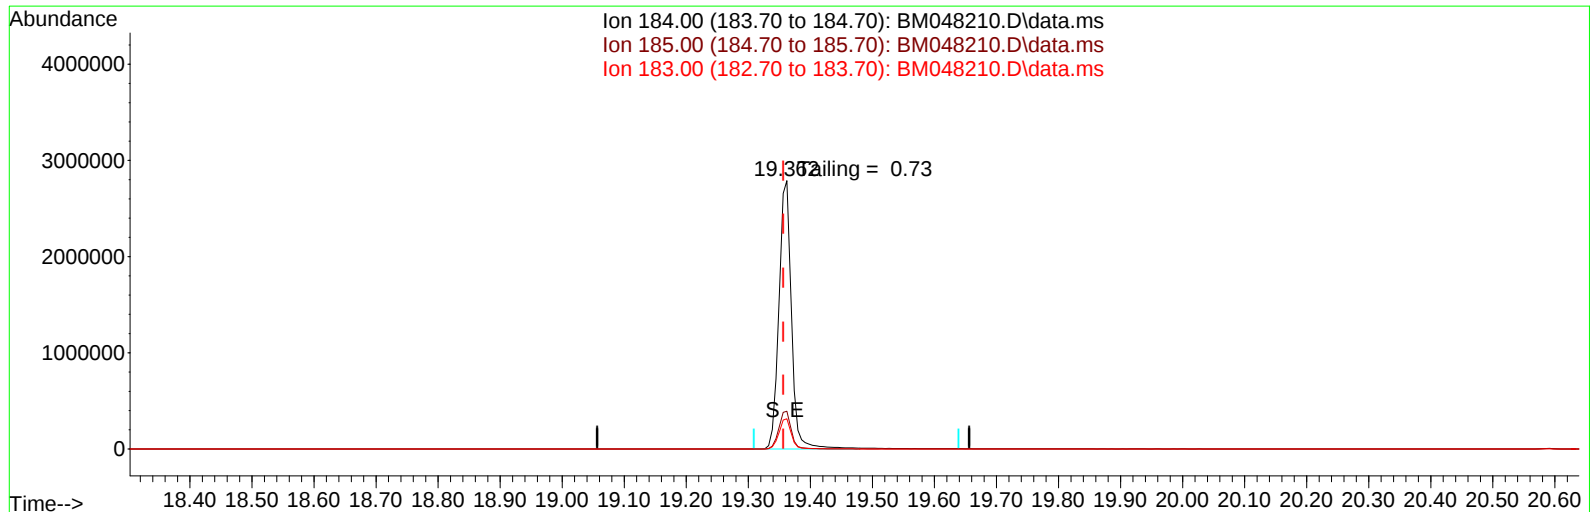

TIC: BM048210.D\data.ms

(77) Benzidine**19.362min (+ 0.006) 54520.09 ng****response 3968464**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.08
183.00	11.20	11.29
0.00	0.00	0.00