

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
 Data File : BM048225.D
 Acq On : 24 Oct 2024 20:26
 Operator : RC/JU
 Sample : PB164366BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB164366BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM048225.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	152	157	163	rBV	170122	230508	2.58%	0.464%
2	4.846	310	316	325	rBV	242250	352697	3.95%	0.710%
3	5.304	388	394	408	rBV	4073519	6082293	68.10%	12.249%
4	6.898	655	665	681	rBV	3634889	6042603	67.66%	12.169%
5	7.716	797	804	812	rBV	753189	1228417	13.75%	2.474%
6	8.875	993	1001	1014	rBV	2178800	3710998	41.55%	7.473%
7	10.510	1270	1279	1293	rBV	830587	1576611	17.65%	3.175%
8	12.980	1692	1699	1716	rBV	5171813	8145078	91.20%	16.403%
9	14.363	1927	1934	1948	rBV	1255745	1987492	22.25%	4.003%
10	15.851	2180	2187	2201	rBV	3559599	5492597	61.50%	11.061%
11	17.110	2394	2401	2412	rBV	1264629	2054834	23.01%	4.138%
12	19.733	2841	2847	2862	rVB	6650507	8931117	100.00%	17.986%
13	20.498	2974	2977	2982	rBV2	77642	104908	1.17%	0.211%
14	21.333	3113	3119	3131	rBV	1109287	1943650	21.76%	3.914%
15	24.280	3613	3620	3635	rVB	659941	1772415	19.85%	3.569%




Sum of corrected areas: 49656218

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048225.D
Acq On : 24 Oct 2024 20:26
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164366BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

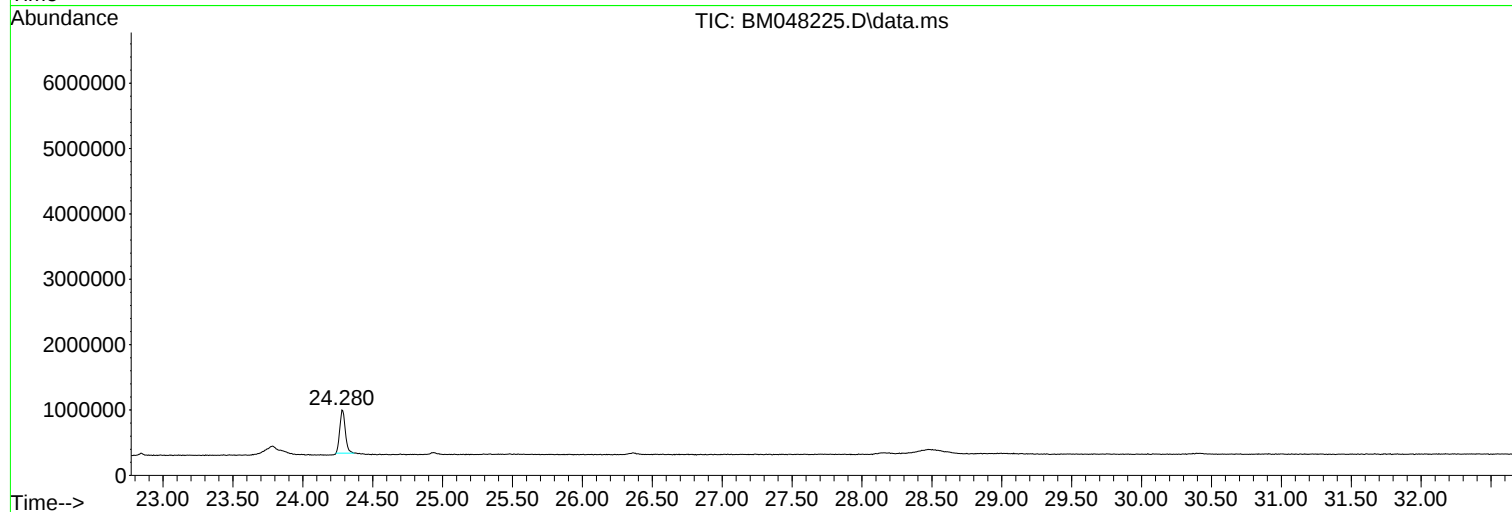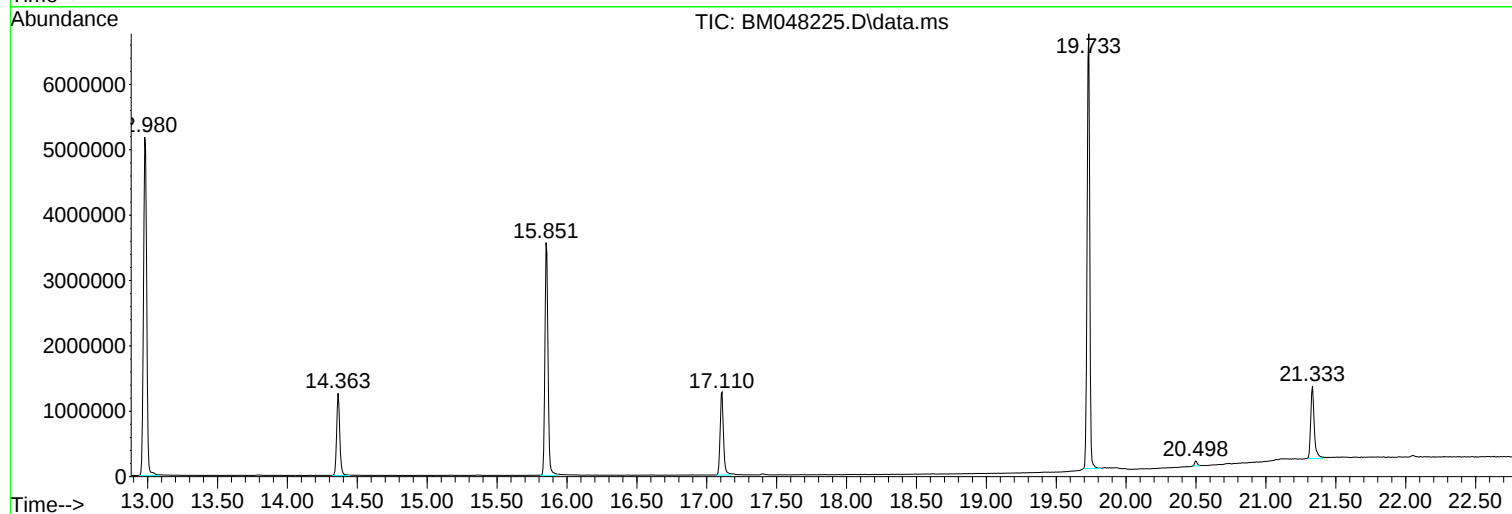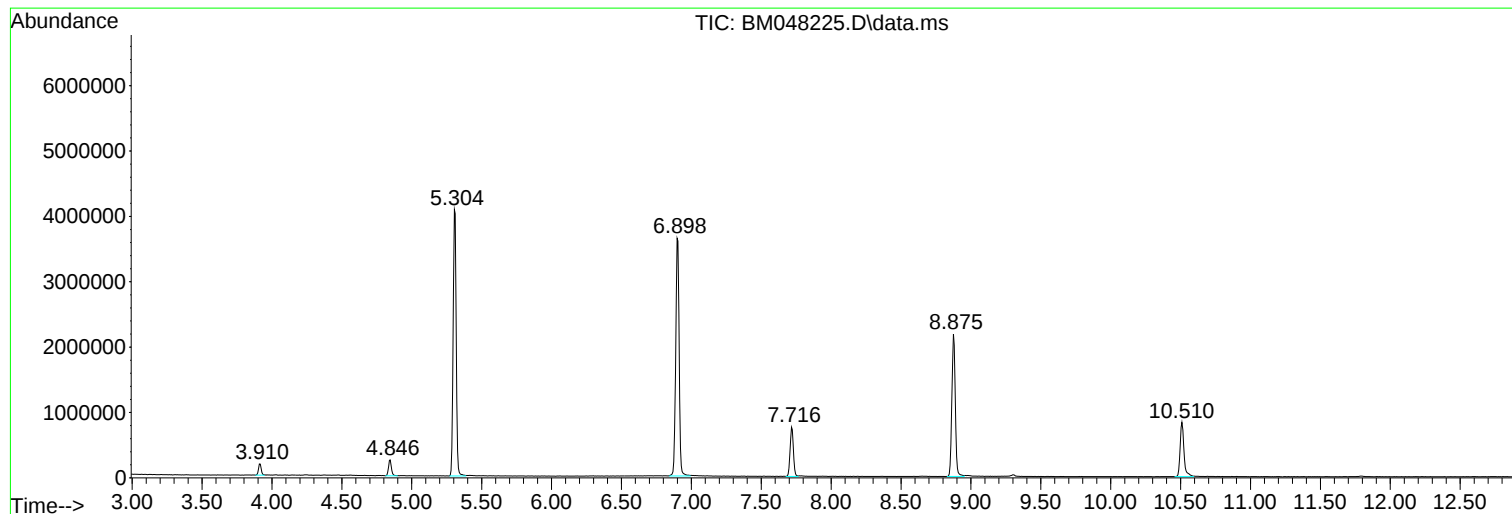

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048225.D
Acq On : 24 Oct 2024 20:26
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164366BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.846	5.74 ng	352697	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	35
3			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4			1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5			(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9

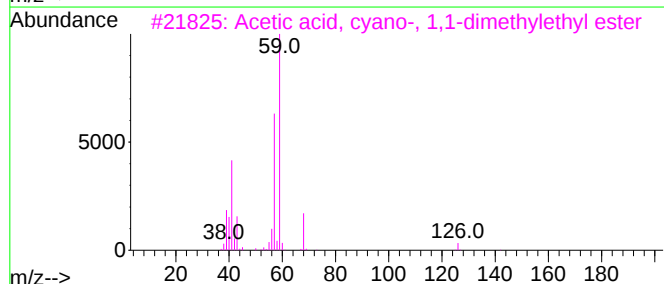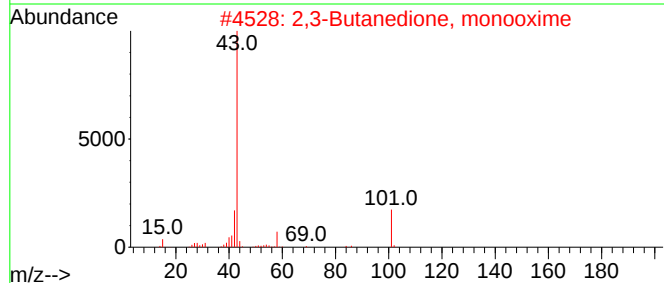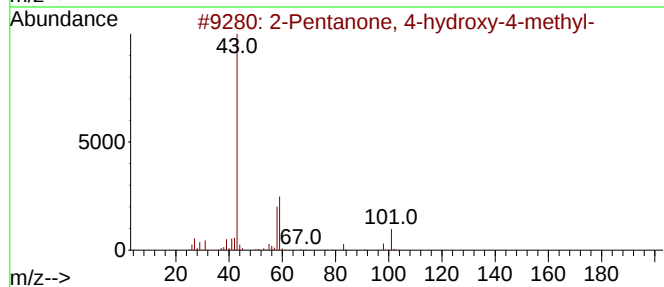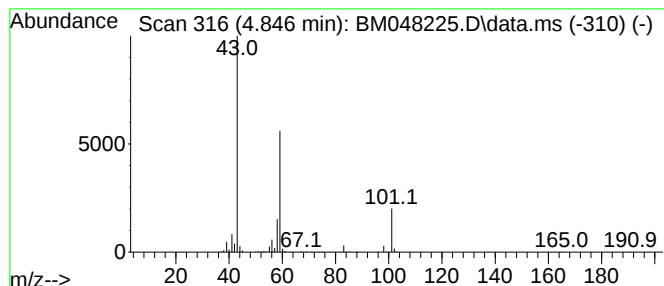

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102424\
Data File : BM048225.D
Acq On : 24 Oct 2024 20:26
Operator : RC/JU
Sample : PB164366BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164366BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.846	5.7	ng	352697	1	7.716	1228420	20.0