

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
 Data File : BM032695.D
 Acq On : 25 Oct 2021 15:34
 Operator : CG/JU
 Sample : M4304-06
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P064-TW001-01

Quant Time: Oct 25 16:11:12 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 10:44:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	3773	0.400	ng/ul	0.00
4) Naphthalene-d8	10.325	136	12431	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.202	164	7007	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.936	188	13454	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.113	240	8659	0.400	ng/ul	0.00
23) Perylene-d12	23.244	264	8867	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.913	96	21016	4.970	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.927	152	6131	0.370	ng/ul	0.00
18) Fluoranthene-d10	18.962	212	12775	0.469	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.974	178	1314	0.029	ng/ul#	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
Data File : BM032695.D
Acq On : 25 Oct 2021 15:34
Operator : CG/JU
Sample : M4304-06
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P064-TW001-01


Quant Time: Oct 25 16:11:12 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 10:44:54 2021
Response via : Initial Calibration

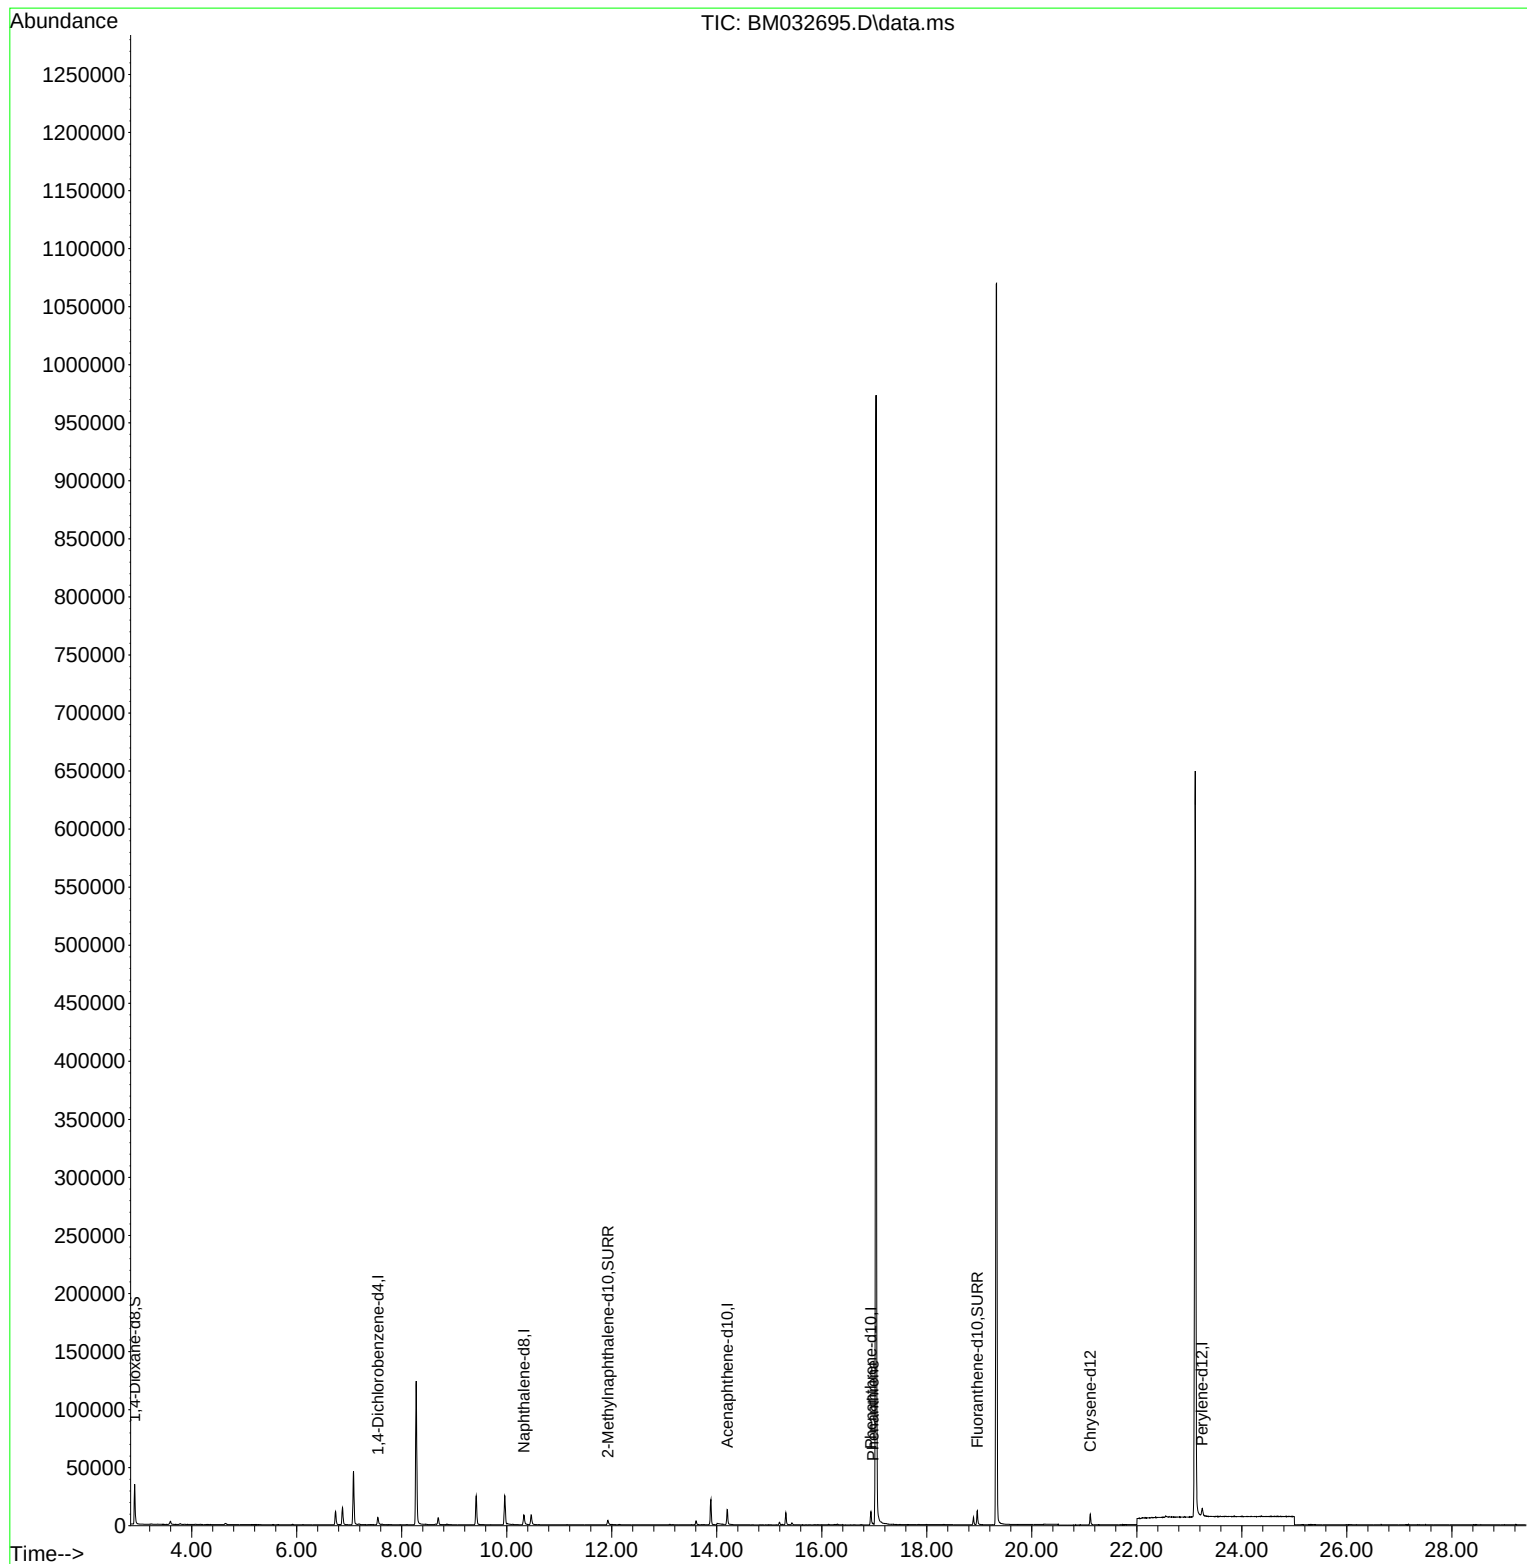

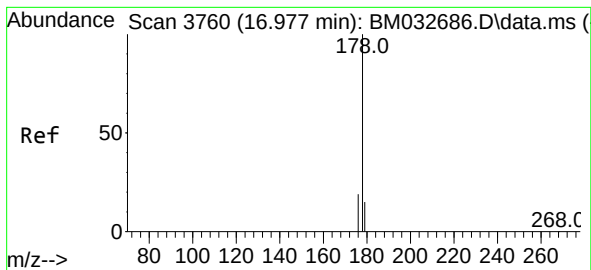

#15
 Phenanthrene
 Concen: 0.029 ng/ul
 RT: 16.974 min Scan# 3759
 Delta R.T. -0.003 min
 Lab File: BM032695.D
 Acq: 25 Oct 2021 15:34

Instrument :
 BNA_M
 ClientSampleId :
 P064-TW001-01

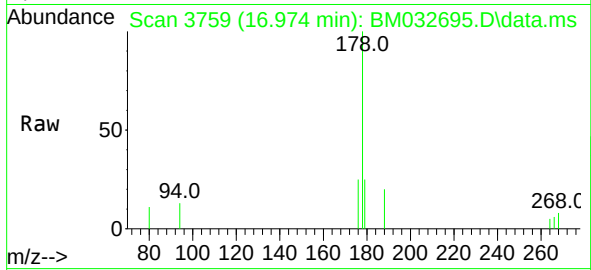

Tgt Ion:178 Resp: 1314
 Ion Ratio Lower Upper
 178 100
 179 25.1 12.9 19.3#
 176 24.9 16.1 24.1#

