

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
 Data File : BM032701.D
 Acq On : 25 Oct 2021 19:12
 Operator : CG/JU
 Sample : M4291-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P022-TW001-02

Quant Time: Oct 26 01:41:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 10:44:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.546	152	4586	0.400	ng/ul	0.00
4) Naphthalene-d8	10.326	136	15465	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.202	164	8245	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.936	188	14645	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.113	240	9420	0.400	ng/ul	0.00
23) Perylene-d12	23.242	264	10043	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.916	96	22876	4.450	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.922	152	6028	0.292	ng/ul	0.00
18) Fluoranthene-d10	18.958	212	11569	0.390	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.974	178	2777	0.056	ng/ul#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
Data File : BM032701.D
Acq On : 25 Oct 2021 19:12
Operator : CG/JU
Sample : M4291-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P022-TW001-02


Quant Time: Oct 26 01:41:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 10:44:54 2021
Response via : Initial Calibration

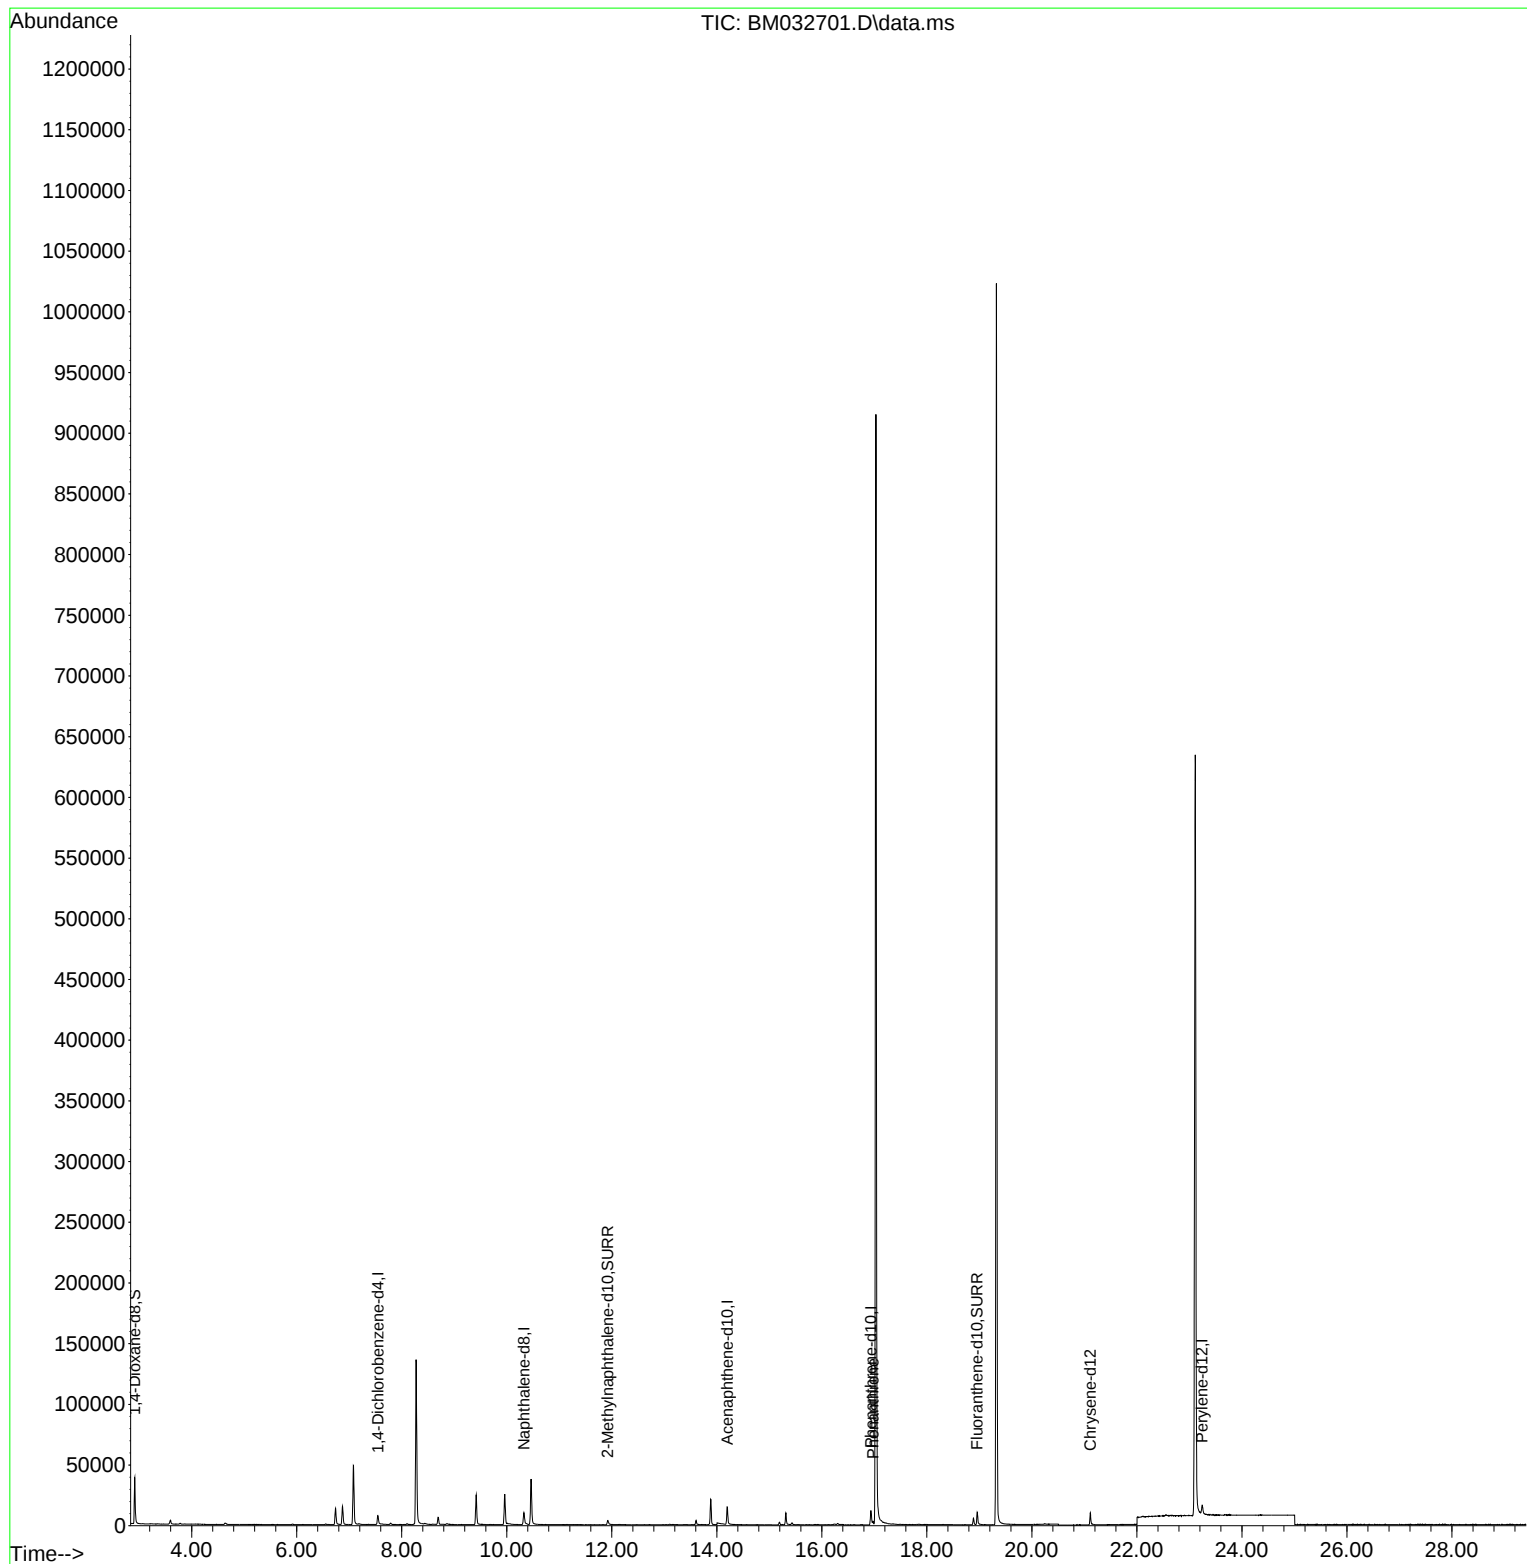

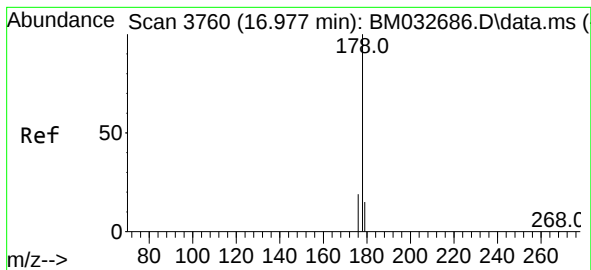

#15
 Phenanthrene
 Concen: 0.056 ng/ul
 RT: 16.974 min Scan# 3759
 Delta R.T. -0.003 min
 Lab File: BM032701.D
 Acq: 25 Oct 2021 19:12

Instrument :
 BNA_M
 ClientSampleId :
 P022-TW001-02

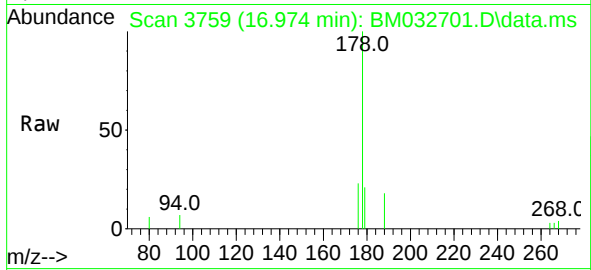

Tgt Ion:178 Resp: 2777
 Ion Ratio Lower Upper
 178 100
 179 21.0 12.9 19.3#
 176 23.0 16.1 24.1

