

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
 Data File : BM032714.D
 Acq On : 26 Oct 2021 03:37
 Operator : CG/JU
 Sample : M4291-17
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P045-TW001-01

Quant Time: Oct 26 04:50:17 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 10:44:54 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.543	152	5349	0.400	ng/ul	0.00
4) Naphthalene-d8	10.321	136	17810	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.194	164	9722	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.932	188	17967	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.106	240	11211	0.400	ng/ul	0.00
23) Perylene-d12	23.235	264	11822	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.913	96	27366	4.565	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.922	152	7459	0.314	ng/ul	0.00
18) Fluoranthene-d10	18.958	212	15514	0.440	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.970	178	2190	0.036	ng/ul#	Qvalue 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
Data File : BM032714.D
Acq On : 26 Oct 2021 03:37
Operator : CG/JU
Sample : M4291-17
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P045-TW001-01


Quant Time: Oct 26 04:50:17 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 10:44:54 2021
Response via : Initial Calibration

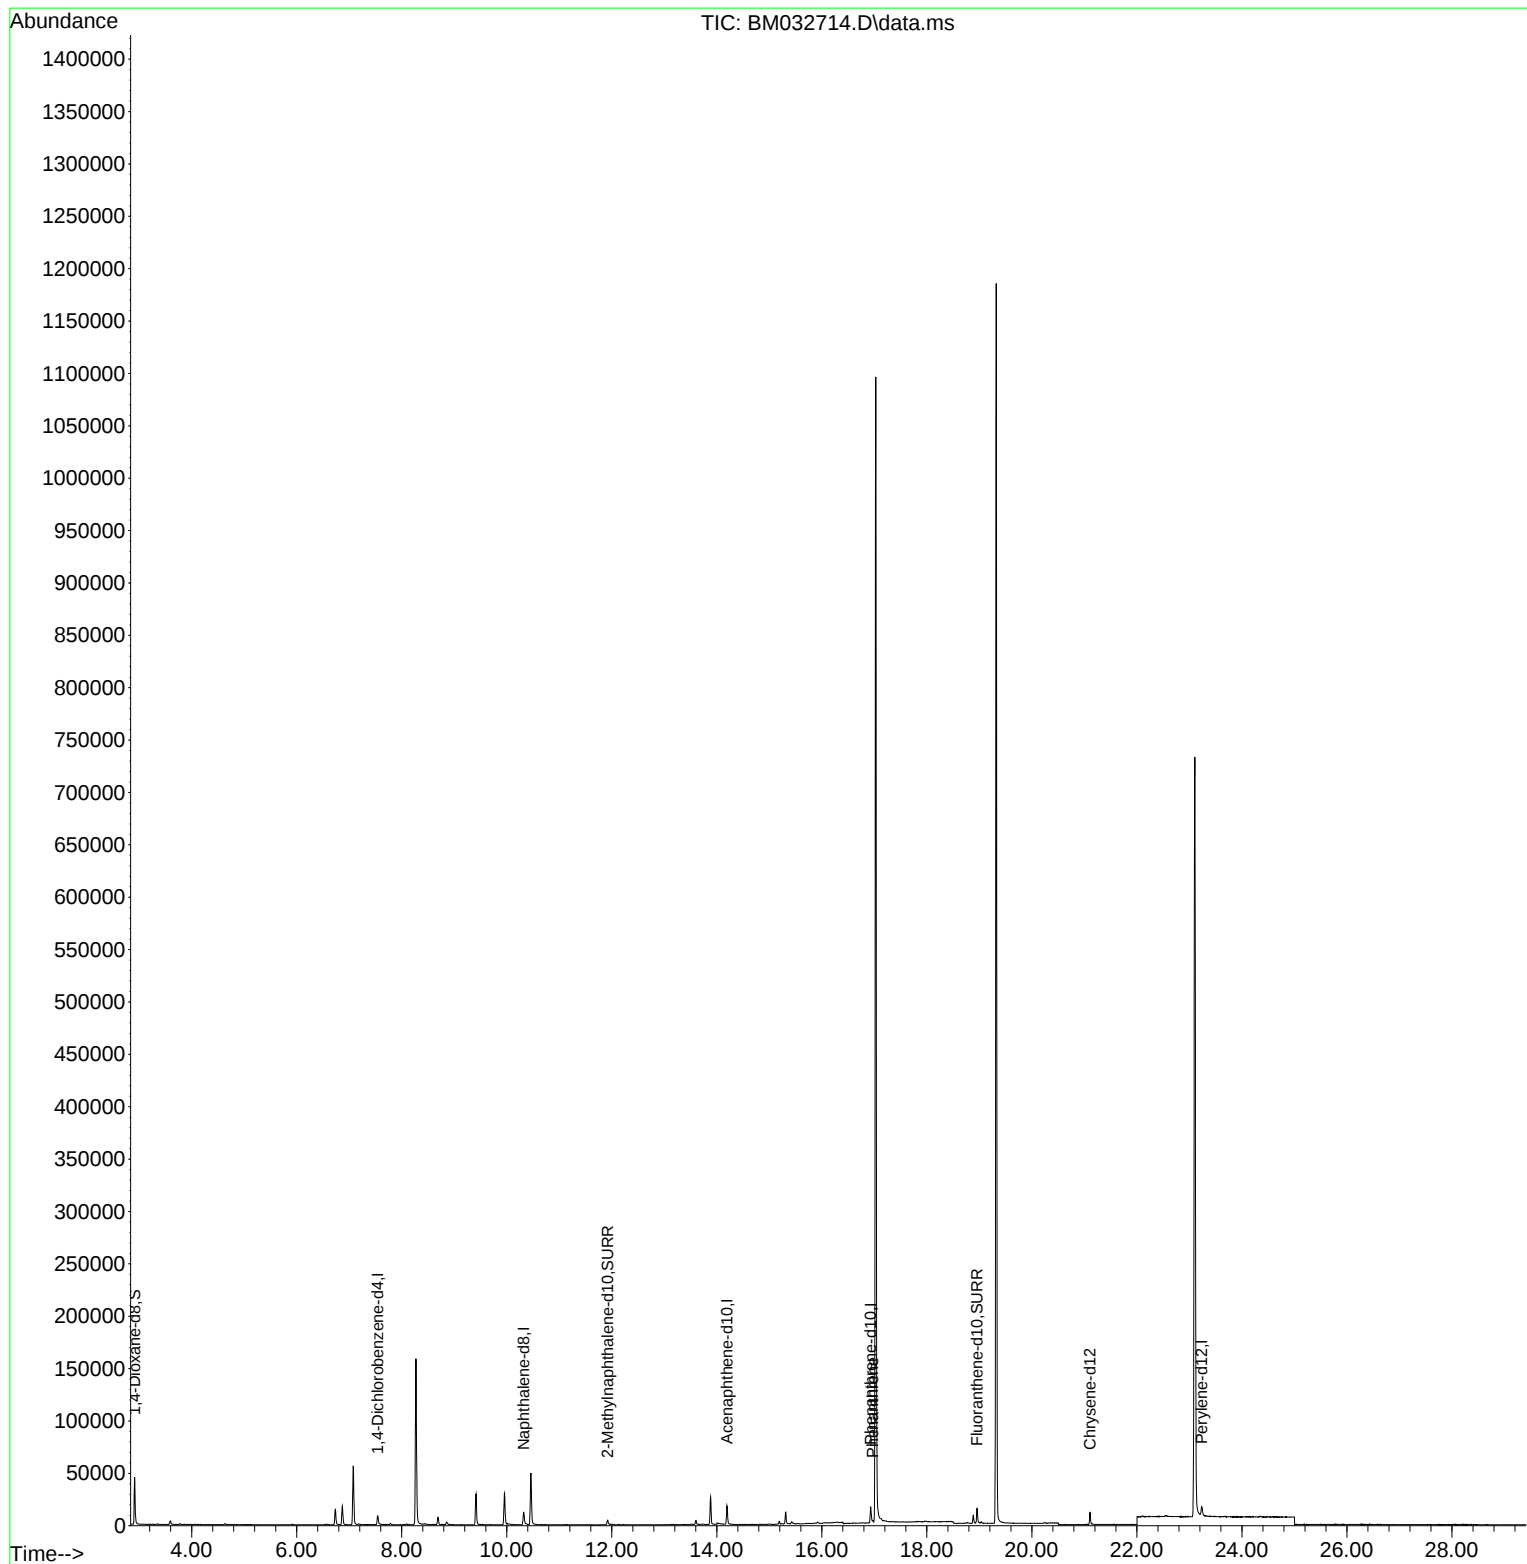

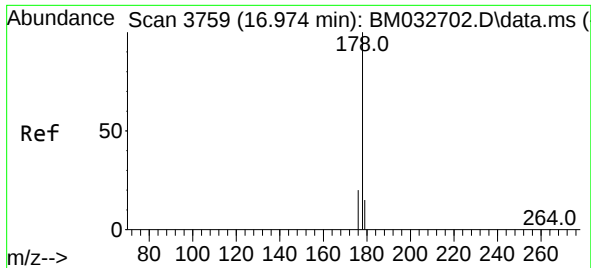

#15
 Phenanthrene
 Concen: 0.036 ng/ul
 RT: 16.970 min Scan# 3758
 Delta R.T. -0.007 min
 Lab File: BM032714.D
 Acq: 26 Oct 2021 03:37

Instrument :
 BNA_M
 ClientSampleId :
 P045-TW001-01

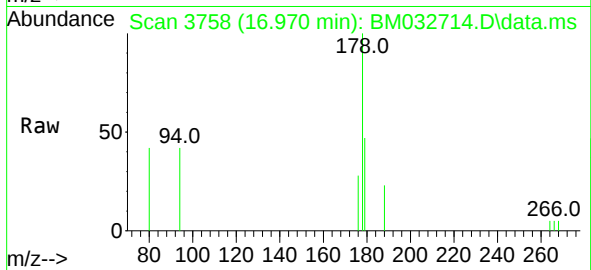

Tgt Ion:178 Resp: 2190
 Ion Ratio Lower Upper
 178 100
 179 47.3 12.9 19.3#
 176 27.5 16.1 24.1#

