

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
 Data File : BM032719.D
 Acq On : 26 Oct 2021 09:52
 Operator : CG/JU
 Sample : M4291-01
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P001-TW001-05

Quant Time: Oct 26 10:40:39 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 26 10:19:48 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.543	152	3615	0.400	ng/ul	0.00
4) Naphthalene-d8	10.321	136	11968	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.194	164	5841	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.929	188	9760	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.111	240	6679	0.400	ng/ul	0.00
23) Perylene-d12	23.240	264	7149	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.913	96	19903	4.912	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.922	152	4026	0.252	ng/ul	0.00
18) Fluoranthene-d10	18.958	212	7469	0.355	ng/ul	0.00
Target Compounds						
						Qvalue
5) Naphthalene	10.371	128	2257	0.062	ng/ul#	89
15) Phenanthrene	16.970	178	1153	0.035	ng/ul#	83


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
Data File : BM032719.D
Acq On : 26 Oct 2021 09:52
Operator : CG/JU
Sample : M4291-01
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P001-TW001-05

Quant Time: Oct 26 10:40:39 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 26 10:19:48 2021
Response via : Initial Calibration




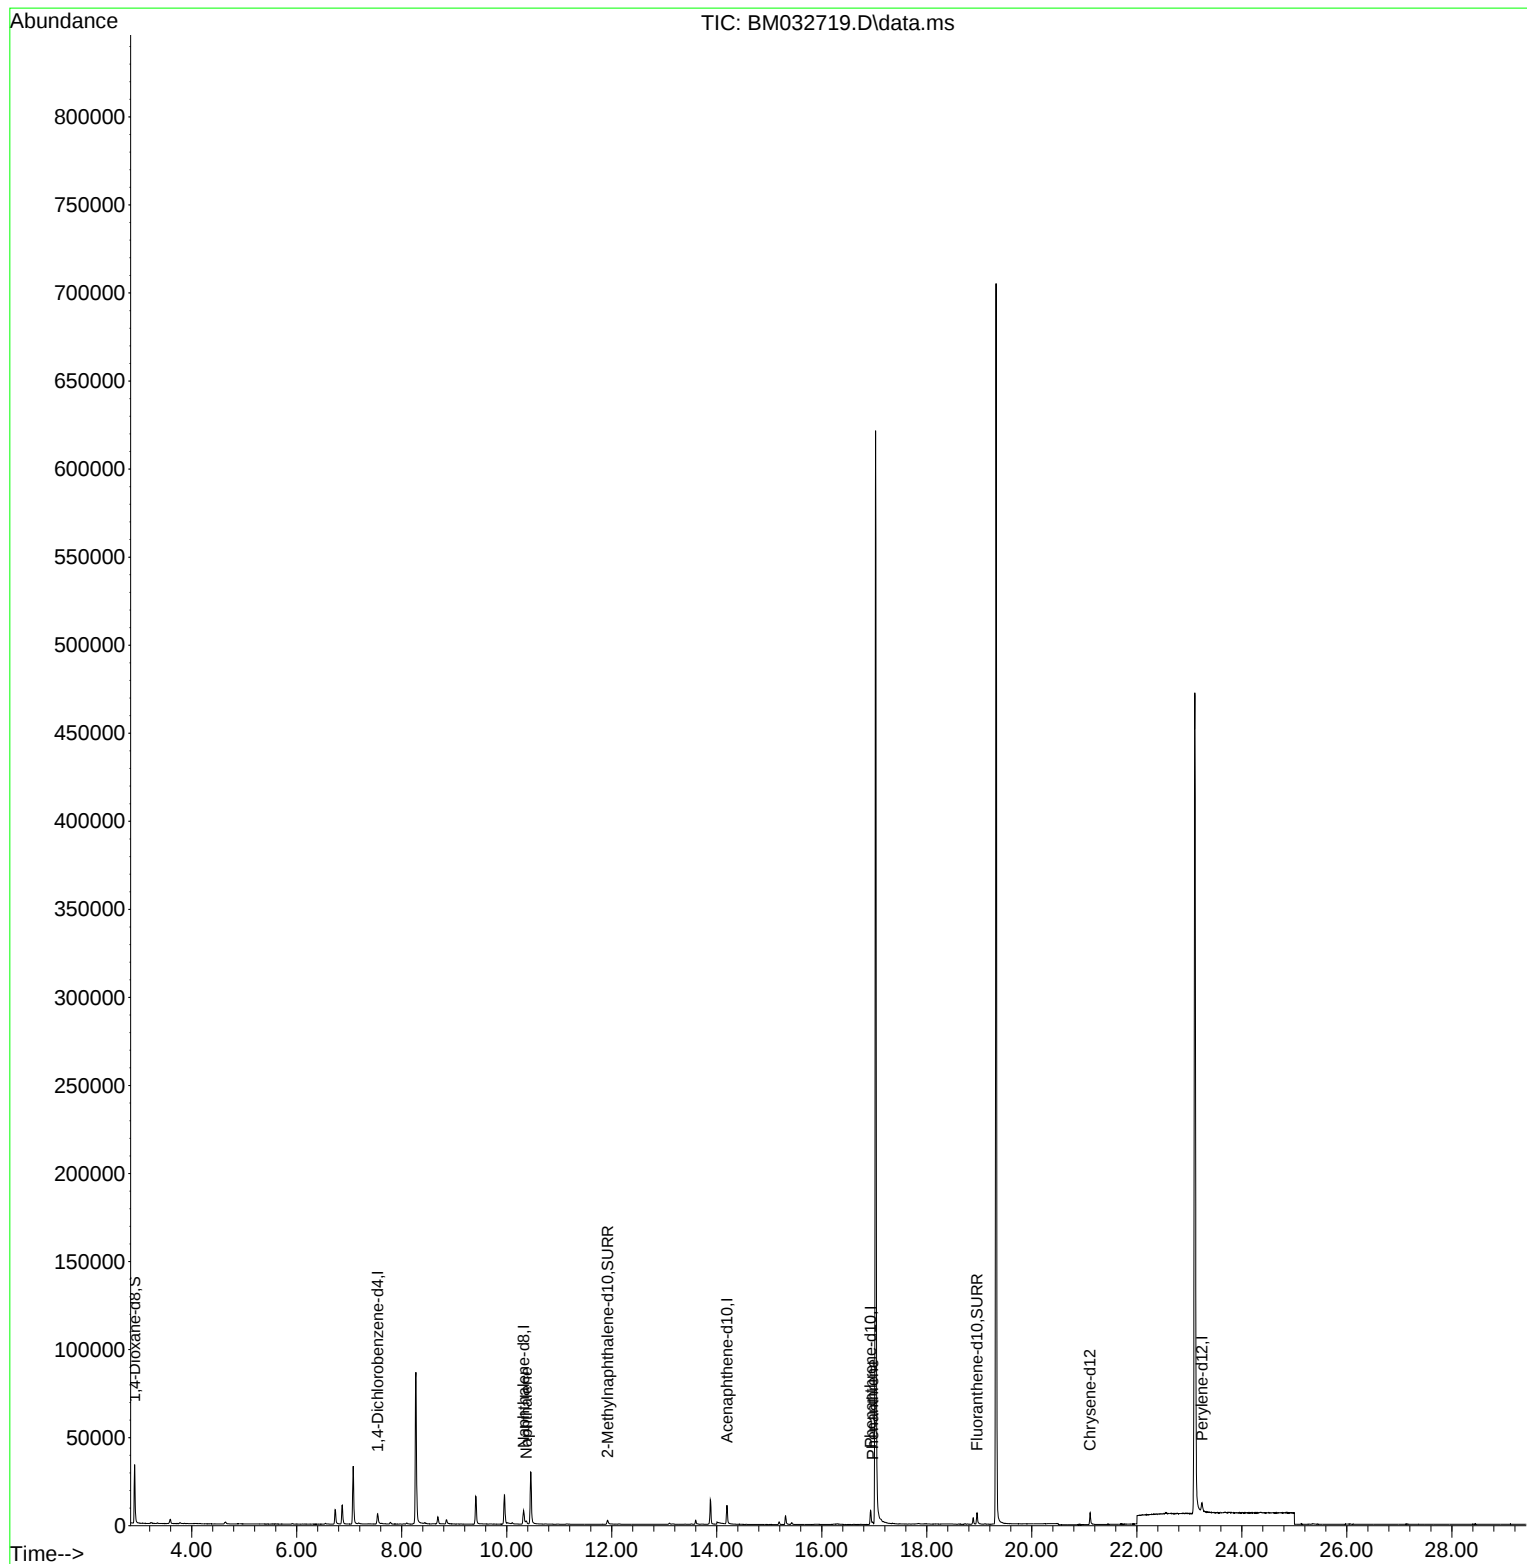


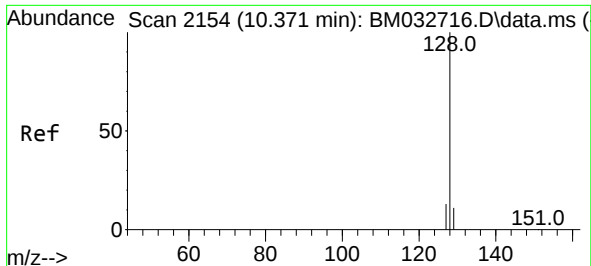

#5
Naphthalene
Concen: 0.062 ng/u1
RT: 10.371 min Scan# 2154
Delta R.T. 0.000 min
Lab File: BM032719.D
Acq: 26 Oct 2021 09:52

Instrument :
BNA_M
ClientSampleId :
P001-TW001-05

Tgt Ion:128 Resp: 2257
Ion Ratio Lower Upper
128 100
129 17.0 9.1 13.7#
127 17.0 11.1 16.7#

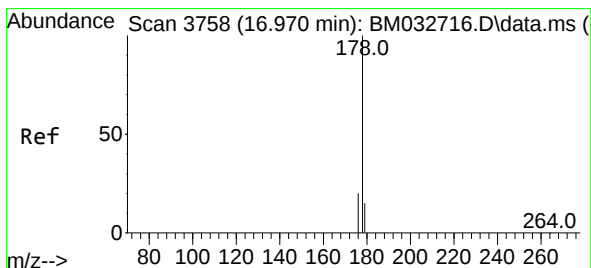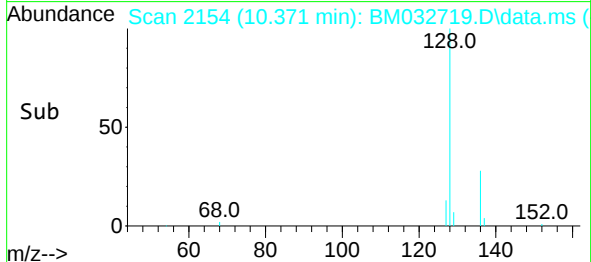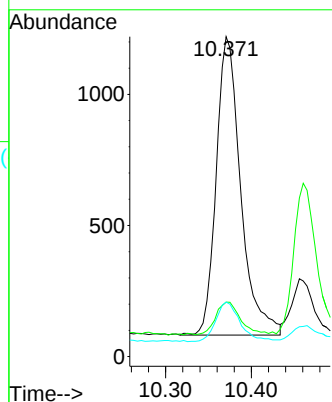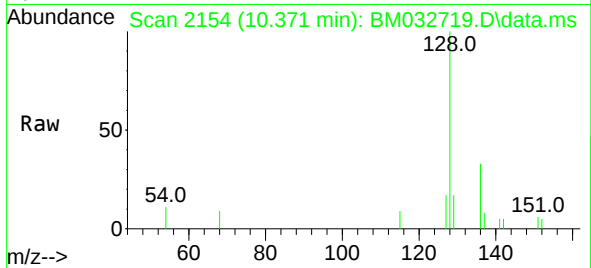

#15
Phenanthrene
Concen: 0.035 ng/u1
RT: 16.970 min Scan# 3758
Delta R.T. 0.000 min
Lab File: BM032719.D
Acq: 26 Oct 2021 09:52

Tgt Ion:178 Resp: 1153
Ion Ratio Lower Upper
178 100
179 25.6 12.9 19.3#
176 25.8 16.1 24.1#

