

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
 Data File : BM032737.D
 Acq On : 26 Oct 2021 20:48
 Operator : CG/JU
 Sample : M4303-06
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P012-TW001-02

Quant Time: Oct 27 03:03:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Oct 26 17:09:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.539	152	4514	0.400	ng/ul	0.00
4) Naphthalene-d8	10.321	136	15794	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.194	164	8648	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.929	188	15084	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.106	240	9110	0.400	ng/ul	0.00
23) Perylene-d12	23.232	264	9071	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.913	96	23035	4.553	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.918	152	6100	0.290	ng/ul	0.00
18) Fluoranthene-d10	18.954	212	12345	0.430	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.967	178	2596	0.051	ng/ul#	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102521\
Data File : BM032737.D
Acq On : 26 Oct 2021 20:48
Operator : CG/JU
Sample : M4303-06
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P012-TW001-02


Quant Time: Oct 27 03:03:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Oct 26 17:09:29 2021
Response via : Initial Calibration

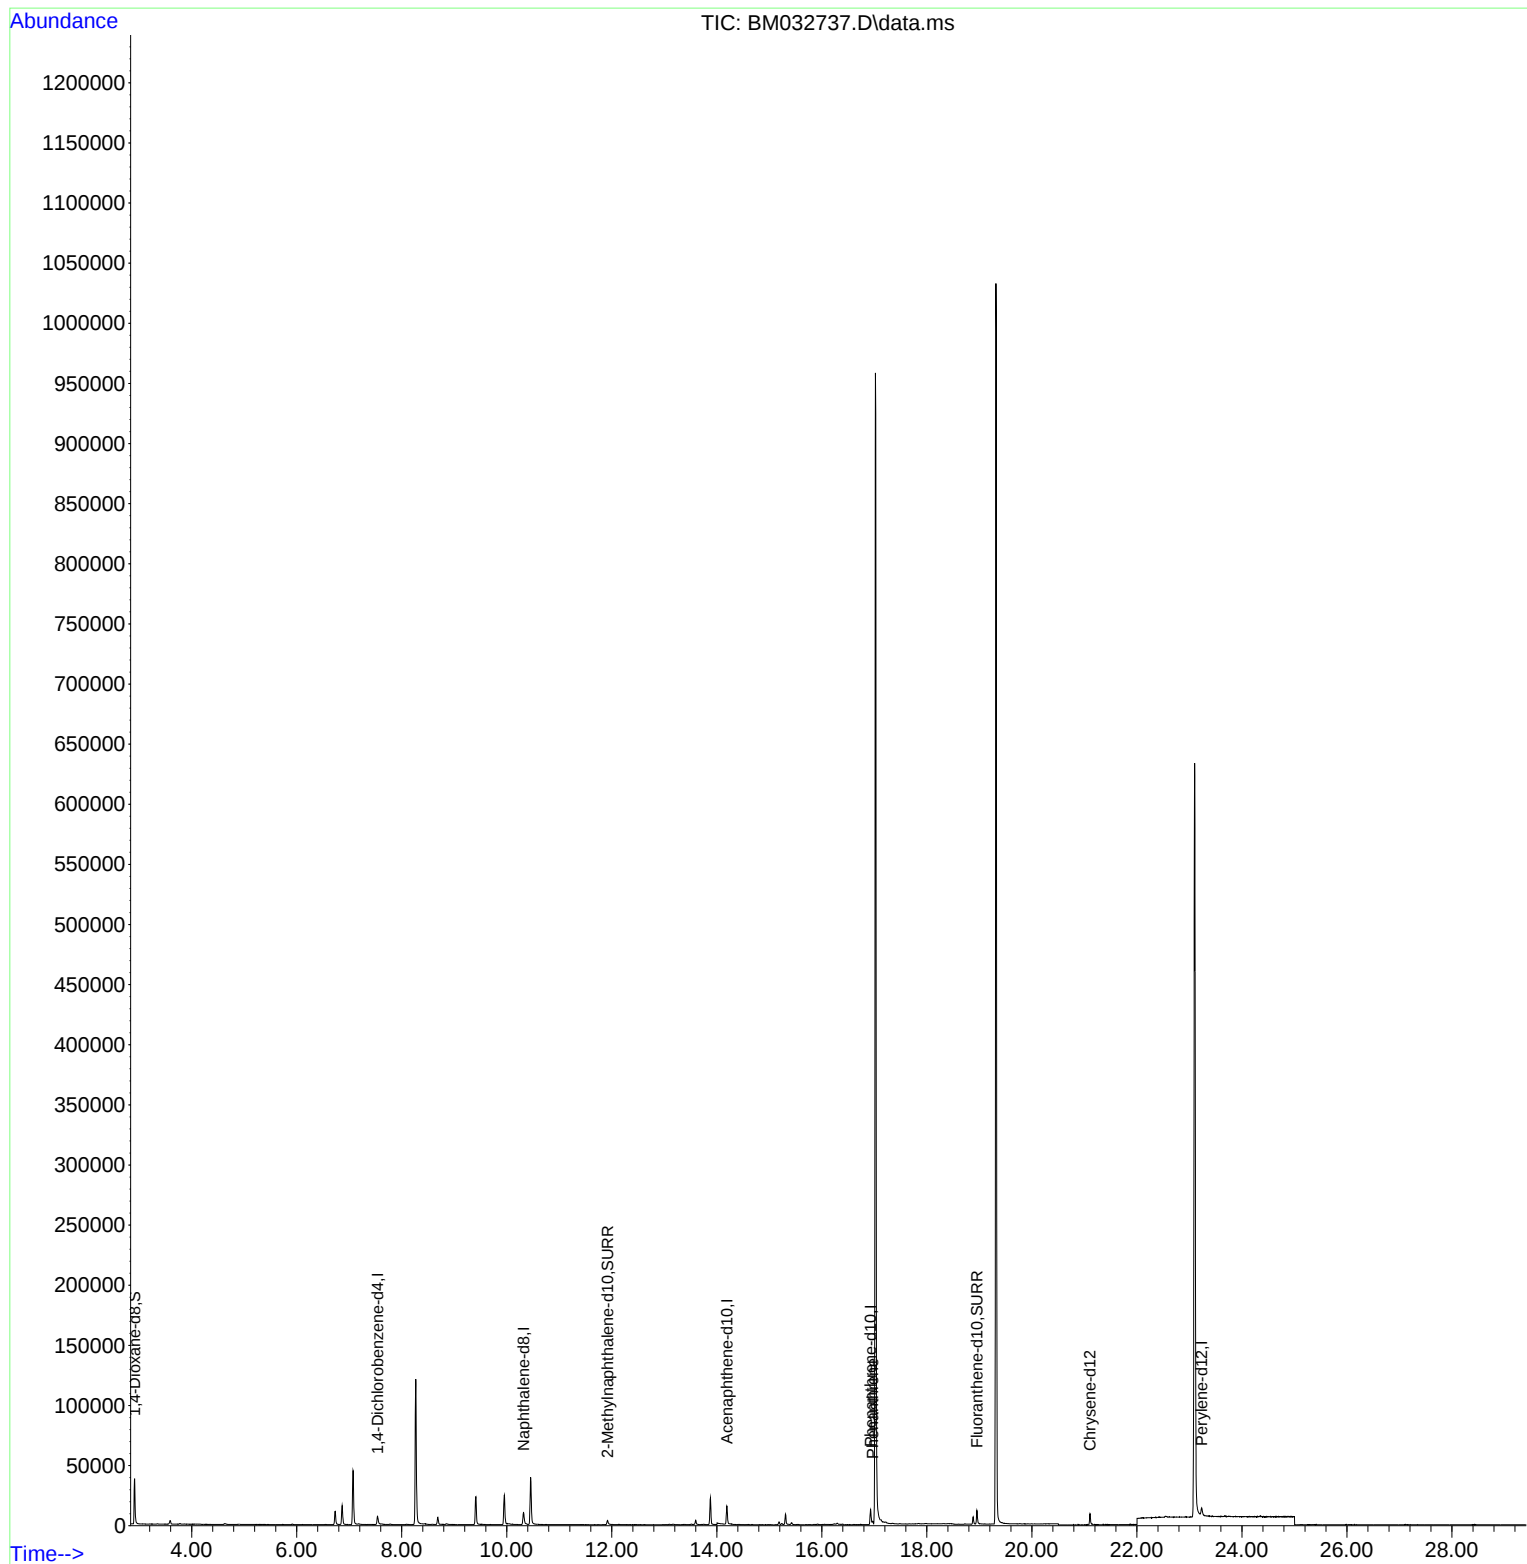

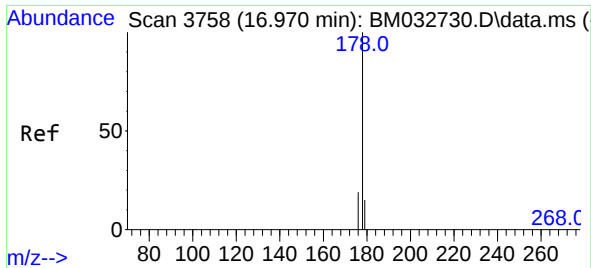

#15
 Phenanthrene
 Concen: 0.051 ng/ul
 RT: 16.967 min Scan# 3757
 Delta R.T. -0.003 min
 Lab File: BM032737.D
 Acq: 26 Oct 2021 20:48

Instrument :
 BNA_M
 ClientSampleId :
 P012-TW001-02

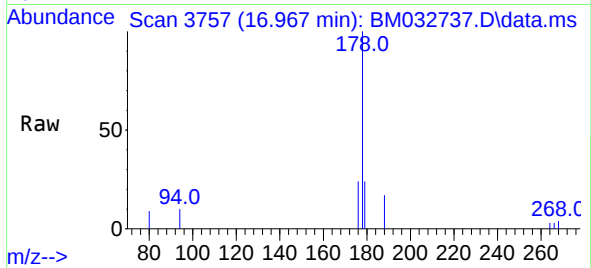

Tgt Ion:	178	Resp:	2596
Ion	Ratio	Lower	Upper
178	100		
179	24.0	12.9	19.3#
176	23.9	16.1	24.1

