

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102522\
 Data File : BM037221.D
 Acq On : 25 Oct 2022 10:41
 Operator : CG/JU
 Sample : PB148455BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 26 07:31:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 22 03:34:37 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.896	152	5011	0.400	ng/ul	0.00
4) Naphthalene-d8	10.699	136	15463	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.530	164	8530	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.268	188	14998	0.400	ng/ul	0.00
17) Chrysene-d12	21.449	240	10140	0.400	ng/ul	0.00
23) Perylene-d12	23.820	264	11423	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.310	96	32702	5.352	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.288	152	6687	0.304	ng/ul	0.00
18) Fluoranthene-d10	19.295	212	10929	0.356	ng/ul	0.00
Target Compounds						
					Qvalue	
12) Fluorene	15.520	166	2340	0.060	ng/ul#	14
20) Pyrene	19.657	202	2023	0.045	ng/ul#	1
26) Benzo(a)pyrene	23.665	252	4283	0.088	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102522\
Data File : BM037221.D
Acq On : 25 Oct 2022 10:41
Operator : CG/JU
Sample : PB148455BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :


Quant Time: Oct 26 07:31:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM101922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 22 03:34:37 2022
Response via : Initial Calibration

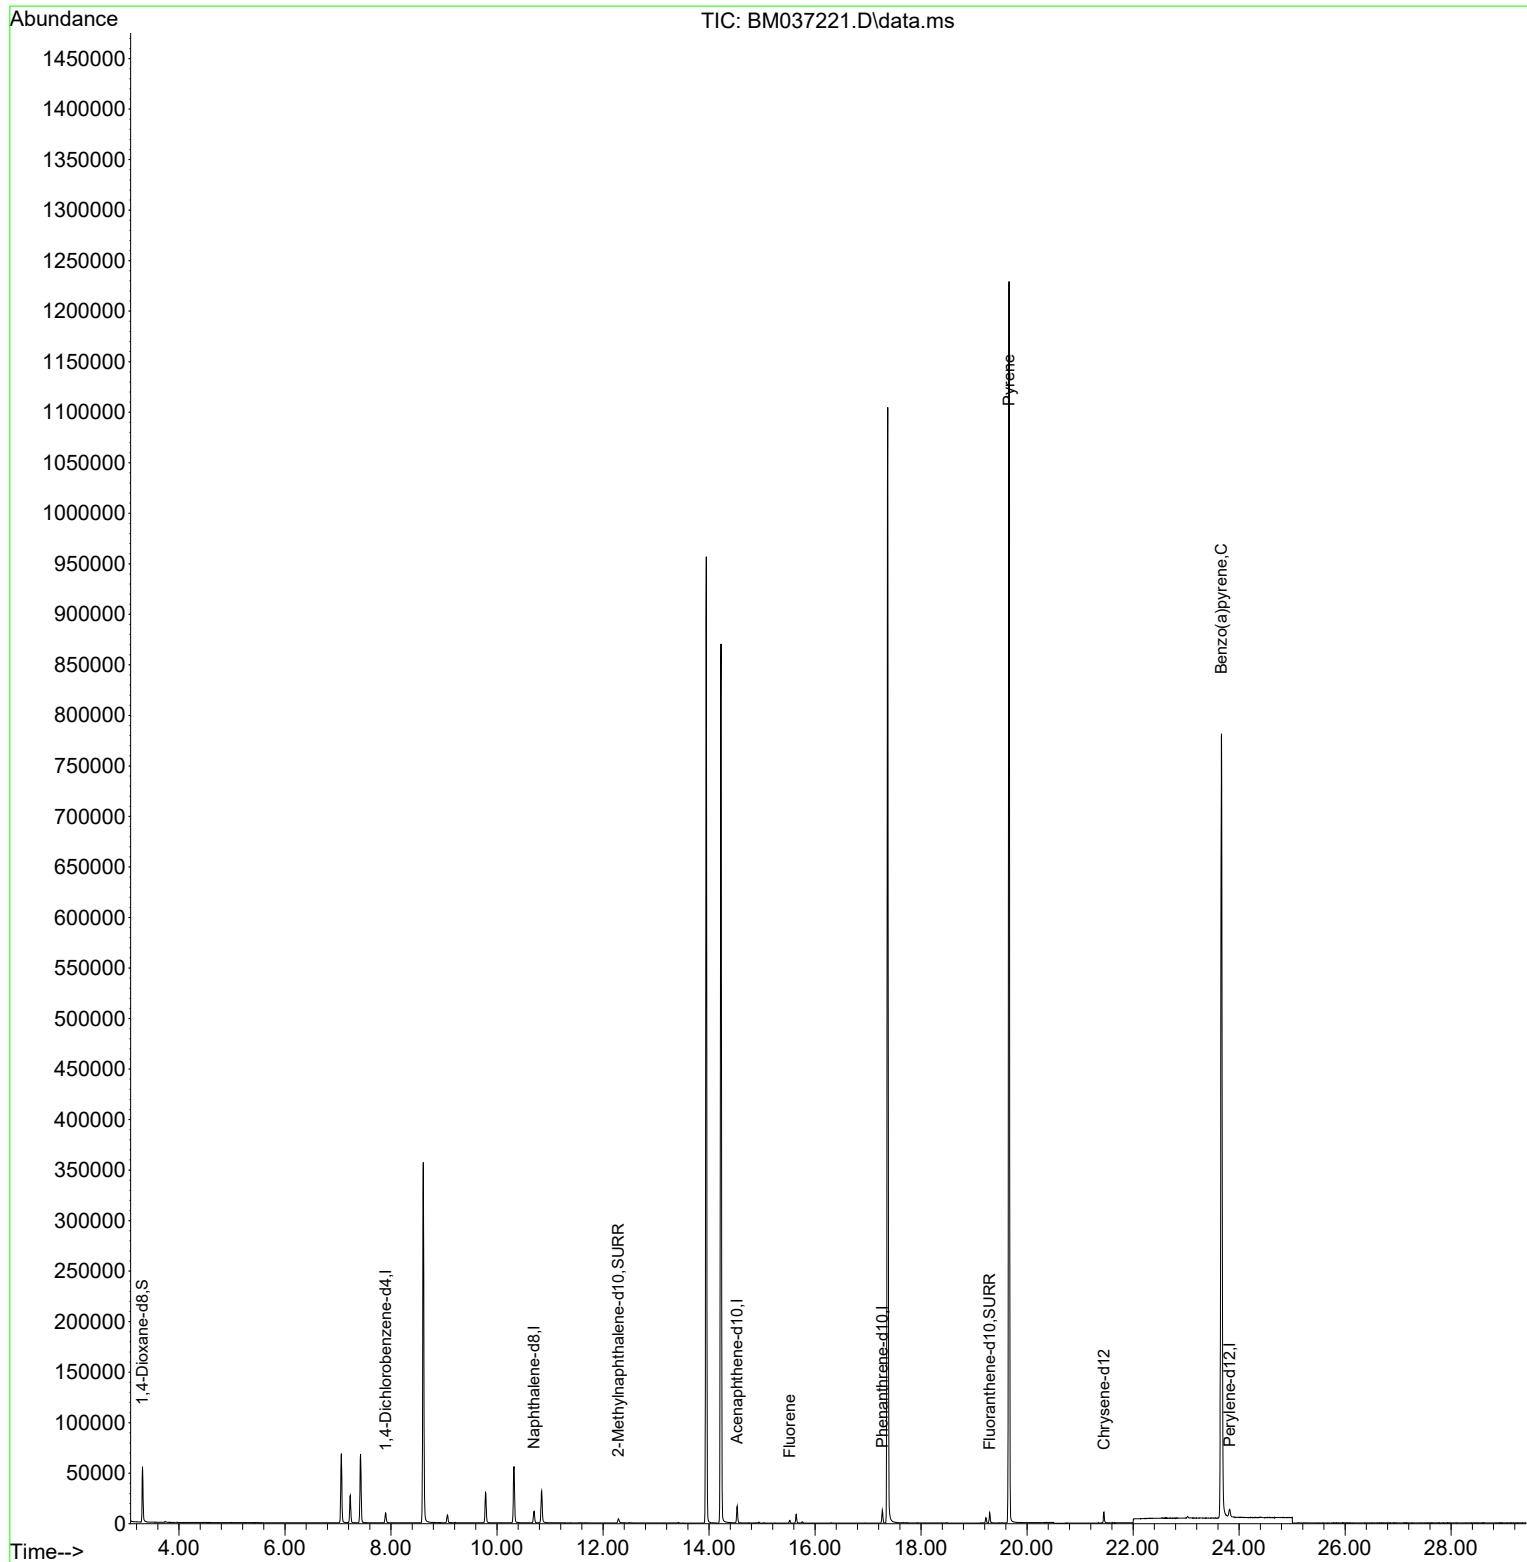



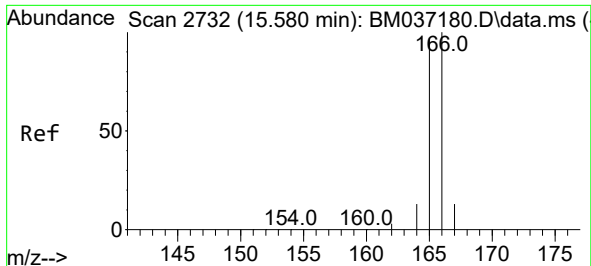


#12
Fluorene
Concen: 0.060 ng/ul
RT: 15.520 min Scan# 21
Delta R.T. -0.060 min
Lab File: BM037221.D
Acq: 25 Oct 2022 10:41

Instrument :
BNA_M
ClientSampleId :



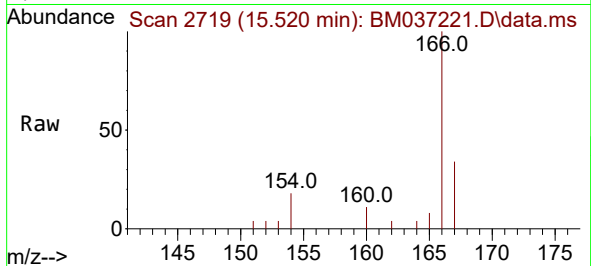



Tgt Ion:166 Resp: 2340
Ion Ratio Lower Upper
166 100
165 8.3 79.4 119.2#
167 33.5 11.3 16.9#

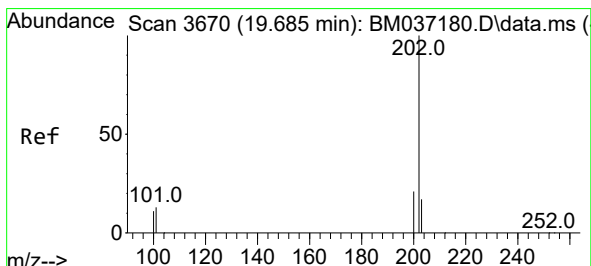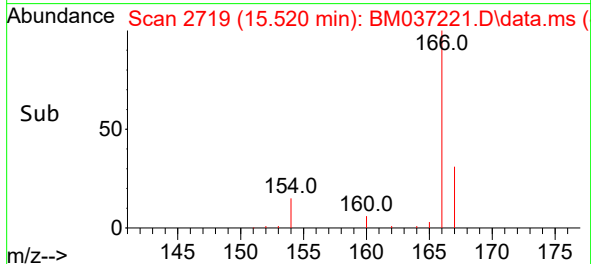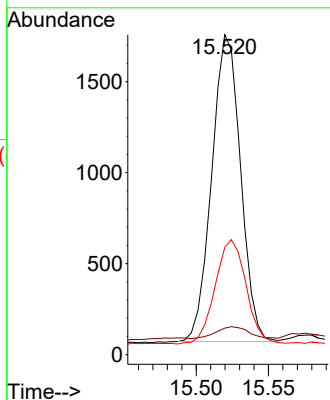

#20
Pyrene
Concen: 0.045 ng/ul
RT: 19.657 min Scan# 3664
Delta R.T. -0.028 min
Lab File: BM037221.D
Acq: 25 Oct 2022 10:41


Tgt Ion:202 Resp: 2023
Ion Ratio Lower Upper
202 100
101 145.8 9.7 14.5#
100 1066.0 7.8 11.8#

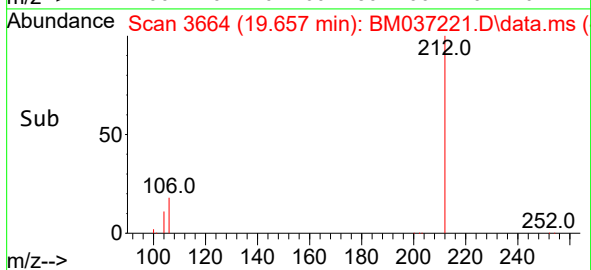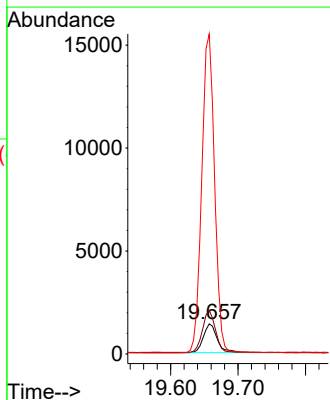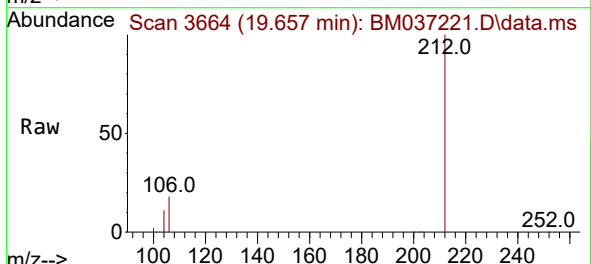

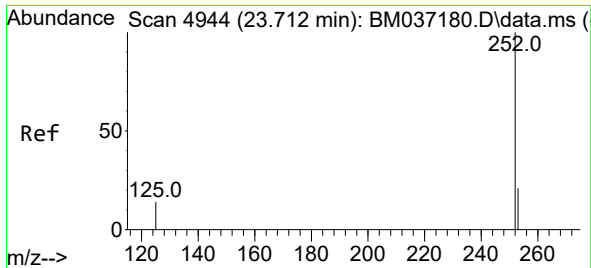

#26
Benzo(a)pyrene
Concen: 0.088 ng/ul
RT: 23.665 min Scan# 4944
Delta R.T. -0.047 min
Lab File: BM037221.D
Acq: 25 Oct 2022 10:41

Instrument :
BNA_M
ClientSampleId :

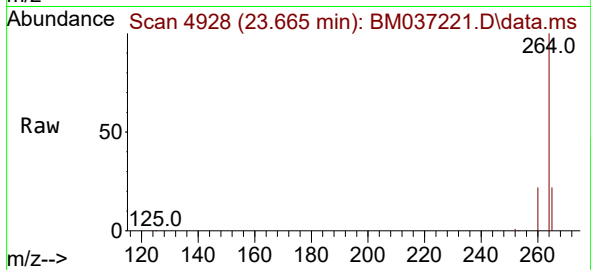

Tgt Ion:252 Resp: 4283
Ion Ratio Lower Upper
252 100
253 48.0 22.1 33.1#
125 44.5 17.6 26.4#

