
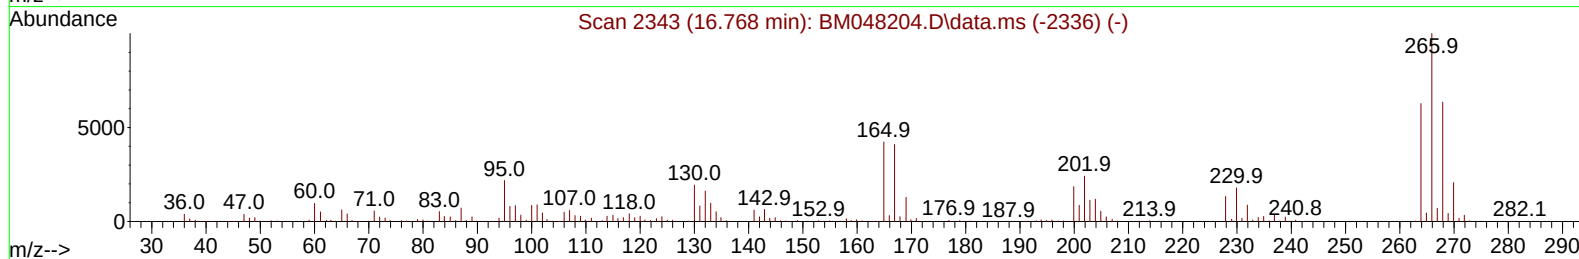
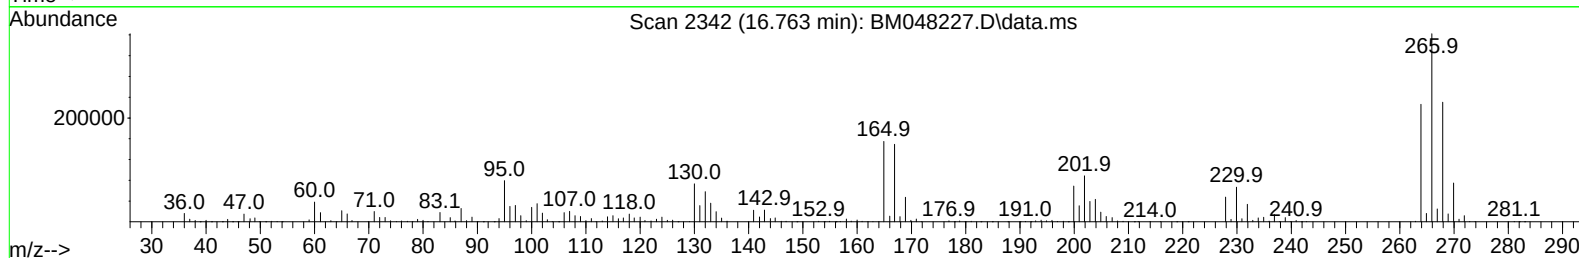


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048227.D
Acq On : 25 Oct 2024 08:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 13:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

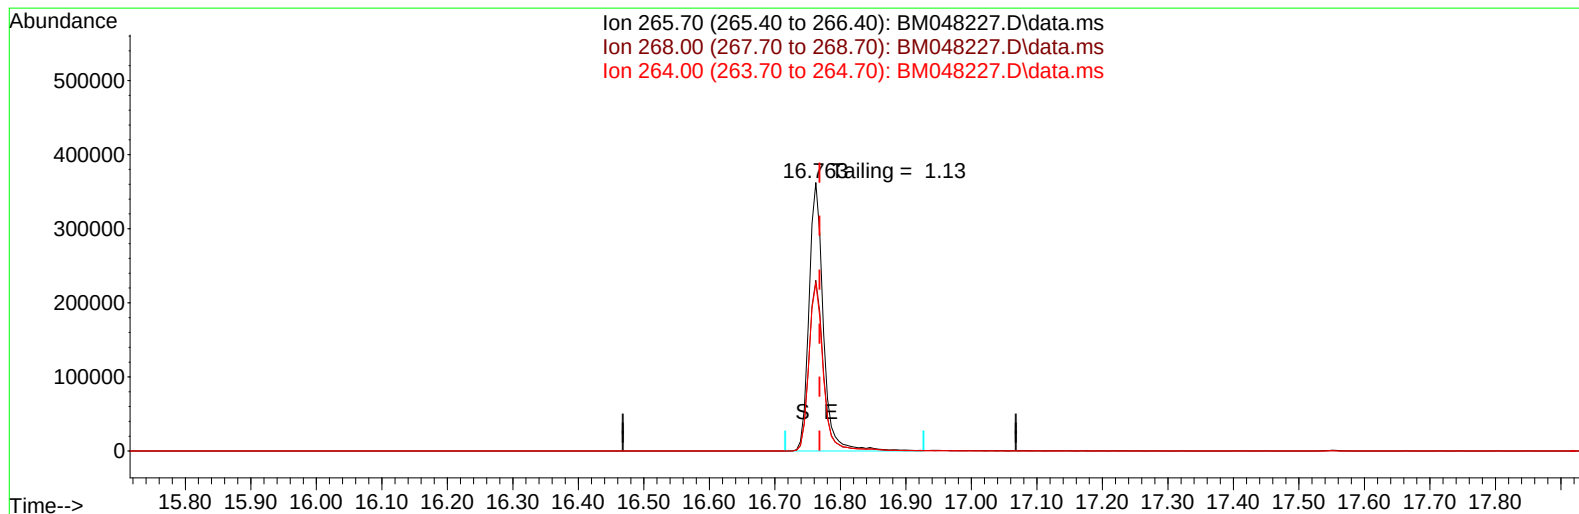

TIC: BM048227.D\data.ms

(70) Pentachlorophenol (C)




16.763min (-0.006) 395736.19 ng

response 550504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.50	63.55
264.00	62.70	62.51
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048227.D
Acq On : 25 Oct 2024 08:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 13:12:55 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 23 18:21:59 2024
Response via : Initial Calibration

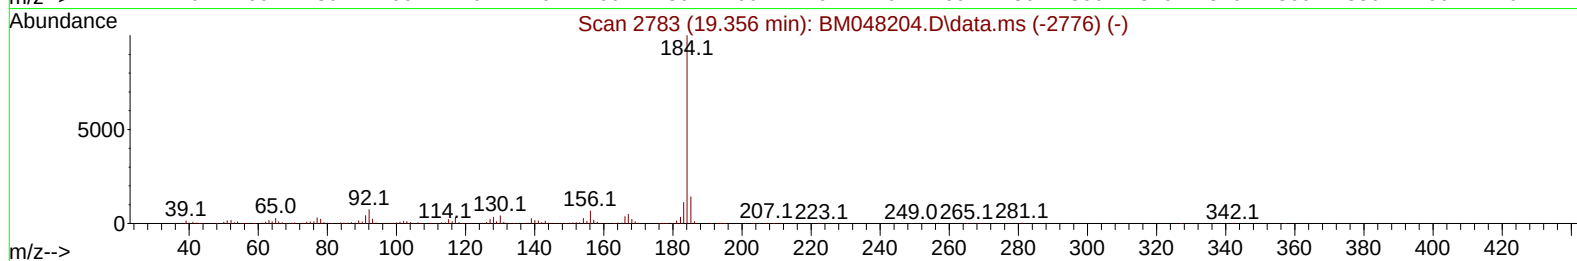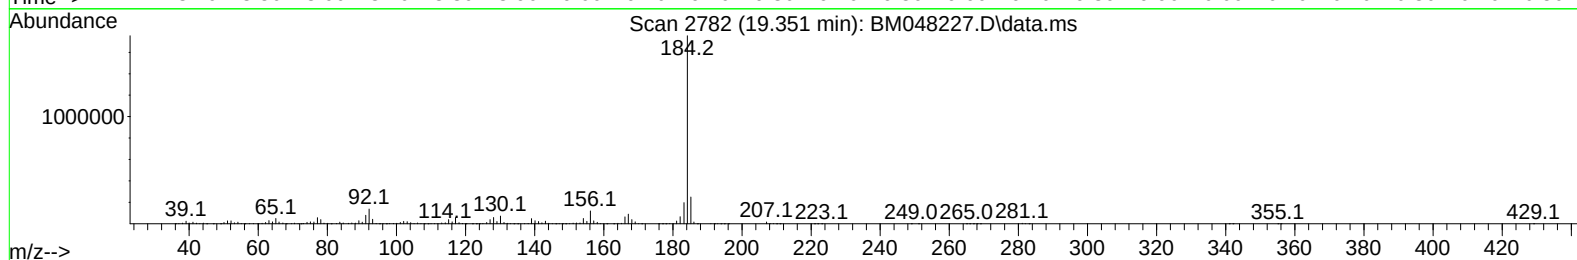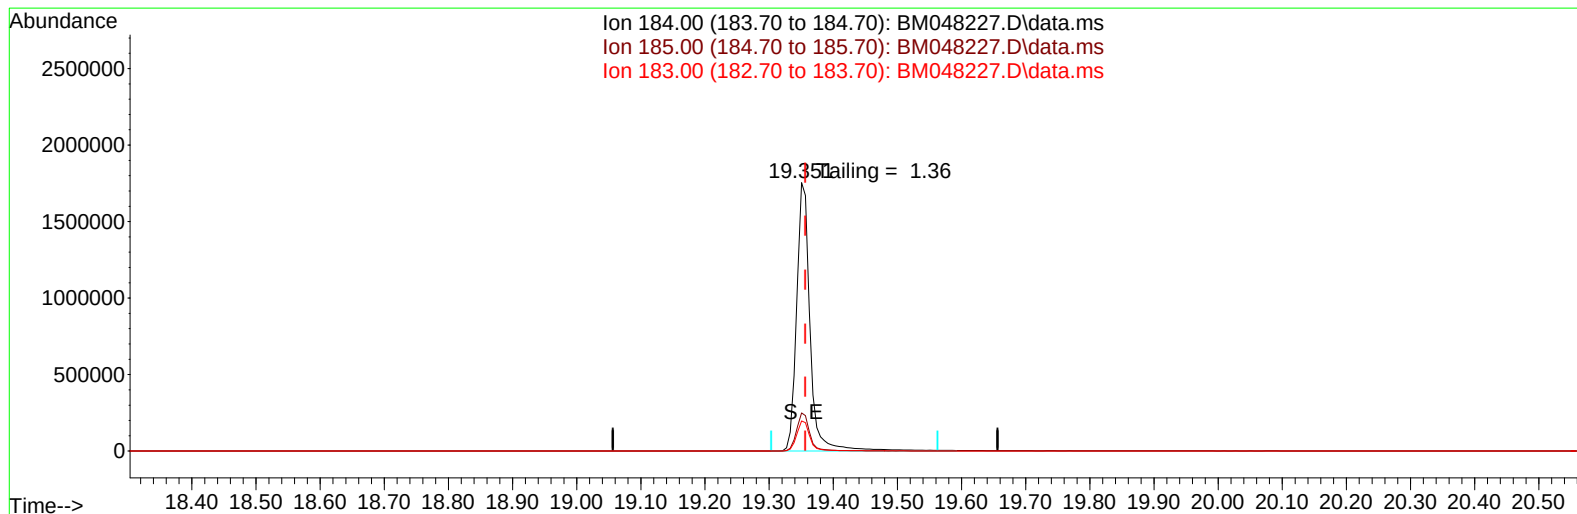

TIC: BM048227.D\data.ms

(77) Benzidine**19.351min (-0.006) 261475.58 ng****response 2555981**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.22
183.00	11.20	11.24
0.00	0.00	0.00