

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048229.D
Acq On : 25 Oct 2024 09:28
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164382BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM048229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.304	387	394	411	rBV	4372094	6427894	66.84%	12.498%
2	6.898	658	665	681	rBV	3875963	6312585	65.64%	12.274%
3	7.716	797	804	812	rBV	792029	1253677	13.04%	2.438%
4	8.875	993	1001	1014	rBV	2319650	3924664	40.81%	7.631%
5	10.510	1271	1279	1299	rBV	852581	1625545	16.90%	3.161%
6	12.980	1692	1699	1721	rBV	5445198	8498894	88.37%	16.525%
7	14.363	1927	1934	1950	rBV	1268544	1994061	20.73%	3.877%
8	15.851	2180	2187	2212	rBV	3837029	5846444	60.79%	11.368%
9	17.104	2394	2400	2421	rBV	1250987	2093406	21.77%	4.070%
10	19.733	2840	2847	2860	rBV	7253261	9617319	100.00%	18.699%
11	21.333	3113	3119	3133	rBV2	1134563	2006231	20.86%	3.901%
12	24.280	3613	3620	3634	rVB	690312	1830326	19.03%	3.559%




Sum of corrected areas: 51431046

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048229.D
Acq On : 25 Oct 2024 09:28
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

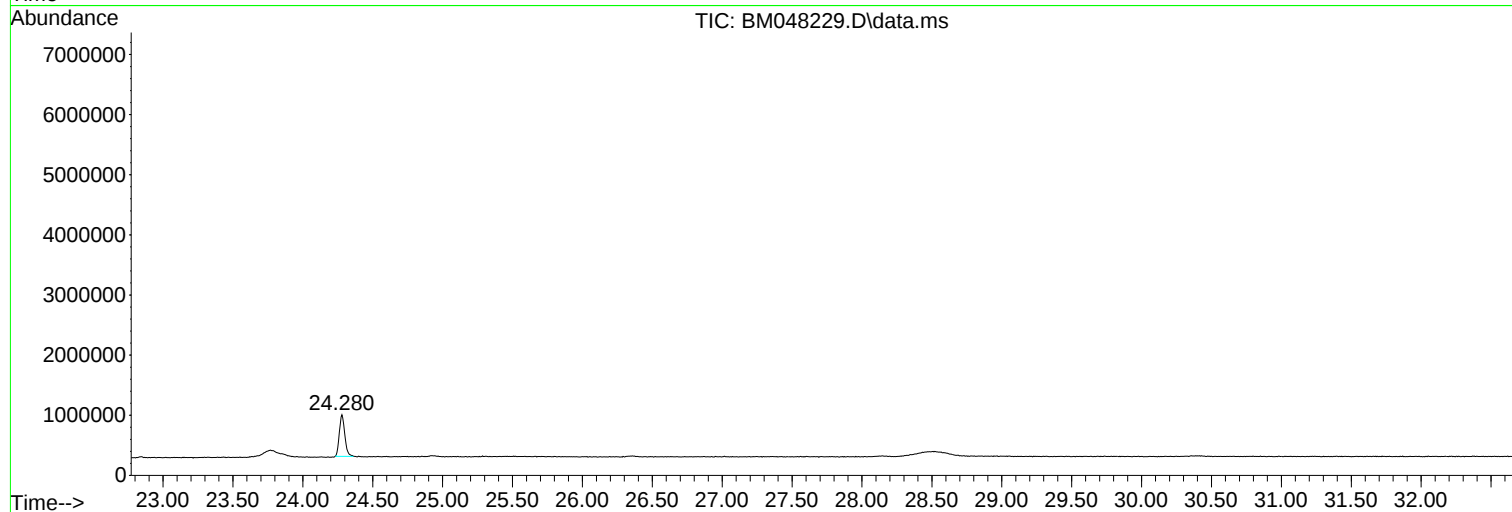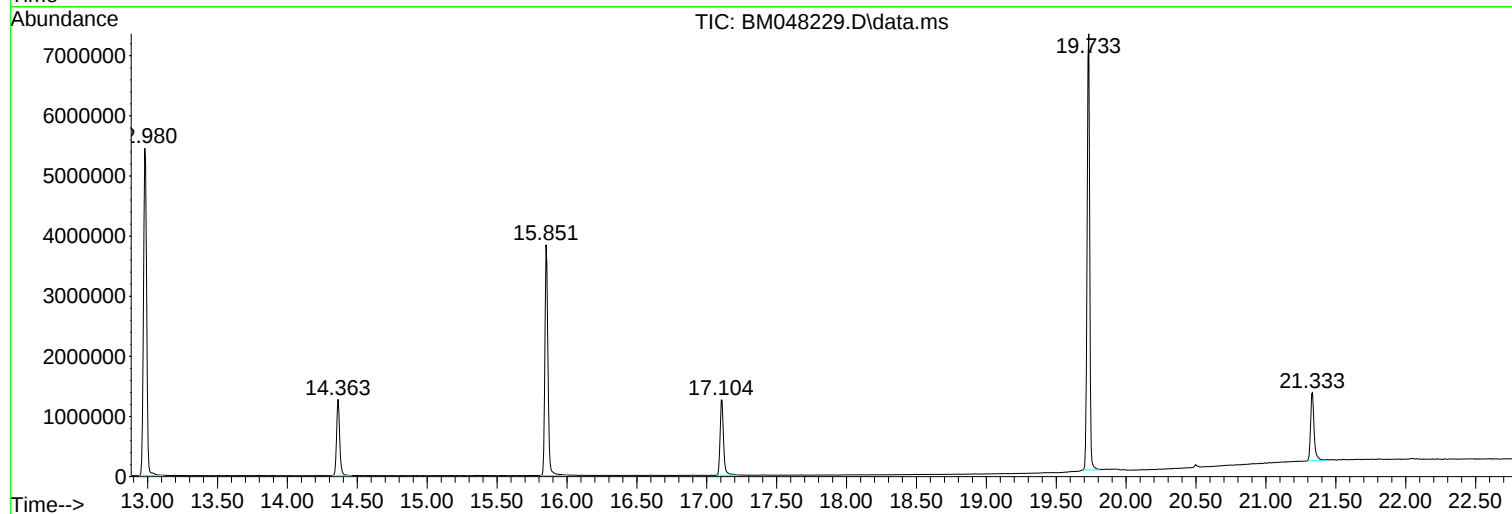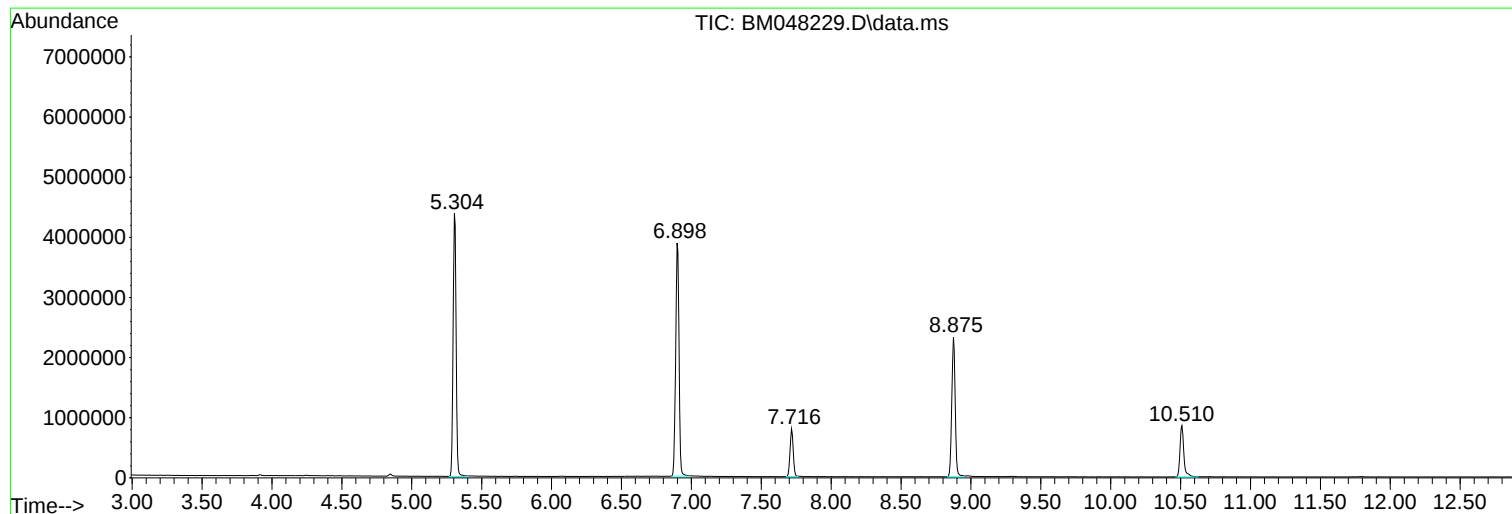

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048229.D
Acq On : 25 Oct 2024 09:28
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048229.D
Acq On : 25 Oct 2024 09:28
Operator : RC/JU
Sample : PB164382BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164382BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------