

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
 Data File : BM048234.D
 Acq On : 25 Oct 2024 13:38
 Operator : RC/JU
 Sample : PB164401BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB164401BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM048234.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	152	157	164	rBV	176153	228053	2.38%	0.429%
2	4.840	310	315	324	rBV	259510	363030	3.78%	0.683%
3	5.304	387	394	408	rBV	4435762	6450801	67.20%	12.134%
4	6.898	653	665	682	rBV	3936823	6549528	68.23%	12.319%
5	7.716	796	804	812	rBV	821829	1305575	13.60%	2.456%
6	8.875	991	1001	1016	rBV	2371315	4029155	41.97%	7.579%
7	9.298	1068	1073	1080	rVB	77249	120392	1.25%	0.226%
8	10.510	1268	1279	1297	rBV	889758	1706934	17.78%	3.211%
9	12.980	1692	1699	1715	rBV	5700079	8612006	89.71%	16.199%
10	14.363	1927	1934	1946	rBV	1349969	2095627	21.83%	3.942%
11	15.851	2180	2187	2207	rBV	3769323	5812961	60.55%	10.934%
12	17.104	2393	2400	2420	rBV	1390921	2242436	23.36%	4.218%
13	19.733	2841	2847	2859	rBV	7228046	9599520	100.00%	18.056%
14	21.333	3113	3119	3130	rBV	1214112	2048786	21.34%	3.854%
15	24.280	3613	3620	3634	rVB	758205	1999543	20.83%	3.761%




Sum of corrected areas: 53164347

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048234.D
Acq On : 25 Oct 2024 13:38
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

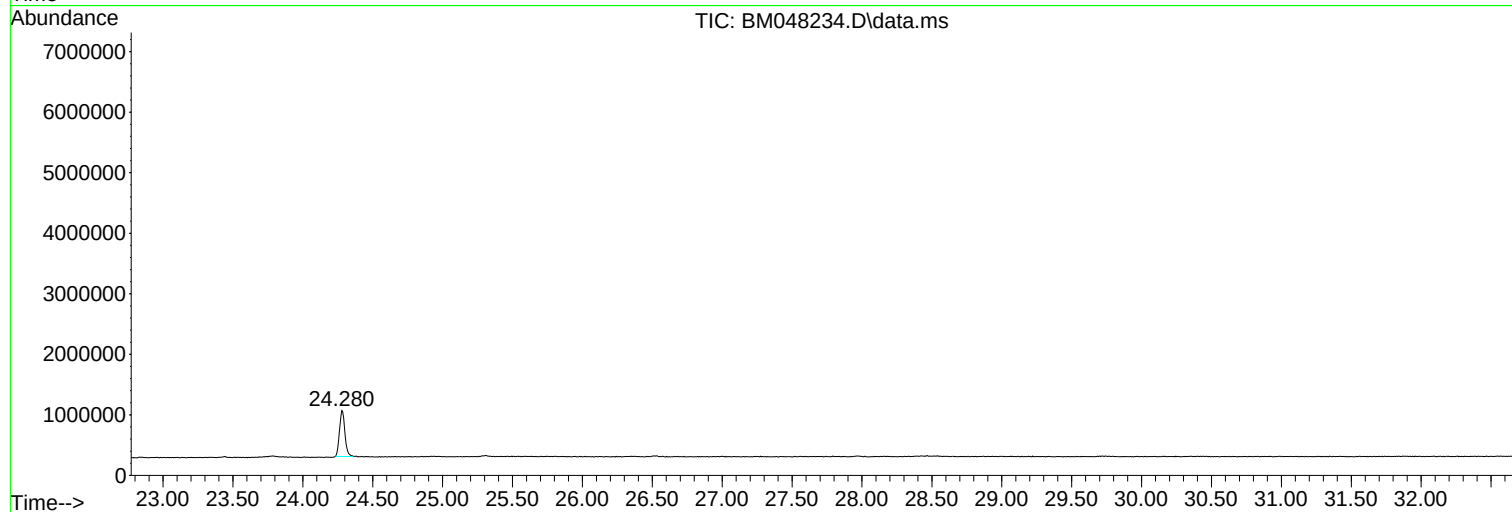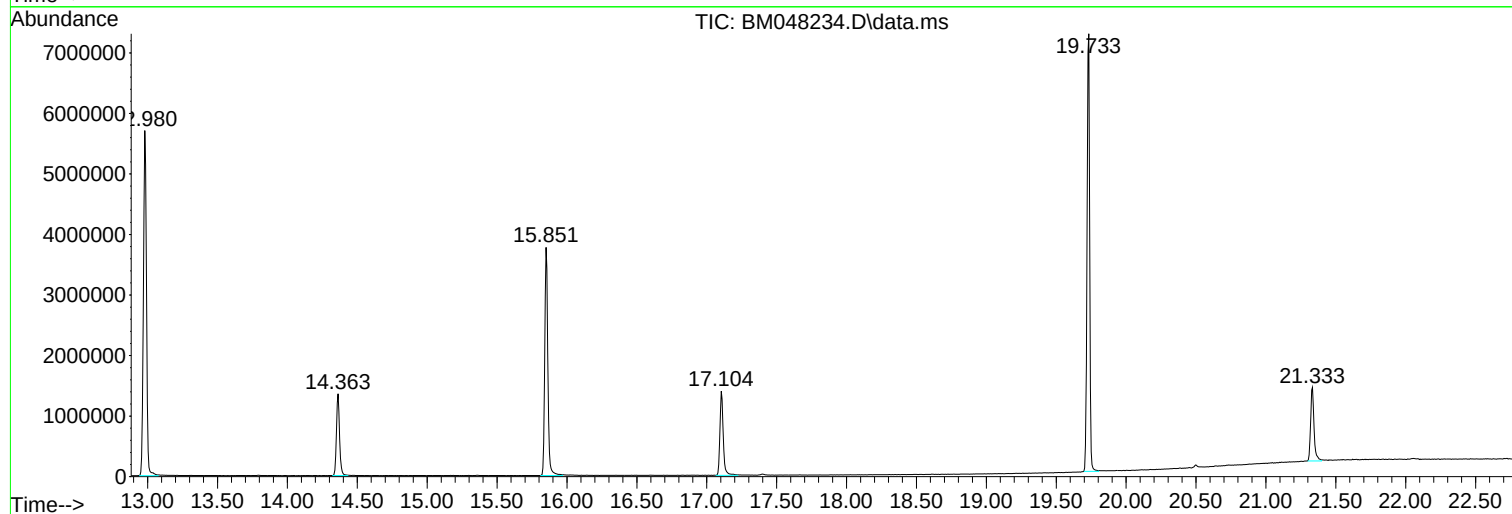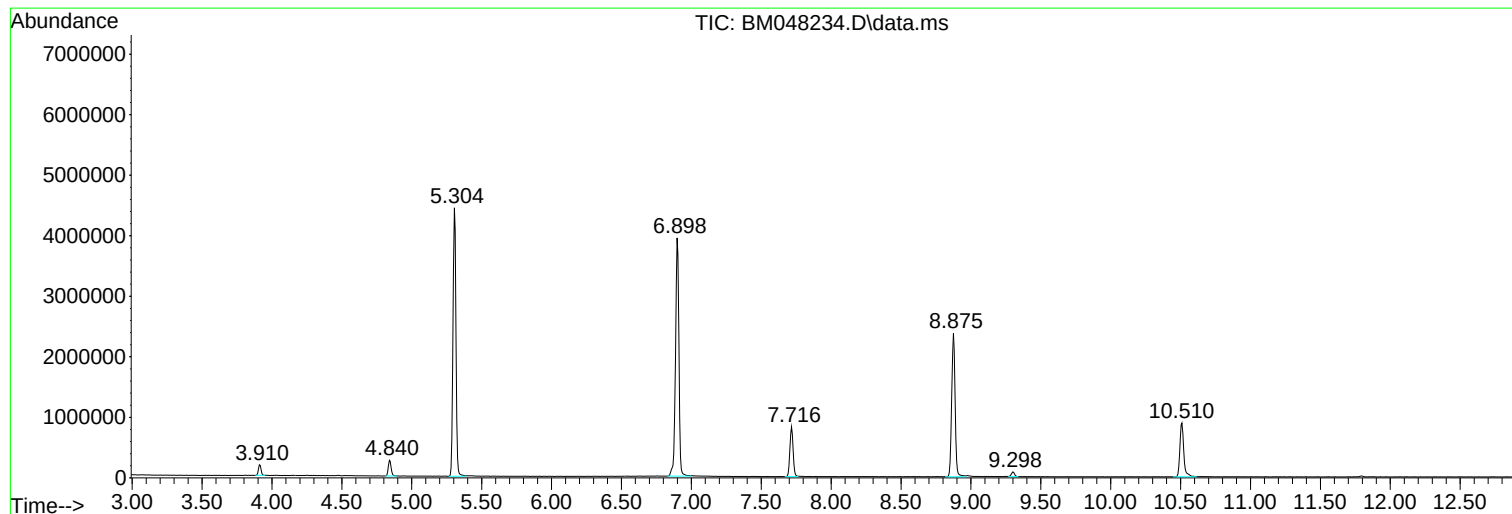

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048234.D
Acq On : 25 Oct 2024 13:38
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164401BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.840	5.56 ng	363030	1,4-Dichlorobenzene-d4	7.716

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2			Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17
3			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
4			5-Hexen-2-one	98	C6H10O	000109-49-9	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

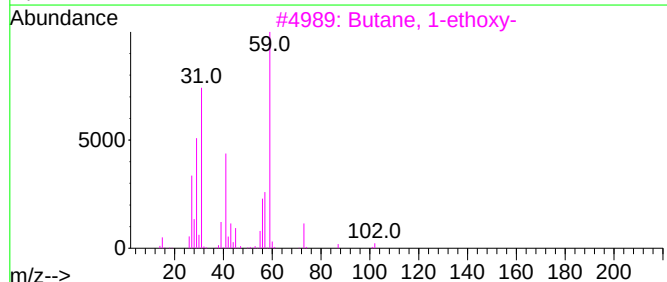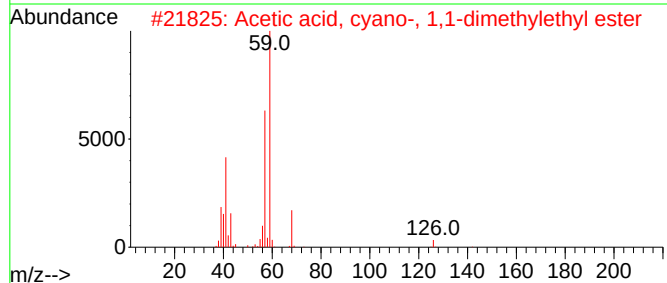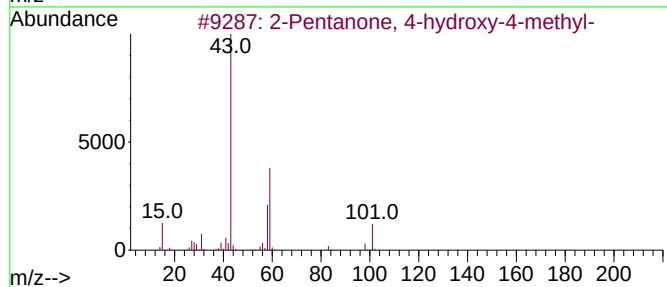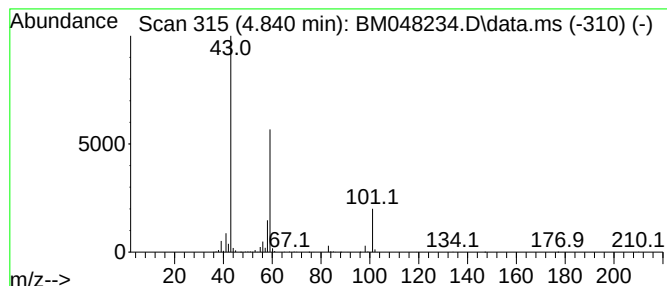

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102524\
Data File : BM048234.D
Acq On : 25 Oct 2024 13:38
Operator : RC/JU
Sample : PB164401BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB164401BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.840	5.6	ng	363030	1	7.716	1305580	20.0