

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
 Data File : BM037242.D
 Acq On : 26 Oct 2022 17:15
 Operator : CG/JU
 Sample : PB148383BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB148383BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM037242.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.458	396	403	415	rBV	3262110	4686439	33.93%	8.117%
2	7.057	668	675	686	rBV	3114975	4839947	35.04%	8.383%
3	7.887	809	816	827	rBV	921037	1424839	10.32%	2.468%
4	9.057	1007	1015	1028	rBV	2821993	4600776	33.31%	7.969%
5	10.692	1283	1293	1309	rBV	1123110	1944484	14.08%	3.368%
6	13.151	1704	1711	1723	rBV	8371164	11492873	83.21%	19.907%
7	14.522	1937	1944	1957	rBV	1718526	2491362	18.04%	4.315%
8	16.010	2190	2197	2209	rBV	3650527	5164984	37.39%	8.946%
9	17.263	2403	2410	2423	rBV	1982370	2726735	19.74%	4.723%
10	19.880	2850	2855	2871	rBV	11446741	13812291	100.00%	23.924%
11	21.433	3115	3119	3128	rBV	1888323	2409185	17.44%	4.173%
12	23.803	3516	3522	3536	rVB2	1066364	2139247	15.49%	3.705%




Sum of corrected areas: 57733162

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
Data File : BM037242.D
Acq On : 26 Oct 2022 17:15
Operator : CG/JU
Sample : PB148383BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB148383BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

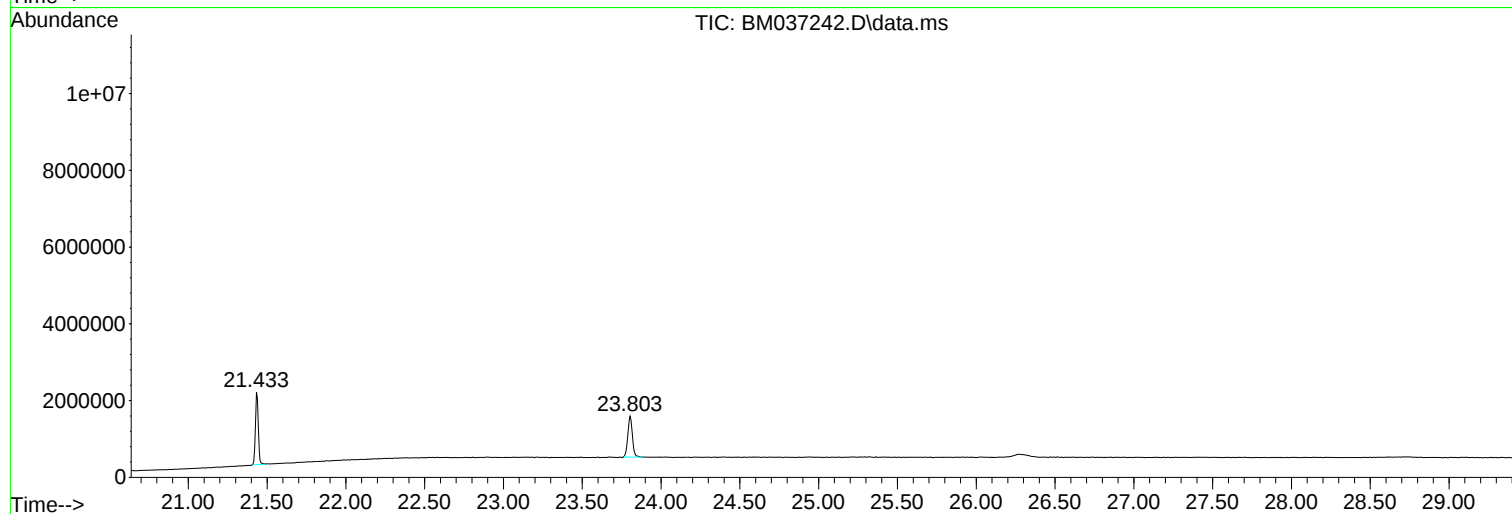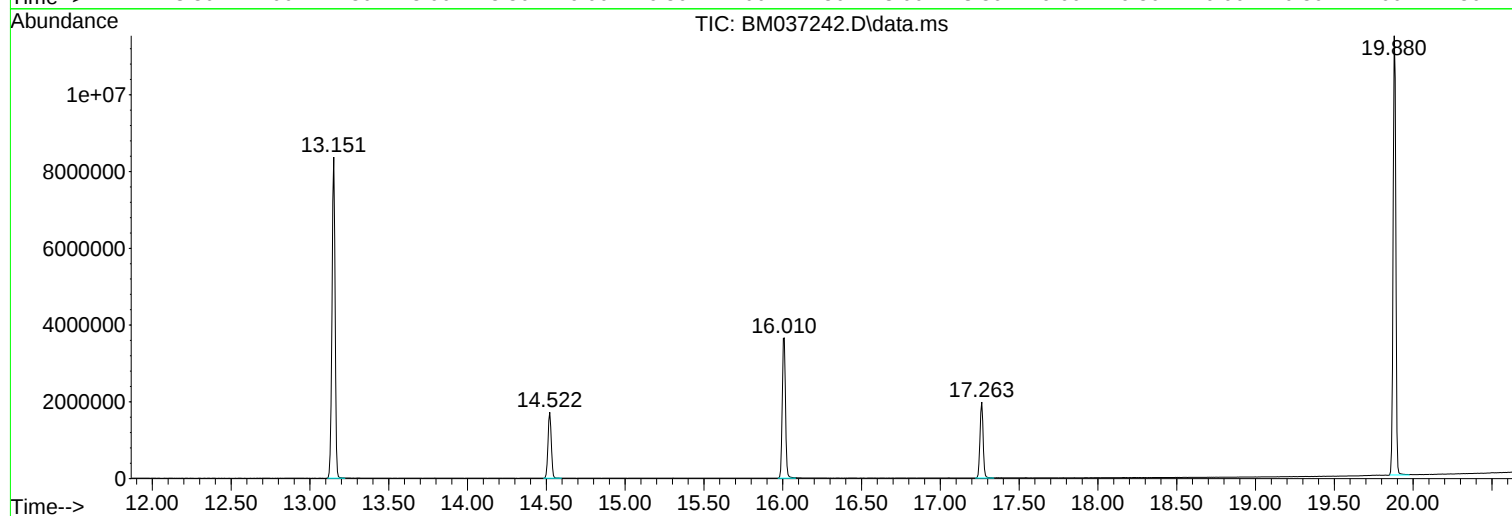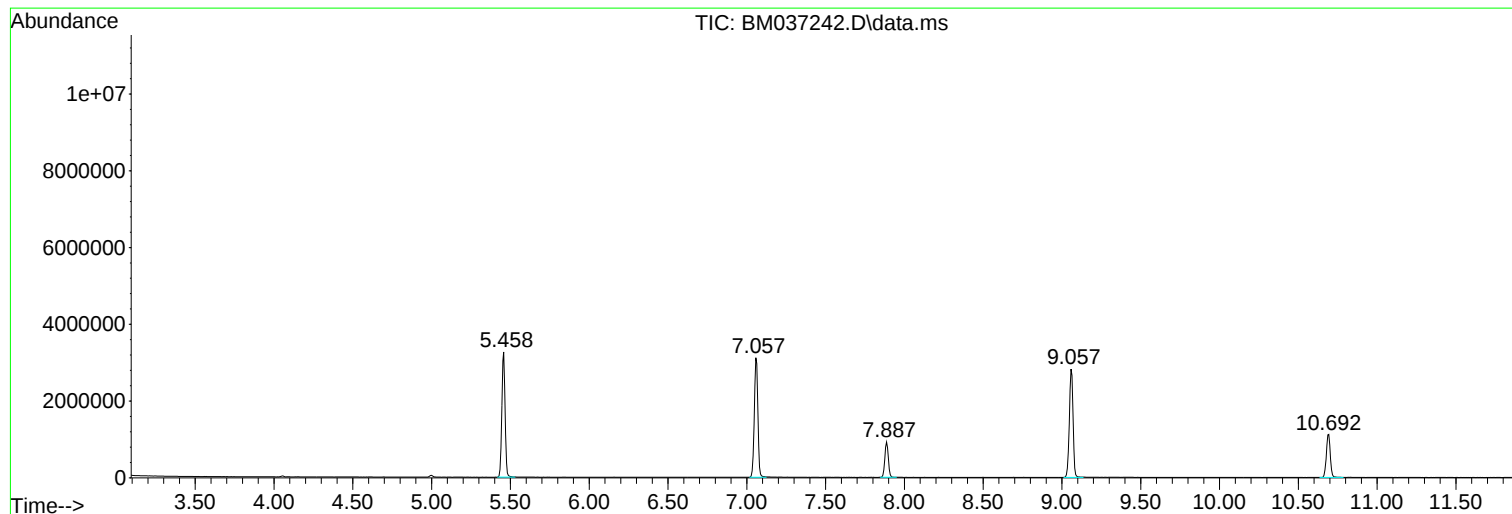

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
Data File : BM037242.D
Acq On : 26 Oct 2022 17:15
Operator : CG/JU
Sample : PB148383BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB148383BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
Data File : BM037242.D
Acq On : 26 Oct 2022 17:15
Operator : CG/JU
Sample : PB148383BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB148383BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------