
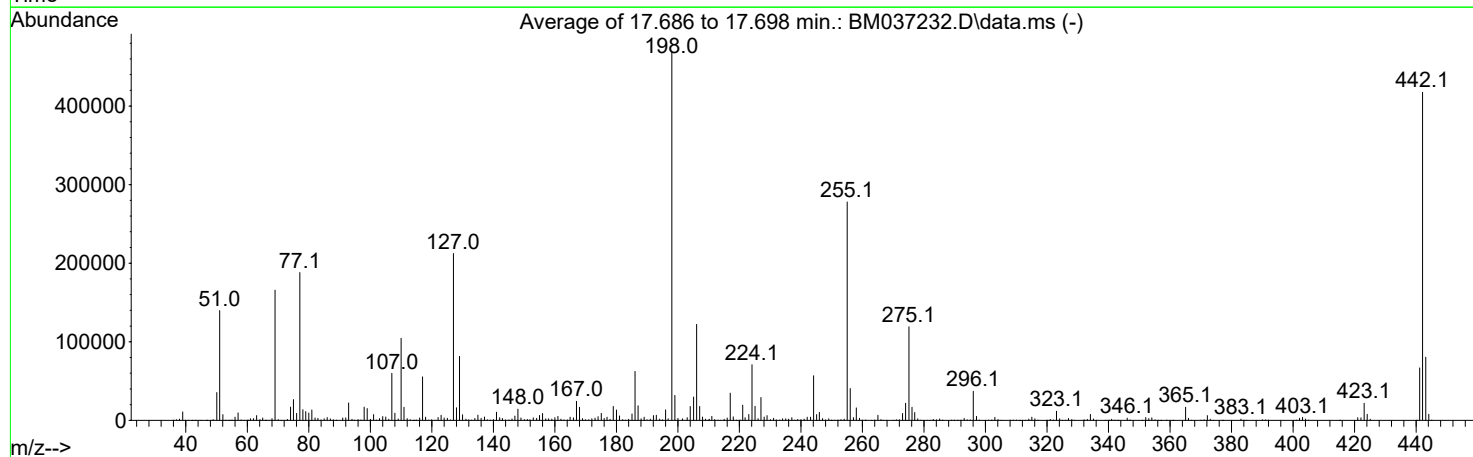


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
 Data File : BM037232.D
 Acq On : 26 Oct 2022 11:07
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM102622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 26 17:18:26 2022

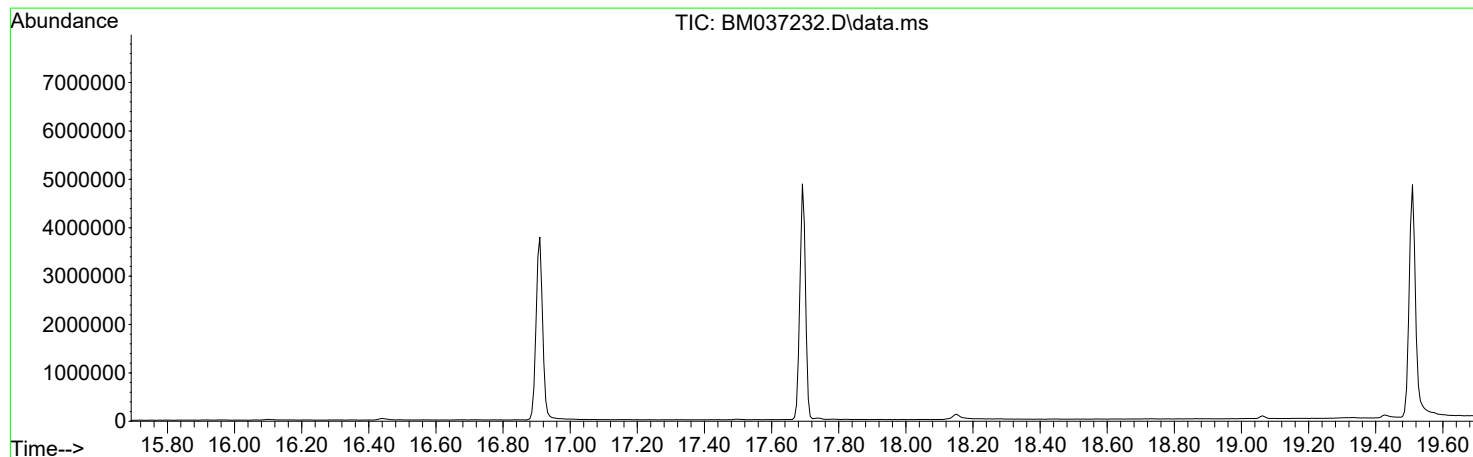




AutoFind: Scans 2482, 2483, 2484; Background Corrected with Scan 2475

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.8	139645	PASS
68	69	0.00	2	1.4	2342	PASS
69	198	0.00	100	35.4	165847	PASS
70	69	0.00	2	0.6	960	PASS
127	198	10	80	45.4	212331	PASS
197	198	0.00	2	0.5	2116	PASS
198	198	100	100	100.0	468139	PASS
199	198	5	9	6.8	31840	PASS
275	198	10	60	25.4	119117	PASS
365	198	1	100	3.6	16711	PASS
441	198	0.01	100	14.3	66816	PASS
442	442	50	100	100.0	417685	PASS
443	442	15	24	19.3	80405	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
Data File : BM037232.D
Acq On : 26 Oct 2022 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 26 18:38:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

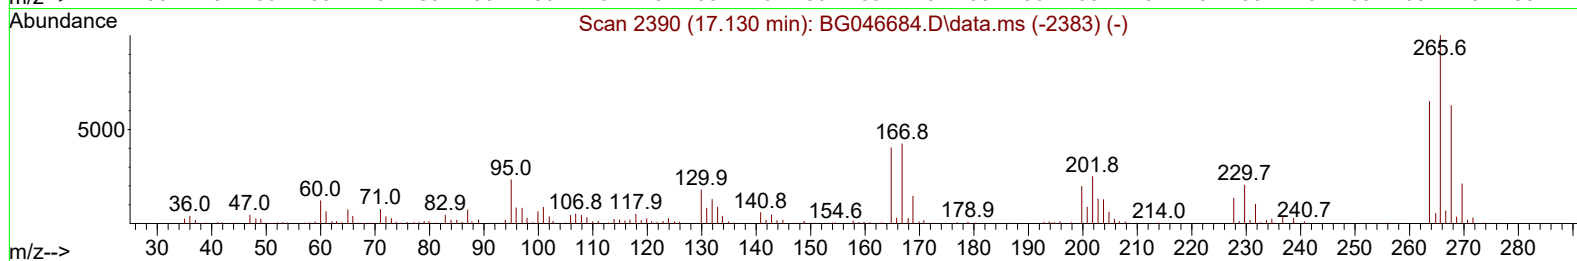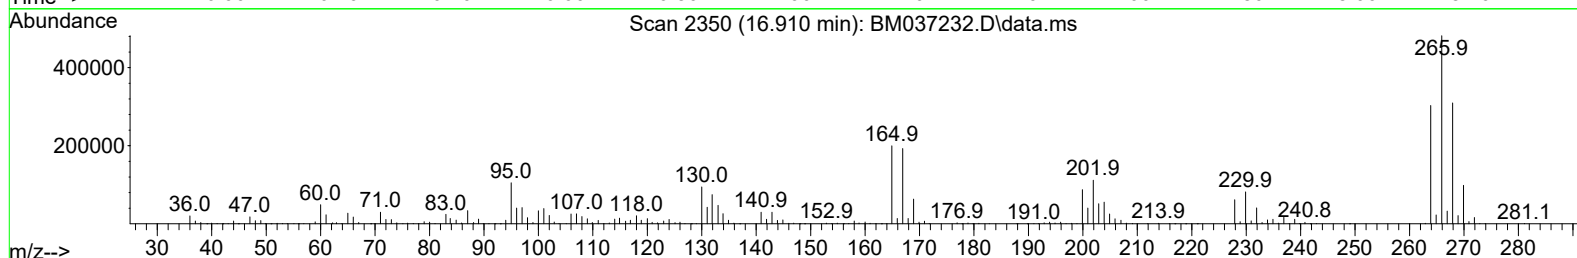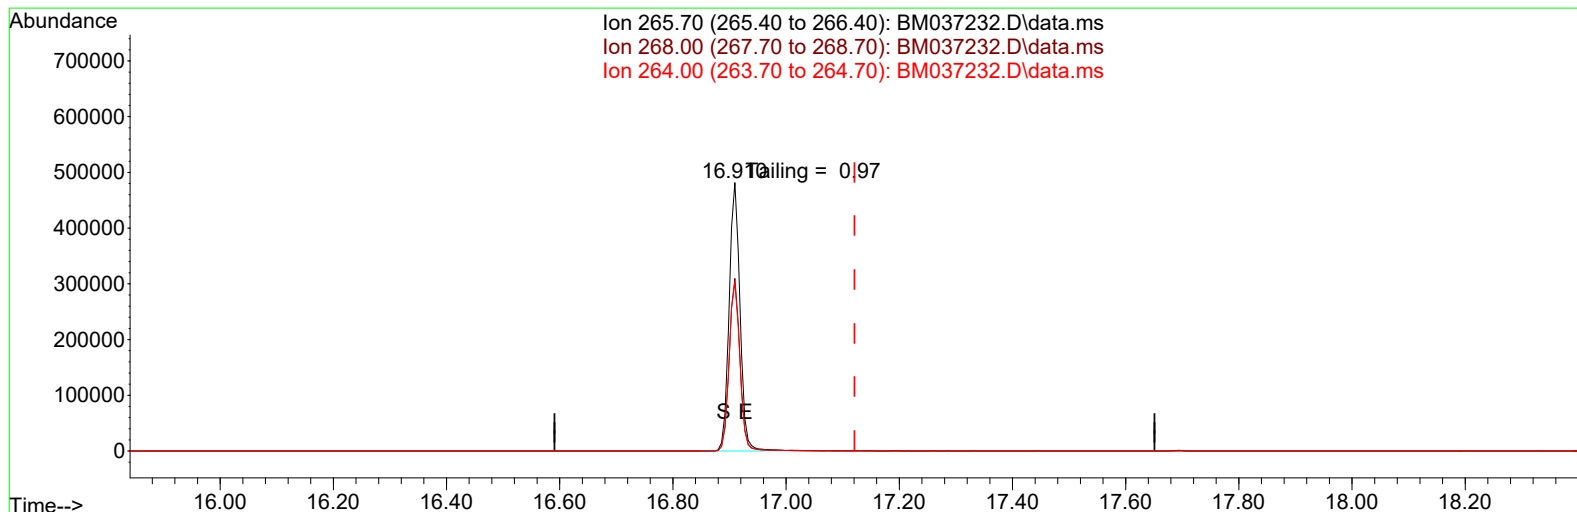

TIC: BM037232.D\data.ms

(70) Pentachlorophenol (C)

16.910min (-0.211) 29169.12 ng




response 644387

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.26
264.00	61.60	62.94
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102622\
Data File : BM037232.D
Acq On : 26 Oct 2022 11:07
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Oct 26 18:38:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

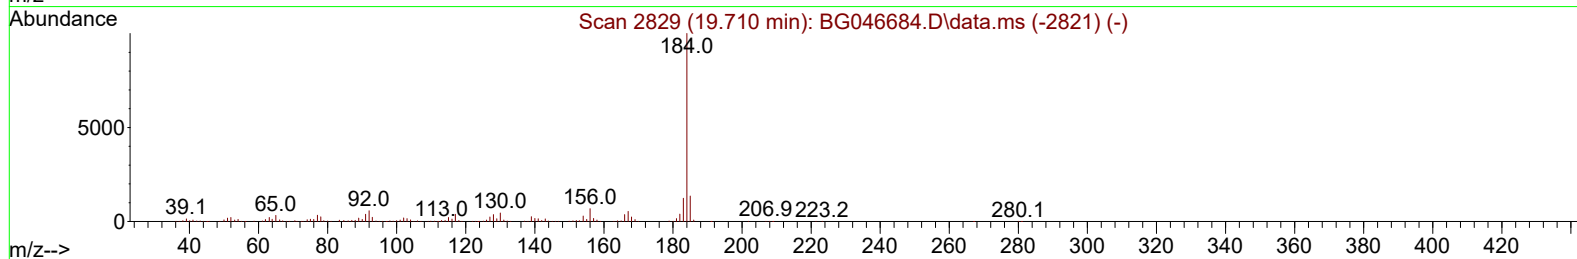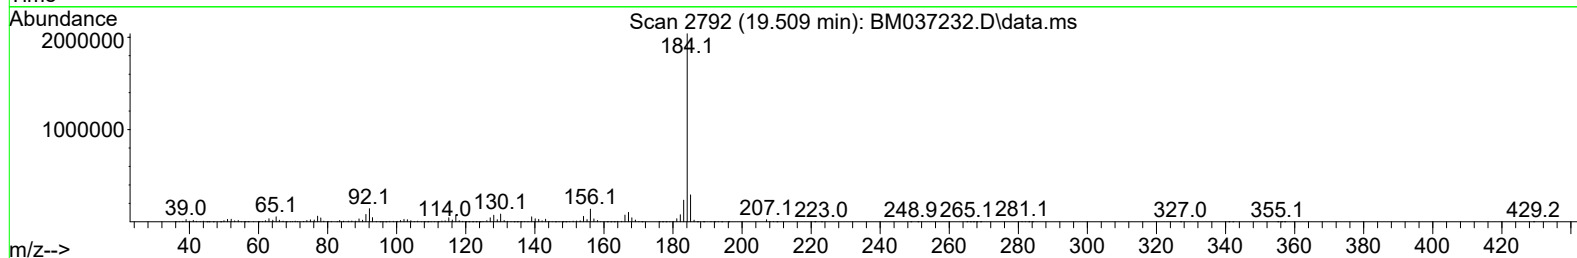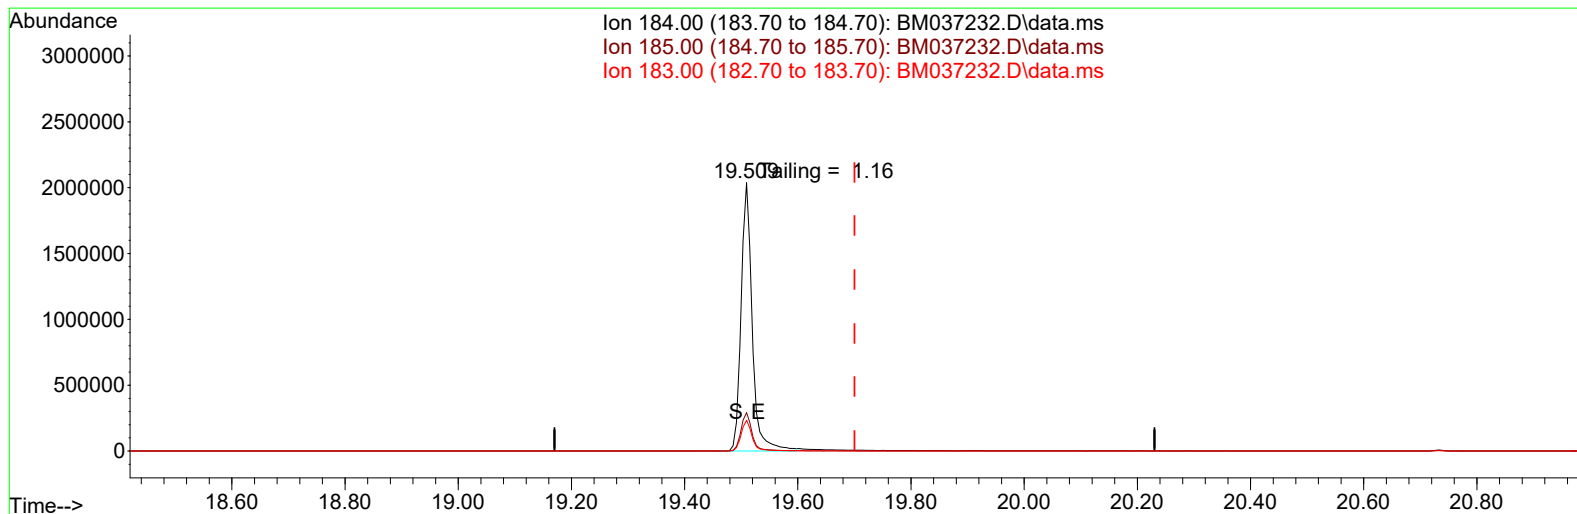

TIC: BM037232.D\data.ms

(77) Benzidine

19.509min (-0.191) 0.00 ng

response 2858363

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.33
183.00	13.20	11.46
0.00	0.00	0.00