
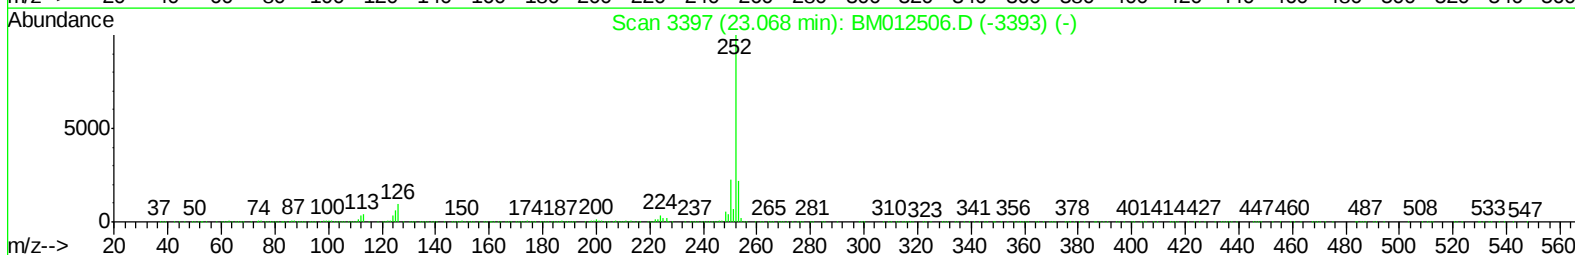
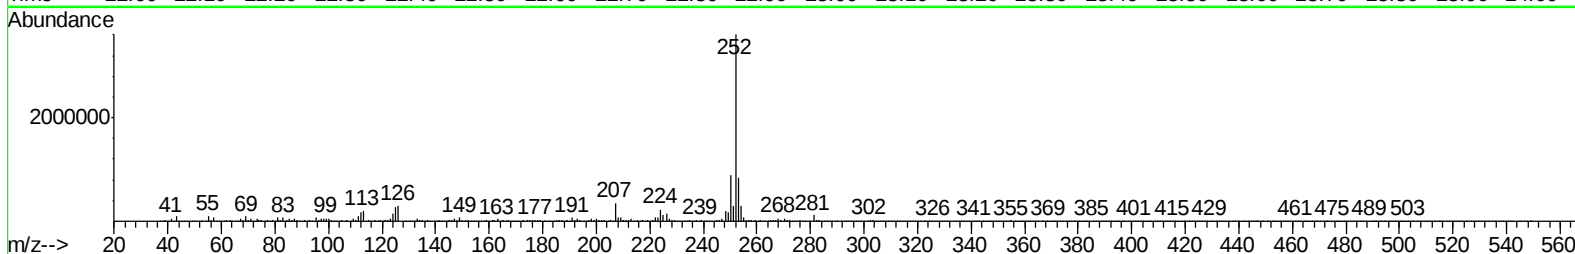


Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012515.D
Acq On : 28 Oct 2017 09:03
Operator : SJ/JU
Sample : I5786-02MS 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Quant Time: Oct 30 07:02:56 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 30 05:30:34 2017
Response via : Initial Calibration

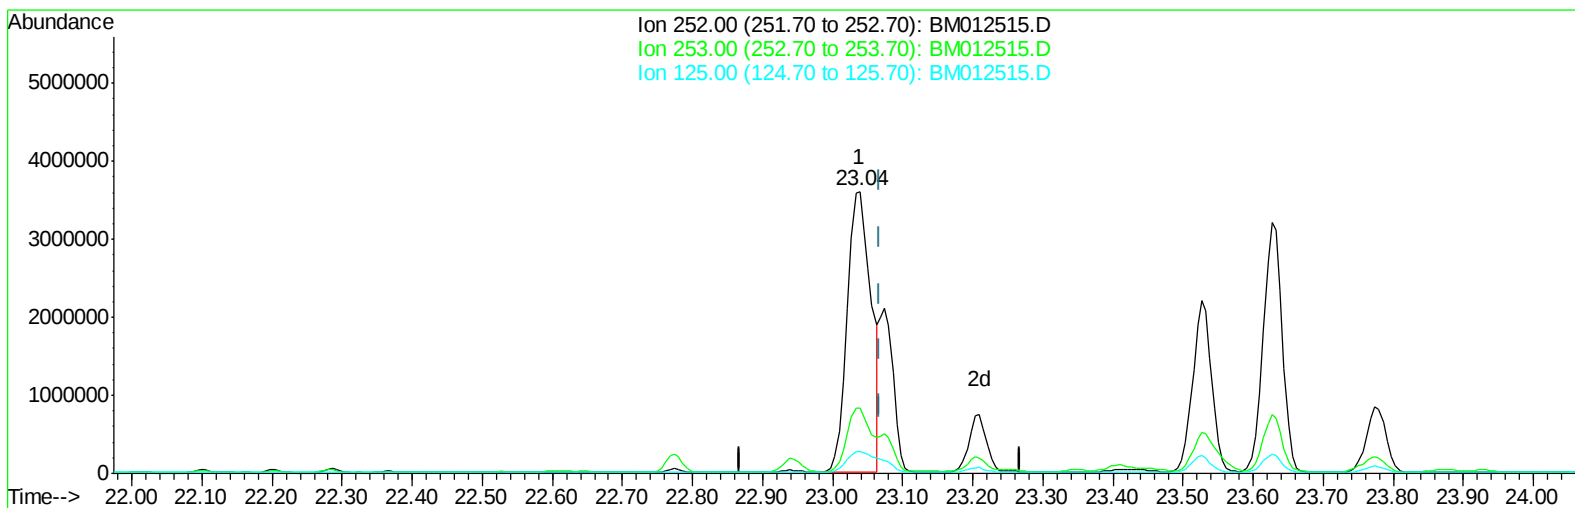

TIC: BM012515.D

(86) Benzo(k)fluoranthene

23.039min (-0.029) 46.91ng/ul

response 8458713

Ion	Exp%	Act%
252.00	100	100
253.00	21.40	23.26
125.00	4.30	7.62#
0.00	0.00	0.00