

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
 Data File : BM012491.D
 Acq On : 27 Oct 2017 18:43
 Operator : SJ/JU
 Sample : PB103703BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 28 02:44:30 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 09:35:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	465314	20.00	ng/ul	0.00
18) Naphthalene-d8	10.67	136	1912629	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.51	164	1196396	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.25	188	2754105	20.00	ng/ul	0.00
75) Chrysene-d12	21.42	240	2637585	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	2696729	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	81636	8.96	ng/uL	0.00
5) Phenol-d5	7.05	99	1573291	40.47	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.21	67	984650	42.67	ng/ul	0.00
9) 2-Chlorophenol-d4	7.41	132	1273867	43.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.59	113	1317795	39.67	ng/ul	0.00
19) Nitrobenzene-d5	9.03	128	640531	53.47	ng/ul	0.00
22) 2-Nitrophenol-d4	9.75	143	752596	60.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.29	165	1336685	40.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.80	131	1732871	50.27	ng/ul	0.00
43) Dimethylphthalate-d6	13.92	166	4478466	42.85	ng/ul	0.00
46) Acenaphthylene-d8	14.20	160	5271348	42.64	ng/ul	0.00
51) 4-Nitrophenol-d4	14.71	143	702862	45.24	ng/ul	0.00
57) Fluorene-d10	15.50	176	3701309	41.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	715365	53.67	ng/ul	0.00
70) Anthracene-d10	17.35	188	5877216	44.78	ng/ul	0.00
76) Pyrene-d10	19.64	212	6071141	50.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.59	264	5569860	43.47	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.58	70	37349	1.31	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012491.D
Acq On : 27 Oct 2017 18:43
Operator : SJ/JU
Sample : PB103703BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :

Quant Time: Oct 28 02:44:30 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 09:35:31 2017
Response via : Initial Calibration

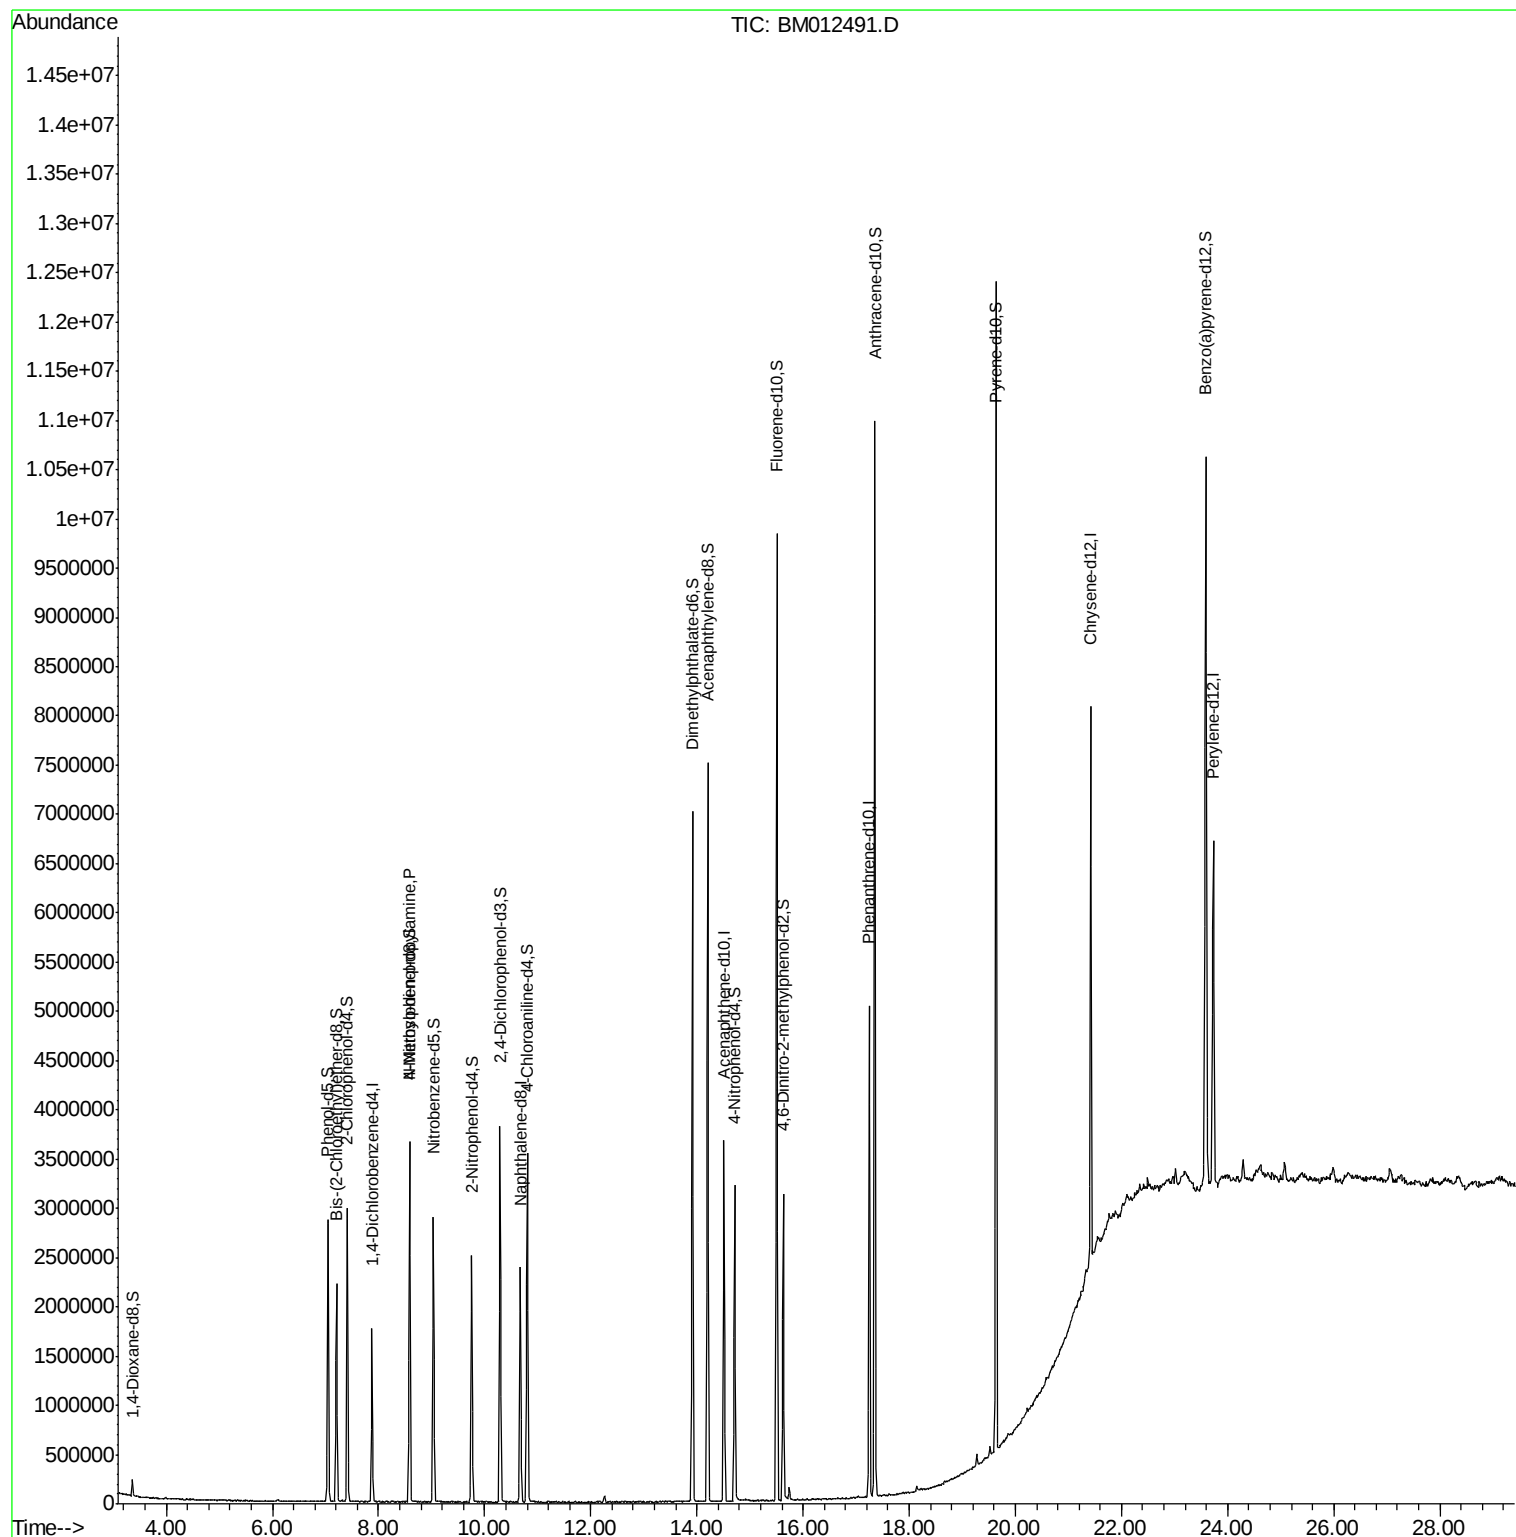

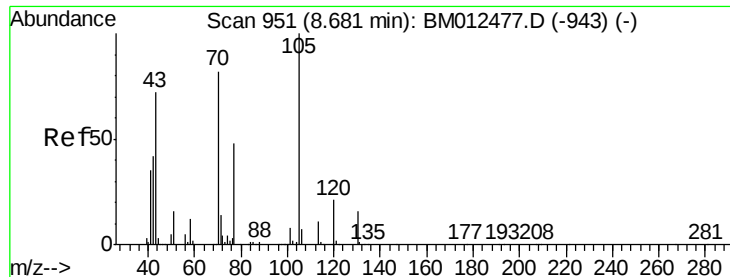

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.31 ng/ul
 RT: 8.58 min Scan# 934
 Delta R.T. -0.11 min
 Lab File: BM012491.D
 Acq: 27 Oct 2017 18:43

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion: 70 Resp: 37349
 Ion Ratio Lower Upper
 70 100
 42 334.9 76.0 114.0#
 101 0.0 6.7 10.1#
 130 0.0 14.6 22.0#

