

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
 Data File : BM012483.D
 Acq On : 27 Oct 2017 13:07
 Operator : SJ/JU
 Sample : I5719-16
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B-26(0.5-1.5)-100517

Quant Time: Oct 28 01:08:45 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 26 09:35:31 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.88	152	399564	20.00	ng/ul	0.00
18) Naphthalene-d8	10.66	136	1478354	20.00	ng/ul	-0.01
35) Acenaphthene-d10	14.50	164	829420	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.25	188	1810727	20.00	ng/ul	0.00
75) Chrysene-d12	21.42	240	2049071	20.00	ng/ul	0.00
83) Perylene-d12	23.73	264	2411212	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.36	96	38225	4.89	ng/uL	0.00
5) Phenol-d5	7.04	99	657507	19.70	ng/ul	-0.01
7) Bis-(2-Chloroethyl)ether-d	7.20	67	450468	22.73	ng/ul	0.00
9) 2-Chlorophenol-d4	7.41	132	552449	22.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.58	113	275391	9.65	ng/ul	-0.01
19) Nitrobenzene-d5	9.03	128	269992	29.16	ng/ul	0.00
22) 2-Nitrophenol-d4	9.75	143	289700	30.37	ng/ul	-0.01
26) 2,4-Dichlorophenol-d3	10.29	165	514894	20.38	ng/ul	-0.01
29) 4-Chloroaniline-d4	10.80	131	180236	6.76	ng/ul	0.00
43) Dimethylphthalate-d6	13.91	166	1703785	23.51	ng/ul	0.00
46) Acenaphthylene-d8	14.20	160	2075778	24.22	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	98655	9.16	ng/ul	-0.01
57) Fluorene-d10	15.49	176	1446636	23.59	ng/ul	-0.01
62) 4,6-Dinitro-2-methylphenol	15.61	200	57758	6.59	ng/ul	-0.01
70) Anthracene-d10	17.34	188	2111864	24.47	ng/ul	-0.01
76) Pyrene-d10	19.63	212	2409701	25.63	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.58	264	2783441	24.30	ng/ul	0.00

Target Compounds


					Ovalue	
6) Phenol	7.07	94	185441	5.336	ng/ul#	86
14) Acetophenone	8.69	105	63571	1.418	ng/ul	86
44) Dimethylphthalate	13.96	163	951626	13.277	ng/ul	99
69) Phenanthrene	17.29	178	319241	3.260	ng/ul	99
74) Fluoranthene	19.30	202	206412	1.860	ng/ul#	96
77) Pyrene	19.66	202	224741	1.929	ng/ul#	88
82) Chrysene	21.45	228	297511	2.727	ng/ul#	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012483.D
Acq On : 27 Oct 2017 13:07
Operator : SJ/JU
Sample : I5719-16
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B-26(0.5-1.5)-100517

Quant Time: Oct 28 01:08:45 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 26 09:35:31 2017
Response via : Initial Calibration

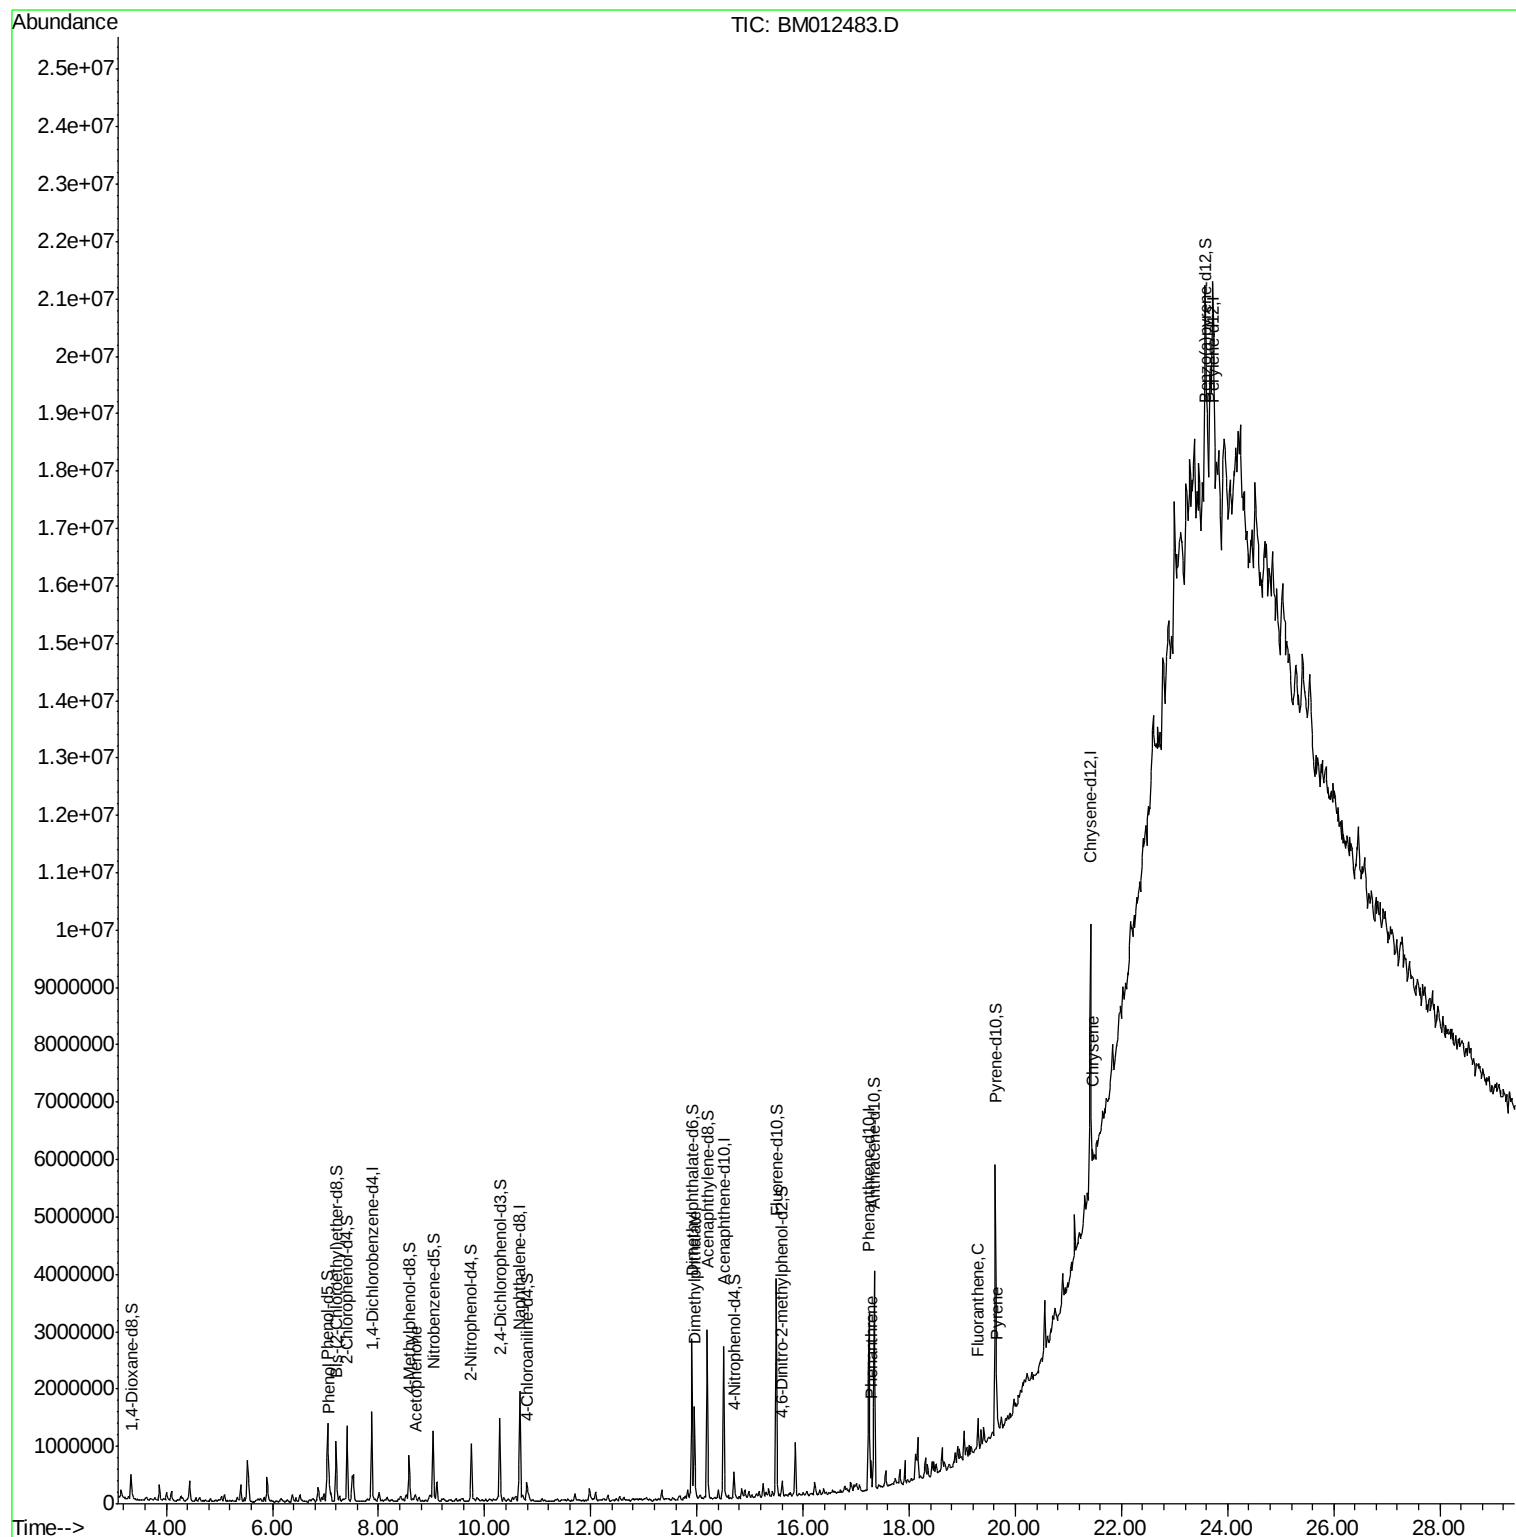

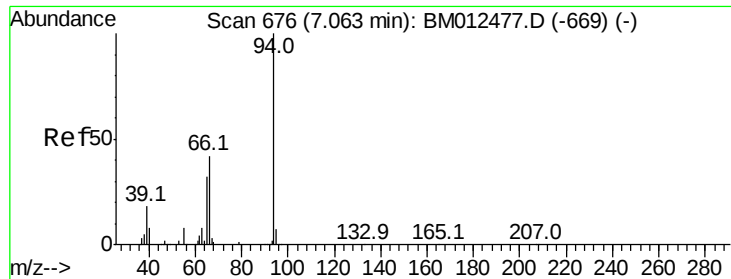

#6

Phenol

Concen: 5.336 ng/ul

RT: 7.07 min Scan# 677

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07

Instrument :

BNA_M

ClientSampleId :

B-26(0.5-1.5)-100517


Tot Ion: 94 Resp: 185441

Ion Ratio Lower Upper

94 100

65 32.5 28.2 42.4

66 44.2 47.2 70.8#

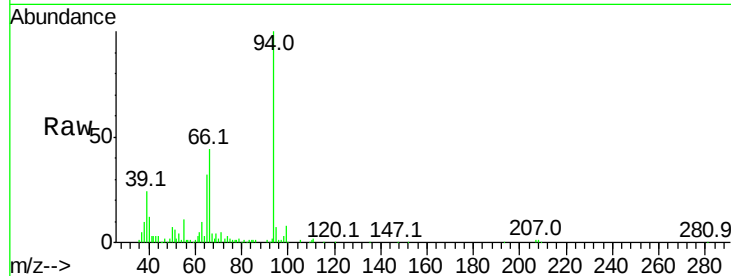

Abundance Ion 94.00 (93.70 to 94.70): BM012477.D (-669) (-)

Ion 65.00 (64.70 to 65.70): BM012477.D (-669) (-)

Ion 66.00 (65.70 to 66.70): BM012477.D (-669) (-)

7.07

150000



100000

50000

0

7.00 7.05 7.10

Time-->

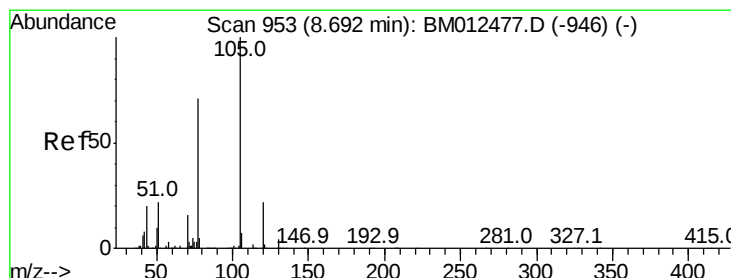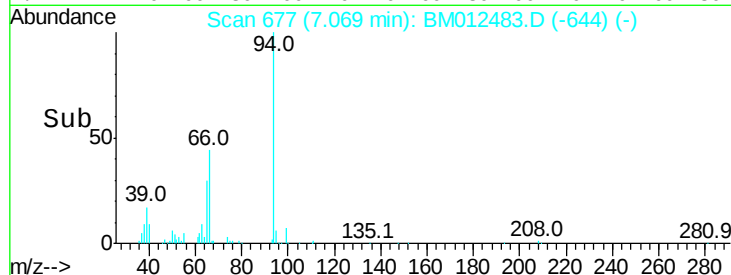

#14

Acetophenone

Concen: 1.418 ng/ul

RT: 8.69 min Scan# 952

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07


Tgt Ion:105 Resp: 63571

Ion Ratio Lower Upper

105 100

77 76.3 74.2 111.4

51 26.7 23.4 35.2

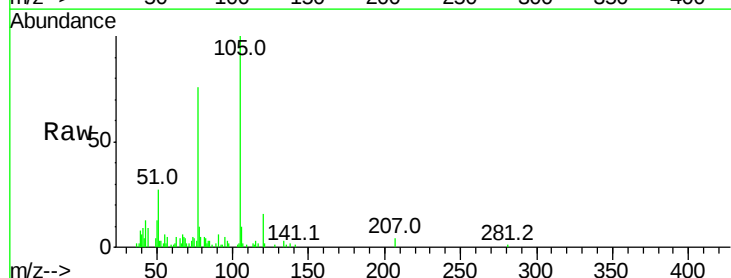

Abundance Ion 105.00 (104.70 to 105.70): BM012477.D (-946) (-)

Ion 77.00 (76.70 to 77.70): BM012477.D (-946) (-)

Ion 51.00 (50.70 to 51.70): BM012477.D (-946) (-)

8.69

40000

30000


20000


10000

0

8.60 8.65 8.70 8.75

Time-->

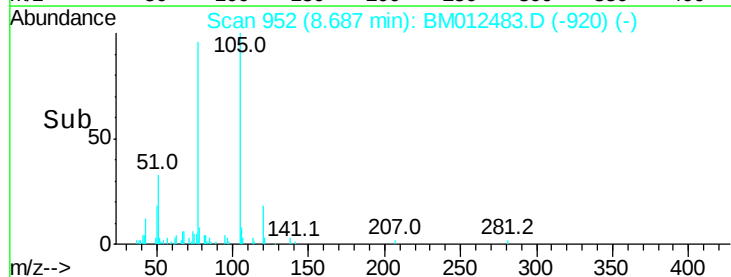

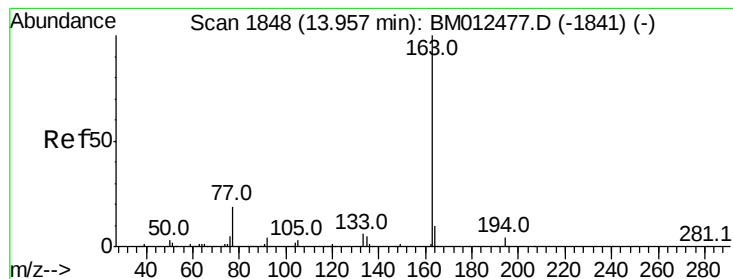

#44

Dimethylphthalate

Concen: 13.277 ng/ul

RT: 13.96 min Scan# 1848

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07

Instrument :

BNA_M

ClientSampleId :

B-26(0.5-1.5)-100517


Tot Ion:163 Resp: 951626

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3




164 10.0 8.2 12.4

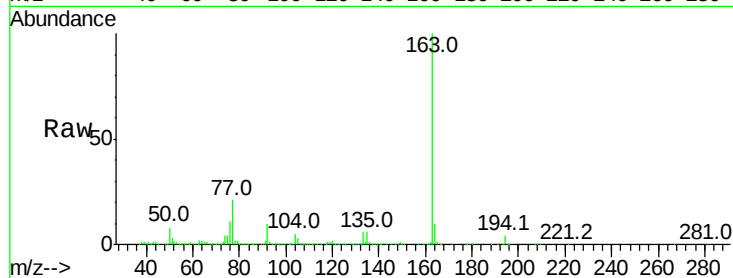

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

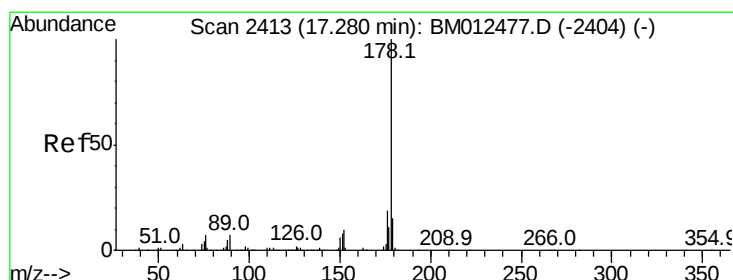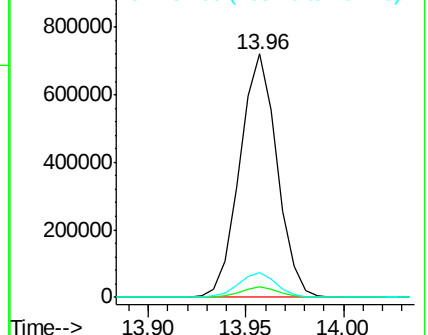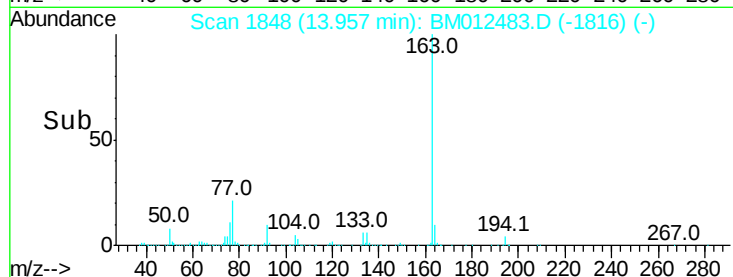

#69

Phenanthrene

Concen: 3.260 ng/ul

RT: 17.29 min Scan# 2414

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07


Tgt Ion:178 Resp: 319241

Ion Ratio Lower Upper

178 100

179 16.2 12.6 19.0



176 19.1 14.9 22.3

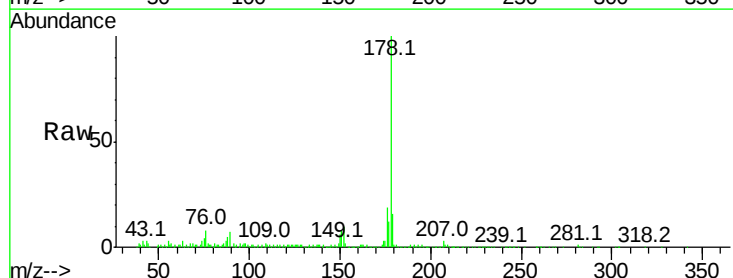


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

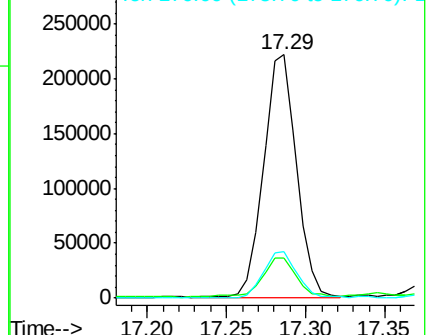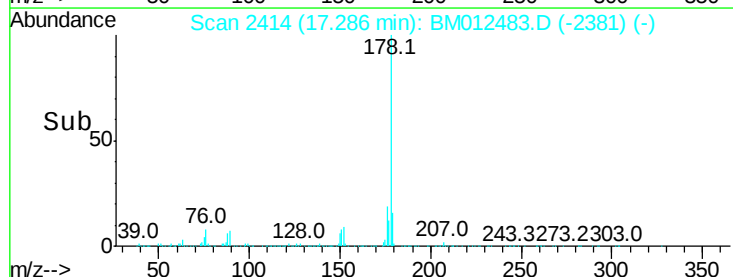

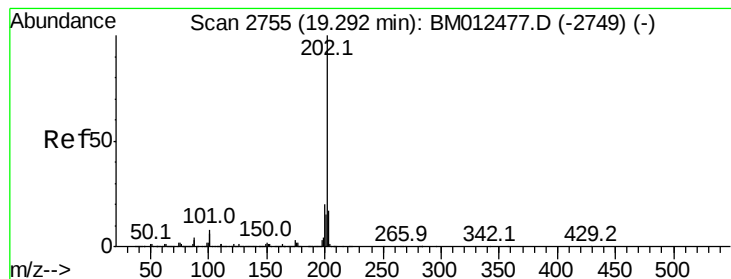

#74

Fluoranthene

Concen: 1.860 ng/ul

RT: 19.30 min Scan# 2756

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07

Instrument :

BNA_M

ClientSampleId :

B-26(0.5-1.5)-100517


Tot Ion:202 Resp: 206412

Ion Ratio Lower Upper

202 100

101 7.2 4.6 7.0#




100 5.6 3.4 5.2#

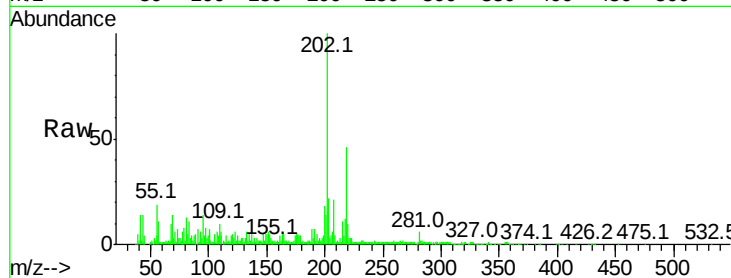

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

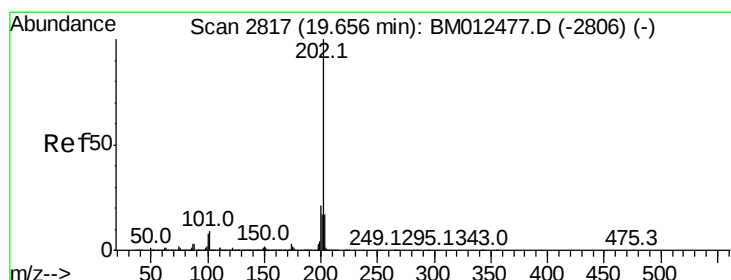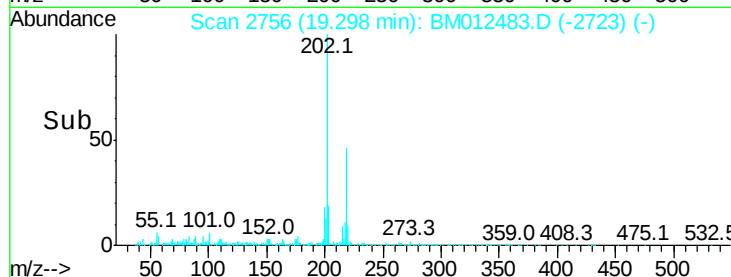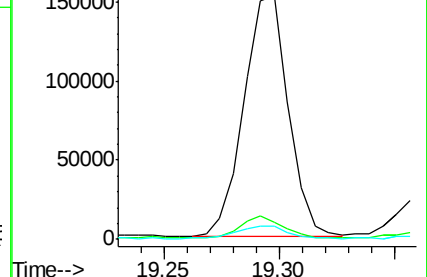

#77

Pyrene

Concen: 1.929 ng/ul

RT: 19.66 min Scan# 2817

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07


Tgt Ion:202 Resp: 224741

Ion Ratio Lower Upper

202 100

101 10.6 5.1 7.7#



100 9.9 4.9 7.3#

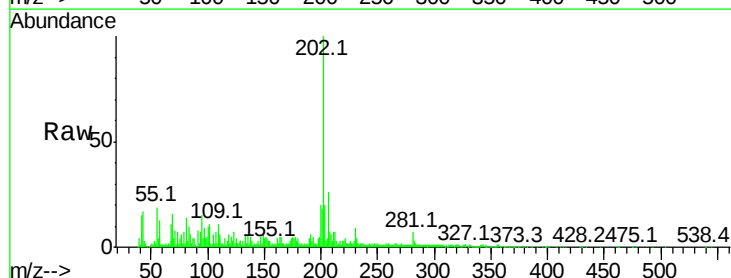


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

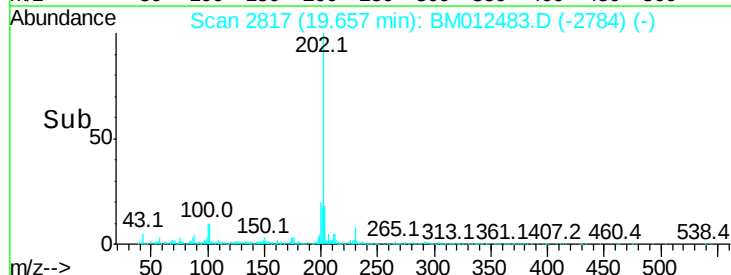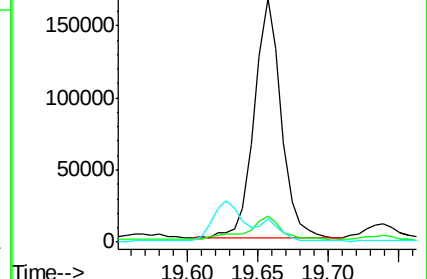

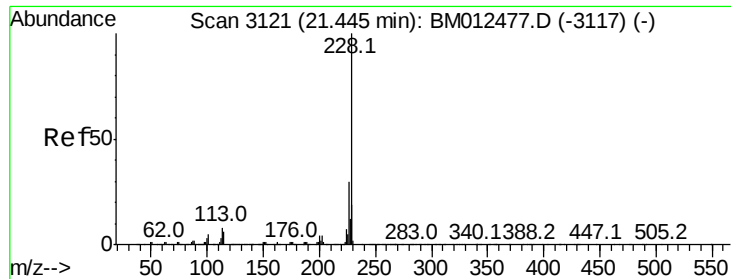

#82

Chrysene

Concen: 2.727 ng/ul

RT: 21.45 min Scan# 3122

Delta R.T. -0.01 min

Lab File: BM012483.D

Acq: 27 Oct 2017 13:07

Instrument :

BNA_M

ClientSampleId :

B-26(0.5-1.5)-100517


Tot Ion:228 Resp: 297511

Ion Ratio Lower Upper

228 100

226 33.2 23.4 35.2

229 27.4 15.5 23.3#

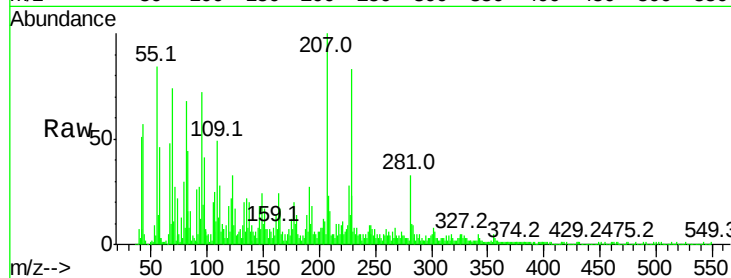

Abundance Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

