

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
 Data File : BM012491.D
 Acq On : 27 Oct 2017 18:43
 Operator : SJ/JU
 Sample : PB103703BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK03

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	43	47	57	rVB	170653	252148	1.57%	0.155%
2	7.045	666	673	682	rBV	2867186	4590161	28.57%	2.823%
3	7.210	692	701	712	rBV	2218493	3454213	21.50%	2.124%
4	7.410	729	735	745	rVB	2981945	4795293	29.84%	2.949%
5	7.875	807	814	823	rBV	1761859	2849887	17.74%	1.753%
6	8.581	927	934	943	rBV	3653948	5913104	36.80%	3.636%
7	9.034	1003	1011	1021	rBV	2898174	4759250	29.62%	2.927%
8	9.751	1126	1133	1148	rBV	2505775	4182169	26.03%	2.572%
9	10.292	1218	1225	1236	rBV	3819912	6176949	38.44%	3.799%
10	10.669	1281	1289	1300	rVB	2385997	4053943	25.23%	2.493%
11	10.804	1304	1312	1328	rVB	3539710	6044067	37.61%	3.717%
12	13.916	1835	1841	1855	rVB	7004572	9597090	59.73%	5.902%
13	14.204	1880	1890	1898	rBV	7499692	11065572	68.86%	6.805%
14	14.510	1933	1942	1952	rBV2	3664504	5667865	35.27%	3.486%
15	14.710	1969	1976	1992	rBV	3205250	4758502	29.61%	2.926%
16	15.504	2103	2111	2118	rBV	9812606	13621474	84.77%	8.377%
17	15.627	2124	2132	2143	rBV	3121033	4483992	27.91%	2.758%
18	15.739	2146	2151	2158	rVB	129382	198403	1.23%	0.122%
19	17.251	2401	2408	2415	rBV	4976842	6856850	42.67%	4.217%
20	17.351	2418	2425	2438	rVB	10918339	14935692	92.95%	9.185%
21	19.639	2808	2814	2820	rBV	11869340	16068543	100.00%	9.882%
22	21.421	3112	3117	3122	rBV	5645735	7024045	43.71%	4.320%
23	23.586	3479	3485	3496	rVB	7380880	14515603	90.34%	8.927%
24	23.733	3504	3510	3520	rVB	3484308	6743654	41.97%	4.147%


Sum of corrected areas: 162608469

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012491.D
Acq On : 27 Oct 2017 18:43
Operator : SJ/JU
Sample : PB103703BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampled :
SBLK03

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

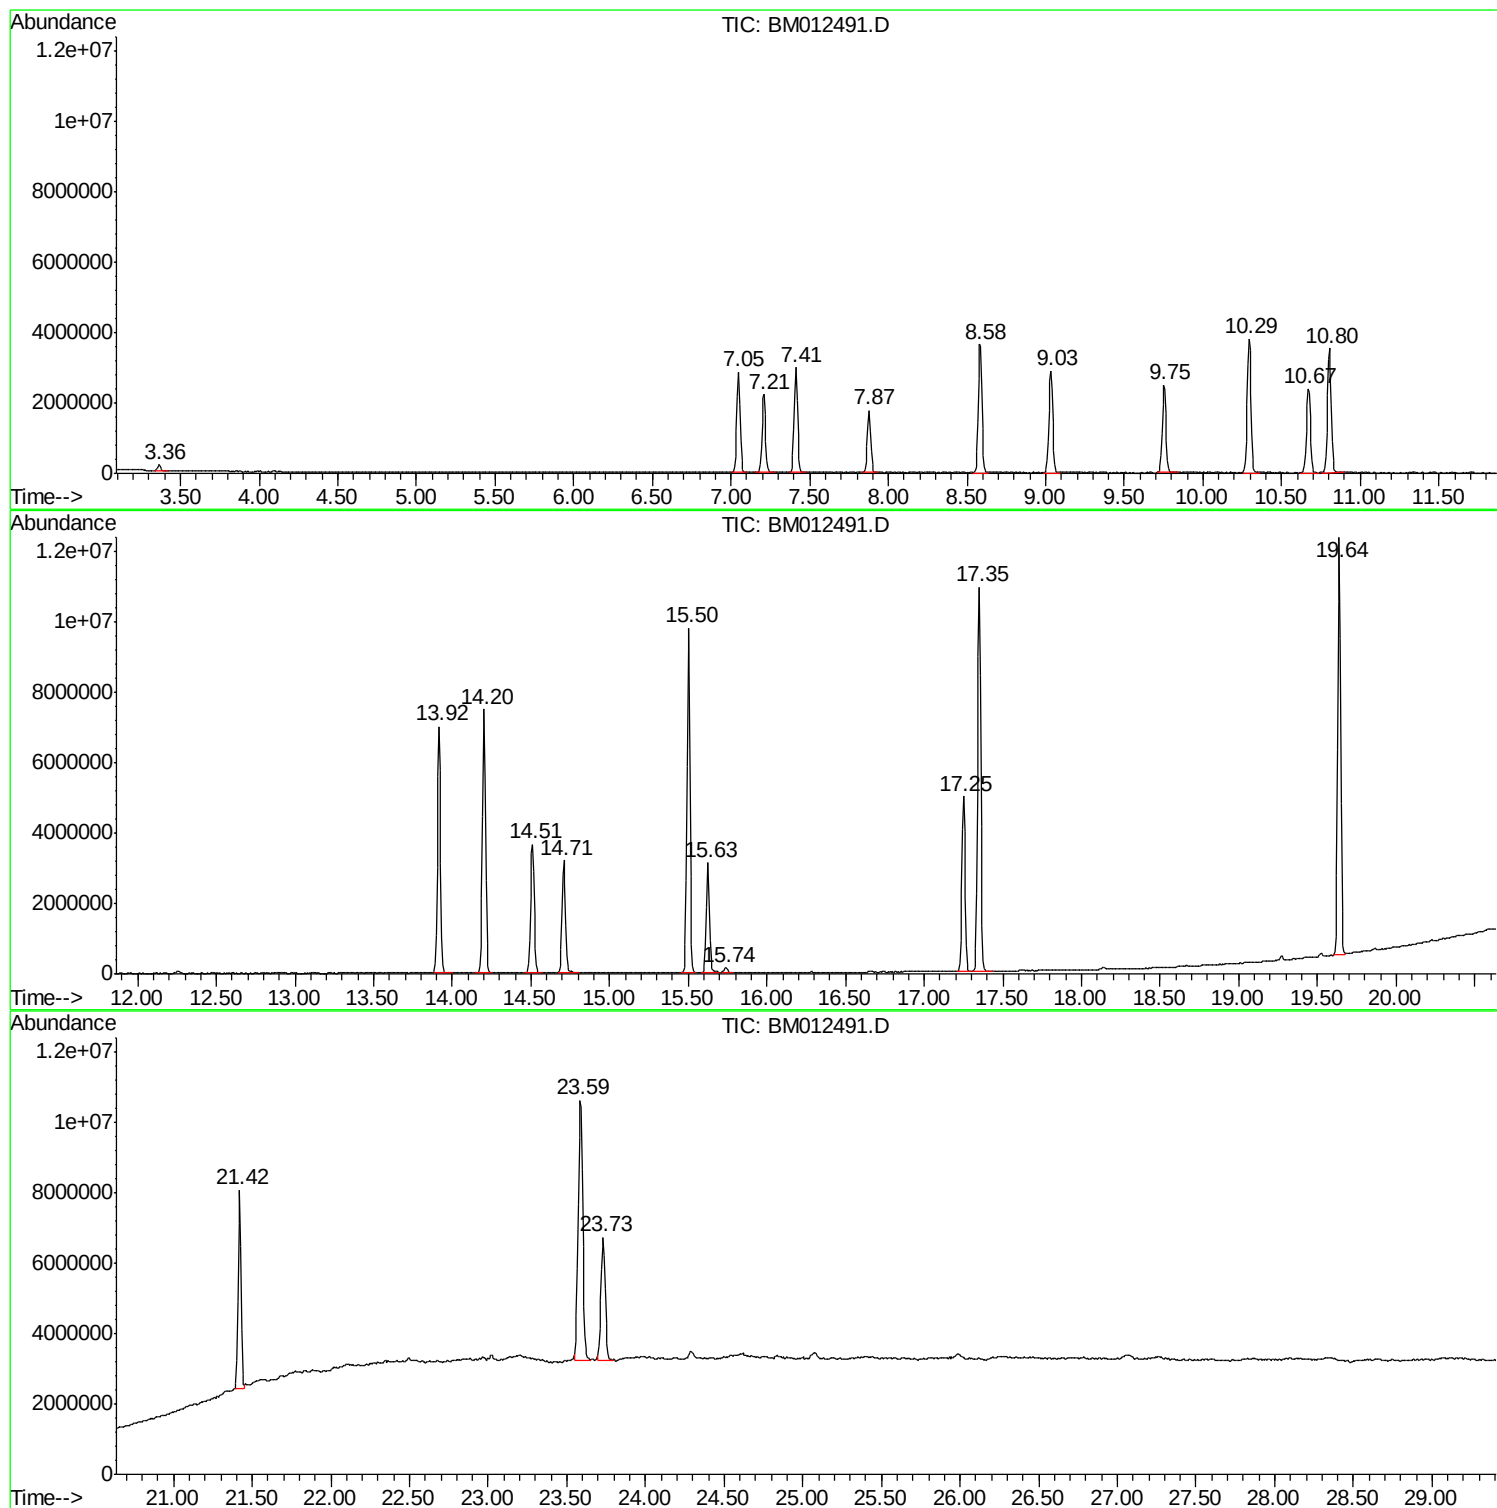

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102717\
Data File : BM012491.D
Acq On : 27 Oct 2017 18:43
Operator : SJ/JU
Sample : PB103703BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK03

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102717\
Data File : BM012491.D
Acq On : 27 Oct 2017 18:43
Operator : SJ/JU
Sample : PB103703BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK03

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc