

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012499.D
Acq On : 27 Oct 2017 23:31
Operator : SJ/JU
Sample : I6127-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC6

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0
Filtering: 5
Min Area: 1 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.357	43	46	53	rVB	146497	204775	1.50%	0.160%
2	7.040	664	672	681	rBV	623339	970163	7.12%	0.756%
3	7.204	692	700	710	rBV	1910209	2914712	21.39%	2.272%
4	7.404	726	734	742	rBV	2155434	3420347	25.10%	2.666%
5	7.875	806	814	821	rBV	1890182	3040142	22.31%	2.370%
6	8.575	923	933	943	rBV	1721208	2735794	20.07%	2.132%
7	9.028	1002	1010	1021	rBV	2495540	4104846	30.12%	3.200%
8	9.745	1124	1132	1142	rBV	2172687	3556011	26.09%	2.772%
9	10.286	1215	1224	1234	rBV	3082945	5069725	37.20%	3.952%
10	10.663	1280	1288	1298	rBV	2463064	4137632	30.36%	3.225%
11	13.910	1833	1840	1851	rBV	5893671	8101867	59.44%	6.315%
12	14.192	1881	1888	1895	rBV	6283410	9541129	70.00%	7.437%
13	14.504	1934	1941	1949	rBV2	3701633	5581706	40.95%	4.351%
14	14.698	1967	1974	1985	rBV	561632	875516	6.42%	0.682%
15	15.498	2103	2110	2119	rBV	7974102	11733670	86.09%	9.146%
16	15.615	2123	2130	2142	rVV	2616433	3650668	26.79%	2.846%
17	15.733	2145	2150	2156	rVB	108049	156035	1.14%	0.122%
18	17.245	2400	2407	2413	rBV2	4729442	6506403	47.74%	5.071%
19	17.345	2417	2424	2432	rBV	8737488	12654811	92.85%	9.864%
20	19.268	2746	2751	2755	rBV	110675	171936	1.26%	0.134%
21	19.633	2806	2813	2819	rBV	9828248	13629264	100.00%	10.623%
22	21.415	3111	3116	3121	rBV	5288119	6731111	49.39%	5.247%
23	23.574	3477	3483	3494	rVB2	6698283	12462271	91.44%	9.714%
24	23.715	3502	3507	3520	rVB	3149368	6344334	46.55%	4.945%


Sum of corrected areas: 128294868

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102717\
Data File : BM012499.D
Acq On : 27 Oct 2017 23:31
Operator : SJ/JU
Sample : I6127-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC6

Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

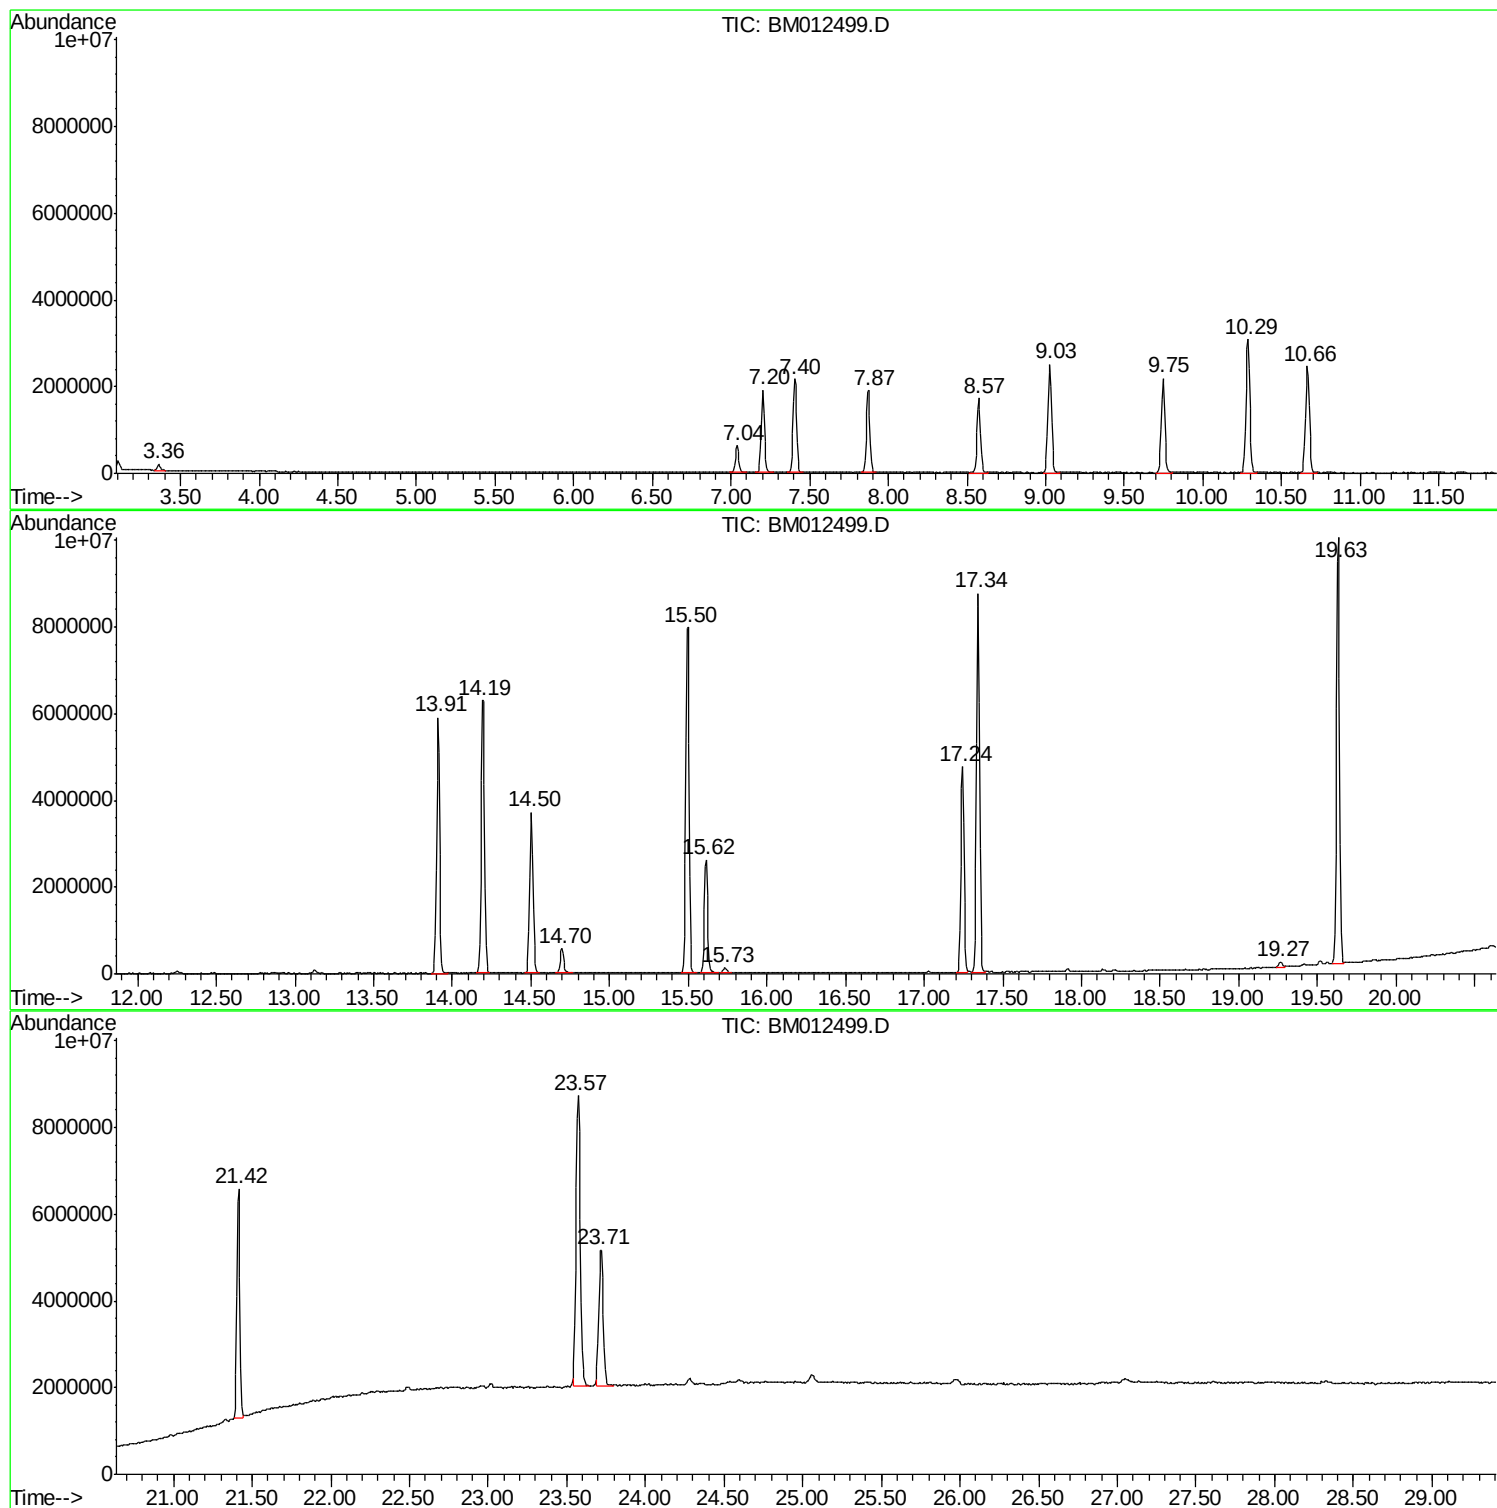

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102717\
Data File : BM012499.D
Acq On : 27 Oct 2017 23:31
Operator : SJ/JU
Sample : I6127-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102717\
Data File : BM012499.D
Acq On : 27 Oct 2017 23:31
Operator : SJ/JU
Sample : I6127-04
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
BDEC6

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc