

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
 Data File : BM032766.D
 Acq On : 27 Oct 2021 18:26
 Operator : CG/JU
 Sample : M4304-08
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P067-TW001-01

Quant Time: Oct 28 05:09:02 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 27 15:49:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.536	152	2407	0.400	ng/ul	0.00
4) Naphthalene-d8	10.317	136	9026	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.187	164	5804	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.922	188	12372	0.400	ng/ul	0.00
17) Chrysene-d12	21.104	240	10495	0.400	ng/ul	0.00
23) Perylene-d12	23.227	264	11775	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.906	96	12696	4.047	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.913	152	4376	0.350	ng/ul	0.00
18) Fluoranthene-d10	18.950	212	14669	0.510	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.963	178	2403	0.058	ng/ul#	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
Data File : BM032766.D
Acq On : 27 Oct 2021 18:26
Operator : CG/JU
Sample : M4304-08
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P067-TW001-01


Quant Time: Oct 28 05:09:02 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 27 15:49:57 2021
Response via : Initial Calibration

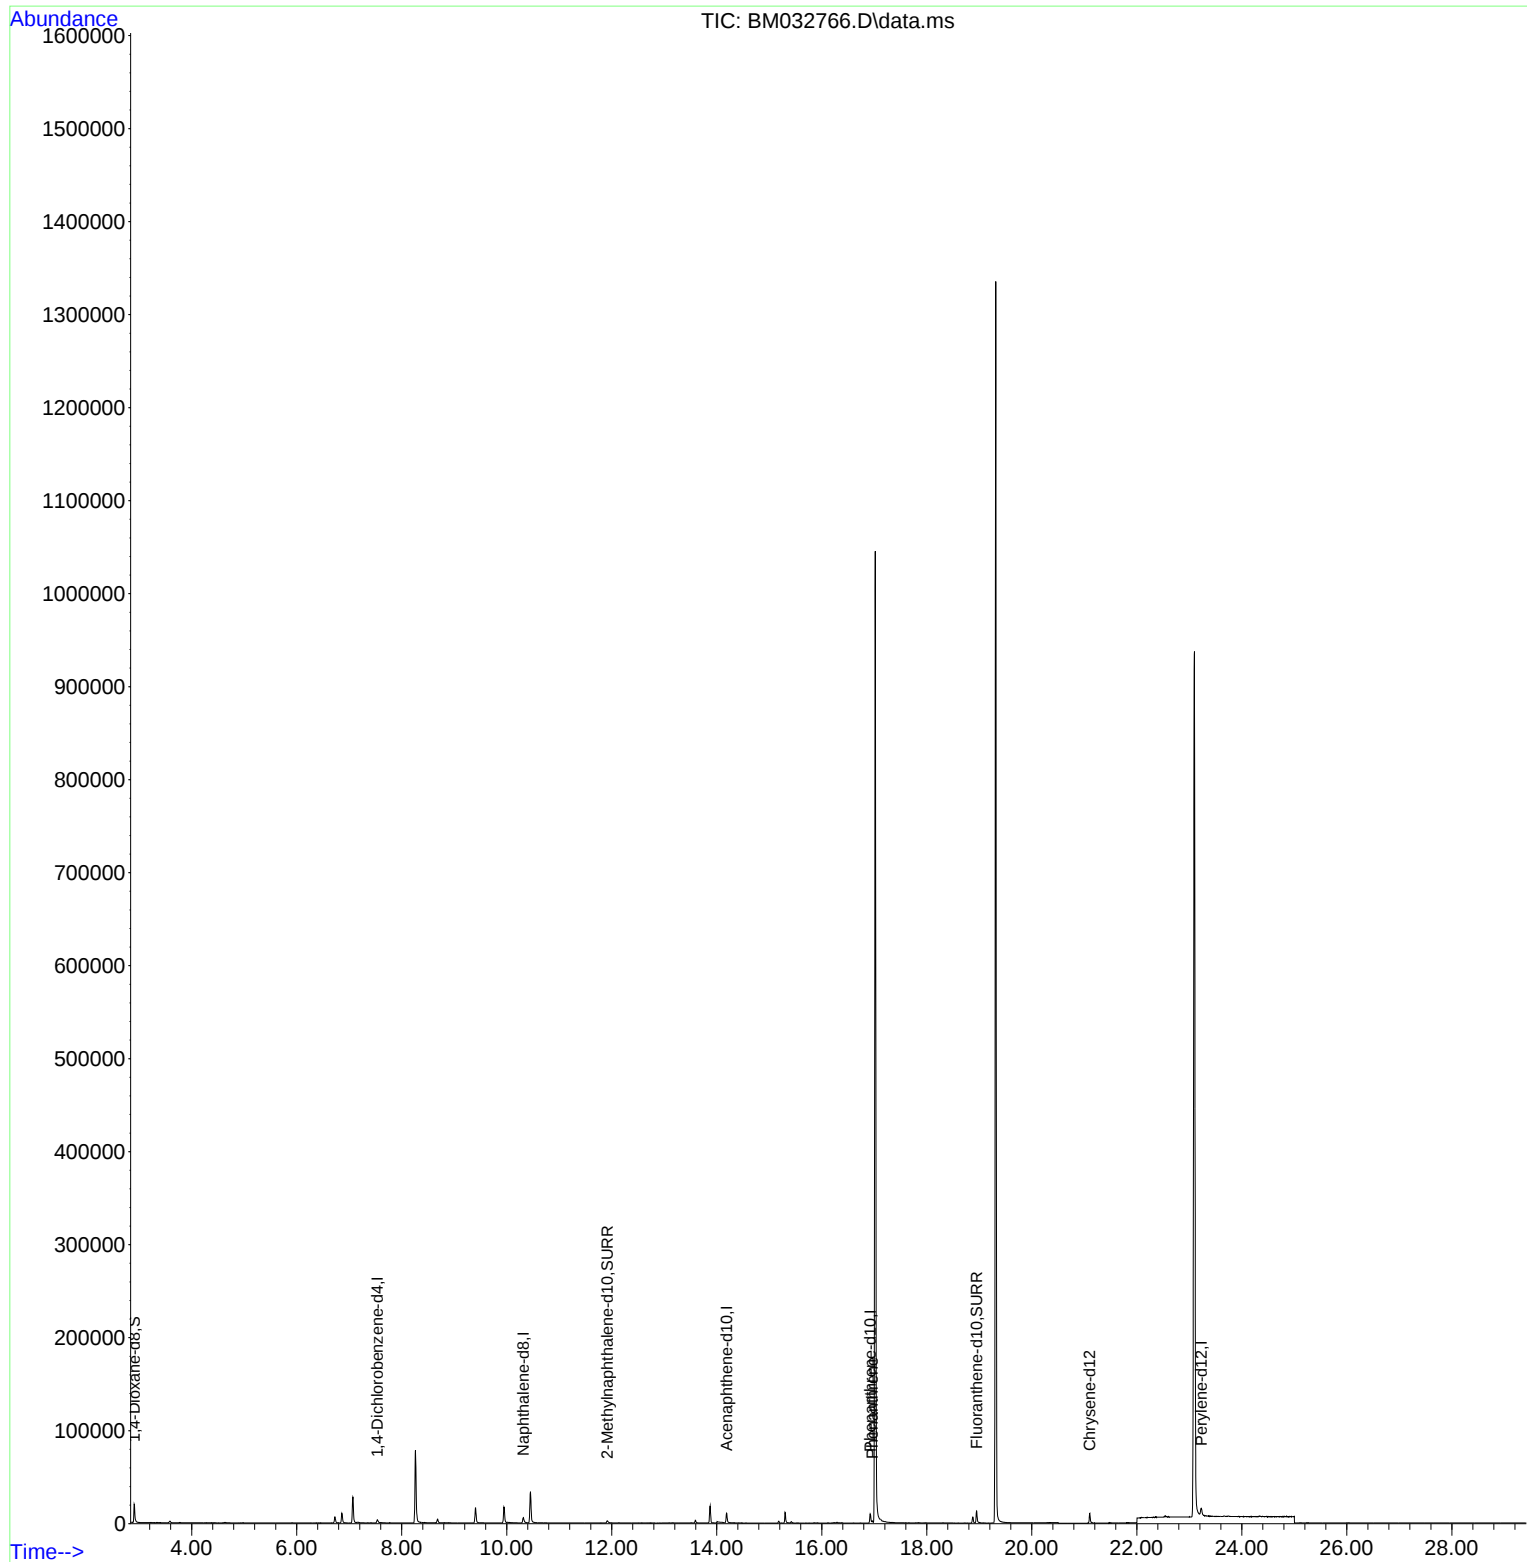

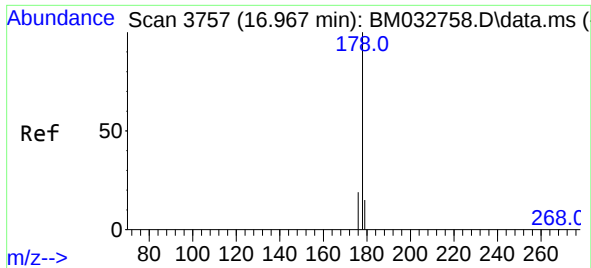

#15
Phenanthrene
Concen: 0.058 ng/ul
RT: 16.963 min Scan# 3756
Delta R.T. -0.004 min
Lab File: BM032766.D
Acq: 27 Oct 2021 18:26

Instrument :
BNA_M
ClientSampleId :
P067-TW001-01

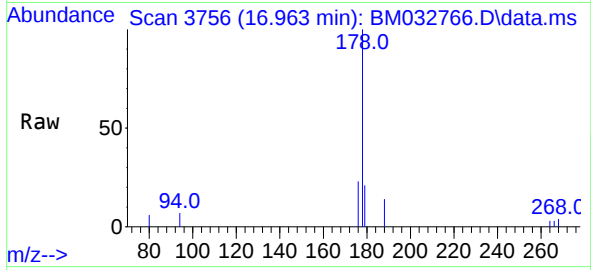

Tgt Ion:178	Resp:	2403
Ion	Ratio	Lower Upper
178	100	
179	20.6	12.6 18.8#
176	23.0	16.0 24.0

