

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
 Data File : BM032778.D
 Acq On : 28 Oct 2021 02:17
 Operator : CG/JU
 Sample : M4319-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P024-TW001-02

Quant Time: Oct 28 05:10:47 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 27 15:49:57 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.532	152	3831	0.400	ng/ul	0.00
4) Naphthalene-d8	10.312	136	14868	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.183	164	9276	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.918	188	20139	0.400	ng/ul	0.00
17) Chrysene-d12	21.096	240	17511	0.400	ng/ul	0.00
23) Perylene-d12	23.218	264	18667	0.400	ng/ul	#-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.906	96	22462	4.499	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.909	152	6789	0.330	ng/ul	0.00
18) Fluoranthene-d10	18.943	212	23545	0.490	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.960	178	1752	0.026	ng/ul#	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
Data File : BM032778.D
Acq On : 28 Oct 2021 02:17
Operator : CG/JU
Sample : M4319-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P024-TW001-02


Quant Time: Oct 28 05:10:47 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 27 15:49:57 2021
Response via : Initial Calibration

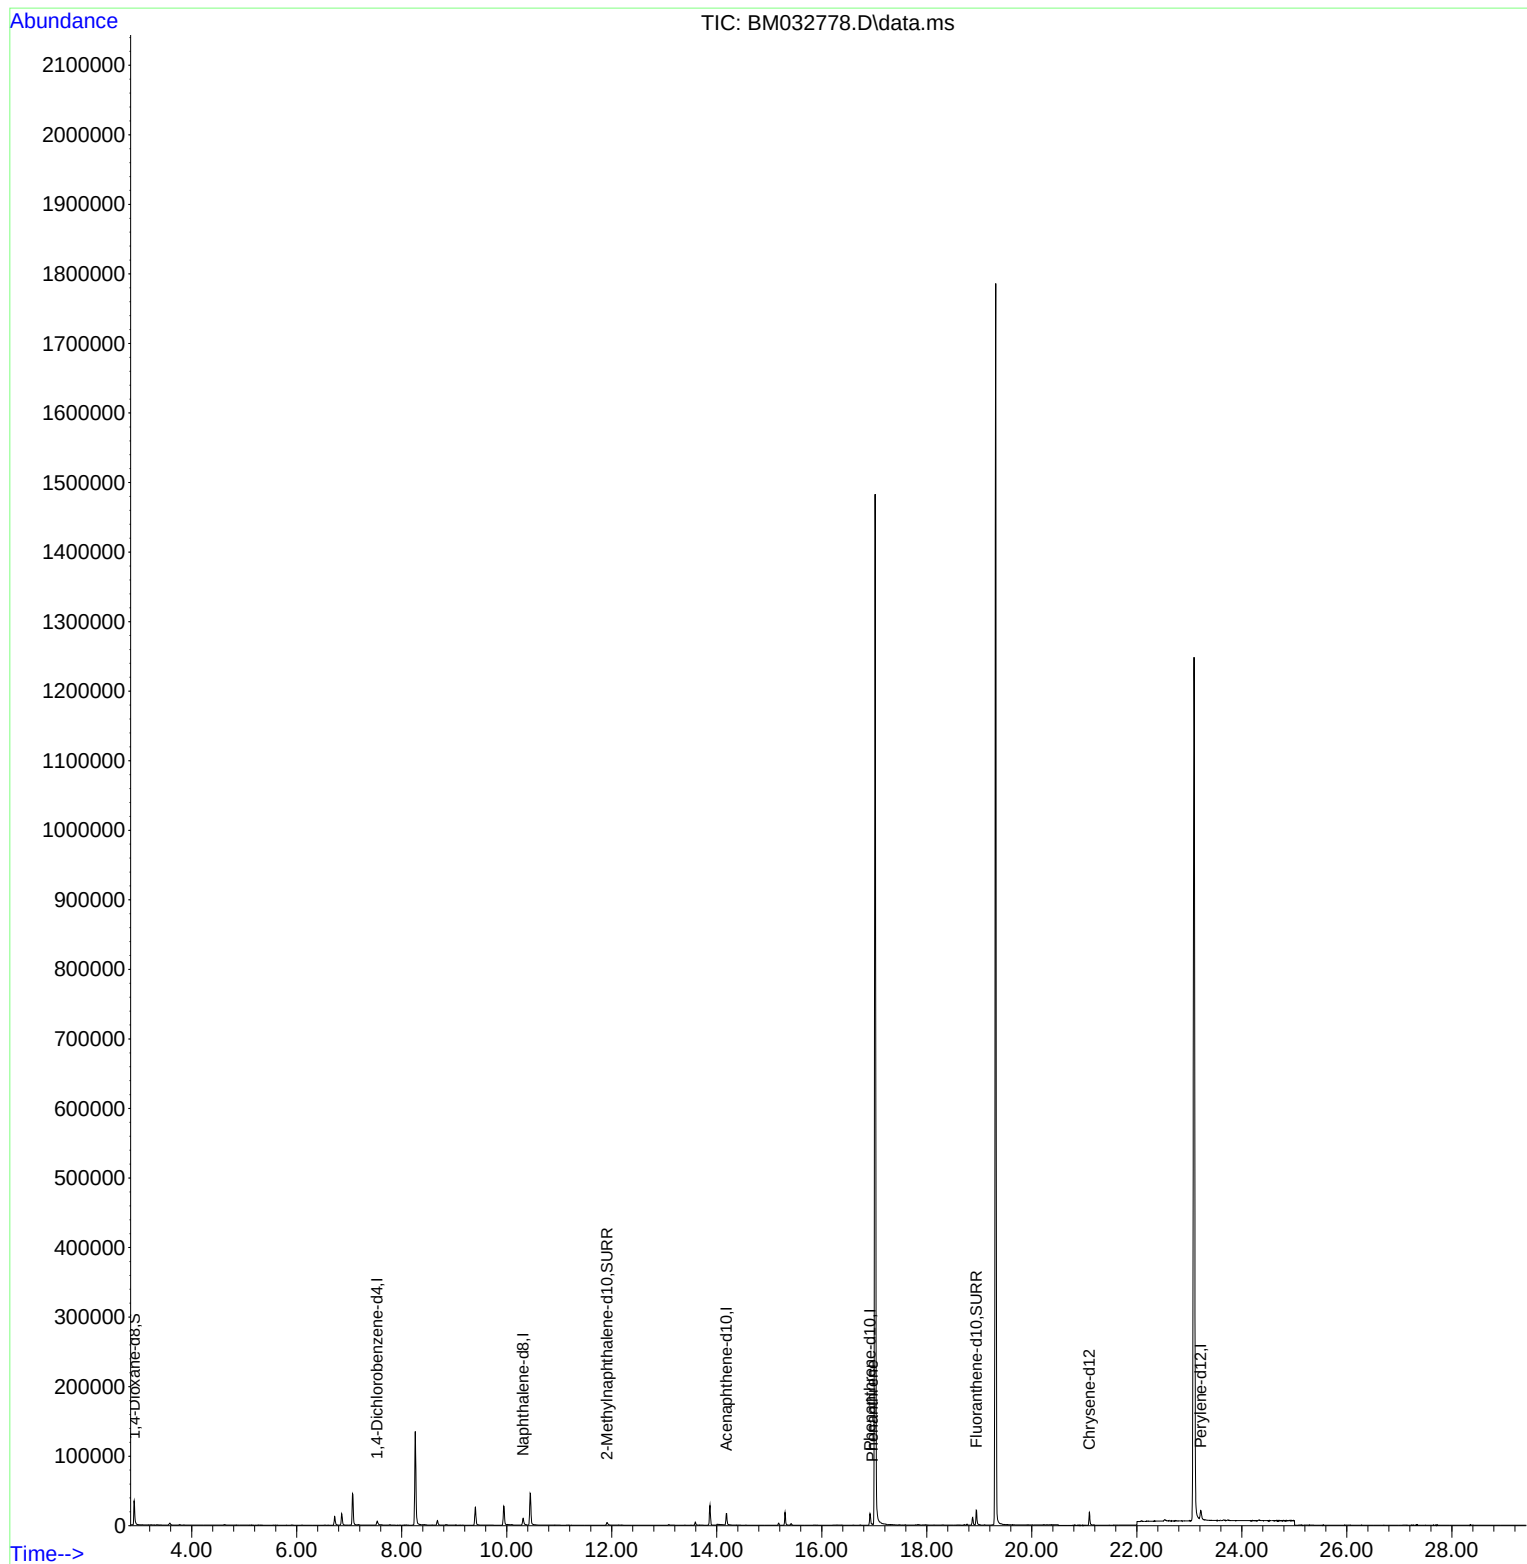

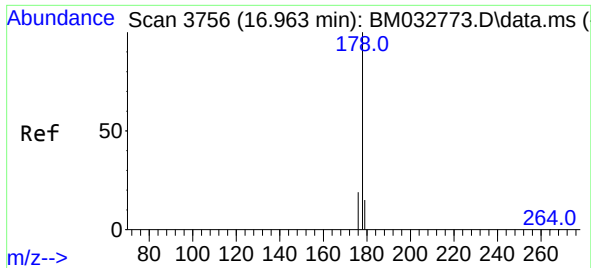

#15
Phenanthrene
Concen: 0.026 ng/ul
RT: 16.960 min Scan# 3755
Delta R.T. -0.007 min
Lab File: BM032778.D
Acq: 28 Oct 2021 02:17

Instrument :
BNA_M
ClientSampleId :
P024-TW001-02

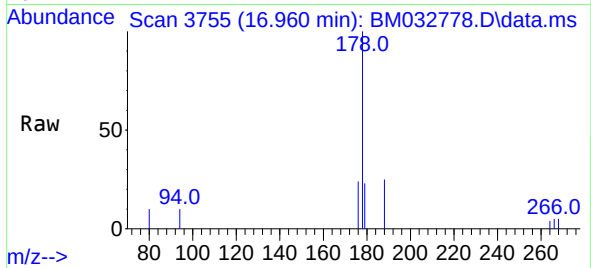

Tgt Ion:178 Resp: 1752
Ion Ratio Lower Upper
178 100
179 22.6 12.6 18.8#
176 23.7 16.0 24.0

