

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
 Data File : BM032803.D
 Acq On : 28 Oct 2021 17:56
 Operator : CG/JU
 Sample : M4319-08
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 P051-TW001-01

Quant Time: Oct 28 18:26:34 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 11:26:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.529	152	2478	0.400	ng/ul	0.00
4) Naphthalene-d8	10.308	136	9543	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.179	164	6107	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	16.915	188	13011	0.400	ng/ul	0.00
17) Chrysene-d12	21.096	240	11037	0.400	ng/ul	0.00
23) Perylene-d12	23.218	264	11387	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.903	96	11570	3.583	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.904	152	4033	0.305	ng/ul	0.00
18) Fluoranthene-d10	18.943	212	13354	0.441	ng/ul	0.00
Target Compounds						
15) Phenanthrene	16.956	178	1456	0.034	ng/ul#	Qvalue 87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
Data File : BM032803.D
Acq On : 28 Oct 2021 17:56
Operator : CG/JU
Sample : M4319-08
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
P051-TW001-01


Quant Time: Oct 28 18:26:34 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 11:26:23 2021
Response via : Initial Calibration

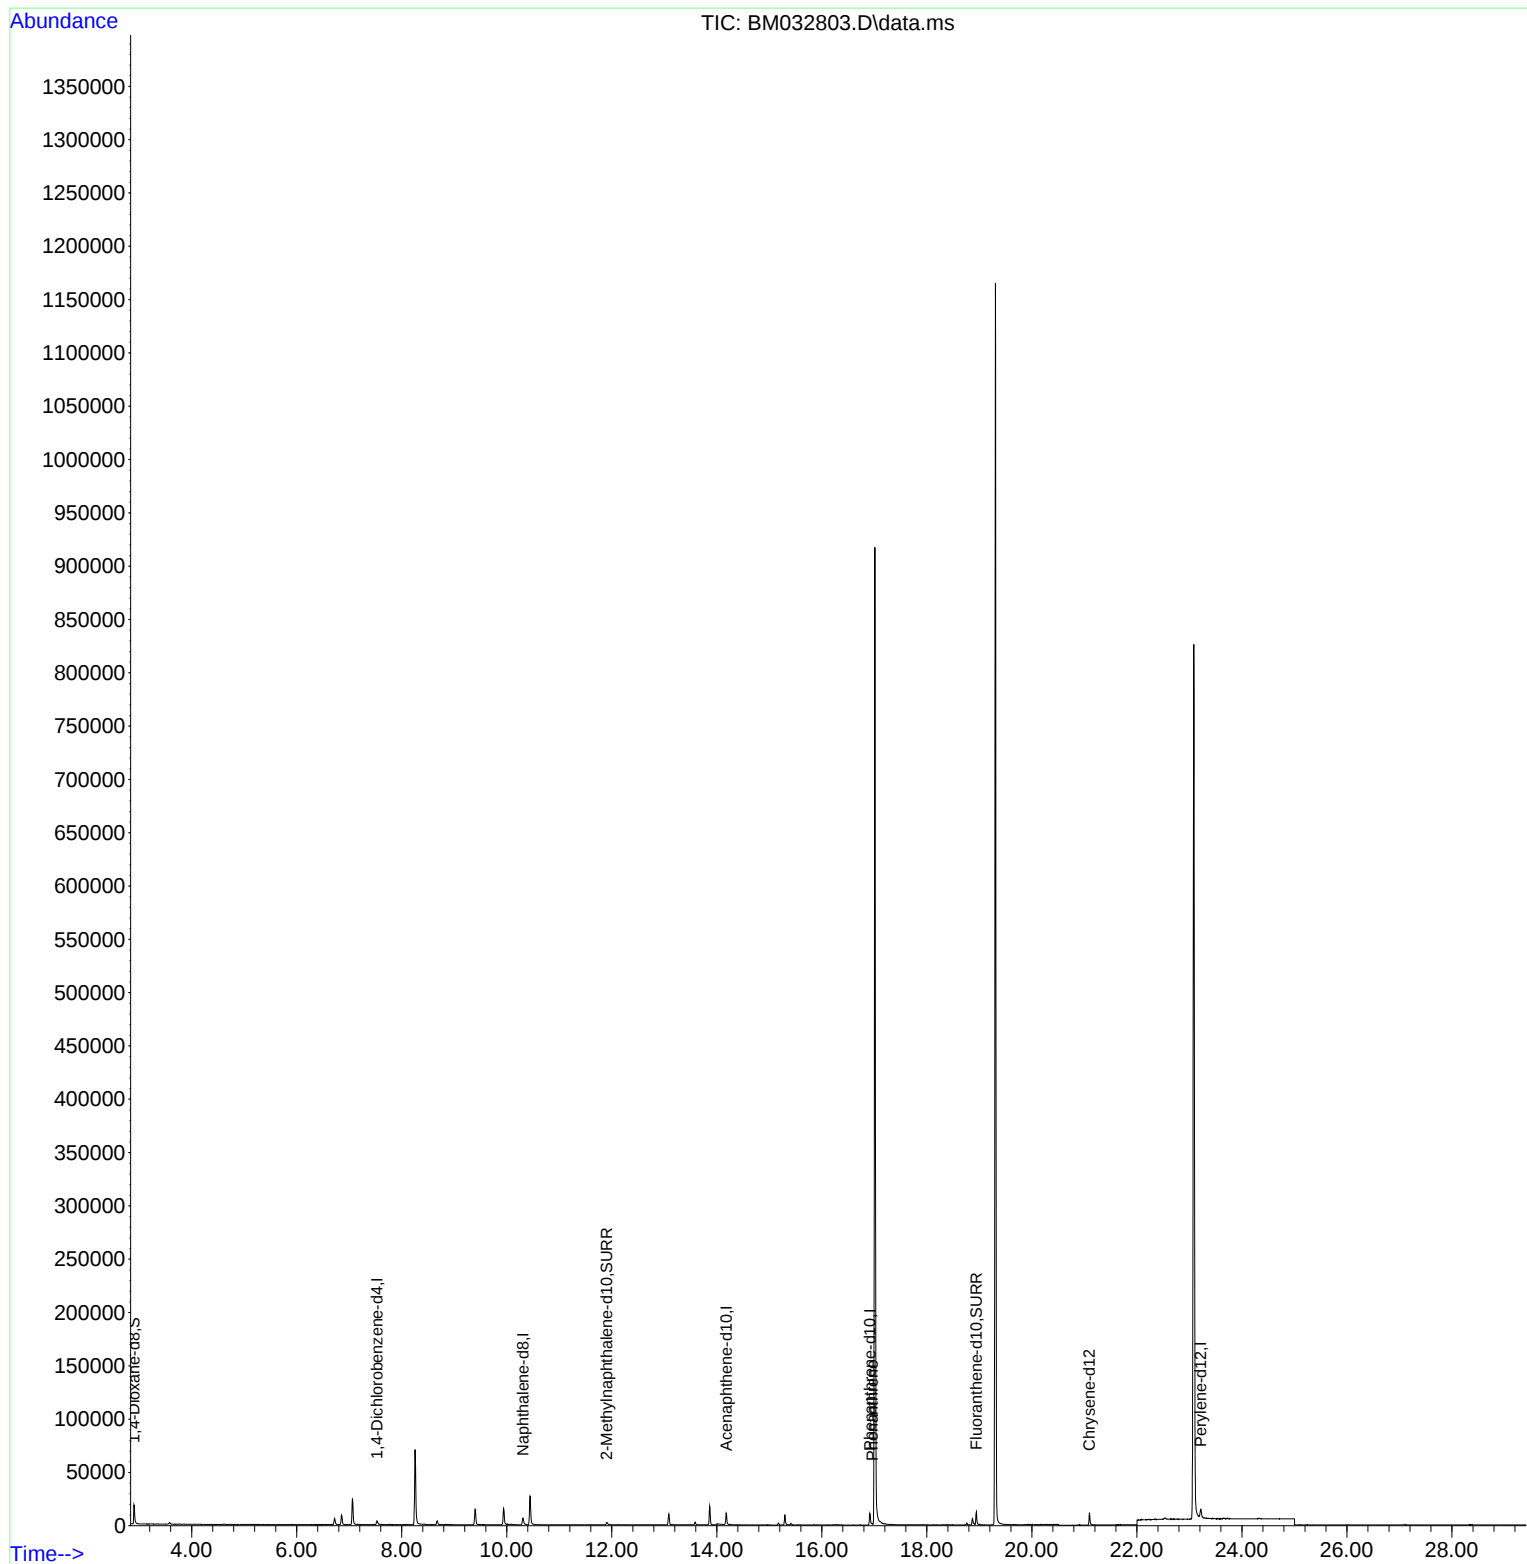

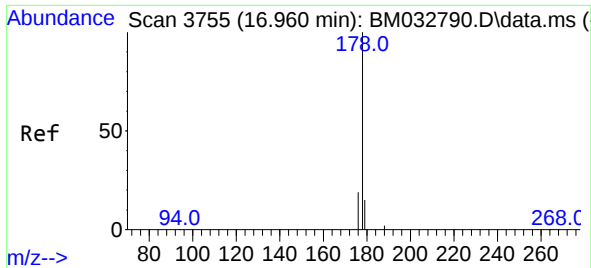

#15
 Phenanthrene
 Concen: 0.034 ng/ul
 RT: 16.956 min Scan# 3754
 Delta R.T. -0.003 min
 Lab File: BM032803.D
 Acq: 28 Oct 2021 17:56

Instrument :
 BNA_M
 ClientSampleId :
 P051-TW001-01

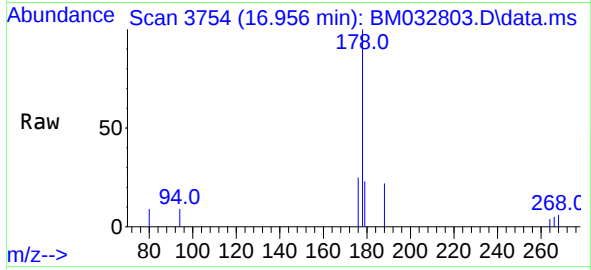

Tgt Ion:	178	Resp:	1456
Ion	Ratio	Lower	Upper
178	100		
179	22.6	12.6	18.8#
176	24.6	16.0	24.0#

