

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
 Data File : BM032815.D
 Acq On : 29 Oct 2021 01:45
 Operator : CG/JU
 Sample : M4215-10
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 JDGC9

Quant Time: Oct 29 02:25:04 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Oct 28 11:26:23 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.529	152	2272	0.400	ng/ul	0.00
4) Naphthalene-d8	10.307	136	9234	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.179	164	6178	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.915	188	13557	0.400	ng/ul	0.00
17) Chrysene-d12	21.089	240	12279	0.400	ng/ul	0.00
23) Perylene-d12	23.208	264	12558	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.906	96	1714	0.579	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.904	152	2904	0.227	ng/ul	0.00
18) Fluoranthene-d10	18.939	212	8129	0.241	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.357	128	962	0.035	ng/ul#	72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102721\
Data File : BM032815.D
Acq On : 29 Oct 2021 01:45
Operator : CG/JU
Sample : M4215-10
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
JDGC9


Quant Time: Oct 29 02:25:04 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM102721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 28 11:26:23 2021
Response via : Initial Calibration

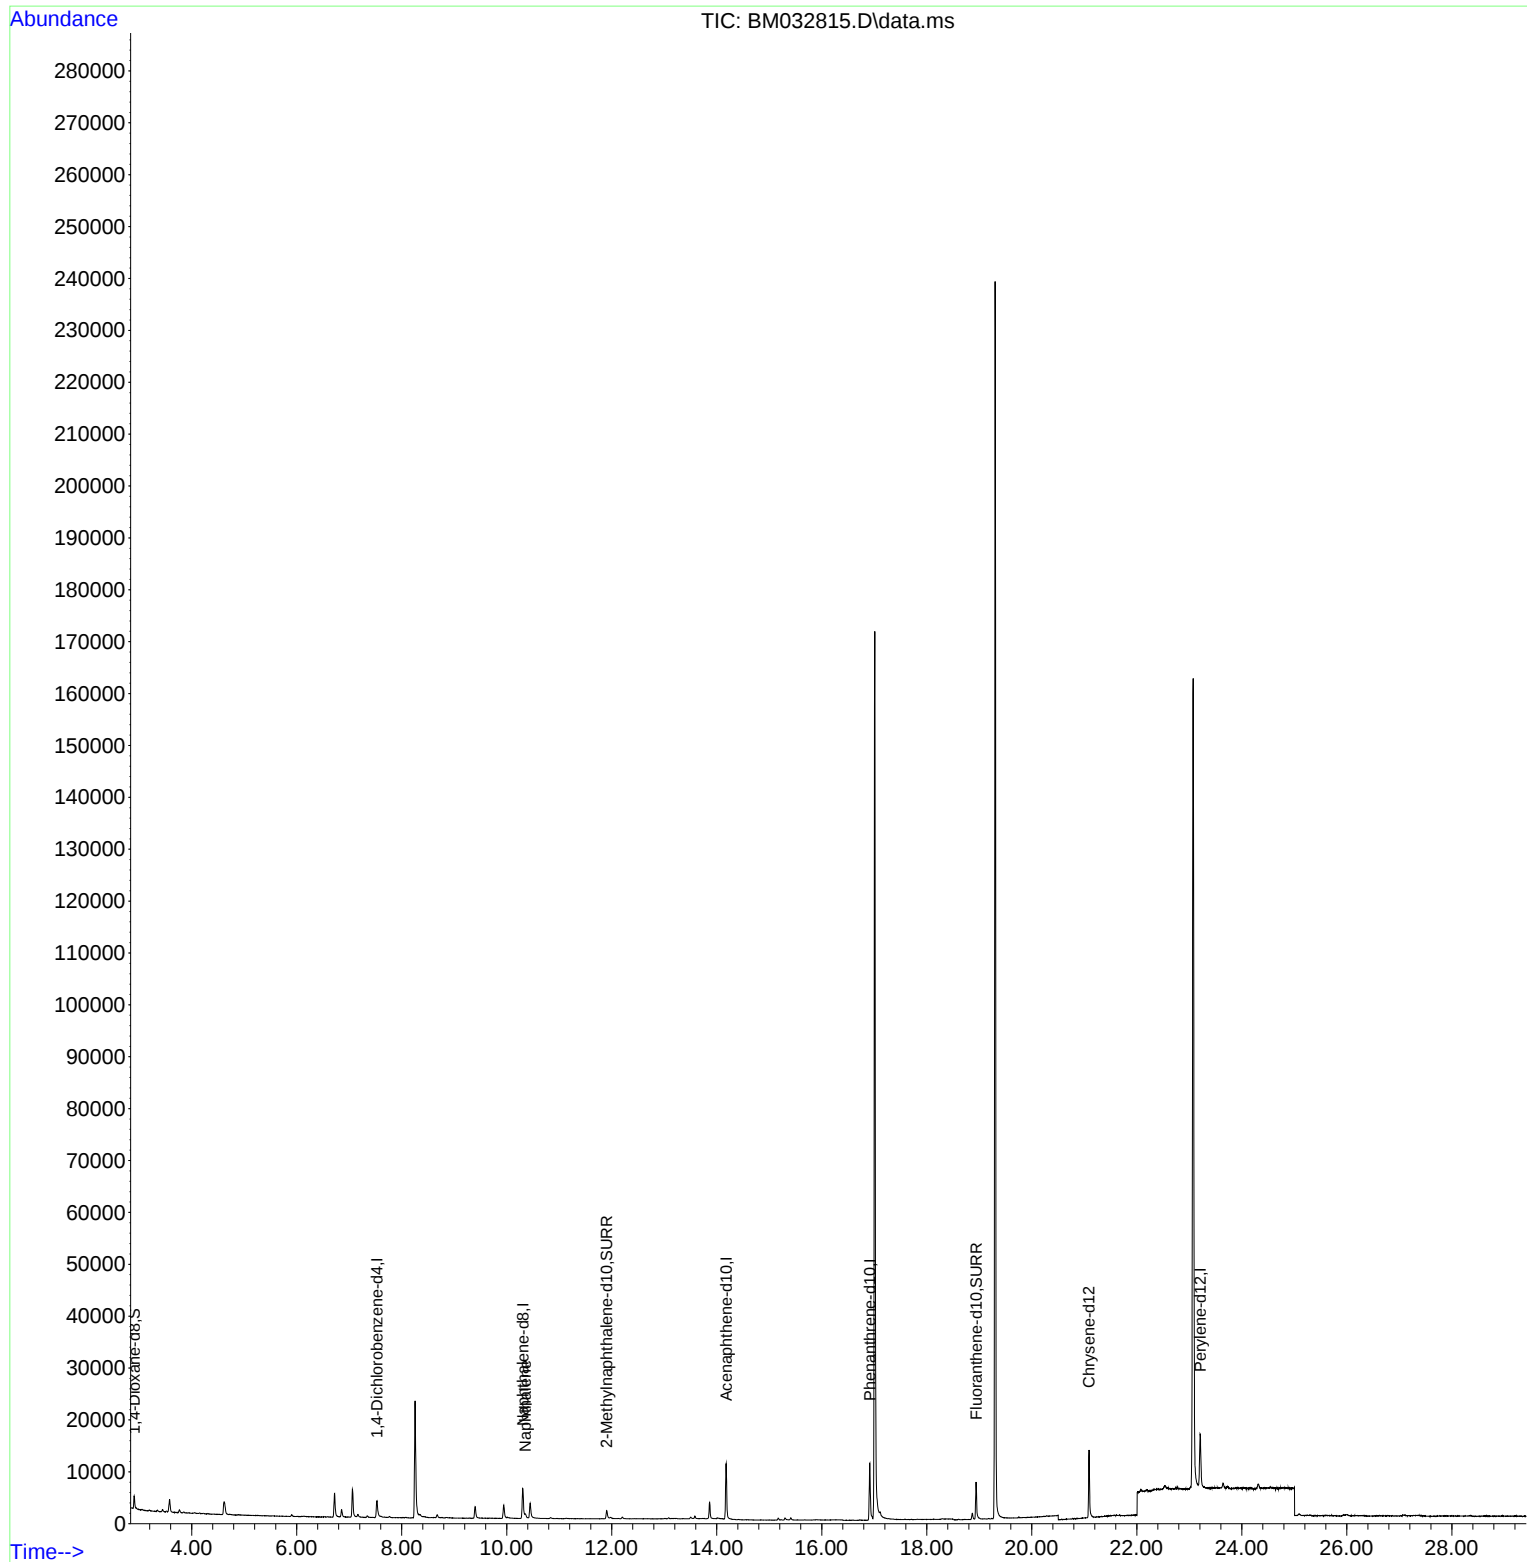

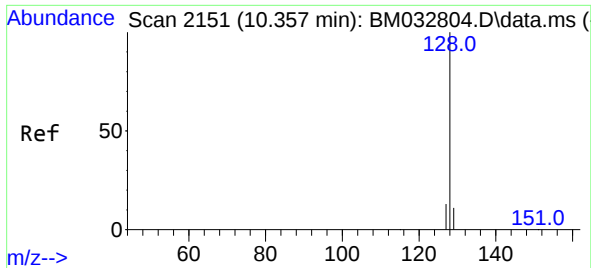

#5
Naphthalene
Concen: 0.035 ng/ul
RT: 10.357 min Scan# 2151
Delta R.T. -0.000 min
Lab File: BM032815.D
Acq: 29 Oct 2021 01:45

Instrument :
BNA_M
ClientSampleId :
JDGC9

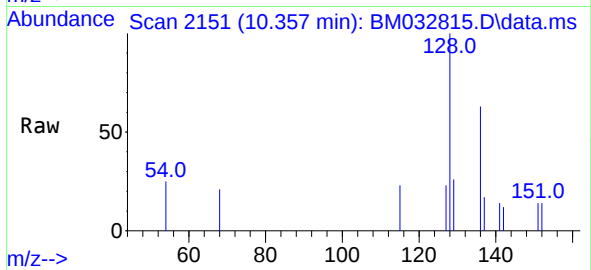

Tgt Ion:128 Resp: 962
Ion Ratio Lower Upper
128 100
129 25.9 9.6 14.4#
127 22.6 11.0 16.6#

