

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102816\
 Data File : BM007747.D
 Acq On : 28 Oct 2016 18:11
 Operator : UM/SJ
 Sample : PB94366BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK66

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.293	116	120	126	rBV	46235	69987	1.40%	0.145%
2	6.934	732	739	754	rBV	808262	1355547	27.10%	2.810%
3	7.093	760	766	779	rBV	656135	1019421	20.38%	2.113%
4	7.287	792	799	816	rVB	852590	1454138	29.07%	3.014%
5	7.751	871	878	888	rBV	686408	1107320	22.14%	2.295%
6	8.457	991	998	1015	rBV	1033599	1736768	34.72%	3.600%
7	8.910	1067	1075	1083	rBV	781171	1332817	26.64%	2.763%
8	9.628	1189	1197	1211	rBV	648495	1123349	22.46%	2.329%
9	10.163	1281	1288	1301	rBV	975534	1744622	34.88%	3.616%
10	10.534	1344	1351	1362	rVB	883976	1472589	29.44%	3.053%
11	10.675	1368	1375	1393	rBV	916095	1696529	33.91%	3.517%
12	13.798	1900	1906	1917	rBV	1723294	2472770	49.43%	5.126%
13	14.080	1946	1954	1965	rBV	1954023	2914823	58.27%	6.042%
14	14.386	2000	2006	2013	rBV	1286372	1901566	38.01%	3.942%
15	14.604	2038	2043	2063	rBV	522426	1071897	21.43%	2.222%
16	15.380	2169	2175	2183	rVB	2490545	3583733	71.64%	7.429%
17	15.521	2193	2199	2212	rBV	418851	667809	13.35%	1.384%
18	17.133	2467	2473	2481	rBV	1558769	2213808	44.26%	4.589%
19	17.233	2483	2490	2502	rVV2	2796660	3982431	79.61%	8.255%
20	17.404	2515	2519	2530	rBV4	29725	84250	1.68%	0.175%
21	19.533	2875	2881	2888	rBV	3228366	4632001	92.60%	9.602%
22	21.321	3180	3185	3192	rBV	2151581	2800680	55.99%	5.806%
23	23.433	3538	3544	3556	rVB2	2529250	5002330	100.00%	10.369%
24	23.574	3563	3568	3576	rVB2	1470002	2799625	55.97%	5.803%


Sum of corrected areas: 48240810

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102816\
Data File : BM007747.D
Acq On : 28 Oct 2016 18:11
Operator : UM/SJ
Sample : PB94366BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

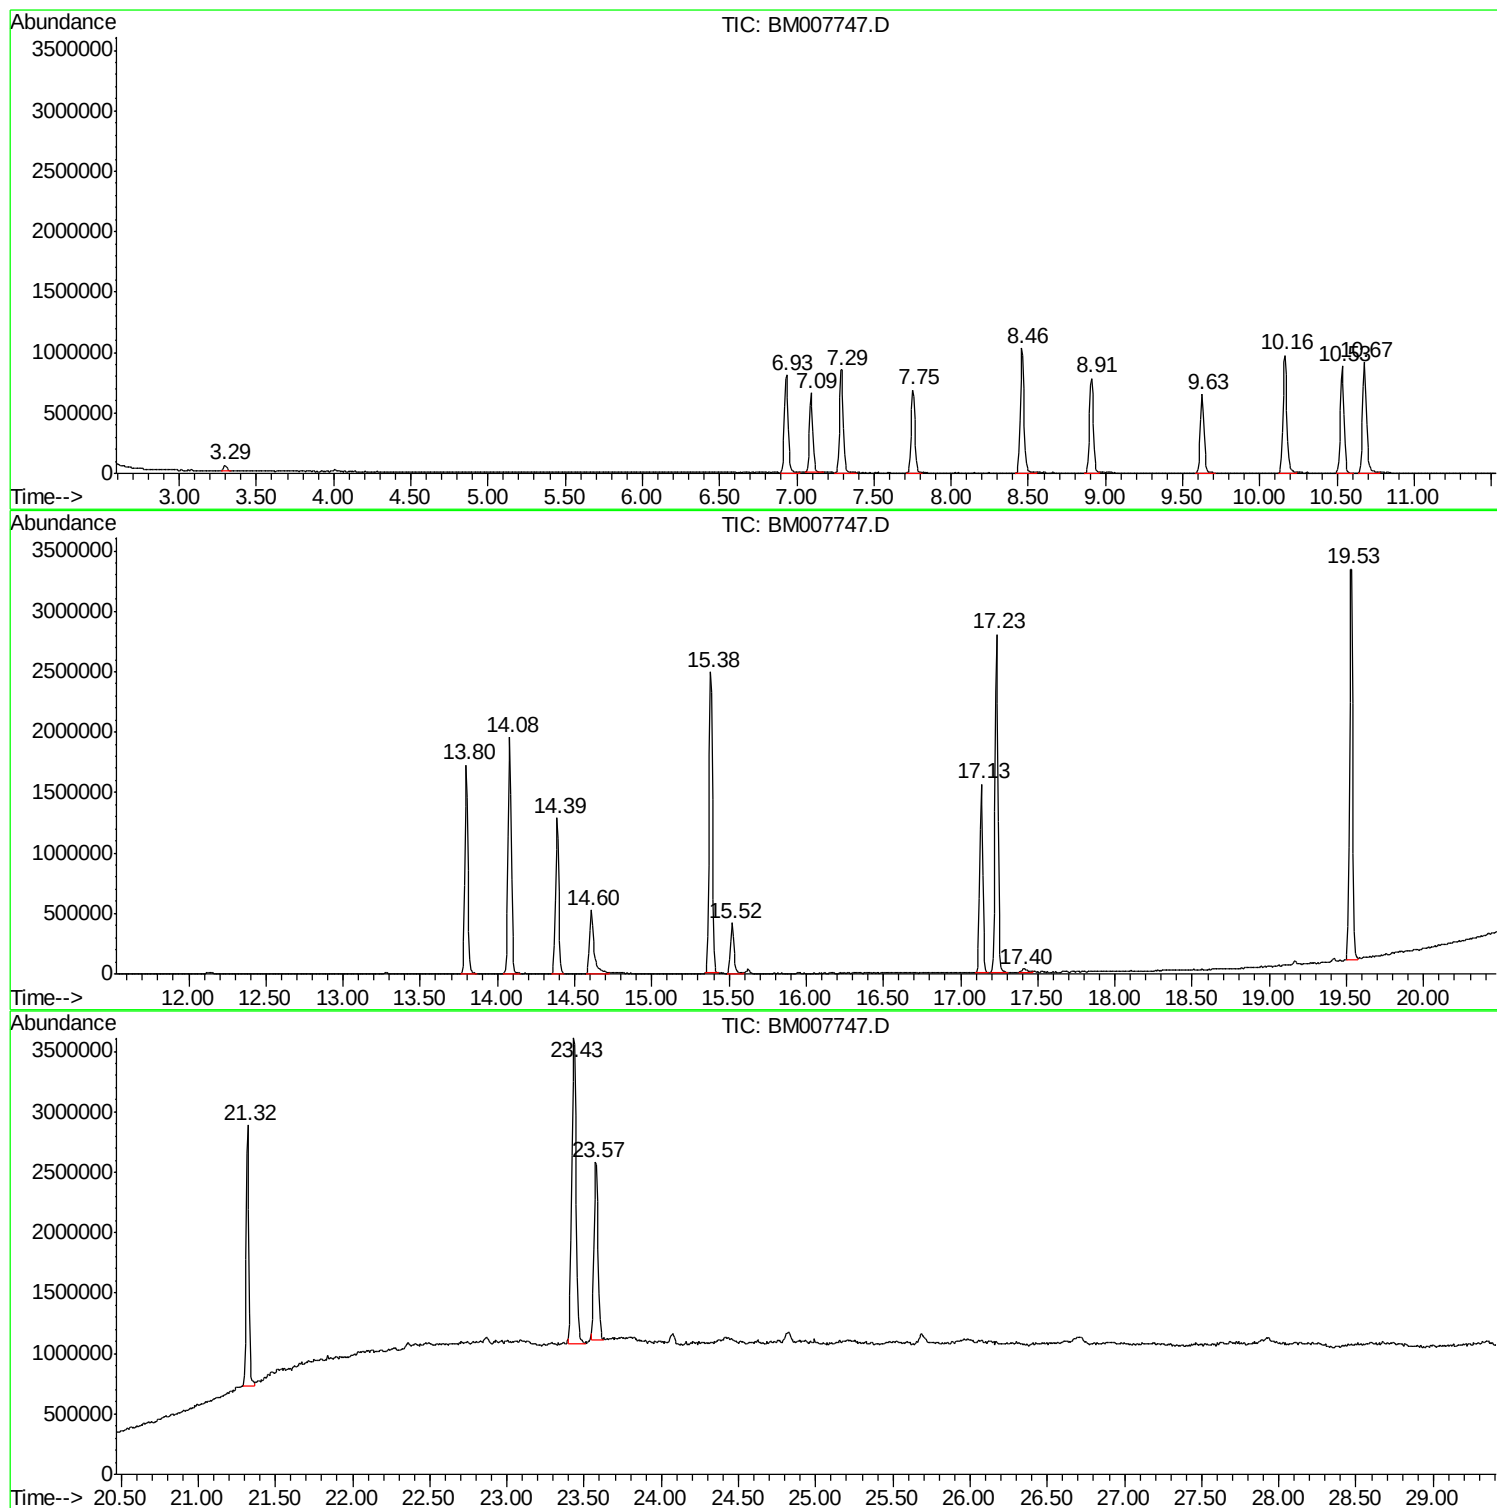

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102816\
Data File : BM007747.D
Acq On : 28 Oct 2016 18:11
Operator : UM/SJ
Sample : PB94366BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM102816\
Data File : BM007747.D
Acq On : 28 Oct 2016 18:11
Operator : UM/SJ
Sample : PB94366BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK66

Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM102016.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc