

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102817\
 Data File : BM012534.D
 Acq On : 28 Oct 2017 20:55
 Operator : SJ/JU
 Sample : I5119-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Oct 30 08:31:26 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 30 08:26:05 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	440625	20.00	ng/ul	0.00
18) Naphthalene-d8	10.66	136	1747181	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.50	164	1059501	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	2464262	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	2150619	20.00	ng/ul	0.00
83) Perylene-d12	23.71	264	2011975	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	49842	5.78	ng/uL	0.00
5) Phenol-d5	7.03	99	1085703	29.49	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	667401	30.54	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	864691	31.36	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	929448	29.54	ng/ul	-0.01
19) Nitrobenzene-d5	9.02	128	428996	39.21	ng/ul	0.00
22) 2-Nitrophenol-d4	9.75	143	473058	41.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.28	165	933691	31.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	1031036	32.74	ng/ul	0.00
43) Dimethylphthalate-d6	13.91	166	3109909	33.60	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	3738158	34.14	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	532178	38.68	ng/ul	0.00
57) Fluorene-d10	15.49	176	2692943	34.37	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	377614	31.66	ng/ul	-0.01
70) Anthracene-d10	17.34	188	4495375	38.28	ng/ul	0.00
76) Pyrene-d10	19.63	212	4732031	47.96	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	3713548	38.85	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.06	94	96483	2.52	ng/ul#	85
44) Dimethylphthalate	13.95	163	346017	3.78	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102817\
Data File : BM012534.D
Acq On : 28 Oct 2017 20:55
Operator : SJ/JU
Sample : I5119-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Oct 30 08:31:26 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 30 08:26:05 2017
Response via : Initial Calibration

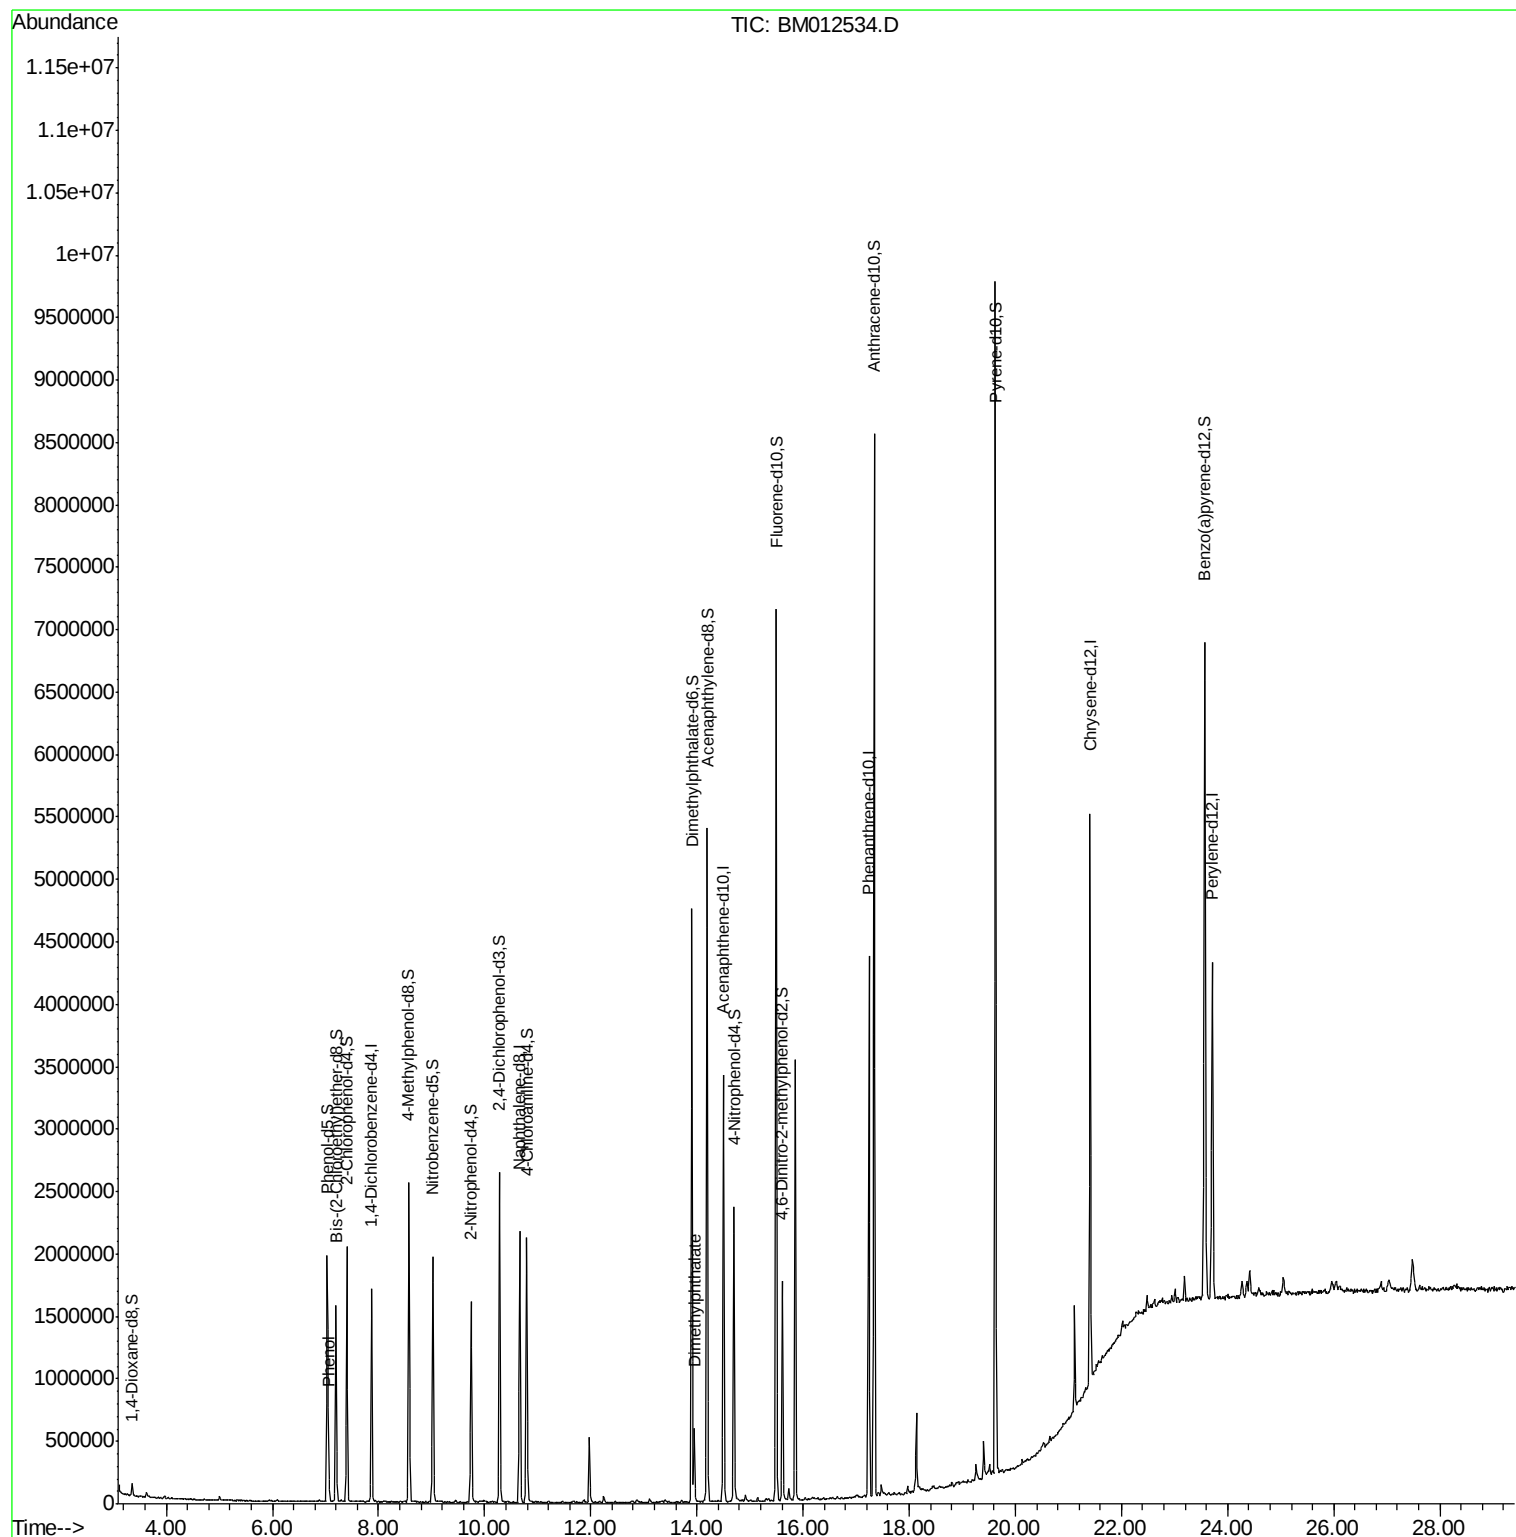

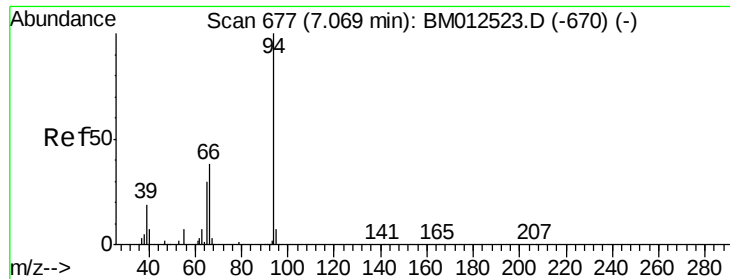

#6

Phenol

Concen: 2.52 ng/ul

RT: 7.06 min Scan# 676

Delta R.T. -0.01 min

Lab File: BM012534.D

Acq: 28 Oct 2017 20:55

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 96483

Ion Ratio Lower Upper

94 100

65 32.6 28.2 42.4




66 43.3 47.2 70.8#

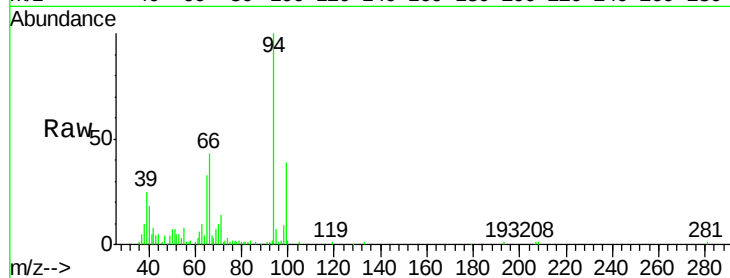

Abundance Ion 94.00 (93.70 to 94.70): BM012523.D (-670) (-)

Ion 65.00 (64.70 to 65.70): BM012523.D (-670) (-)

Ion 66.00 (65.70 to 66.70): BM012523.D (-670) (-)

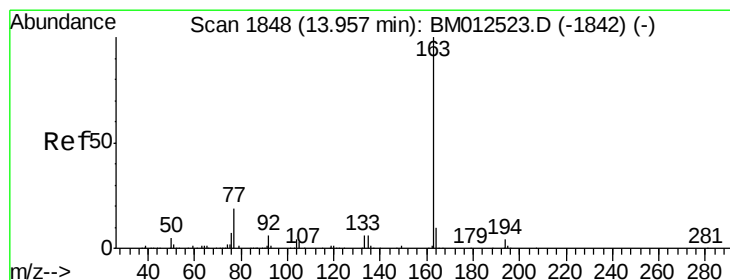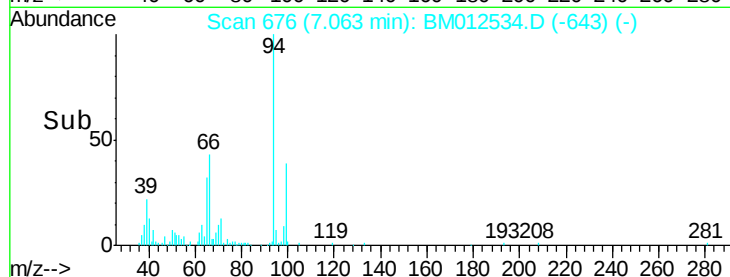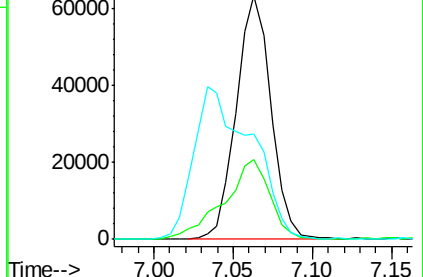

#44

Dimethylphthalate

Concen: 3.78 ng/ul

RT: 13.95 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BM012534.D

Acq: 28 Oct 2017 20:55


Tgt Ion: 163 Resp: 346017

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.2 8.2 12.4

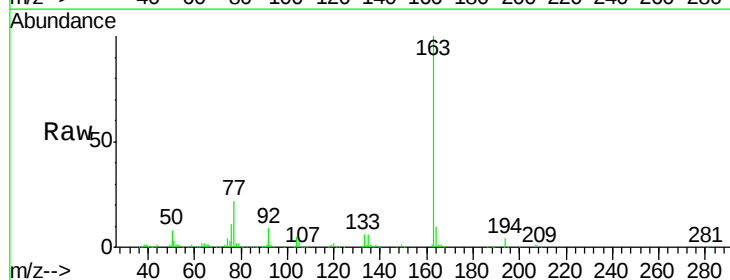

Abundance Ion 163.00 (162.70 to 163.70): BM012523.D (-1842) (-)

Ion 194.00 (193.70 to 194.70): BM012523.D (-1842) (-)

Ion 164.00 (163.70 to 164.70): BM012523.D (-1842) (-)

