

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102817\
 Data File : BM012557.D
 Acq On : 29 Oct 2017 10:48
 Operator : SJ/JU
 Sample : I5887-13
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 B0DE7

Quant Time: Oct 30 16:51:45 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 30 16:46:58 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.86	152	571115	20.00	ng/ul	0.00
18) Naphthalene-d8	10.66	136	2120416	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.50	164	1199542	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.24	188	2674369	20.00	ng/ul	0.00
75) Chrysene-d12	21.41	240	3085379	20.00	ng/ul	0.00
83) Perylene-d12	23.72	264	3502243	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.36	96	26463	2.37	ng/uL	0.00
5) Phenol-d5	7.03	99	639008	13.39	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.19	67	361746	12.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	508869	14.24	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	328255	8.05	ng/ul	0.00
19) Nitrobenzene-d5	9.02	128	227723	17.15	ng/ul	0.00
22) 2-Nitrophenol-d4	9.74	143	249450	18.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.28	165	533415	14.72	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	540158	14.14	ng/ul	0.00
43) Dimethylphthalate-d6	13.90	166	1625050	15.51	ng/ul	0.00
46) Acenaphthylene-d8	14.19	160	2119164	17.10	ng/ul	0.00
51) 4-Nitrophenol-d4	14.69	143	357118	22.92	ng/ul	0.00
57) Fluorene-d10	15.49	176	1768843	19.94	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.61	200	263821	20.38	ng/ul	0.00
70) Anthracene-d10	17.33	188	3350313	26.29	ng/ul	0.00
76) Pyrene-d10	19.63	212	4211053	29.75	ng/ul	0.00
87) Benzo(a)pyrene-d12	23.57	264	4971611	29.88	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
6) Phenol	7.06	94	70757	1.424	ng/ul#	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM102817\
Data File : BM012557.D
Acq On : 29 Oct 2017 10:48
Operator : SJ/JU
Sample : I5887-13
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
B0DE7

Quant Time: Oct 30 16:51:45 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM102417.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 30 16:46:58 2017
Response via : Initial Calibration

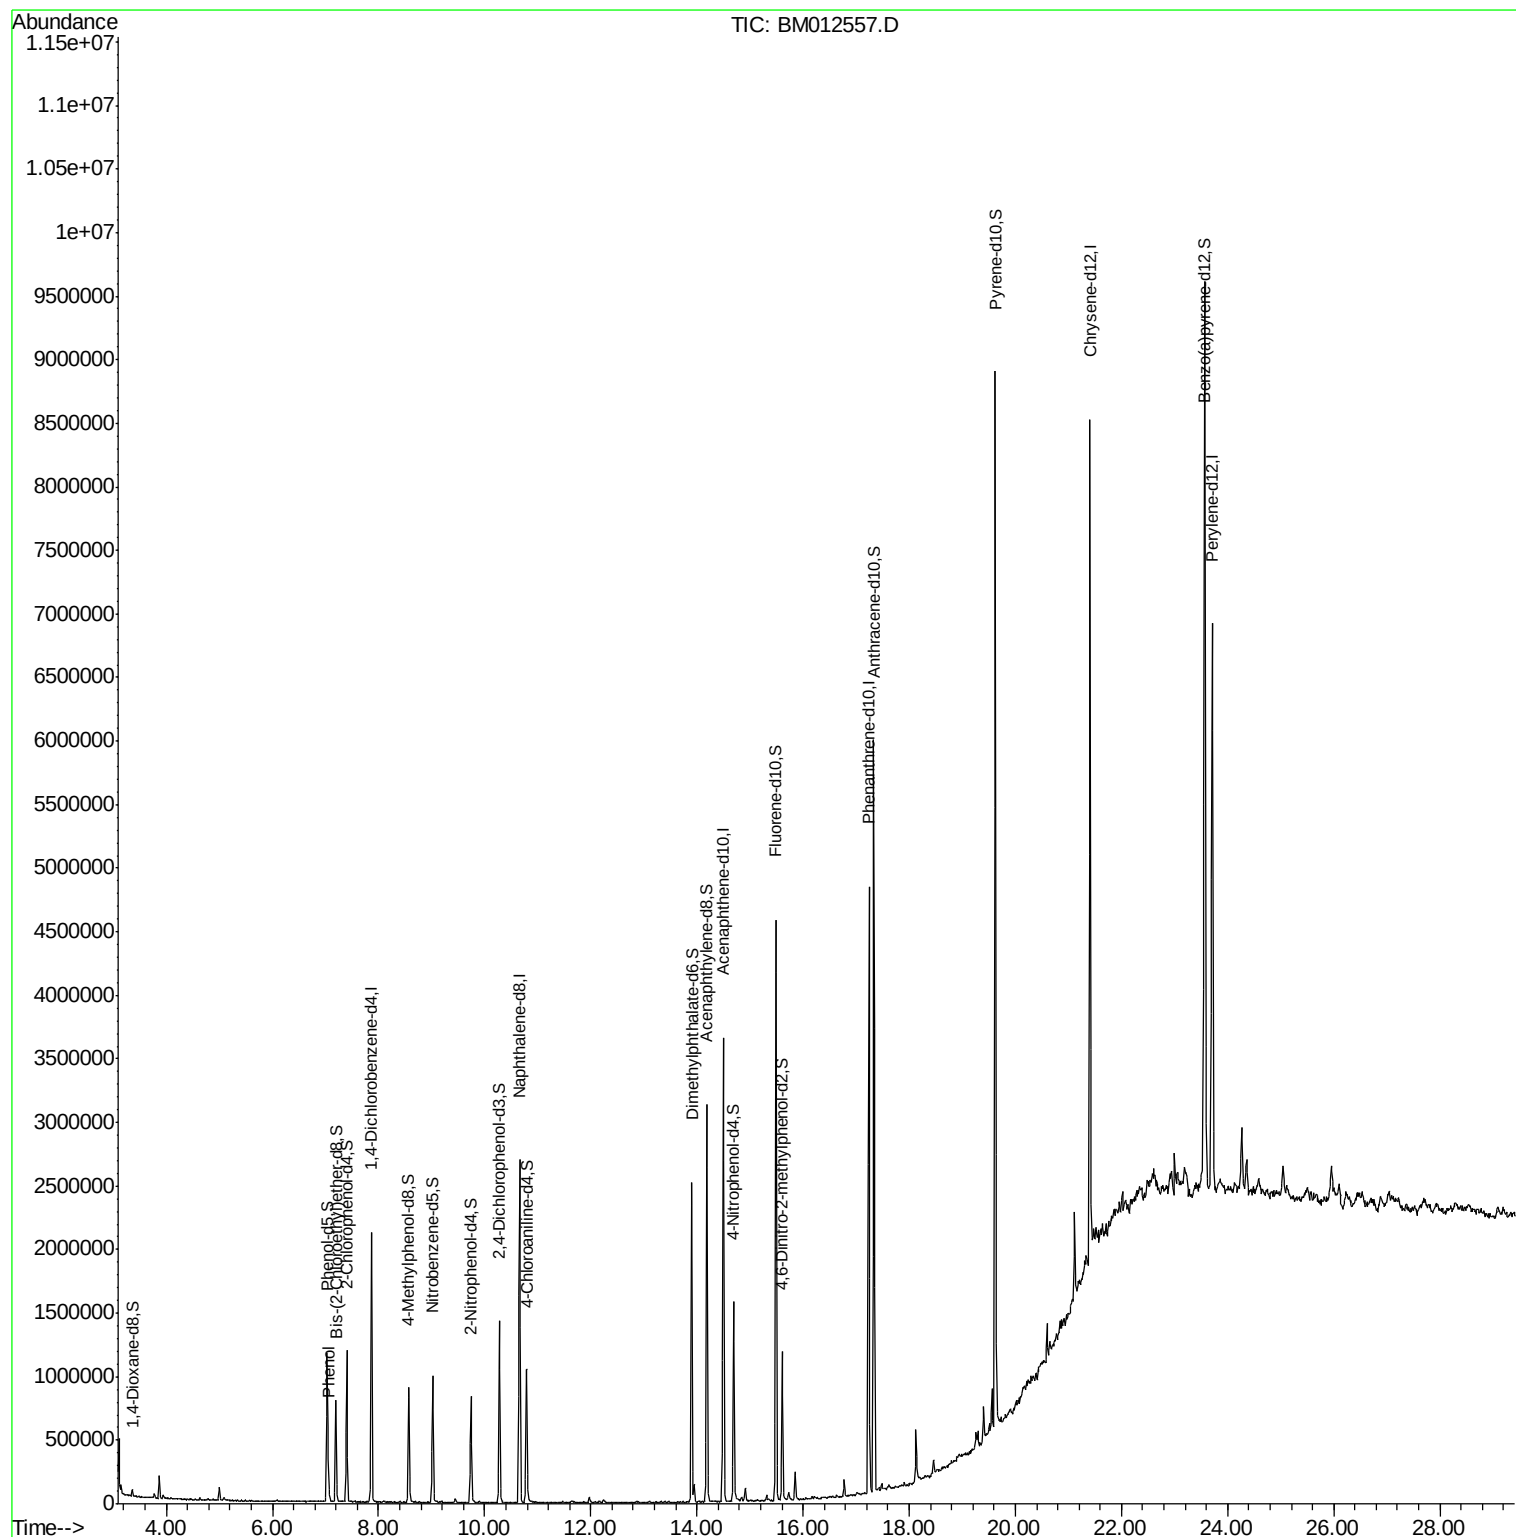

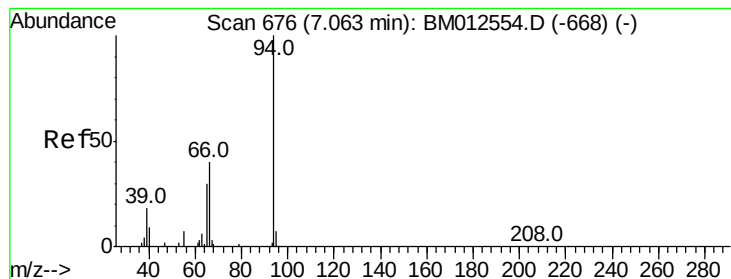


#6

Phenol

Concen: 1.424 ng/ul
 RT: 7.06 min Scan# 675
 Delta R.T. -0.01 min
 Lab File: BM012557.D
 Acq: 29 Oct 2017 10:48

Instrument :
 BNA_M
 ClientSampleId :
 B0DE7

Tot Ion: 94 Resp: 70757
 Ion Ratio Lower Upper
 94 100
 65 26.6 28.2 42.4#
 66 41.7 47.2 70.8#

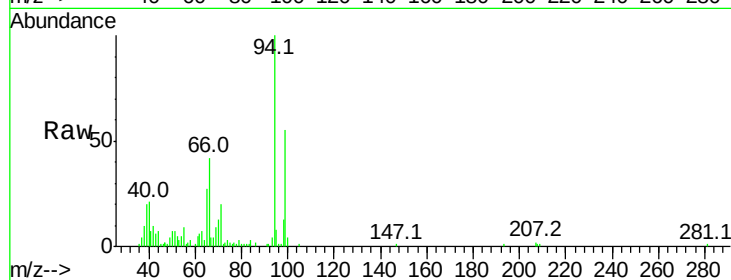

Abundance Ion 94.00 (93.70 to 94.70): BM0
 Ion 65.00 (64.70 to 65.70): BM0
 Ion 66.00 (65.70 to 66.70): BM0

