

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048282.D
 Acq On : 29 Oct 2024 10:09
 Operator : RC/JU
 Sample : P4532-18
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNZ6

Quant Time: Oct 29 11:17:33 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 27 23:39:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	177559	20.000	ng/u1	0.00
20) Naphthalene-d8	10.504	136	731463	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.357	164	444495	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.104	188	858344	20.000	ng/u1	0.00
79) Chrysene-d12	21.327	240	724576	20.000	ng/u1	0.00
88) Perylene-d12	24.274	264	811583	20.000	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	29230	6.481	ng/uL	0.00
4) Pyridine-d5	3.587	84	430719	32.948	ng/u1	0.00
7) Phenol-d5	6.893	99	520523	34.123	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.051	67	332222	35.158	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	430243	34.682	ng/u1	0.00
15) 4-Methylphenol-d8	8.428	113	416638	34.019	ng/u1	-0.01
21) Nitrobenzene-d5	8.875	128	210827	35.156	ng/u1	0.00
24) 2-Nitrophenol-d4	9.592	143	227093	34.956	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.134	165	384247	32.412	ng/u1	0.00
31) 4-Chloroaniline-d4	10.645	131	582071	35.359	ng/u1	0.00
46) Dimethylphthalate-d6	13.774	166	1240597	37.347	ng/u1	0.00
49) Acenaphthylene-d8	14.051	160	1377184	36.770	ng/u1	0.00
54) 4-Nitrophenol-d4	14.580	143	160058	26.349	ng/u1	0.00
60) Fluorene-d10	15.357	176	1055217	37.595	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.480	200	171902	30.305	ng/u1	0.00
73) Anthracene-d10	17.198	188	1646783	40.573	ng/u1	-0.01
81) Pyrene-d10	19.492	212	1779214	40.465	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	1785669	41.715	ng/u1	-0.01
Target Compounds						
2) 1,4-Dioxane	3.205	88	27136	5.692	ng/uL	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048282.D
Acq On : 29 Oct 2024 10:09
Operator : RC/JU
Sample : P4532-18
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ6


Quant Time: Oct 29 11:17:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 27 23:39:58 2024
Response via : Initial Calibration

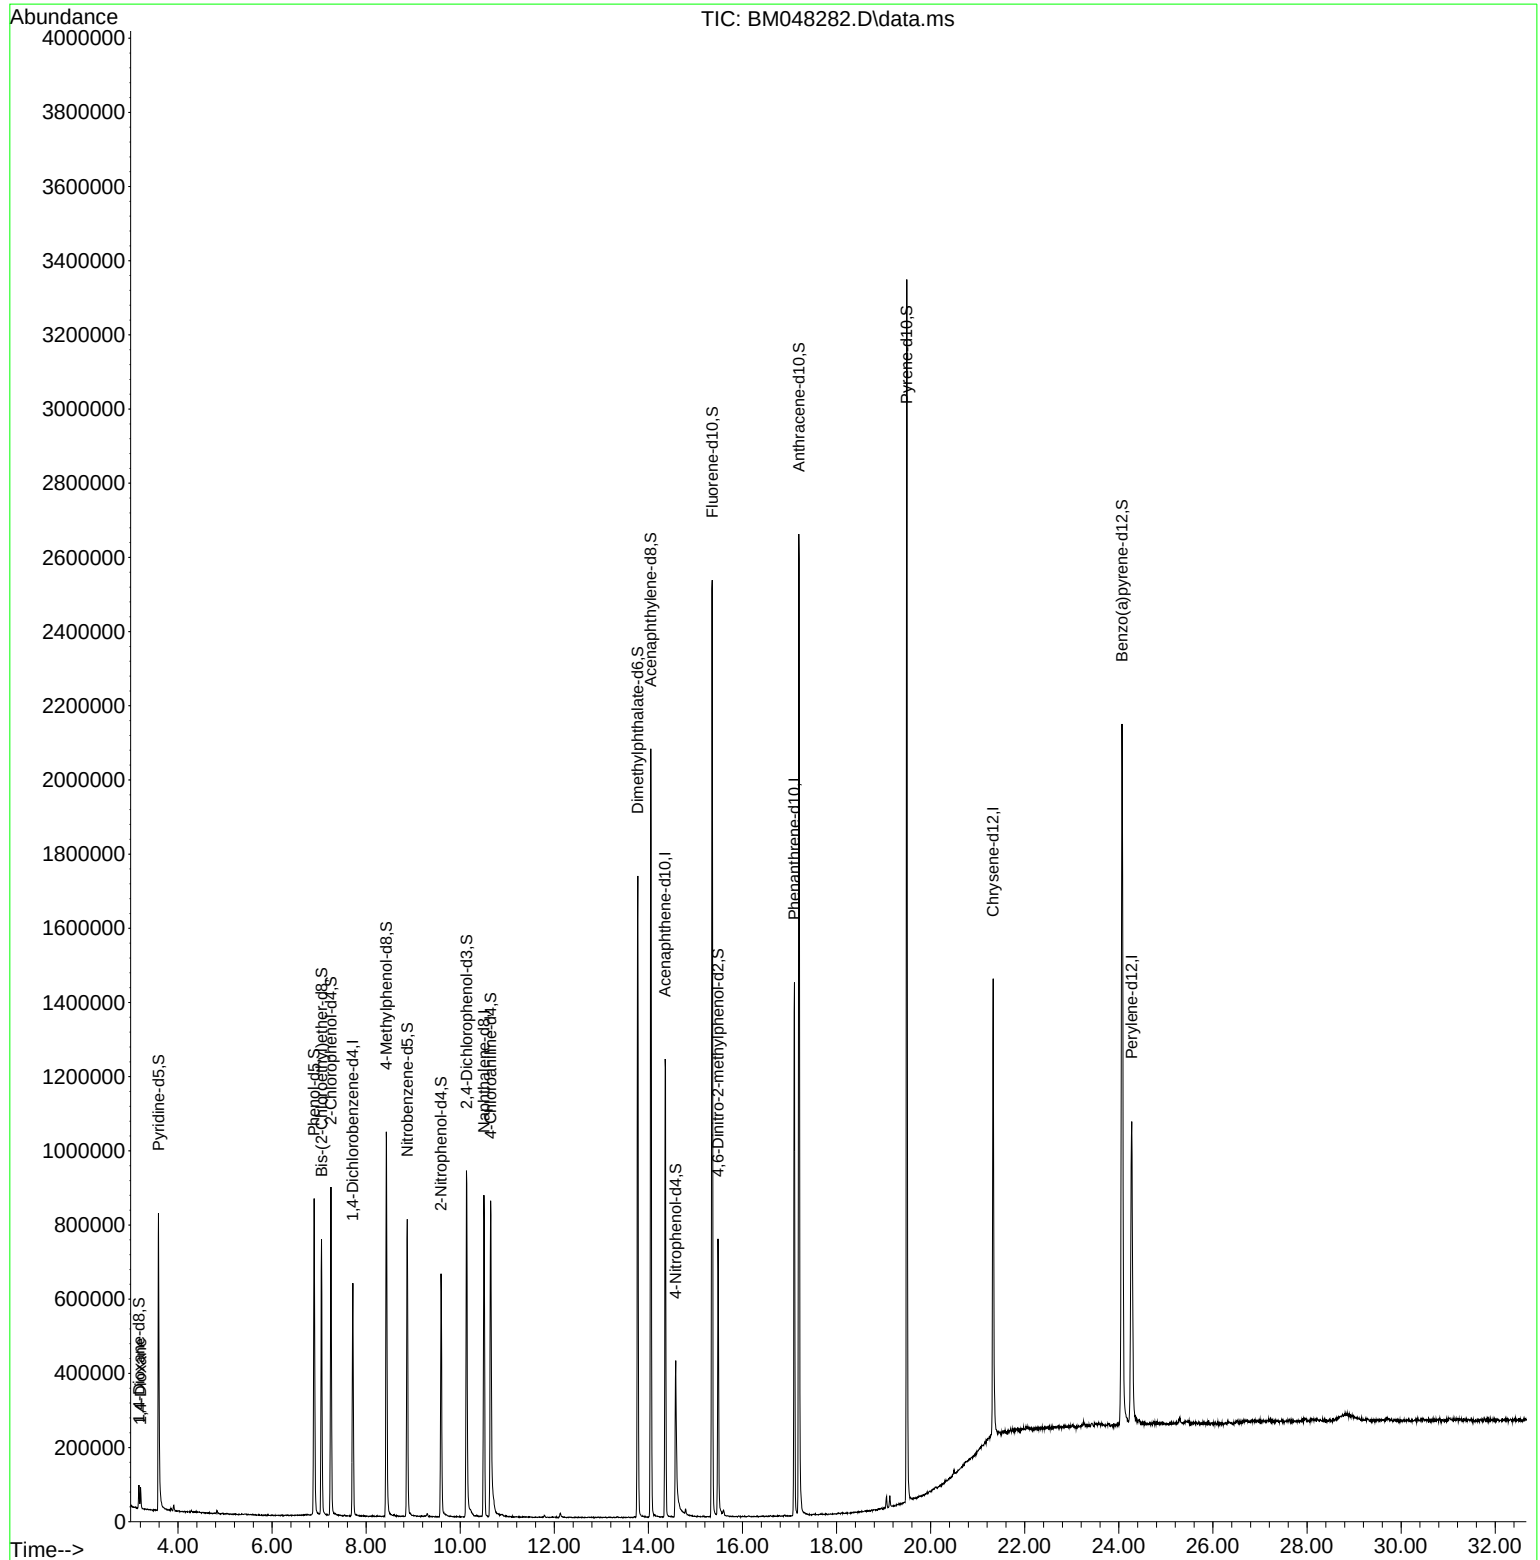

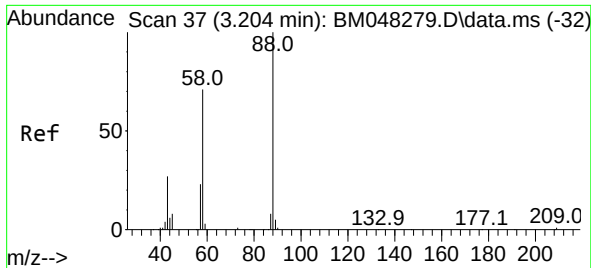

#2
1,4-Dioxane
Concen: 5.692 ng/uL
RT: 3.205 min Scan# 31
Delta R.T. 0.001 min
Lab File: BM048282.D
Acq: 29 Oct 2024 10:09

Instrument :
BNA_M
ClientSampleId :
GCNZ6

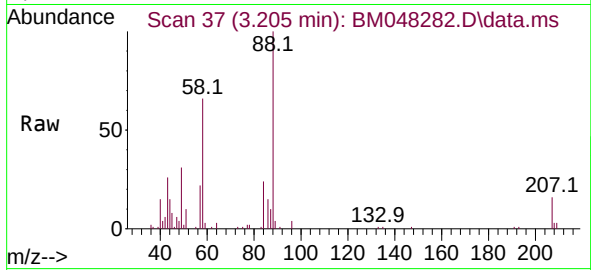

Tgt Ion:	88	Resp:	27136
Ion	Ratio	Lower	Upper
88	100		
43	26.3	22.3	33.5
58	66.4	58.7	88.1

