

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048297.D
 Acq On : 29 Oct 2024 21:20
 Operator : RC/JU
 Sample : P4529-20
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 F7H48

Quant Time: Oct 29 22:54:45 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Oct 27 23:39:58 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.716	152	218605	20.000	ng/u1	0.00
20) Naphthalene-d8	10.504	136	942570	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.357	164	598459	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.098	188	1128442	20.000	ng/u1	-0.01
79) Chrysene-d12	21.327	240	857945	20.000	ng/u1	0.00
88) Perylene-d12	24.268	264	905693	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.169	96	28545	5.141	ng/uL	0.00
4) Pyridine-d5	3.593	84	114489	7.114	ng/u1	0.00
7) Phenol-d5	6.892	99	142781	7.603	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.051	67	370520	31.849	ng/u1	0.00
11) 2-Chlorophenol-d4	7.251	132	421862	27.622	ng/u1	0.00
15) 4-Methylphenol-d8	8.428	113	290438	19.262	ng/u1	-0.01
21) Nitrobenzene-d5	8.869	128	244206	31.601	ng/u1	-0.01
24) 2-Nitrophenol-d4	9.592	143	268447	32.066	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.133	165	455914	29.844	ng/u1	0.00
31) 4-Chloroaniline-d4	10.645	131	601599	28.360	ng/u1	0.00
46) Dimethylphthalate-d6	13.768	166	1595569	35.676	ng/u1	-0.01
49) Acenaphthylene-d8	14.051	160	1688847	33.491	ng/u1	0.00
54) 4-Nitrophenol-d4	14.592	143	36947	4.517	ng/u1	0.01
60) Fluorene-d10	15.351	176	1324785	35.056	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.480	200	224288	30.076	ng/u1	0.00
73) Anthracene-d10	17.198	188	2060346	38.612	ng/u1	-0.01
81) Pyrene-d10	19.492	212	2146702	41.233	ng/u1	0.00
92) Benzo(a)pyrene-d12	24.068	264	1914901	40.085	ng/u1	-0.01
Target Compounds						
					Qvalue	
35) 4-Chloro-3-methylphenol	11.816	107	35711	2.271	ng/u1	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048297.D
Acq On : 29 Oct 2024 21:20
Operator : RC/JU
Sample : P4529-20
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
F7H48

Quant Time: Oct 29 22:54:45 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Oct 27 23:39:58 2024
Response via : Initial Calibration

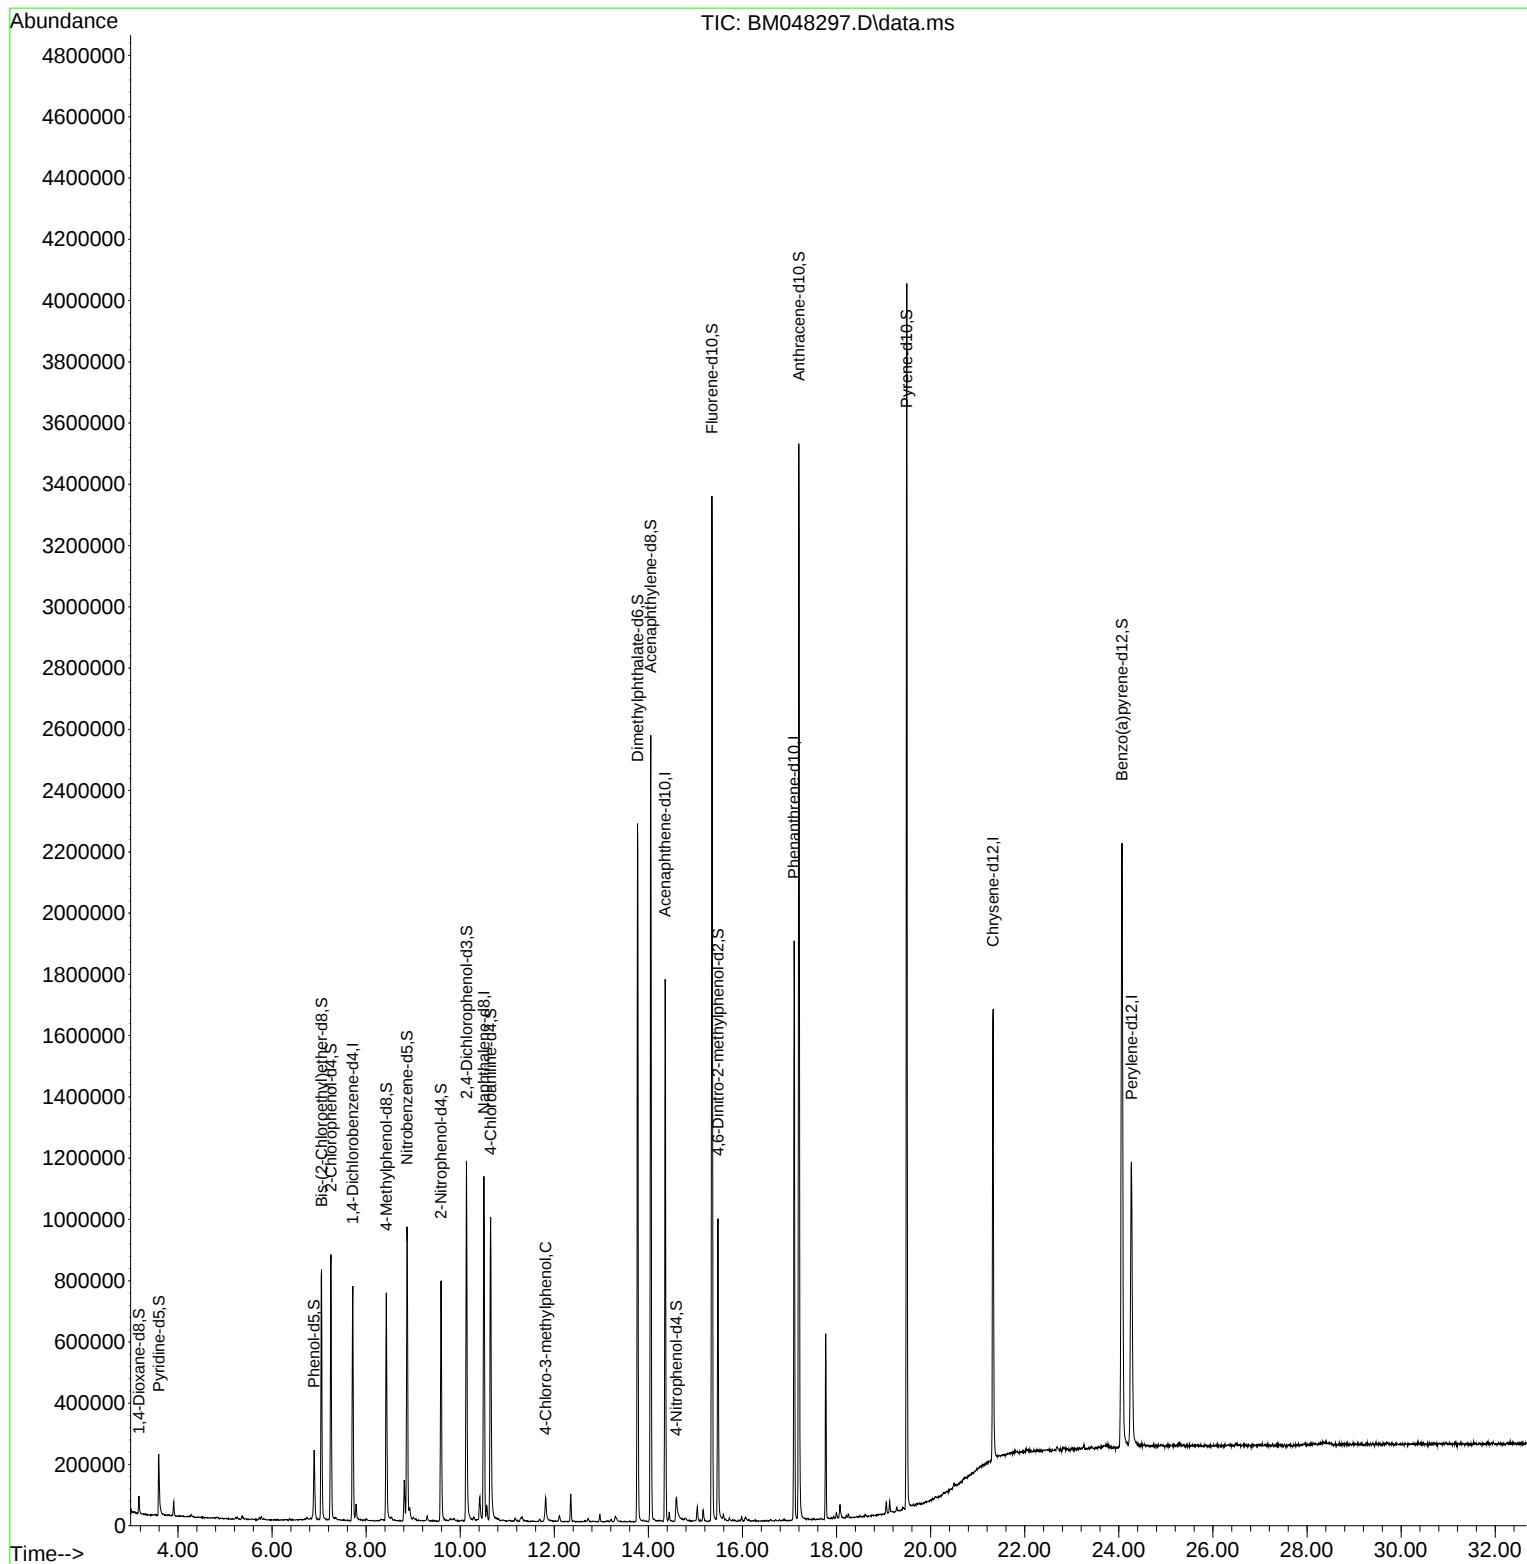

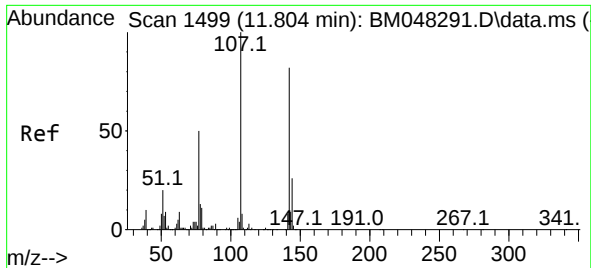

#35
4-Chloro-3-methylphenol
Concen: 2.271 ng/ul
RT: 11.816 min Scan# 11
Delta R.T. 0.000 min
Lab File: BM048297.D
Acq: 29 Oct 2024 21:20

Instrument :
BNA_M
ClientSampleId :
F7H48

Tgt Ion:	107	Resp:	35711
Ion	Ratio	Lower	Upper
107	100		
144	25.7	20.9	31.3
142	78.4	65.3	97.9

