

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048250.D
 Acq On : 28 Oct 2024 11:23
 Operator : RC/JU
 Sample : PB164422BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK422

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	39	rVB	70438	95109	2.16%	0.188%
2	3.587	98	102	125	rBV	827950	1203447	27.31%	2.375%
3	3.910	154	157	164	rVB2	13759	20728	0.47%	0.041%
4	6.898	656	665	677	rBV	814852	1341948	30.45%	2.648%
5	7.051	685	691	703	rVB	690927	1122365	25.47%	2.215%
6	7.257	717	726	740	rBV	843034	1416976	32.15%	2.796%
7	7.722	797	805	817	rBV	820569	1363268	30.93%	2.690%
8	7.939	837	842	845	rBV5	3320	4788	0.11%	0.009%
9	8.433	919	926	944	rBV	969877	1654623	37.55%	3.265%
10	8.875	994	1001	1015	rBV	775463	1318230	29.91%	2.601%
11	9.045	1026	1030	1036	rVB7	2649	5232	0.12%	0.010%
12	9.304	1069	1074	1078	rBV7	3759	6186	0.14%	0.012%
13	9.598	1115	1124	1137	rBV	619596	1074515	24.38%	2.120%
14	10.139	1209	1216	1229	rBV	888677	1558279	35.36%	3.075%
15	10.357	1251	1253	1260	rVB8	4643	5938	0.13%	0.012%
16	10.510	1271	1279	1293	rBV	1128948	1917041	43.50%	3.783%
17	10.651	1296	1303	1322	rBV	803540	1639943	37.21%	3.236%
18	11.798	1493	1498	1505	rVB8	5763	8752	0.20%	0.017%
19	12.133	1548	1555	1561	rBV3	10209	19864	0.45%	0.039%
20	12.363	1589	1594	1600	rBV3	4701	8513	0.19%	0.017%
21	13.774	1827	1834	1849	rBV	1589159	2302178	52.24%	4.542%
22	14.057	1875	1882	1898	rBV	1863949	2831588	64.25%	5.587%
23	14.363	1927	1934	1949	rBV	1699456	2492392	56.55%	4.918%
24	14.580	1966	1971	1998	rBV	370479	939779	21.32%	1.854%
25	15.186	2068	2074	2076	rBV4	2586	4775	0.11%	0.009%
26	15.357	2096	2103	2119	rBV	2336670	3470535	78.75%	6.848%
27	15.486	2119	2125	2140	rVV	676735	1065578	24.18%	2.103%
28	15.598	2140	2144	2151	rVB5	16486	31580	0.72%	0.062%
29	15.921	2193	2199	2204	rBV5	2975	6690	0.15%	0.013%
30	16.898	2361	2365	2367	rBV3	4749	4895	0.11%	0.010%
31	17.104	2394	2400	2411	rBV	1954440	2815486	63.89%	5.555%
32	17.204	2411	2417	2443	rVB	2444202	3719494	84.40%	7.339%
33	19.062	2729	2733	2740	rBV3	28334	44586	1.01%	0.088%
34	19.133	2742	2745	2750	rBV	23348	34199	0.78%	0.067%
35	19.497	2801	2807	2817	rBV	3130948	4281674	97.16%	8.448%
36	21.333	3113	3119	3129	rBV	1868043	3072028	69.71%	6.061%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048250.D
Acq On : 28 Oct 2024 11:23
Operator : RC/JU
Sample : PB164422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK422

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	24.074	3577	3585	3600	rBV	1835411	4407032	100.00%	8.696%
38	24.280	3612	3620	3636	rVB	1316060	3371194	76.50%	6.652%




Sum of corrected areas: 50681428

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048250.D
Acq On : 28 Oct 2024 11:23
Operator : RC/JU
Sample : PB164422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

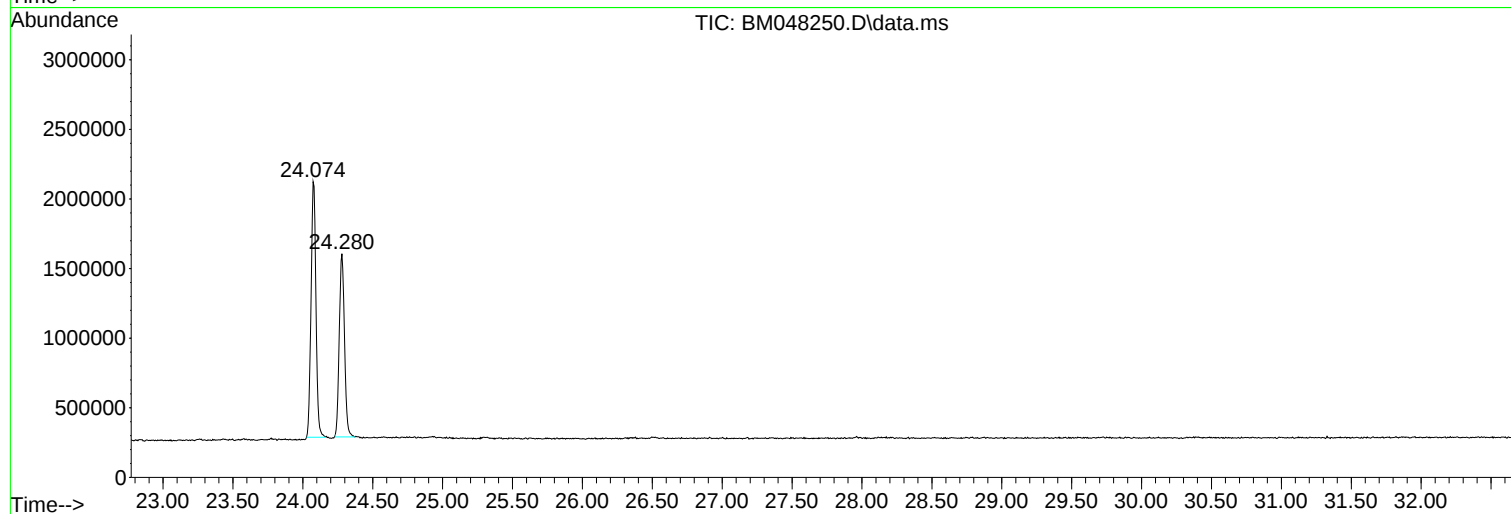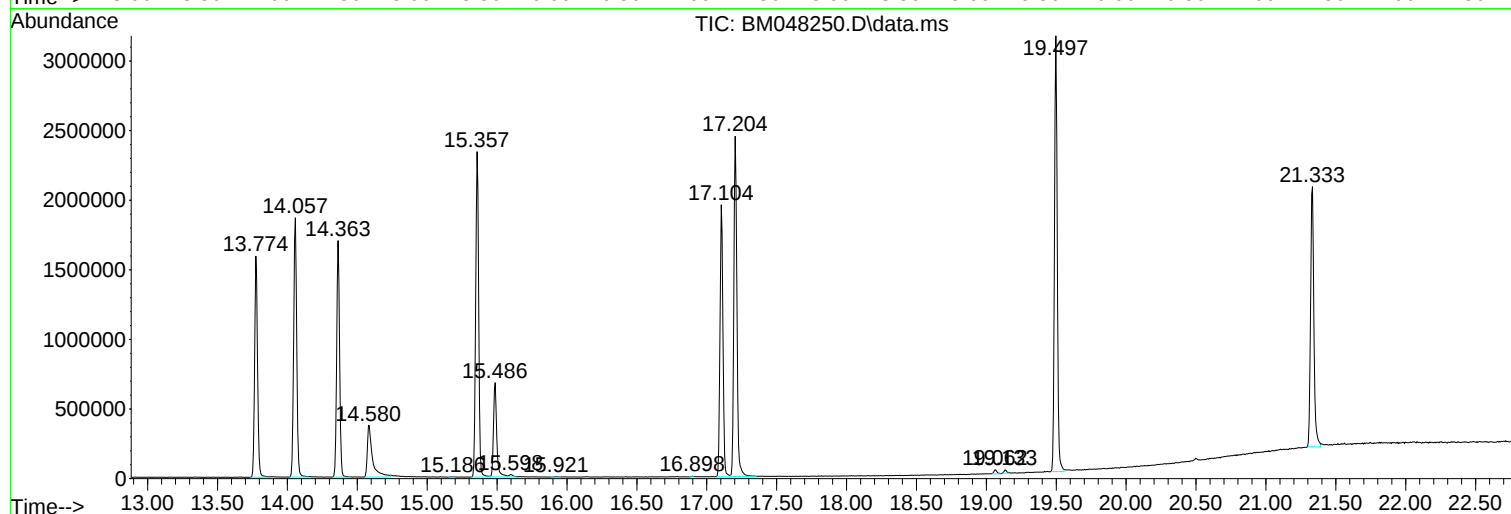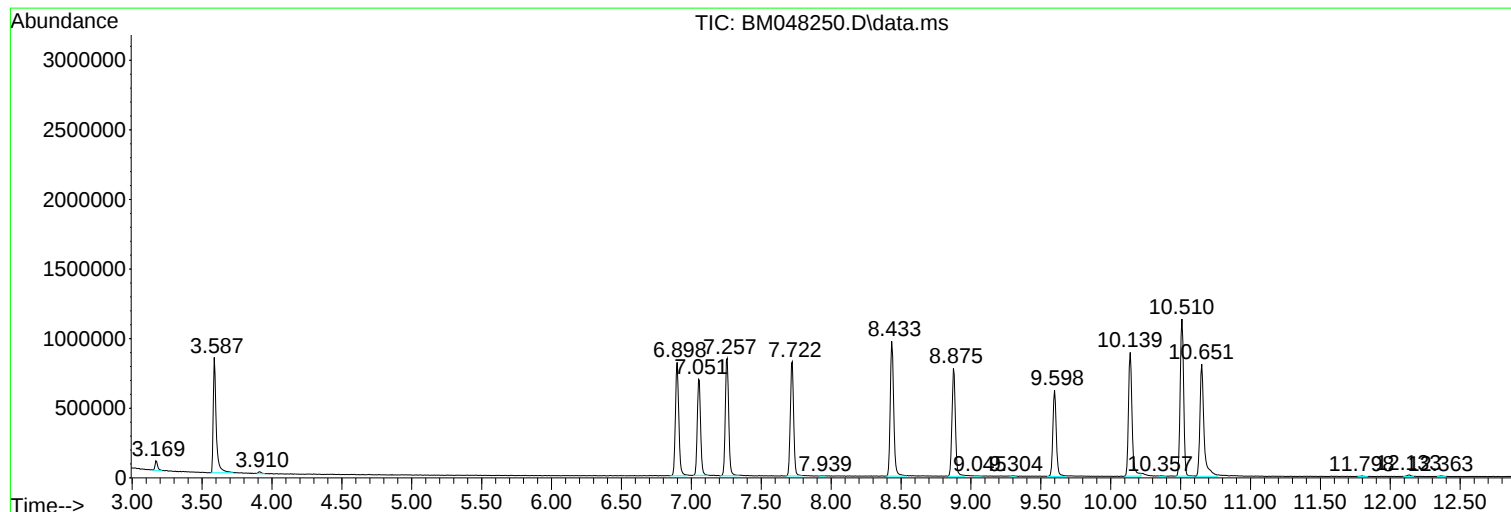

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048250.D
Acq On : 28 Oct 2024 11:23
Operator : RC/JU
Sample : PB164422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048250.D
Acq On : 28 Oct 2024 11:23
Operator : RC/JU
Sample : PB164422BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK422

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc