

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048251.D
 Acq On : 28 Oct 2024 12:02
 Operator : RC/JU
 Sample : P4559-13
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNY8

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048251.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	40	rVB	61100	81741	1.28%	0.143%
2	3.593	100	103	120	rBV	184818	313671	4.92%	0.550%
3	3.910	154	157	161	rVB	10735	14341	0.22%	0.025%
4	4.834	311	314	320	rVB3	6233	9868	0.15%	0.017%
5	6.898	655	665	678	rBV	231276	417708	6.55%	0.733%
6	7.051	684	691	705	rBV	833495	1377528	21.61%	2.418%
7	7.257	718	726	737	rBV	884183	1472222	23.09%	2.584%
8	7.345	739	741	749	rVB7	7467	12672	0.20%	0.022%
9	7.722	797	805	814	rBV	676183	1125936	17.66%	1.976%
10	8.434	918	926	939	rBV	737465	1242029	19.48%	2.180%
11	8.875	993	1001	1010	rBV	961966	1623190	25.46%	2.849%
12	9.016	1019	1025	1033	rBV	33149	60972	0.96%	0.107%
13	9.304	1067	1074	1079	rVB2	42492	67032	1.05%	0.118%
14	9.598	1115	1124	1138	rBV	795610	1358635	21.31%	2.384%
15	10.139	1208	1216	1227	rBV	1124516	1986525	31.16%	3.486%
16	10.510	1272	1279	1290	rBV	1004206	1695486	26.59%	2.976%
17	10.651	1294	1303	1325	rBV	898933	1783972	27.98%	3.131%
18	10.886	1340	1343	1348	rBV6	5797	8112	0.13%	0.014%
19	11.339	1414	1420	1424	rBV5	4897	8086	0.13%	0.014%
20	11.798	1490	1498	1503	rBV2	18523	31778	0.50%	0.056%
21	12.128	1548	1554	1561	rBV2	14682	28835	0.45%	0.051%
22	13.774	1827	1834	1851	rBV	2259145	3282474	51.48%	5.761%
23	14.057	1874	1882	1898	rBV	2640067	3875272	60.78%	6.801%
24	14.363	1927	1934	1944	rBV	1611272	2338634	36.68%	4.104%
25	14.592	1968	1973	1983	rBV2	93672	241031	3.78%	0.423%
26	15.357	2096	2103	2115	rBV	3440720	4935067	77.40%	8.661%
27	15.486	2118	2125	2140	rVV	1108474	1676633	26.30%	2.943%
28	15.598	2140	2144	2150	rVB3	19582	32453	0.51%	0.057%
29	16.533	2293	2303	2308	rBV9	5259	12996	0.20%	0.023%
30	16.786	2342	2346	2350	rBV7	4889	8568	0.13%	0.015%
31	17.104	2393	2400	2411	rBV	1947214	2752502	43.17%	4.831%
32	17.204	2411	2417	2433	rVV	3817116	5501149	86.28%	9.655%
33	17.404	2448	2451	2455	rVB5	5075	6960	0.11%	0.012%
34	18.004	2548	2553	2559	rBV2	55182	83617	1.31%	0.147%
35	18.074	2562	2565	2574	rVB2	11223	18395	0.29%	0.032%
36	19.062	2729	2733	2738	rVB	47259	59245	0.93%	0.104%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048251.D
Acq On : 28 Oct 2024 12:02
Operator : RC/JU
Sample : P4559-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNY8

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	19.133	2741	2745	2747	rBV2	47624	64091	1.01%	0.112%
38	19.162	2747	2750	2762	rVB	88792	137499	2.16%	0.241%
39	19.280	2766	2770	2776	rBV2	63004	91334	1.43%	0.160%
40	19.433	2793	2796	2800	rVB2	20934	20731	0.33%	0.036%
41	19.498	2800	2807	2819	rBV	4585339	6375768	100.00%	11.190%
42	19.733	2845	2847	2850	rBV3	12364	13307	0.21%	0.023%
43	21.327	3113	3118	3129	rBV	1741129	2746606	43.08%	4.820%
44	24.080	3577	3586	3606	rVB	2186974	5376872	84.33%	9.436%
45	24.280	3612	3620	3635	rVB	975017	2608318	40.91%	4.578%




Sum of corrected areas: 56979861

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048251.D
Acq On : 28 Oct 2024 12:02
Operator : RC/JU
Sample : P4559-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

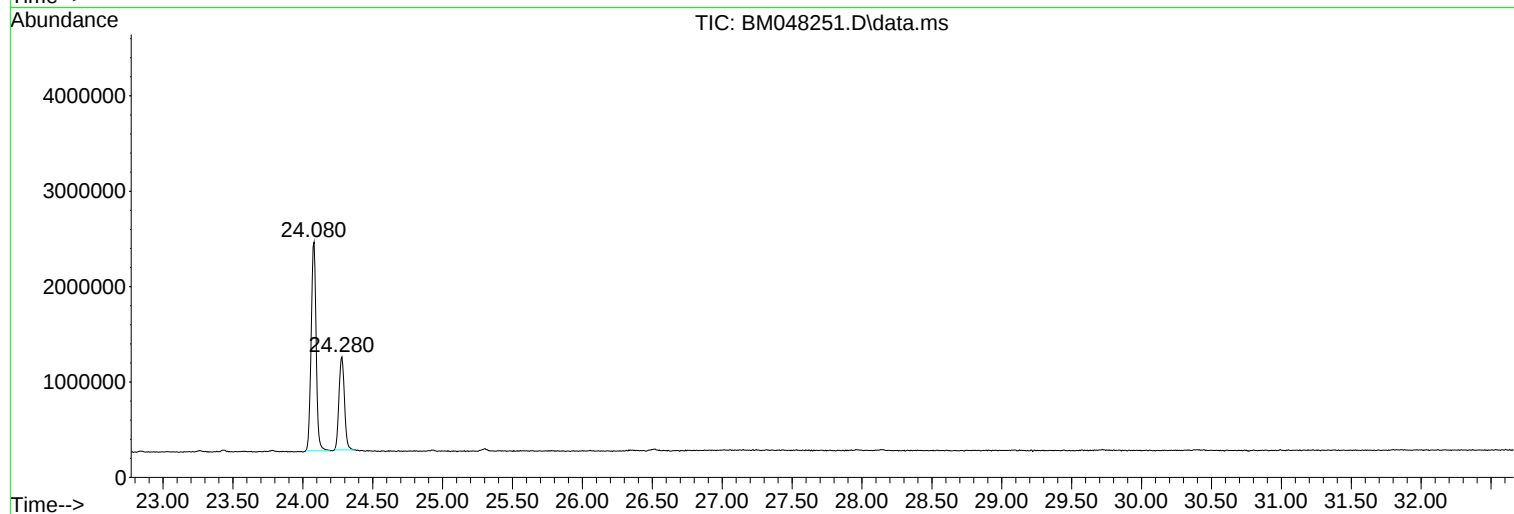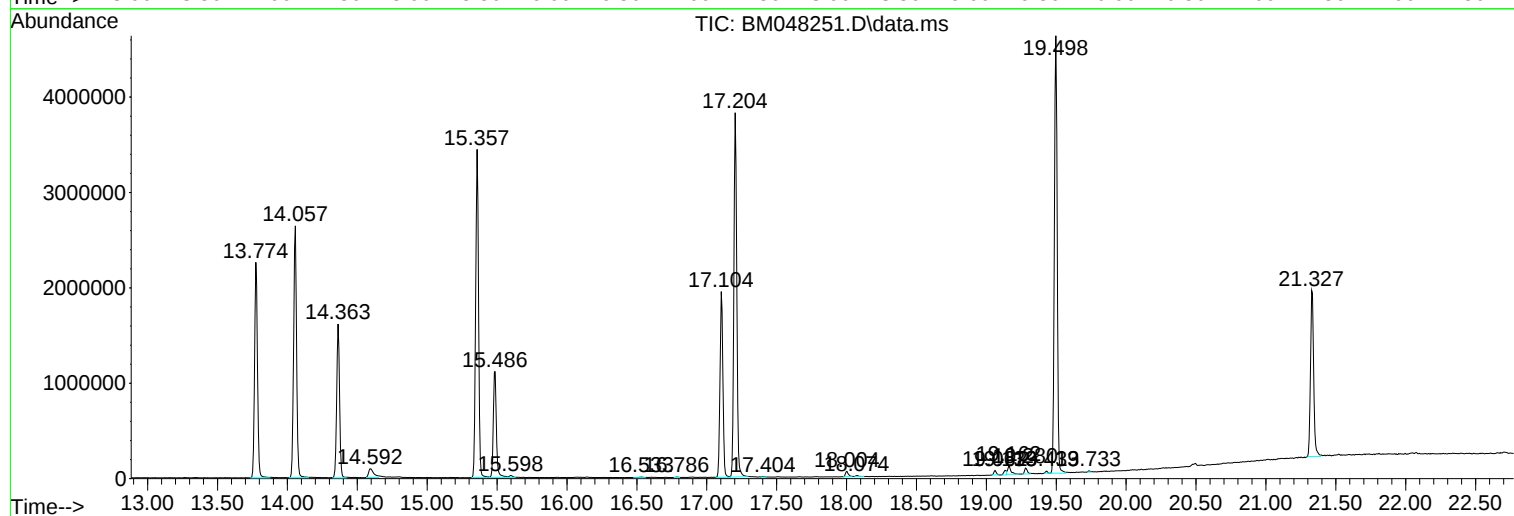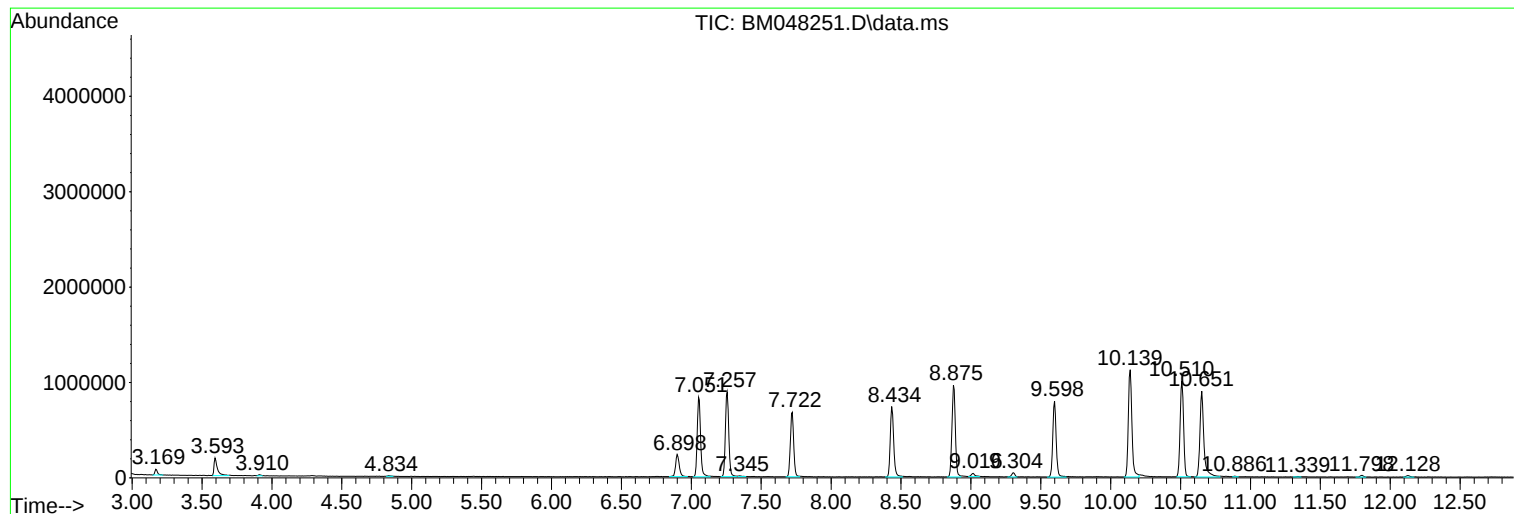

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048251.D
Acq On : 28 Oct 2024 12:02
Operator : RC/JU
Sample : P4559-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048251.D
Acq On : 28 Oct 2024 12:02
Operator : RC/JU
Sample : P4559-13
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNY8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc