

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048253.D
 Acq On : 28 Oct 2024 13:21
 Operator : RC/JU
 Sample : P4559-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048253.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	41	rVB	54488	71840	1.24%	0.126%
2	3.593	100	103	115	rBV	144999	240256	4.13%	0.422%
3	3.910	153	157	162	rVB3	13022	19725	0.34%	0.035%
4	4.281	218	220	229	rVB9	6456	14044	0.24%	0.025%
5	4.840	311	315	321	rVB4	3666	7677	0.13%	0.013%
6	6.898	655	665	681	rBV	234247	423087	7.28%	0.744%
7	7.051	683	691	706	rBV	836011	1397113	24.03%	2.456%
8	7.257	717	726	738	rBV	877219	1496287	25.73%	2.630%
9	7.351	738	742	745	rVB5	6367	10663	0.18%	0.019%
10	7.722	797	805	814	rBV	800561	1322795	22.75%	2.325%
11	8.434	919	926	942	rBV	735812	1237204	21.28%	2.175%
12	8.875	993	1001	1010	rBV	973625	1647215	28.33%	2.895%
13	9.304	1067	1074	1081	rVB	161667	247566	4.26%	0.435%
14	9.598	1117	1124	1141	rBV	818977	1372117	23.60%	2.412%
15	9.710	1141	1143	1150	rVB8	3464	7422	0.13%	0.013%
16	10.139	1209	1216	1241	rBV	1153286	2070981	35.61%	3.640%
17	10.510	1269	1279	1288	rBV	1215511	1966196	33.81%	3.456%
18	10.651	1295	1303	1322	rBV	809236	1663727	28.61%	2.924%
19	10.892	1339	1344	1346	rVB3	6822	7956	0.14%	0.014%
20	11.798	1493	1498	1502	rBV	39483	59066	1.02%	0.104%
21	12.127	1549	1554	1562	rVB4	13634	27299	0.47%	0.048%
22	13.774	1824	1834	1843	rBV	2271760	3229762	55.54%	5.677%
23	14.057	1875	1882	1892	rBV	2579775	3832146	65.90%	6.736%
24	14.363	1926	1934	1946	rBV	1787475	2662161	45.78%	4.679%
25	14.598	1968	1974	1995	rBV2	82958	269298	4.63%	0.473%
26	15.357	2096	2103	2119	rBV	3287695	4860875	83.59%	8.544%
27	15.480	2119	2124	2140	rVV	1004354	1588575	27.32%	2.792%
28	15.598	2140	2144	2151	rVB3	19010	32379	0.56%	0.057%
29	15.727	2160	2166	2172	rVB	37858	55948	0.96%	0.098%
30	16.080	2221	2226	2228	rBV5	5337	8047	0.14%	0.014%
31	16.145	2232	2237	2243	rVB3	10057	18111	0.31%	0.032%
32	16.286	2257	2261	2268	rVB3	13872	20985	0.36%	0.037%
33	16.598	2309	2314	2318	rBV7	3155	6121	0.11%	0.011%
34	16.792	2343	2347	2351	rVB5	5178	6675	0.11%	0.012%
35	17.104	2394	2400	2410	rBV	2067377	2972355	51.11%	5.225%
36	17.204	2411	2417	2440	rVB	3646027	5258087	90.42%	9.242%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048253.D
 Acq On : 28 Oct 2024 13:21
 Operator : RC/JU
 Sample : P4559-15
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNZ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

37	17.509	2462	2469	2473	rBV7	4309	9511	0.16%	0.017%
38	17.609	2483	2486	2490	rBV6	6096	8720	0.15%	0.015%
39	18.004	2548	2553	2560	rBV5	29850	53260	0.92%	0.094%
40	18.074	2563	2565	2570	rVB2	8021	9493	0.16%	0.017%
41	18.303	2600	2604	2608	rVB7	7684	11170	0.19%	0.020%
42	18.851	2694	2697	2703	rVB7	6266	12526	0.22%	0.022%
43	18.939	2708	2712	2715	rVV6	6618	9582	0.16%	0.017%
44	19.062	2728	2733	2739	rBV3	46408	68939	1.19%	0.121%
45	19.133	2741	2745	2748	rBV2	39736	61072	1.05%	0.107%
46	19.162	2748	2750	2754	rVB4	23640	26625	0.46%	0.047%
47	19.286	2767	2771	2779	rBV8	21147	33447	0.58%	0.059%
48	19.433	2793	2796	2799	rVB3	15969	15770	0.27%	0.028%
49	19.498	2801	2807	2820	rVV	4101862	5815162	100.00%	10.222%
50	21.333	3113	3119	3133	rBV	1815234	2872871	49.40%	5.050%
51	24.080	3577	3586	3603	rVB	2021195	4932355	84.82%	8.670%
52	24.274	3612	3619	3638	rVB	1078604	2819065	48.48%	4.955%



Sum of corrected areas: 56891329

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048253.D
Acq On : 28 Oct 2024 13:21
Operator : RC/JU
Sample : P4559-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

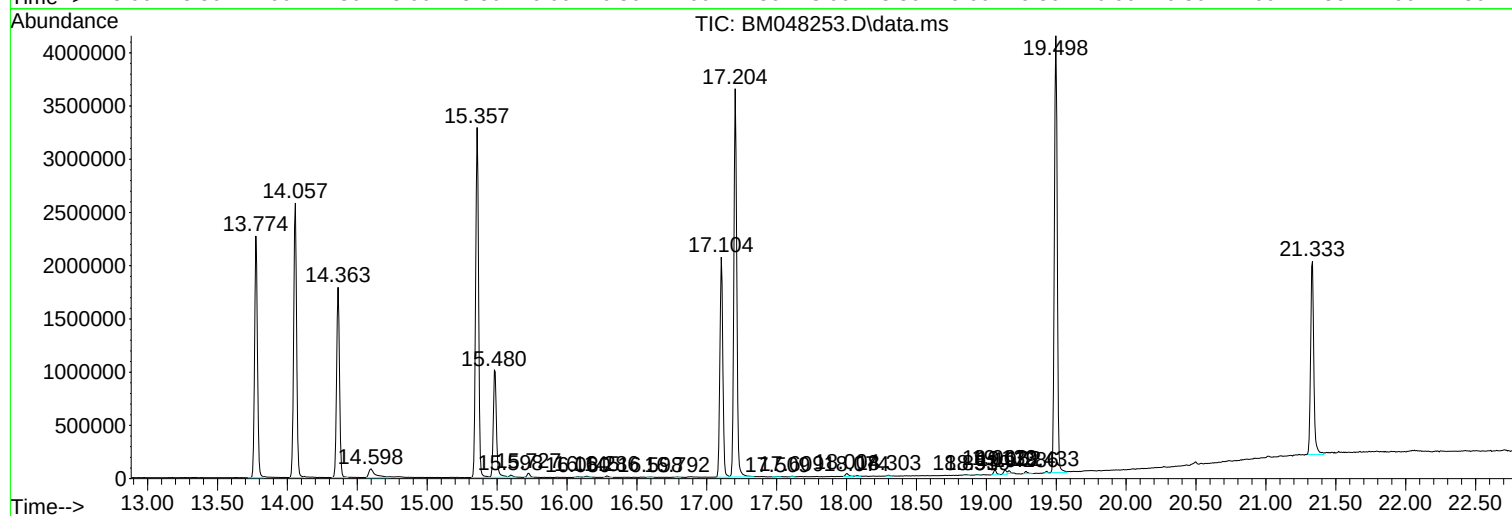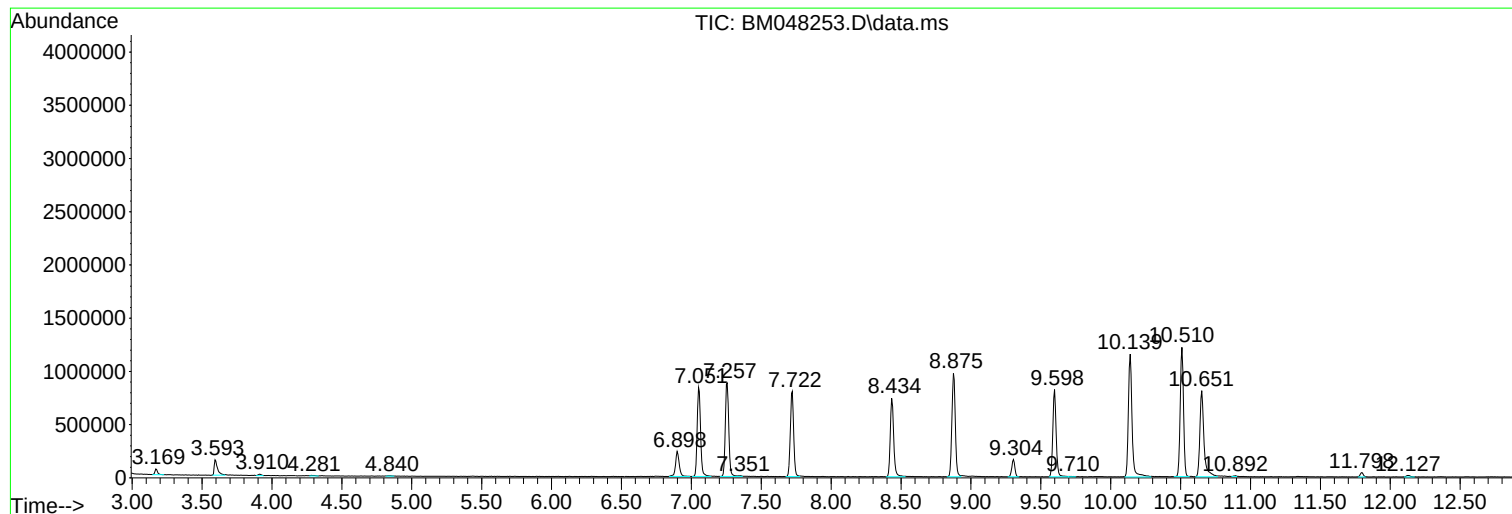

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048253.D
Acq On : 28 Oct 2024 13:21
Operator : RC/JU
Sample : P4559-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048253.D
Acq On : 28 Oct 2024 13:21
Operator : RC/JU
Sample : P4559-15
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc