

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048254.D
 Acq On : 28 Oct 2024 14:00
 Operator : RC/JU
 Sample : P4559-16
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNZ1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	41	rVB	51061	69879	1.16%	0.131%
2	3.593	100	103	114	rBV	125766	207353	3.43%	0.388%
3	3.916	154	158	166	rVB2	11997	21938	0.36%	0.041%
4	6.898	654	665	679	rBV	223049	413517	6.84%	0.774%
5	7.051	685	691	710	rBV	798865	1306148	21.60%	2.446%
6	7.257	717	726	737	rBV	832533	1391420	23.01%	2.606%
7	7.345	738	741	745	rVB6	7010	9184	0.15%	0.017%
8	7.722	798	805	813	rBV	663968	1118456	18.49%	2.095%
9	8.434	919	926	948	rBV	706602	1191319	19.70%	2.231%
10	8.875	991	1001	1010	rBV	908689	1519818	25.13%	2.847%
11	8.951	1010	1014	1018	rVV2	17167	29464	0.49%	0.055%
12	9.010	1019	1024	1034	rVB	32601	60548	1.00%	0.113%
13	9.304	1068	1074	1082	rVB	39439	63360	1.05%	0.119%
14	9.598	1117	1124	1137	rBV	752843	1277221	21.12%	2.392%
15	10.139	1206	1216	1240	rBV	1042414	1962934	32.46%	3.676%
16	10.510	1271	1279	1287	rBV	985913	1689685	27.94%	3.165%
17	10.651	1296	1303	1322	rBV	467507	995572	16.46%	1.865%
18	10.886	1338	1343	1349	rVB8	7873	13027	0.22%	0.024%
19	11.792	1492	1497	1503	rBV3	14664	22855	0.38%	0.043%
20	12.127	1548	1554	1561	rBV	12712	26317	0.44%	0.049%
21	12.363	1590	1594	1599	rBV2	5983	10874	0.18%	0.020%
22	13.774	1828	1834	1849	rBV	2303182	3207209	53.03%	6.007%
23	14.057	1874	1882	1892	rBV	2414967	3645742	60.28%	6.828%
24	14.174	1898	1902	1908	rVB5	6528	11753	0.19%	0.022%
25	14.363	1927	1934	1945	rBV	1561641	2270582	37.55%	4.253%
26	14.598	1967	1974	1988	rBV2	92661	258140	4.27%	0.483%
27	15.357	2096	2103	2118	rBV	3406559	4788550	79.18%	8.969%
28	15.480	2118	2124	2138	rVV	1038017	1632453	26.99%	3.057%
29	15.598	2140	2144	2154	rVB2	22489	41995	0.69%	0.079%
30	15.786	2171	2176	2179	rBV6	4372	6120	0.10%	0.011%
31	16.063	2218	2223	2233	rBV2	16451	39100	0.65%	0.073%
32	16.139	2233	2236	2240	rVB4	4941	7553	0.12%	0.014%
33	16.886	2358	2363	2365	rBV7	4224	6498	0.11%	0.012%
34	17.104	2393	2400	2411	rBV	1870267	2623681	43.38%	4.914%
35	17.204	2411	2417	2439	rVB	3638997	5314345	87.88%	9.953%
36	17.398	2446	2450	2455	rVB7	5213	8721	0.14%	0.016%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048254.D
Acq On : 28 Oct 2024 14:00
Operator : RC/JU
Sample : P4559-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	17.780	2512	2515	2520	rBV5	8311	12973	0.21%	0.024%
38	18.004	2548	2553	2560	rBV3	31577	55462	0.92%	0.104%
39	18.080	2562	2566	2570	rVB3	6348	10765	0.18%	0.020%
40	19.062	2729	2733	2740	rBV	46325	63485	1.05%	0.119%
41	19.133	2741	2745	2748	rBV	44211	63099	1.04%	0.118%
42	19.162	2748	2750	2754	rVB3	31629	36154	0.60%	0.068%
43	19.280	2766	2770	2775	rBV5	35685	54063	0.89%	0.101%
44	19.433	2793	2796	2800	rVB4	16368	16913	0.28%	0.032%
45	19.498	2801	2807	2822	rBV	4445625	6047570	100.00%	11.327%
46	21.327	3113	3118	3130	rBV	1568831	2488924	41.16%	4.662%
47	24.080	3577	3586	3602	rVB	1955603	4860274	80.37%	9.103%
48	24.280	3612	3620	3637	rVB	932488	2419213	40.00%	4.531%




Sum of corrected areas: 53392226

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048254.D
Acq On : 28 Oct 2024 14:00
Operator : RC/JU
Sample : P4559-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

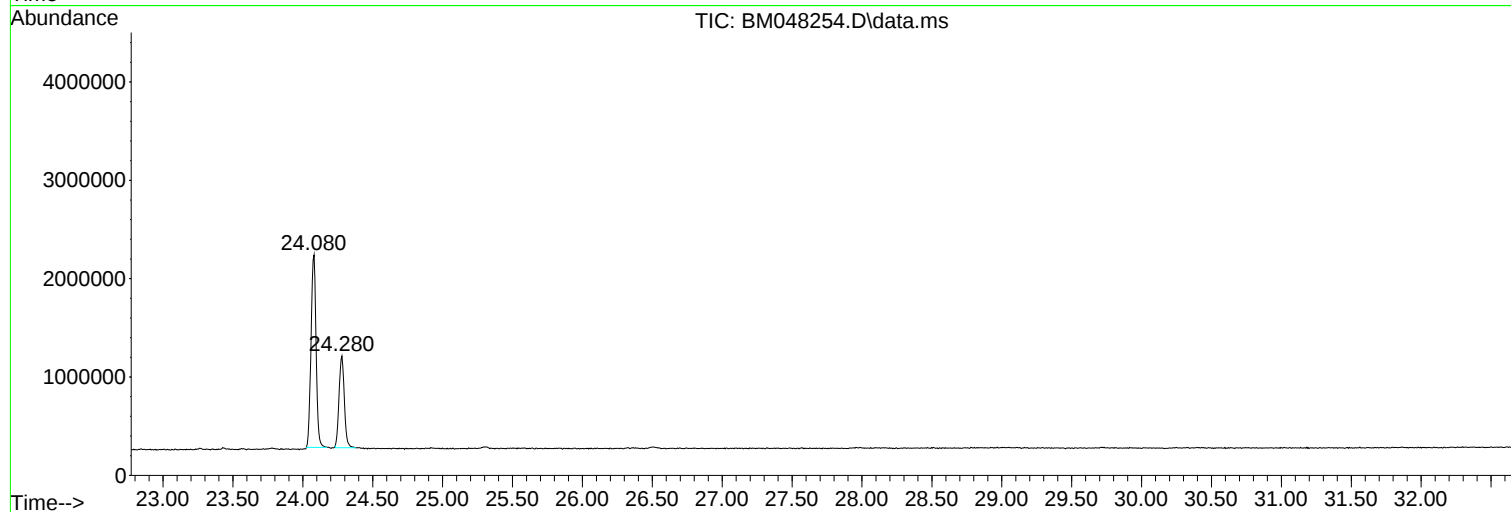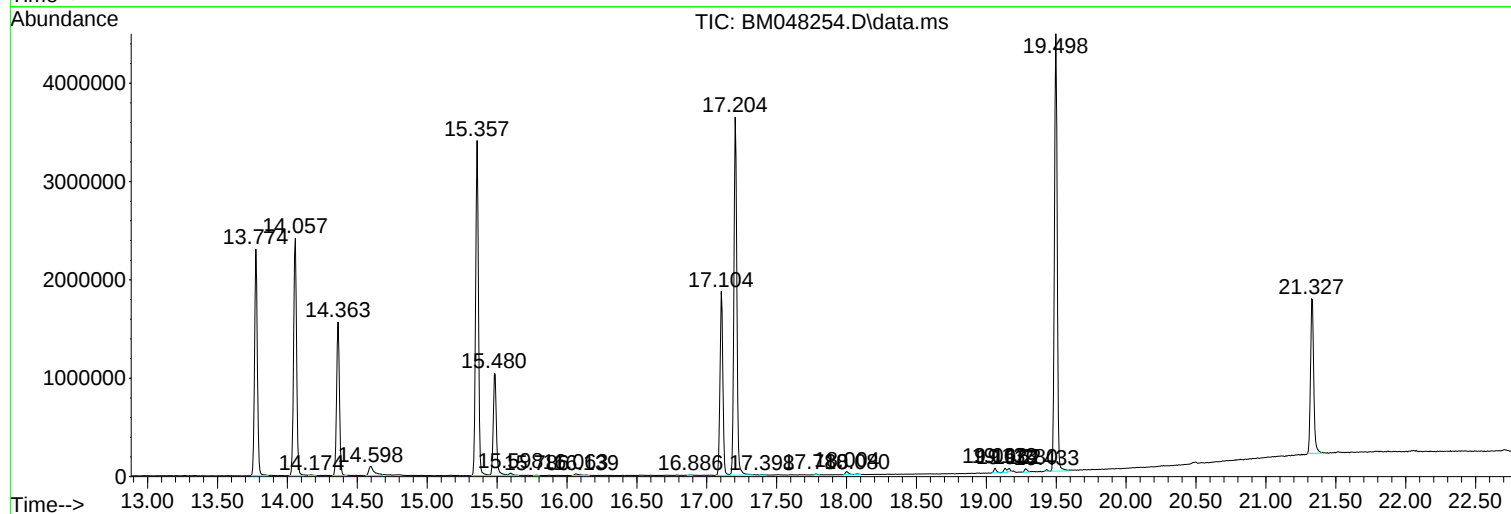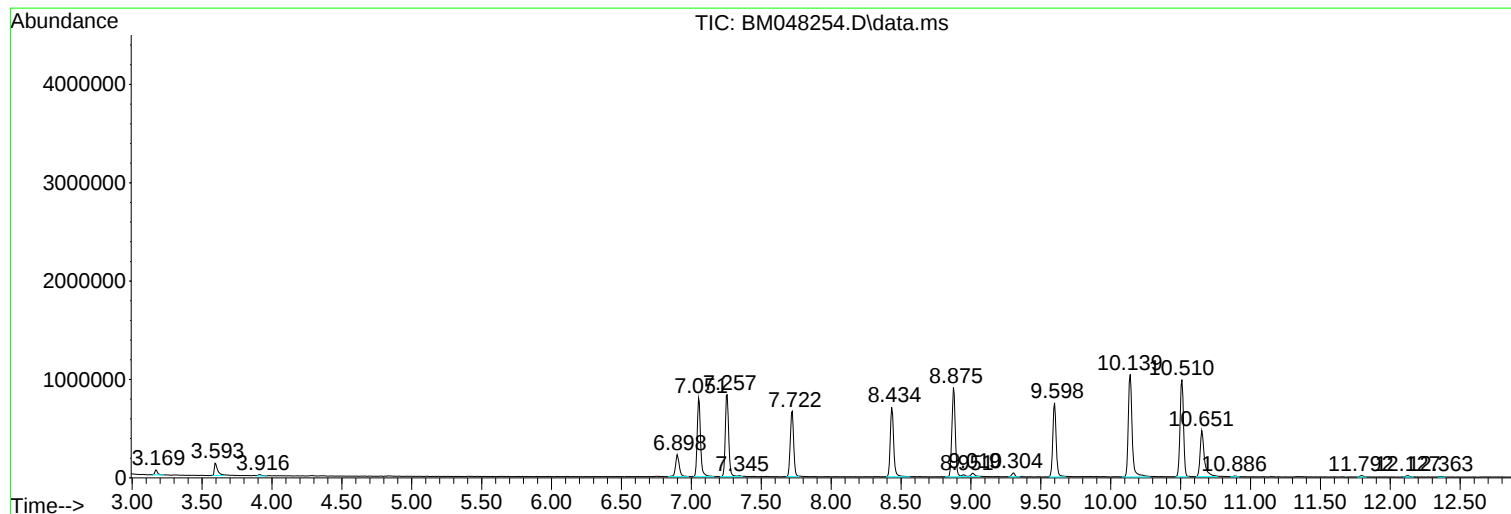

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048254.D
Acq On : 28 Oct 2024 14:00
Operator : RC/JU
Sample : P4559-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048254.D
Acq On : 28 Oct 2024 14:00
Operator : RC/JU
Sample : P4559-16
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
