

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048255.D
 Acq On : 28 Oct 2024 14:40
 Operator : RC/JU
 Sample : P4559-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 GCNZ2

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 0.1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	36	rBV	56977	68847	1.00%	0.111%
2	3.593	99	103	119	rBV	272101	444282	6.48%	0.717%
3	3.910	154	157	163	rVB	12703	17522	0.26%	0.028%
4	4.287	217	221	225	rBV6	5027	7760	0.11%	0.013%
5	6.898	653	665	679	rBV	276385	495136	7.23%	0.799%
6	7.051	684	691	705	rBV	891929	1472494	21.49%	2.376%
7	7.257	718	726	737	rBV	954575	1591659	23.23%	2.568%
8	7.722	796	805	813	rBV	777837	1294339	18.89%	2.089%
9	8.434	919	926	937	rBV	840291	1390465	20.29%	2.244%
10	8.875	994	1001	1012	rBV	1043871	1741102	25.41%	2.810%
11	9.304	1067	1074	1083	rBV	41581	63005	0.92%	0.102%
12	9.598	1115	1124	1135	rBV	880329	1455429	21.24%	2.349%
13	9.892	1171	1174	1183	rBV9	3787	6964	0.10%	0.011%
14	10.139	1207	1216	1227	rBV	1251843	2148419	31.36%	3.467%
15	10.510	1270	1279	1291	rBV	1156236	1944664	28.38%	3.138%
16	10.651	1295	1303	1323	rBV	992404	1945760	28.40%	3.140%
17	10.892	1340	1344	1351	rVB9	5654	10551	0.15%	0.017%
18	11.333	1415	1419	1422	rBV6	4407	8850	0.13%	0.014%
19	11.798	1492	1498	1503	rBV3	18220	29243	0.43%	0.047%
20	12.127	1549	1554	1558	rBV2	14113	25400	0.37%	0.041%
21	13.774	1827	1834	1848	rBV	2457537	3499010	51.07%	5.646%
22	14.057	1875	1882	1898	rBV	2767728	4151216	60.59%	6.699%
23	14.363	1927	1934	1944	rBV	1805676	2683916	39.17%	4.331%
24	14.592	1967	1973	1992	rBV2	115561	334222	4.88%	0.539%
25	15.357	2096	2103	2118	rBV	3661917	5319046	77.64%	8.583%
26	15.486	2118	2125	2140	rVV	1195489	1833520	26.76%	2.959%
27	15.604	2140	2145	2150	rVB2	19230	34298	0.50%	0.055%
28	16.074	2220	2225	2227	rBV4	4586	8021	0.12%	0.013%
29	16.139	2232	2236	2241	rVB7	3871	7532	0.11%	0.012%
30	16.533	2297	2303	2307	rBV7	5669	8964	0.13%	0.014%
31	16.604	2311	2315	2320	rVB5	4810	8114	0.12%	0.013%
32	16.892	2360	2364	2367	rBV5	5707	7588	0.11%	0.012%
33	17.104	2393	2400	2411	rBV	2189032	3135074	45.76%	5.059%
34	17.204	2411	2417	2435	rVV2	4067045	5922625	86.44%	9.557%
35	18.004	2549	2553	2559	rBV5	31390	48974	0.71%	0.079%
36	18.074	2563	2565	2571	rVB3	9909	11215	0.16%	0.018%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048255.D
Acq On : 28 Oct 2024 14:40
Operator : RC/JU
Sample : P4559-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	19.062	2728	2733	2739	rBV2	58383	86939	1.27%	0.140%
38	19.133	2741	2745	2747	rBV	50632	61661	0.90%	0.099%
39	19.162	2747	2750	2754	rVB3	37361	49679	0.73%	0.080%
40	19.280	2767	2770	2778	rBV6	32169	48698	0.71%	0.079%
41	19.433	2793	2796	2800	rVB5	17418	22321	0.33%	0.036%
42	19.498	2800	2807	2822	rBV	5093888	6851328	100.00%	11.056%
43	20.497	2974	2977	2980	rVB	56329	60708	0.89%	0.098%
44	21.333	3113	3119	3132	rBV	1986813	3123221	45.59%	5.040%
45	24.080	3577	3586	3606	rVB	2306714	5563055	81.20%	8.977%
46	24.280	3611	3620	3634	rBV	1117409	2928529	42.74%	4.726%




Sum of corrected areas: 61971365

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048255.D
Acq On : 28 Oct 2024 14:40
Operator : RC/JU
Sample : P4559-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

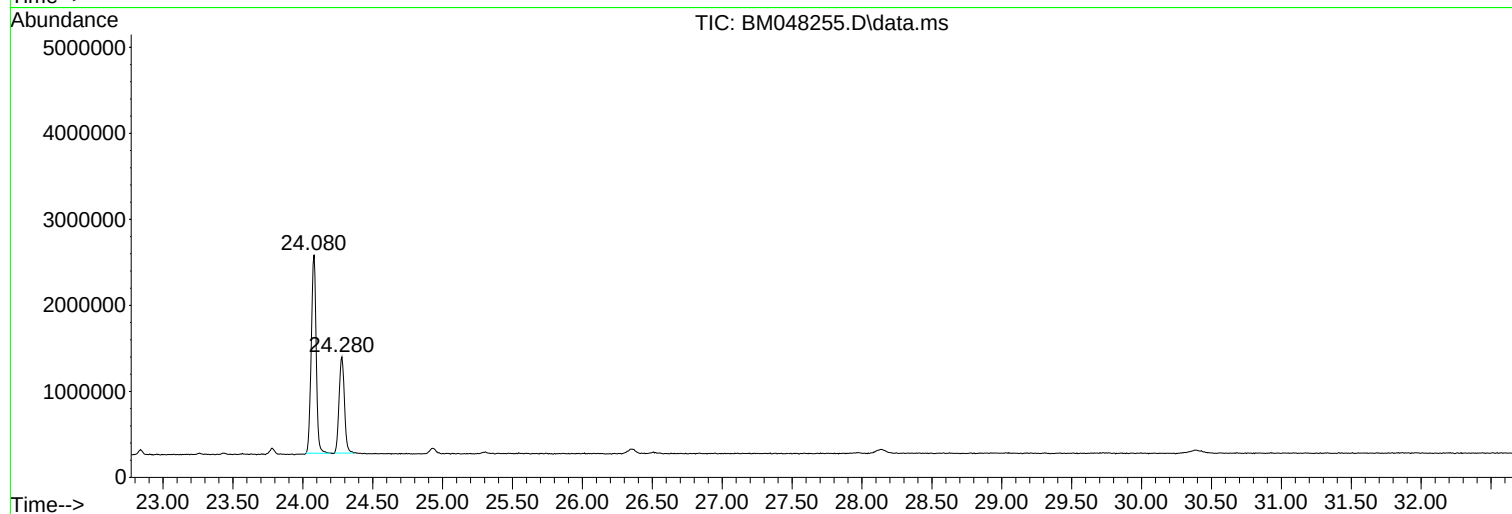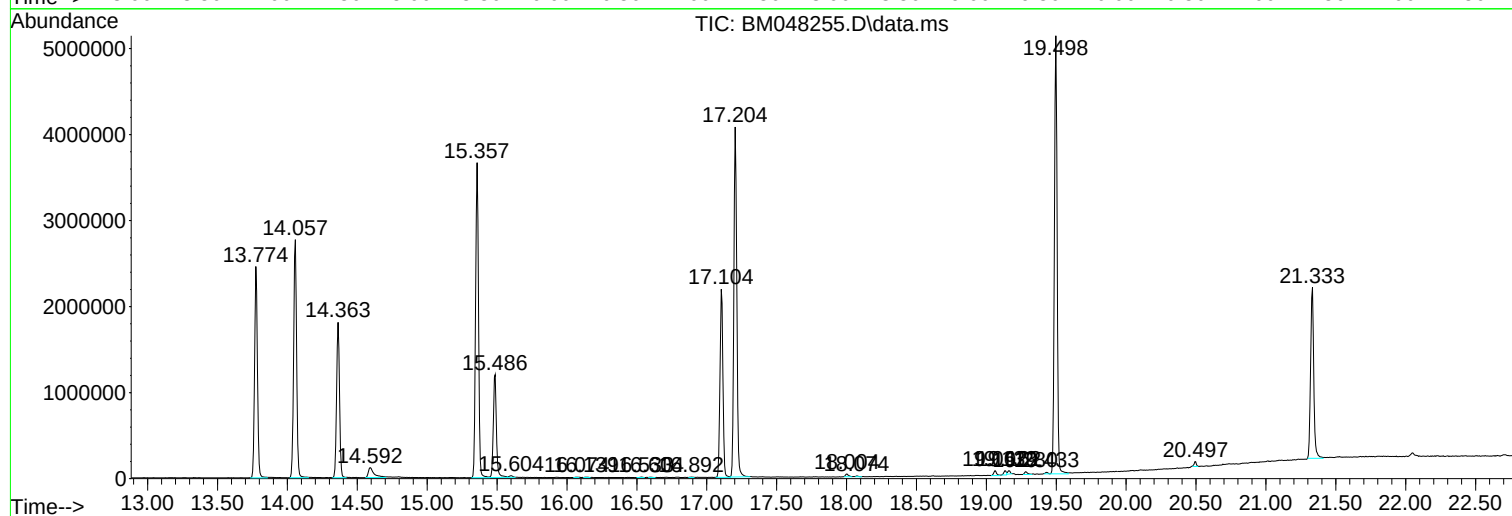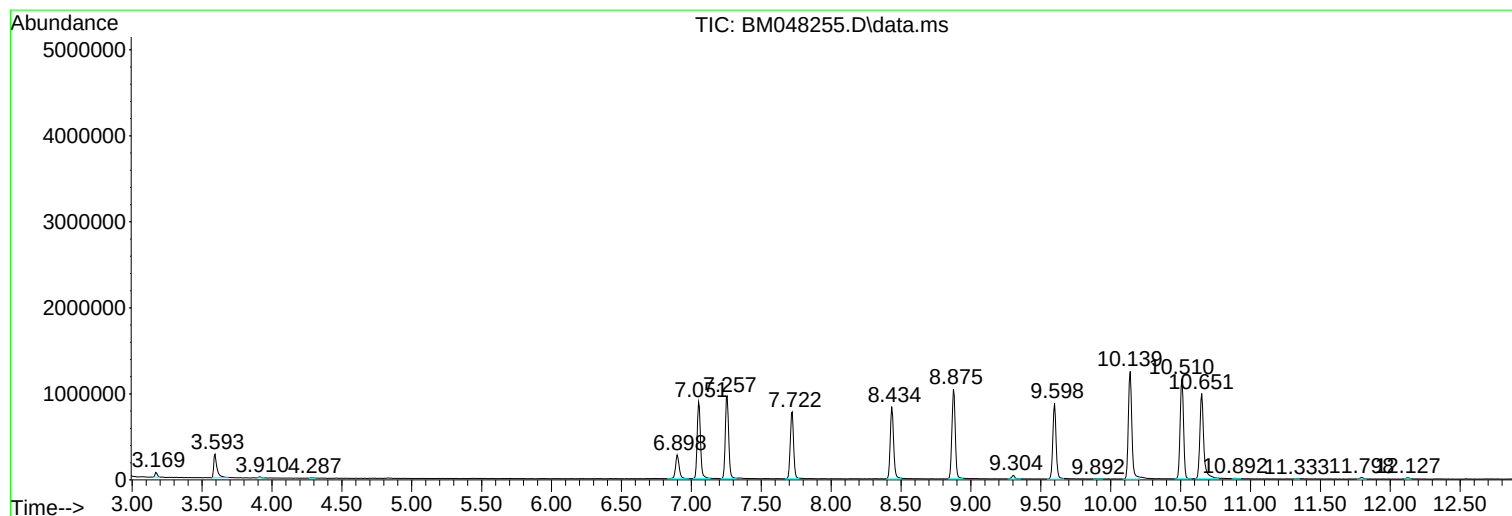

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048255.D
Acq On : 28 Oct 2024 14:40
Operator : RC/JU
Sample : P4559-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048255.D
Acq On : 28 Oct 2024 14:40
Operator : RC/JU
Sample : P4559-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
GCNZ2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc