

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048259.D
 Acq On : 28 Oct 2024 17:17
 Operator : RC/JU
 Sample : P4534-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048259.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	39	rVB	56859	72600	1.31%	0.137%
2	3.593	99	103	116	rBV	177700	289600	5.22%	0.547%
3	3.910	154	157	162	rVB3	12191	15165	0.27%	0.029%
4	4.828	312	313	322	rVB5	5029	6776	0.12%	0.013%
5	6.898	656	665	677	rBV	245011	437296	7.88%	0.826%
6	7.051	683	691	707	rBV	784960	1282791	23.11%	2.423%
7	7.251	719	725	737	rBV	827016	1398738	25.20%	2.642%
8	7.716	795	804	816	rBV	783706	1307448	23.55%	2.469%
9	8.434	919	926	938	rBV	788275	1312547	23.65%	2.479%
10	8.875	994	1001	1012	rBV	893824	1508918	27.18%	2.850%
11	9.304	1068	1074	1079	rVB3	15026	23798	0.43%	0.045%
12	9.598	1117	1124	1138	rBV	732587	1253603	22.58%	2.368%
13	10.139	1208	1216	1228	rBV	1023559	1836732	33.09%	3.469%
14	10.510	1272	1279	1290	rBV	1113175	1857787	33.47%	3.509%
15	10.651	1295	1303	1322	rBV	728258	1509402	27.19%	2.851%
16	11.798	1492	1498	1504	rVB2	13026	20754	0.37%	0.039%
17	12.127	1548	1554	1561	rBV2	13065	25316	0.46%	0.048%
18	12.363	1590	1594	1598	rVB	5538	7221	0.13%	0.014%
19	13.774	1827	1834	1850	rBV	2061670	2903754	52.31%	5.484%
20	14.057	1873	1882	1900	rBV	2162668	3323152	59.87%	6.276%
21	14.363	1927	1934	1949	rBV	1638280	2364830	42.60%	4.466%
22	14.598	1968	1974	1985	rBV2	72894	199042	3.59%	0.376%
23	14.804	2008	2009	2017	rVB8	5666	6554	0.12%	0.012%
24	15.357	2096	2103	2118	rBV	2914225	4269359	76.92%	8.063%
25	15.480	2118	2124	2141	rVV	959110	1458425	26.27%	2.754%
26	15.598	2141	2144	2150	rVB4	17005	27567	0.50%	0.052%
27	16.068	2219	2224	2231	rBV4	10059	24621	0.44%	0.046%
28	16.580	2306	2311	2317	rBV4	30852	54928	0.99%	0.104%
29	16.704	2327	2332	2338	rVB3	20547	31509	0.57%	0.060%
30	16.792	2343	2347	2350	rVB7	4974	6381	0.11%	0.012%
31	16.898	2356	2365	2368	rBV6	6303	13711	0.25%	0.026%
32	16.980	2374	2379	2382	rBV7	3296	6792	0.12%	0.013%
33	17.104	2393	2400	2410	rBV	1819361	2590837	46.68%	4.893%
34	17.204	2410	2417	2435	rVV	3417000	4858246	87.53%	9.175%
35	17.339	2438	2440	2446	rVB7	6115	10750	0.19%	0.020%
36	17.509	2466	2469	2473	rBV5	3684	7098	0.13%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048259.D
Acq On : 28 Oct 2024 17:17
Operator : RC/JU
Sample : P4534-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L78

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	17.604	2482	2485	2490	rBV7	4240	6445	0.12%	0.012%
38	17.692	2497	2500	2505	rVB6	8001	10381	0.19%	0.020%
39	17.774	2512	2514	2521	rVB8	5296	7875	0.14%	0.015%
40	17.998	2546	2552	2557	rBV4	47446	74423	1.34%	0.141%
41	18.286	2596	2601	2607	rBV2	20092	34187	0.62%	0.065%
42	19.062	2728	2733	2738	rBV2	40313	61327	1.10%	0.116%
43	19.133	2741	2745	2749	rBV	43647	64236	1.16%	0.121%
44	19.280	2767	2770	2775	rBV4	44471	56604	1.02%	0.107%
45	19.433	2792	2796	2798	rBV4	19398	21980	0.40%	0.042%
46	19.498	2801	2807	2821	rVV	4000489	5550620	100.00%	10.483%
47	21.333	3113	3119	3130	rBV	1645722	2619454	47.19%	4.947%
48	24.080	3577	3586	3607	rVB	2151356	5362757	96.62%	10.128%
49	24.280	3611	3620	3634	rVB	1055768	2754856	49.63%	5.203%




Sum of corrected areas: 52949193

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048259.D
Acq On : 28 Oct 2024 17:17
Operator : RC/JU
Sample : P4534-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

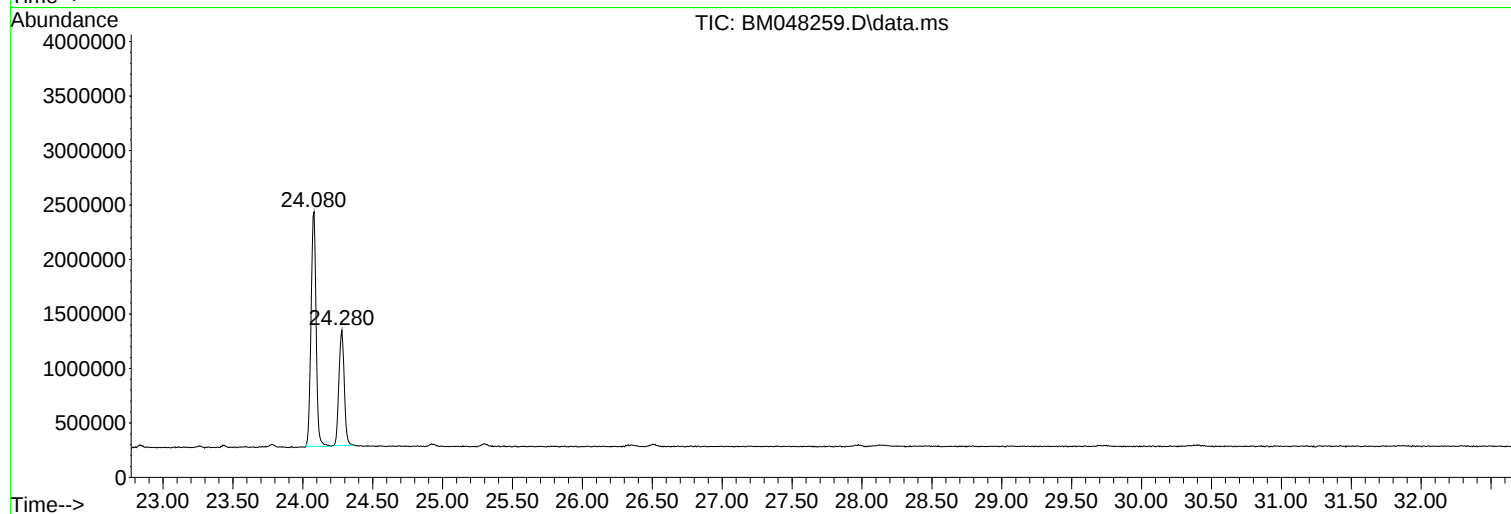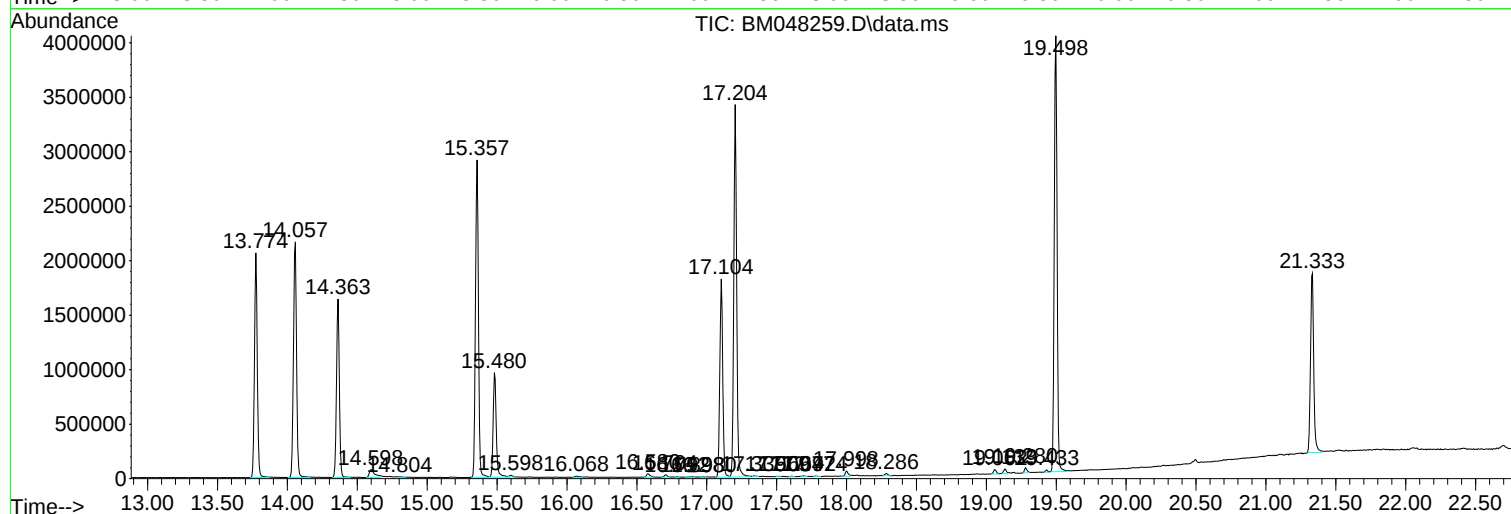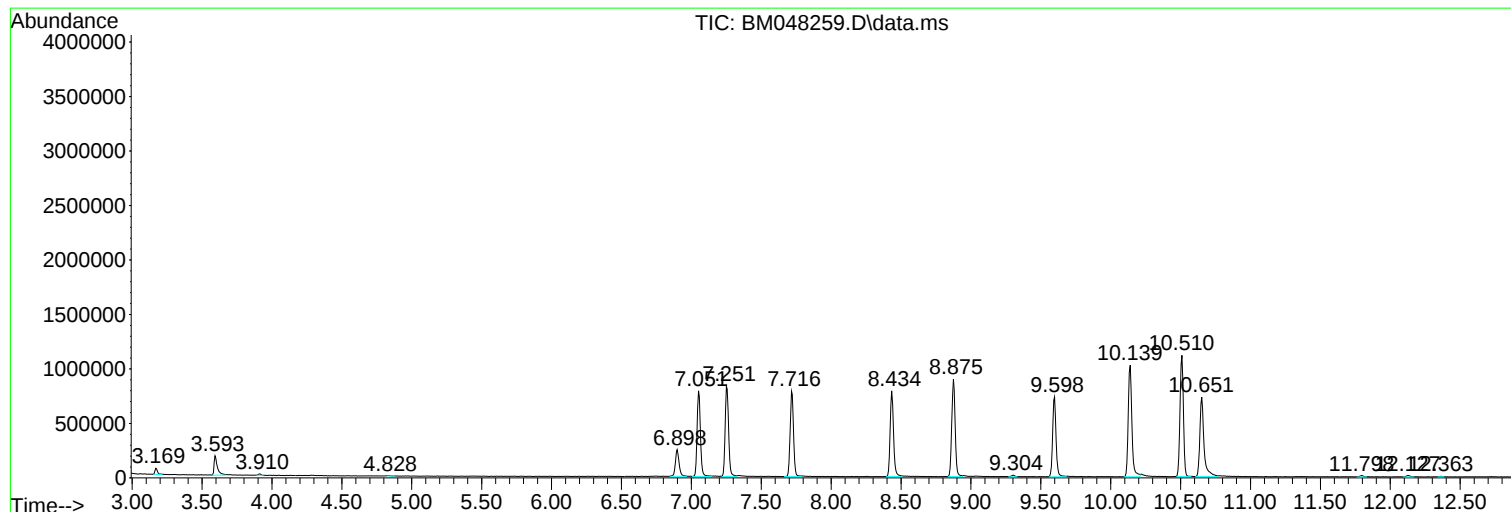

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048259.D
Acq On : 28 Oct 2024 17:17
Operator : RC/JU
Sample : P4534-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048259.D
Acq On : 28 Oct 2024 17:17
Operator : RC/JU
Sample : P4534-07
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L78

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc