

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048260.D
 Acq On : 28 Oct 2024 17:56
 Operator : RC/JU
 Sample : P4534-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E1L98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	28	31	36	rBV	54044	66984	1.10%	0.119%
2	3.593	99	103	124	rBV	190731	318543	5.25%	0.567%
3	3.910	153	157	165	rVB2	13812	22852	0.38%	0.041%
4	6.898	654	665	677	rBV	219842	396783	6.54%	0.706%
5	7.051	685	691	702	rBV	847504	1364992	22.50%	2.430%
6	7.251	719	725	736	rBV	863779	1468973	24.21%	2.615%
7	7.340	738	740	748	rVB7	8576	15137	0.25%	0.027%
8	7.716	797	804	813	rBV	822261	1389373	22.90%	2.473%
9	8.434	918	926	937	rBV	723790	1196097	19.72%	2.129%
10	8.875	994	1001	1010	rBV	980982	1627469	26.83%	2.897%
11	9.304	1066	1074	1078	rBV3	13162	21381	0.35%	0.038%
12	9.598	1116	1124	1140	rBV	771307	1352182	22.29%	2.407%
13	10.139	1209	1216	1228	rBV	1085232	1966415	32.41%	3.500%
14	10.510	1271	1279	1290	rBV	1226652	2058604	33.93%	3.664%
15	10.651	1296	1303	1324	rBV	308801	748772	12.34%	1.333%
16	11.792	1492	1497	1502	rVB	12177	19011	0.31%	0.034%
17	12.122	1548	1553	1561	rBV4	12904	26477	0.44%	0.047%
18	12.363	1590	1594	1600	rVB3	4382	6812	0.11%	0.012%
19	13.774	1827	1834	1844	rBV	2281574	3285511	54.16%	5.848%
20	14.057	1873	1882	1893	rBV	2444518	3728409	61.46%	6.637%
21	14.363	1927	1934	1950	rVB	1890958	2745721	45.26%	4.887%
22	14.592	1967	1973	1990	rBV2	75332	236150	3.89%	0.420%
23	14.804	2007	2009	2014	rVB5	4773	6089	0.10%	0.011%
24	15.169	2066	2071	2072	rBV2	4802	6116	0.10%	0.011%
25	15.357	2095	2103	2118	rBV	3299601	4910683	80.95%	8.741%
26	15.480	2118	2124	2139	rVV	1099856	1690789	27.87%	3.010%
27	15.598	2141	2144	2151	rVB4	19619	33901	0.56%	0.060%
28	16.063	2218	2223	2232	rBV3	12564	30176	0.50%	0.054%
29	16.133	2234	2235	2241	rVB5	5601	6142	0.10%	0.011%
30	16.604	2310	2315	2317	rBV6	5340	7488	0.12%	0.013%
31	16.780	2341	2345	2349	rBV5	4942	8178	0.13%	0.015%
32	16.892	2359	2364	2370	rBV5	5441	10727	0.18%	0.019%
33	17.104	2394	2400	2410	rBV	2165113	3014477	49.69%	5.366%
34	17.204	2410	2417	2433	rVV2	3785004	5509324	90.81%	9.807%
35	18.004	2548	2553	2558	rBV5	24342	42672	0.70%	0.076%
36	18.080	2563	2566	2570	rVB2	5493	6746	0.11%	0.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048260.D
Acq On : 28 Oct 2024 17:56
Operator : RC/JU
Sample : P4534-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L98

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	19.062	2729	2733	2738	rBV2	41448	54106	0.89%	0.096%
38	19.133	2741	2745	2750	rBV	38984	58829	0.97%	0.105%
39	19.286	2768	2771	2778	rBV8	19899	30466	0.50%	0.054%
40	19.427	2793	2795	2800	rVB4	13026	14911	0.25%	0.027%
41	19.498	2800	2807	2819	rBV	4440045	6066648	100.00%	10.799%
42	21.327	3113	3118	3131	rBV2	1677217	2731564	45.03%	4.862%
43	24.080	3577	3586	3600	rVB	2087738	5097271	84.02%	9.073%
44	24.274	3611	3619	3636	rVB	1068201	2778828	45.80%	4.946%




Sum of corrected areas: 56178779

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048260.D
Acq On : 28 Oct 2024 17:56
Operator : RC/JU
Sample : P4534-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

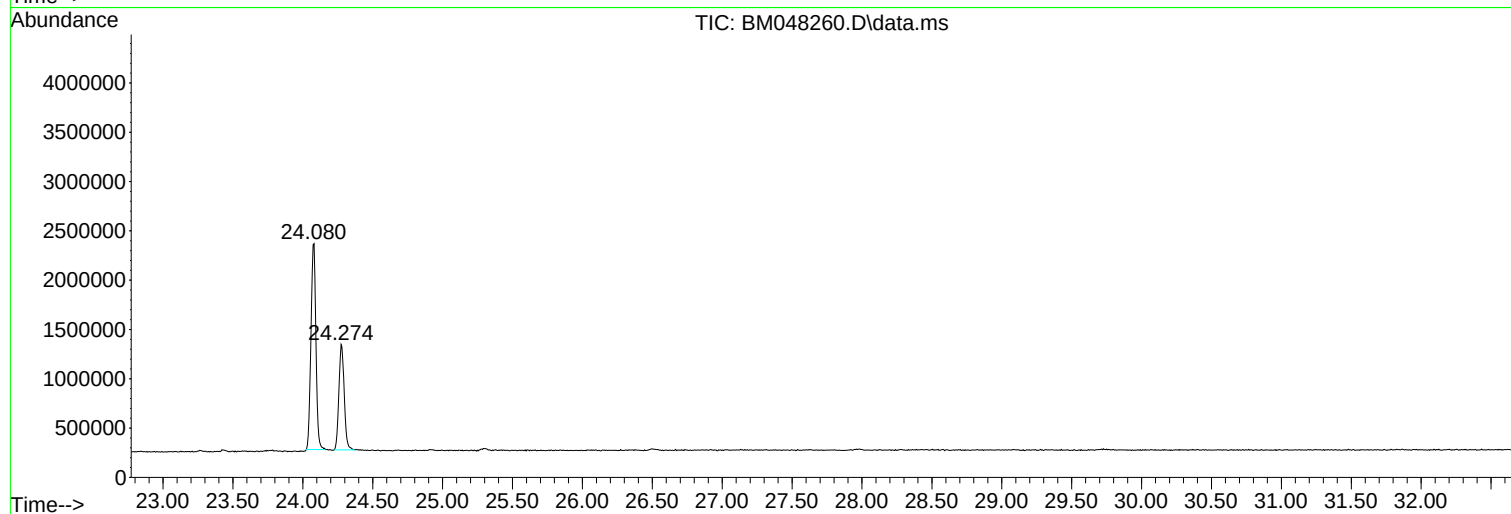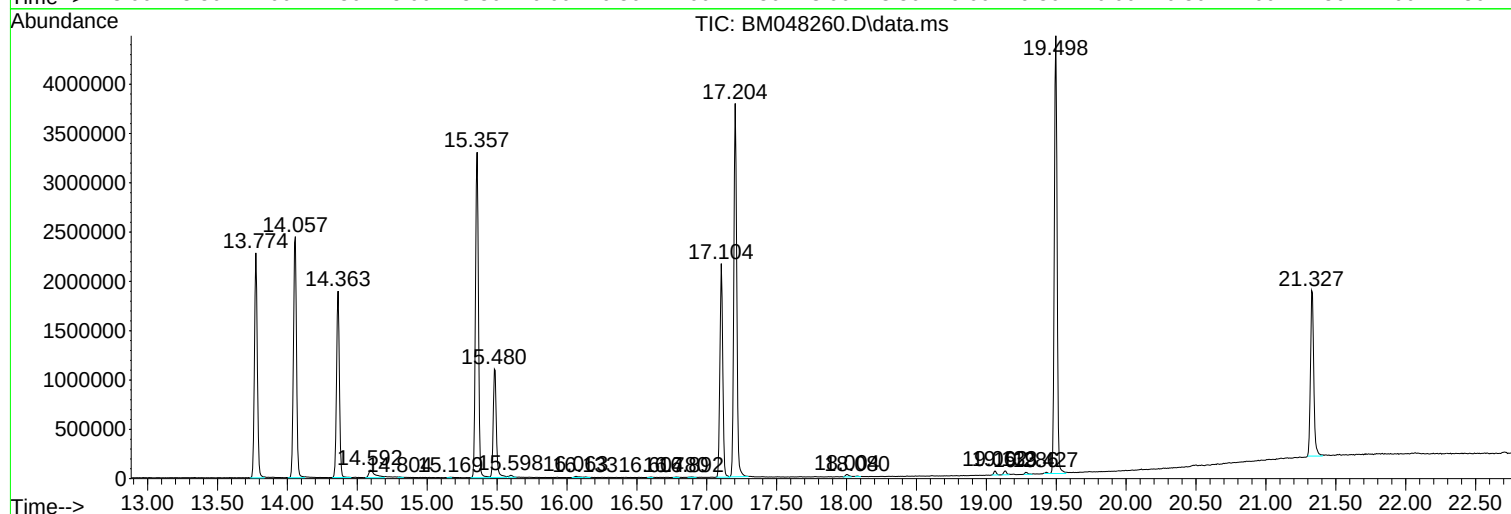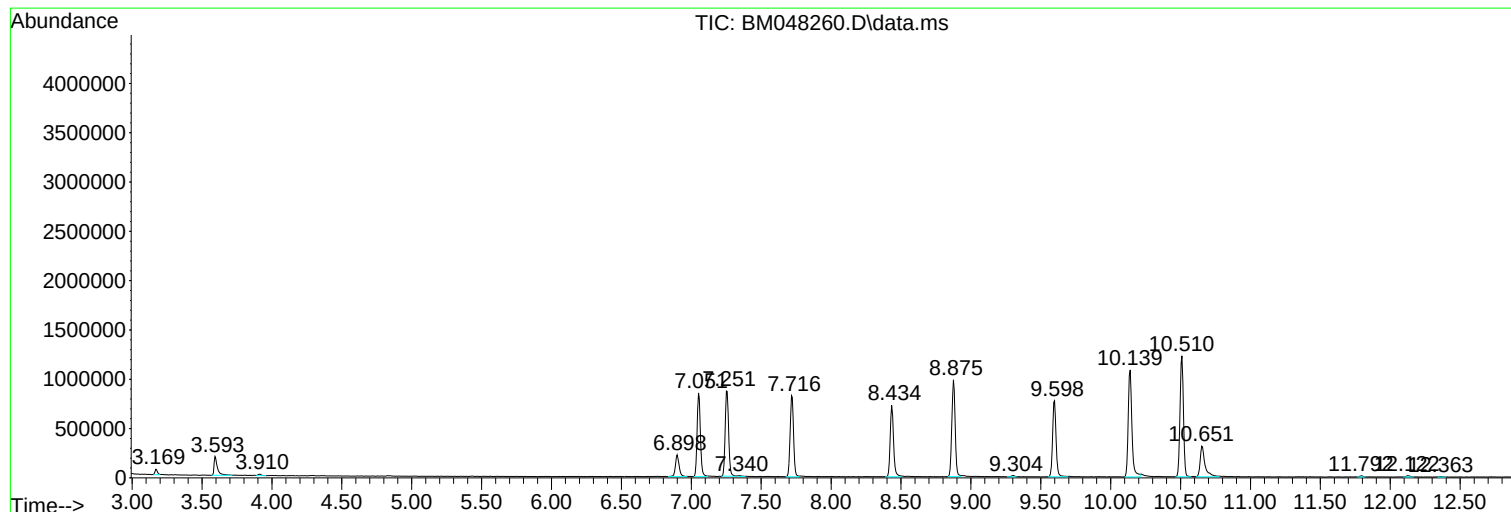

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048260.D
Acq On : 28 Oct 2024 17:56
Operator : RC/JU
Sample : P4534-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048260.D
Acq On : 28 Oct 2024 17:56
Operator : RC/JU
Sample : P4534-08
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E1L98

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc