

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048280.D
 Acq On : 29 Oct 2024 08:51
 Operator : RC/JU
 Sample : PB164388BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK388

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048280.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	39	rVB	67696	89222	2.25%	0.196%
2	3.587	98	102	123	rBV	797628	1242729	31.34%	2.730%
3	3.910	153	157	161	rVB	9860	12882	0.32%	0.028%
4	5.416	411	413	416	rBV3	2855	4324	0.11%	0.009%
5	6.169	538	541	544	rBV6	2926	4039	0.10%	0.009%
6	6.892	654	664	684	rBV	786690	1345396	33.93%	2.956%
7	7.051	684	691	704	rVV	711594	1134067	28.60%	2.492%
8	7.251	717	725	737	rBV	867380	1394130	35.16%	3.063%
9	7.351	740	742	747	rVV5	4769	7036	0.18%	0.015%
10	7.716	797	804	812	rBV	652268	1047912	26.43%	2.302%
11	8.434	918	926	943	rBV	948463	1655849	41.76%	3.638%
12	8.645	958	962	964	rBV4	2925	4127	0.10%	0.009%
13	8.875	994	1001	1010	rBV	769863	1311860	33.09%	2.882%
14	9.192	1052	1055	1058	rVB5	4022	5219	0.13%	0.011%
15	9.310	1069	1075	1076	rBV6	4375	6350	0.16%	0.014%
16	9.598	1116	1124	1135	rBV	618473	1068571	26.95%	2.348%
17	10.133	1209	1215	1227	rBV	854190	1581837	39.90%	3.475%
18	10.504	1270	1278	1289	rBV	917237	1547989	39.04%	3.401%
19	10.645	1294	1302	1323	rBV	789551	1689635	42.62%	3.712%
20	11.798	1493	1498	1502	rVB6	4405	8483	0.21%	0.019%
21	12.127	1548	1554	1564	rBV4	11764	21478	0.54%	0.047%
22	13.339	1755	1760	1761	rBV5	3148	4532	0.11%	0.010%
23	13.651	1808	1813	1818	rBV8	2365	5175	0.13%	0.011%
24	13.774	1827	1834	1849	rBV	1588851	2330216	58.77%	5.120%
25	14.051	1874	1881	1893	rBV	1884683	2899414	73.13%	6.370%
26	14.363	1927	1934	1950	rVB	1347869	1985330	50.07%	4.362%
27	14.586	1965	1972	1994	rBV	321388	854187	21.54%	1.877%
28	15.357	2096	2103	2118	rBV	2386274	3493519	88.11%	7.675%
29	15.480	2118	2124	2135	rBV	584535	915202	23.08%	2.011%
30	15.598	2140	2144	2152	rVB8	15936	31175	0.79%	0.068%
31	16.421	2278	2284	2286	rBV5	3763	6581	0.17%	0.014%
32	16.598	2311	2314	2317	rVB3	5413	5117	0.13%	0.011%
33	16.792	2342	2347	2350	rBV6	3115	4494	0.11%	0.010%
34	17.104	2393	2400	2410	rBV	1495401	2155941	54.38%	4.737%
35	17.204	2410	2417	2434	rVB	2380174	3580039	90.30%	7.865%
36	17.651	2489	2493	2495	rBV4	3684	5720	0.14%	0.013%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048280.D
Acq On : 29 Oct 2024 08:51
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK388

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	17.739	2503	2508	2509	rBV5	2794	4469	0.11%	0.010%
38	18.433	2622	2626	2630	rBV5	4864	8351	0.21%	0.018%
39	19.062	2729	2733	2738	rBV3	27045	36830	0.93%	0.081%
40	19.133	2742	2745	2751	rVB	23686	32536	0.82%	0.071%
41	19.497	2801	2807	2819	rBV	2765913	3964816	100.00%	8.711%
42	20.497	2974	2977	2981	rBV2	34368	36609	0.92%	0.080%
43	21.333	3113	3119	3131	rBV	1259701	2142785	54.05%	4.708%
44	24.074	3577	3585	3602	rVB	1470743	3676036	92.72%	8.076%
45	24.280	3612	3620	3635	rVB	814658	2153667	54.32%	4.732%




Sum of corrected areas: 45515876

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048280.D
Acq On : 29 Oct 2024 08:51
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

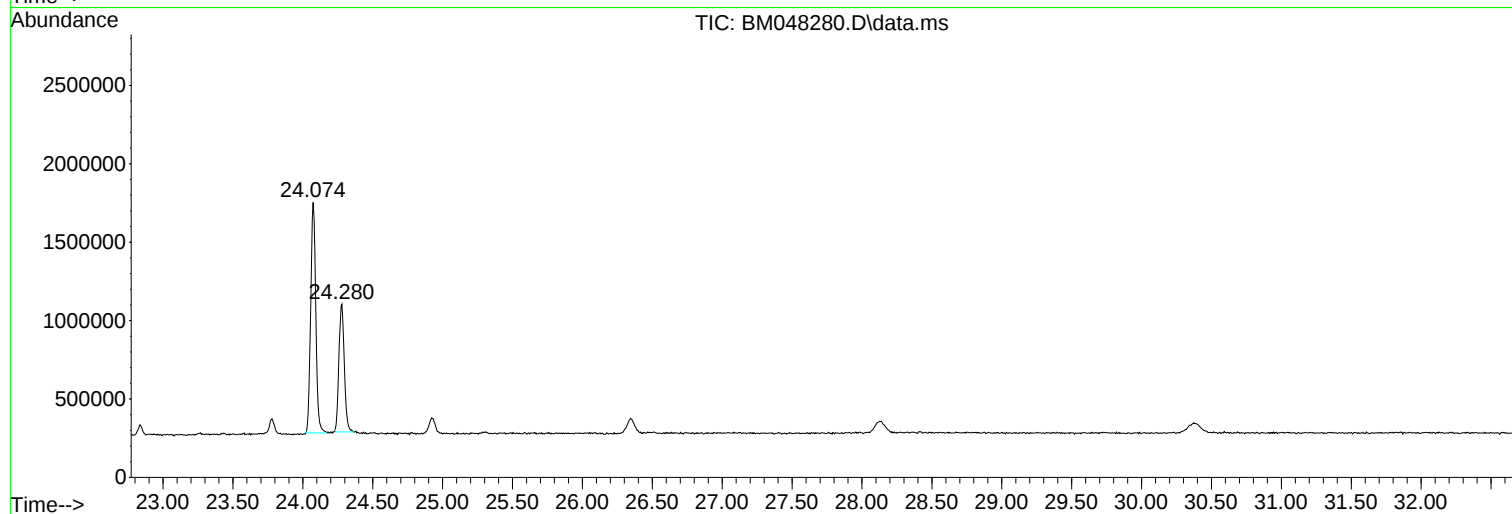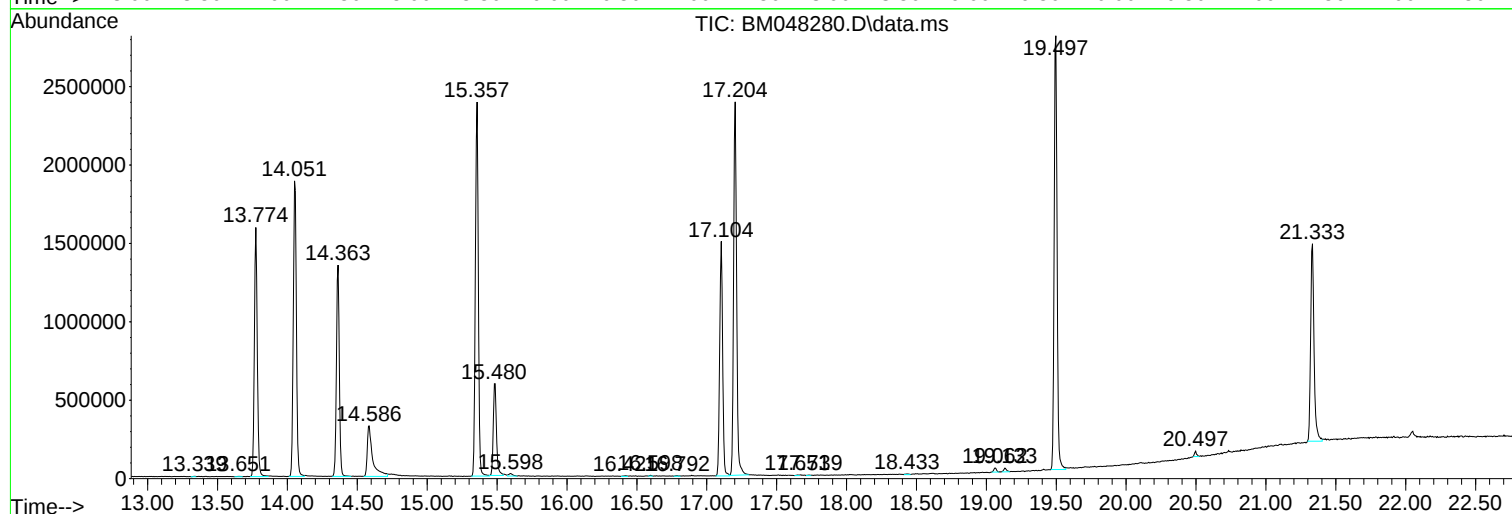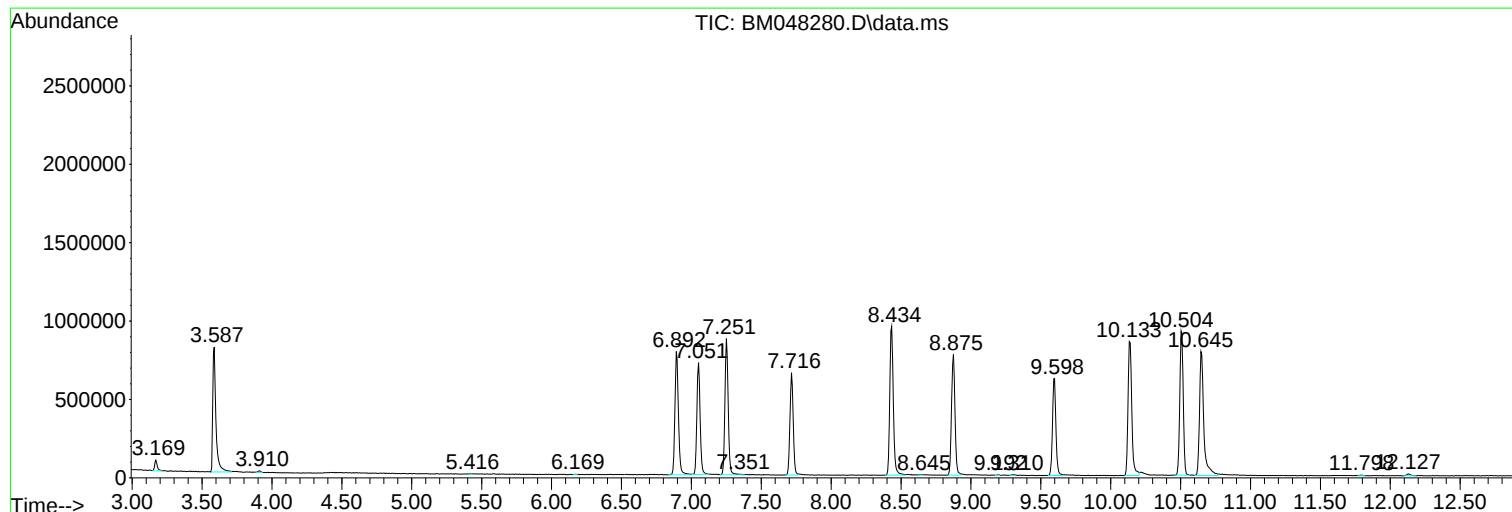

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048280.D
Acq On : 29 Oct 2024 08:51
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048280.D
Acq On : 29 Oct 2024 08:51
Operator : RC/JU
Sample : PB164388BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK388

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc