

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048281.D
 Acq On : 29 Oct 2024 09:30
 Operator : RC/JU
 Sample : PB164417BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK417

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048281.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	37	rVB	65477	83705	2.02%	0.176%
2	3.587	98	102	122	rBV	764892	1191893	28.71%	2.504%
3	3.910	154	157	163	rVB4	10866	16408	0.40%	0.034%
4	6.893	658	664	682	rBV	777871	1293646	31.16%	2.718%
5	7.051	685	691	701	rBV	707231	1110105	26.74%	2.332%
6	7.251	718	725	735	rBV	841769	1352414	32.57%	2.841%
7	7.716	796	804	812	rBV	710164	1144979	27.58%	2.405%
8	7.775	812	814	818	rVB4	5400	6110	0.15%	0.013%
9	8.428	919	925	939	rBV	941586	1635923	39.40%	3.437%
10	8.875	994	1001	1014	rBV	753228	1306973	31.48%	2.746%
11	9.592	1116	1123	1134	rBV	606247	1052802	25.36%	2.212%
12	10.134	1208	1215	1227	rBV	879141	1557489	37.51%	3.272%
13	10.504	1269	1278	1287	rBV	1032163	1731692	41.71%	3.638%
14	10.645	1295	1302	1328	rBV	822340	1735717	41.80%	3.646%
15	10.810	1328	1330	1336	rVB6	3201	5921	0.14%	0.012%
16	12.128	1549	1554	1560	rBV3	12913	26495	0.64%	0.056%
17	13.345	1754	1761	1766	rBV9	2256	6197	0.15%	0.013%
18	13.775	1827	1834	1849	rBV	1736504	2524992	60.81%	5.304%
19	14.051	1874	1881	1898	rBV	2020687	3077344	74.12%	6.465%
20	14.357	1927	1933	1944	rBV	1557067	2338256	56.32%	4.912%
21	14.580	1964	1971	1996	rBV	387573	939714	22.63%	1.974%
22	15.351	2095	2102	2118	rBV	2566409	3768215	90.76%	7.916%
23	15.480	2118	2124	2140	rVV	666080	1044975	25.17%	2.195%
24	15.598	2140	2144	2151	rVB2	17373	29902	0.72%	0.063%
25	16.139	2231	2236	2240	rBV6	3165	5507	0.13%	0.012%
26	16.592	2309	2313	2318	rBV5	2706	5487	0.13%	0.012%
27	16.786	2343	2346	2349	rBV5	3402	5097	0.12%	0.011%
28	16.892	2361	2364	2370	rVB6	5683	7893	0.19%	0.017%
29	17.104	2393	2400	2410	rBV	1782141	2589362	62.37%	5.440%
30	17.198	2410	2416	2431	rVV2	2501499	3881412	93.48%	8.154%
31	19.062	2728	2733	2739	rBV3	27877	43004	1.04%	0.090%
32	19.133	2742	2745	2752	rVB	23540	31345	0.75%	0.066%
33	19.492	2800	2806	2818	rBV	3021080	4151947	100.00%	8.722%
34	21.327	3112	3118	3132	rBV2	1346404	2338378	56.32%	4.912%
35	24.068	3576	3584	3595	rBV	1389354	3412085	82.18%	7.168%
36	24.274	3611	3619	3630	rVB	834882	2147839	51.73%	4.512%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048281.D
Acq On : 29 Oct 2024 09:30
Operator : RC/JU
Sample : PB164417BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK417

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 47601223

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048281.D
Acq On : 29 Oct 2024 09:30
Operator : RC/JU
Sample : PB164417BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

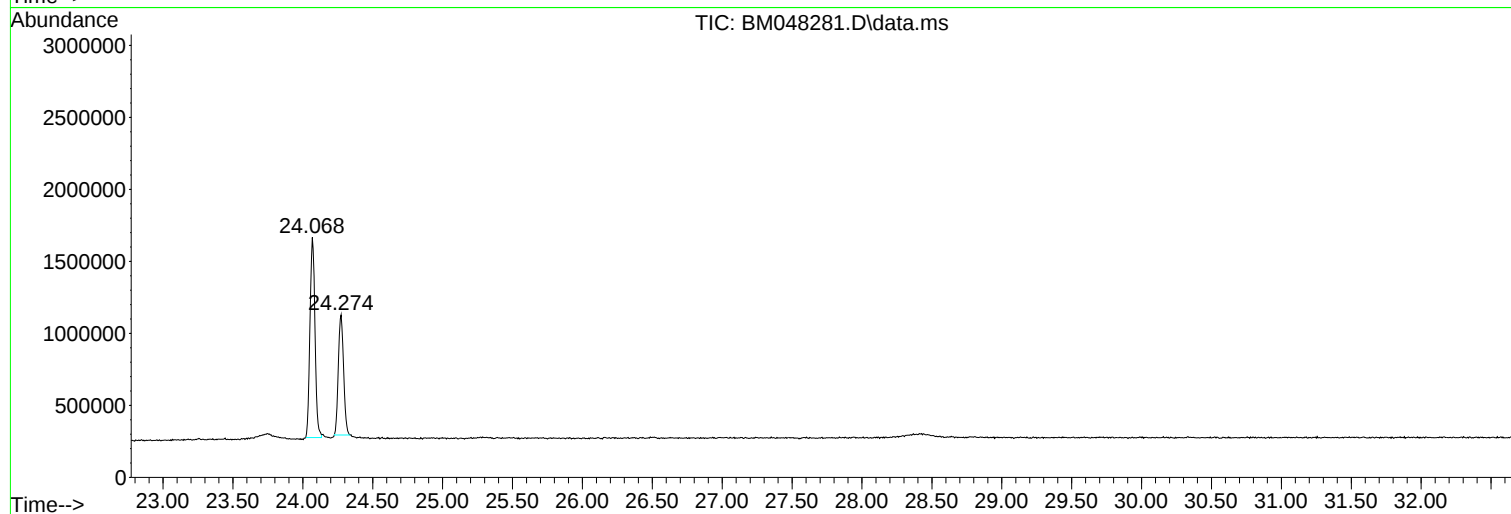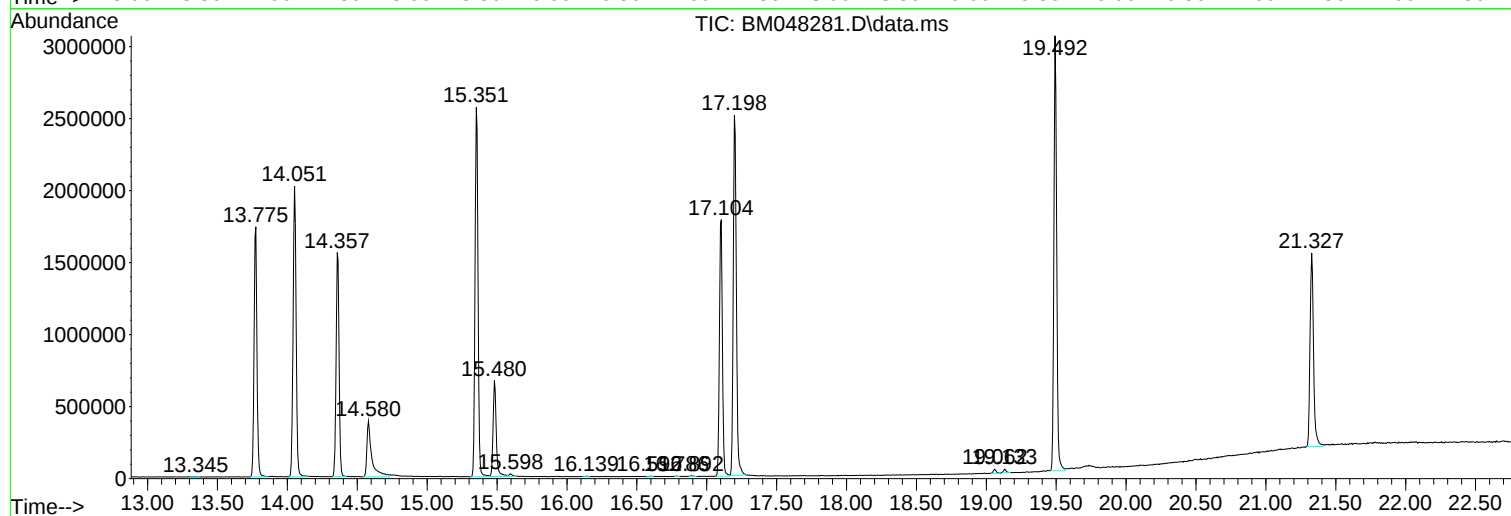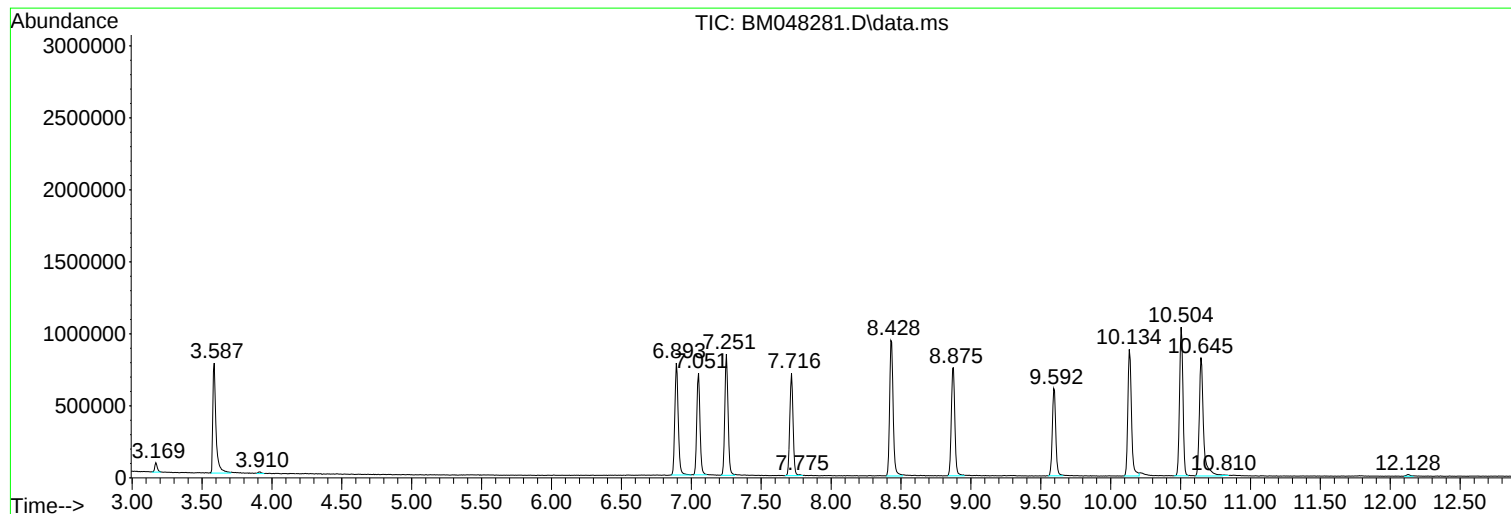

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048281.D
Acq On : 29 Oct 2024 09:30
Operator : RC/JU
Sample : PB164417BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048281.D
Acq On : 29 Oct 2024 09:30
Operator : RC/JU
Sample : PB164417BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK417

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc