

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048292.D
 Acq On : 29 Oct 2024 18:04
 Operator : RC/JU
 Sample : PB164416BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK416

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	36	rBV	60198	73911	2.18%	0.182%
2	3.587	98	102	124	rBV	703140	1093950	32.21%	2.692%
3	3.910	154	157	160	rVB3	8665	12273	0.36%	0.030%
4	4.375	234	236	238	rBV3	5049	4841	0.14%	0.012%
5	6.892	654	664	674	rBV	724790	1212917	35.72%	2.985%
6	7.051	684	691	706	rVB	630723	1031463	30.37%	2.538%
7	7.251	719	725	736	rBV	771038	1254595	36.94%	3.087%
8	7.628	788	789	793	rVB4	3351	3653	0.11%	0.009%
9	7.716	796	804	815	rVV	619853	1011402	29.78%	2.489%
10	8.428	919	925	942	rBV	887057	1522211	44.82%	3.746%
11	8.869	993	1000	1014	rBV	683413	1195001	35.19%	2.940%
12	9.298	1066	1073	1079	rVB2	12315	20710	0.61%	0.051%
13	9.592	1116	1123	1136	rBV	585817	981022	28.89%	2.414%
14	10.004	1190	1193	1196	rVB4	2765	4125	0.12%	0.010%
15	10.133	1208	1215	1238	rBV	812785	1491748	43.93%	3.671%
16	10.504	1269	1278	1288	rBV	877441	1475197	43.44%	3.630%
17	10.645	1295	1302	1323	rBV	737727	1498307	44.12%	3.687%
18	10.810	1328	1330	1333	rVB3	3218	3564	0.10%	0.009%
19	11.786	1489	1496	1501	rBV3	9995	15245	0.45%	0.038%
20	12.122	1548	1553	1559	rBV3	10652	17524	0.52%	0.043%
21	12.433	1604	1606	1611	rBV4	2924	3951	0.12%	0.010%
22	12.922	1686	1689	1692	rBV5	2292	3772	0.11%	0.009%
23	13.339	1755	1760	1762	rVV5	2569	3623	0.11%	0.009%
24	13.769	1827	1833	1845	rBV	1384144	2073862	61.07%	5.103%
25	14.051	1874	1881	1896	rBV	1728338	2582598	76.05%	6.355%
26	14.357	1926	1933	1943	rBV	1278174	1885864	55.53%	4.640%
27	14.439	1945	1947	1951	rVB5	3155	4056	0.12%	0.010%
28	14.580	1965	1971	1993	rBV	267032	728810	21.46%	1.793%
29	15.051	2049	2051	2054	rBV4	2873	3490	0.10%	0.009%
30	15.351	2095	2102	2118	rVV	2158770	3085250	90.85%	7.592%
31	15.480	2118	2124	2140	rVV	548377	836321	24.63%	2.058%
32	15.598	2140	2144	2151	rVB4	14004	24651	0.73%	0.061%
33	16.133	2232	2235	2239	rVB5	3281	4549	0.13%	0.011%
34	16.215	2246	2249	2253	rBV5	2218	3886	0.11%	0.010%
35	16.598	2311	2314	2317	rVB4	4046	4863	0.14%	0.012%
36	16.786	2342	2346	2351	rBV7	2293	3744	0.11%	0.009%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048292.D
Acq On : 29 Oct 2024 18:04
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	16.892	2361	2364	2367	rBV5	3056	4087	0.12%	0.010%
38	17.098	2393	2399	2410	rVV	1375392	1993478	58.70%	4.905%
39	17.198	2410	2416	2434	rVB2	2119018	3108846	91.54%	7.650%
40	17.668	2491	2496	2500	rVB5	3981	6282	0.18%	0.015%
41	18.292	2600	2602	2606	rBV5	2757	4676	0.14%	0.012%
42	19.056	2729	2732	2737	rBV4	23063	31655	0.93%	0.078%
43	19.133	2741	2745	2749	rVV2	18511	26623	0.78%	0.066%
44	19.492	2800	2806	2817	rBV	2575264	3396002	100.00%	8.356%
45	21.327	3112	3118	3129	rBV	1138610	1918979	56.51%	4.722%
46	24.068	3576	3584	3602	rVB	1215402	3089853	90.99%	7.603%
47	24.268	3611	3618	3630	rVB	781293	1882528	55.43%	4.632%




Sum of corrected areas: 40639958

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048292.D
Acq On : 29 Oct 2024 18:04
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

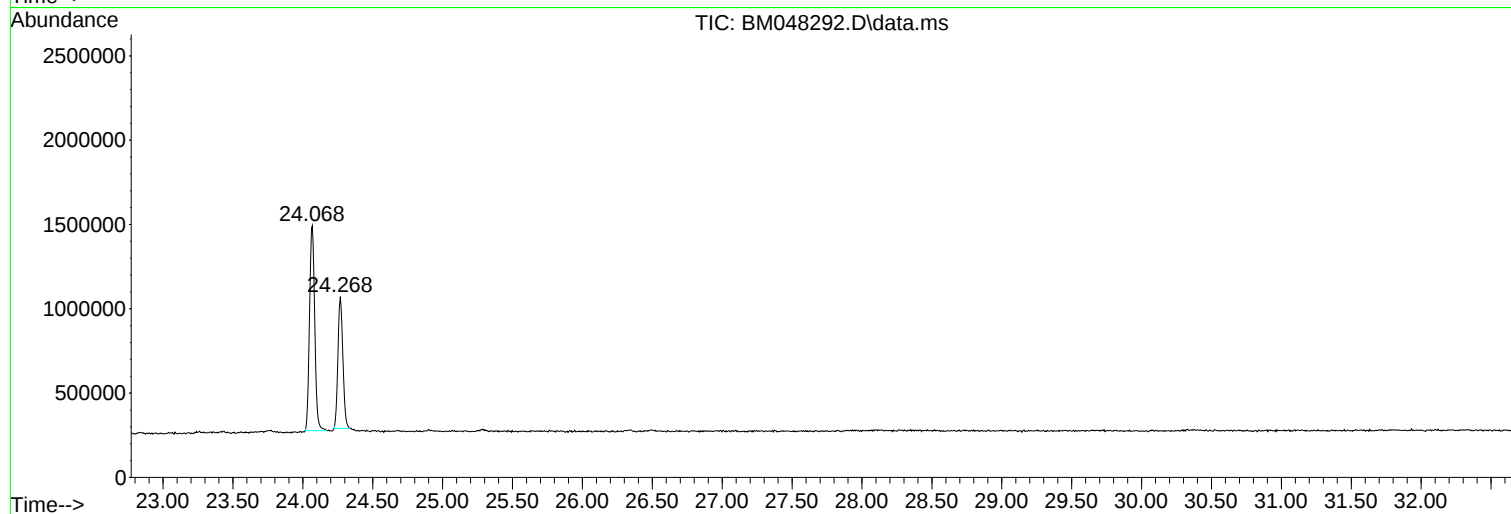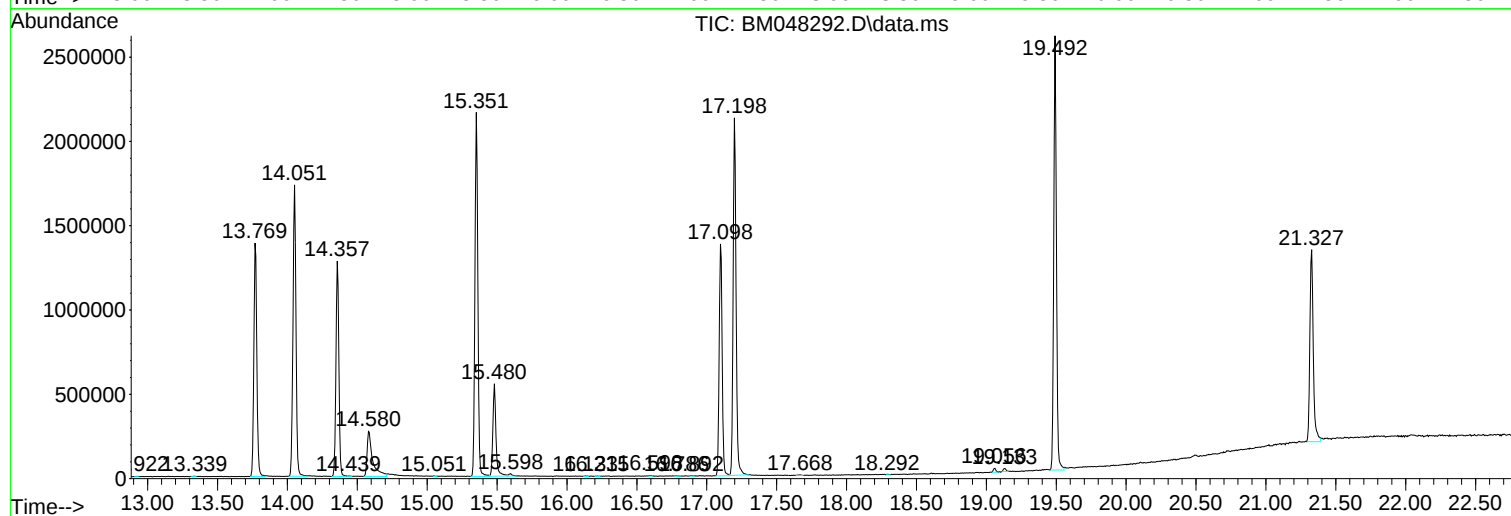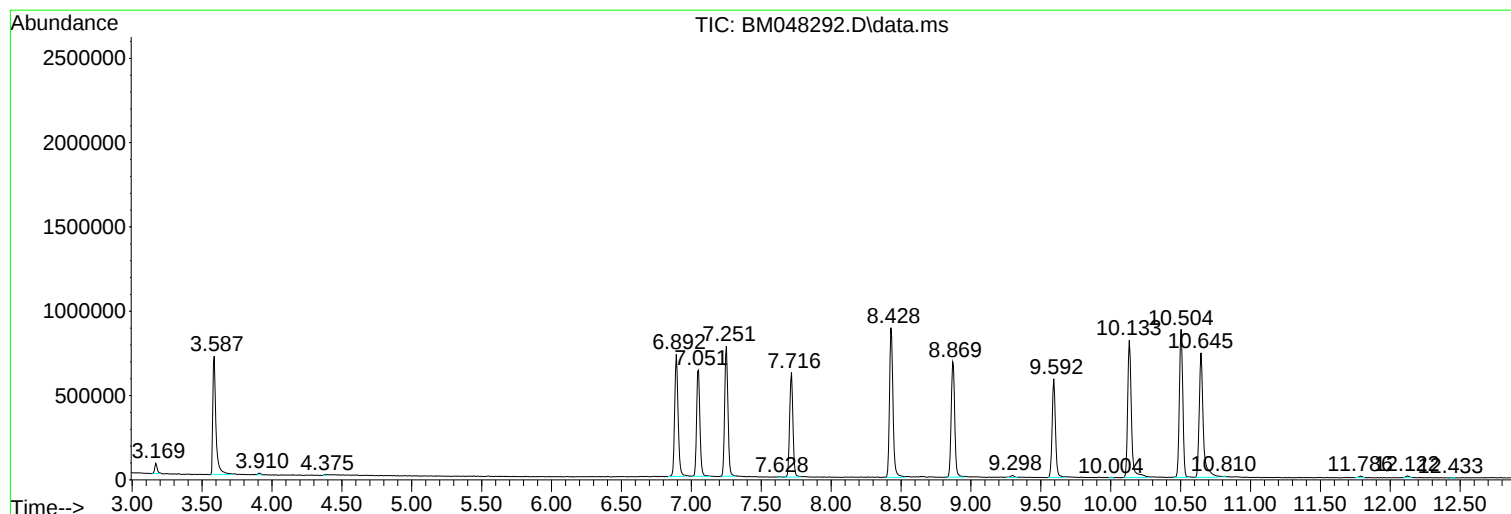

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048292.D
Acq On : 29 Oct 2024 18:04
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048292.D
Acq On : 29 Oct 2024 18:04
Operator : RC/JU
Sample : PB164416BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK416

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc