

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048293.D
 Acq On : 29 Oct 2024 18:43
 Operator : RC/JU
 Sample : PB164419BL
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK419

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.169	27	31	40	rVB	58441	77724	2.29%	0.195%
2	3.587	98	102	121	rBV	679437	1042807	30.70%	2.622%
3	3.910	153	157	161	rVV3	9479	13305	0.39%	0.033%
4	4.187	203	204	209	rBV4	3061	4818	0.14%	0.012%
5	6.116	527	532	535	rBV7	2692	5183	0.15%	0.013%
6	6.892	654	664	679	rBV	690350	1162316	34.22%	2.922%
7	7.051	684	691	703	rVV	604851	973577	28.67%	2.448%
8	7.251	718	725	739	rBV	743939	1214520	35.76%	3.053%
9	7.716	797	804	814	rBV	607989	995395	29.31%	2.503%
10	8.428	919	925	939	rBV	832354	1426031	41.99%	3.585%
11	8.869	992	1000	1014	rBV	643352	1134459	33.40%	2.852%
12	9.298	1069	1073	1078	rVB2	12851	20230	0.60%	0.051%
13	9.480	1102	1104	1110	rVB4	2034	3541	0.10%	0.009%
14	9.592	1116	1123	1137	rBV	533117	921750	27.14%	2.317%
15	9.704	1140	1142	1150	rVB6	3306	6626	0.20%	0.017%
16	10.133	1206	1215	1227	rBV	762960	1368383	40.29%	3.440%
17	10.504	1270	1278	1288	rVV	862713	1433125	42.20%	3.603%
18	10.645	1294	1302	1321	rBV	679428	1405139	41.37%	3.533%
19	11.792	1491	1497	1502	rVB5	11067	17704	0.52%	0.045%
20	12.121	1548	1553	1558	rBV4	10039	19233	0.57%	0.048%
21	13.768	1827	1833	1848	rBV	1314035	1967854	57.94%	4.947%
22	14.051	1874	1881	1895	rBV	1635041	2440493	71.86%	6.136%
23	14.357	1926	1933	1941	rBV	1273298	1830494	53.90%	4.602%
24	14.586	1963	1972	1993	rBV	254573	708095	20.85%	1.780%
25	15.351	2095	2102	2118	rBV	1992451	2969638	87.44%	7.466%
26	15.480	2118	2124	2139	rVV	508230	801234	23.59%	2.014%
27	15.592	2141	2143	2148	rVB6	11813	15633	0.46%	0.039%
28	16.598	2310	2314	2317	rVB5	3257	3741	0.11%	0.009%
29	17.098	2393	2399	2410	rBV	1364795	1975571	58.17%	4.967%
30	17.198	2410	2416	2433	rVB	2058071	3038036	89.45%	7.638%
31	17.515	2466	2470	2473	rBV6	3685	5449	0.16%	0.014%
32	17.656	2492	2494	2499	rVB4	4429	4916	0.14%	0.012%
33	19.056	2728	2732	2737	rBV4	22479	34219	1.01%	0.086%
34	19.133	2741	2745	2749	rBV2	17704	26772	0.79%	0.067%
35	19.492	2800	2806	2816	rBV	2454373	3396269	100.00%	8.539%
36	21.327	3112	3118	3129	rBV	1233645	2010883	59.21%	5.056%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048293.D
Acq On : 29 Oct 2024 18:43
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Title : SVOA CALIBRATION

37	24.068	3576	3584	3603	rVB	1314316	3232198	95.17%	8.126%
38	24.268	3610	3618	3632	rVB	796387	2068309	60.90%	5.200%




Sum of corrected areas: 39775670

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048293.D
Acq On : 29 Oct 2024 18:43
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

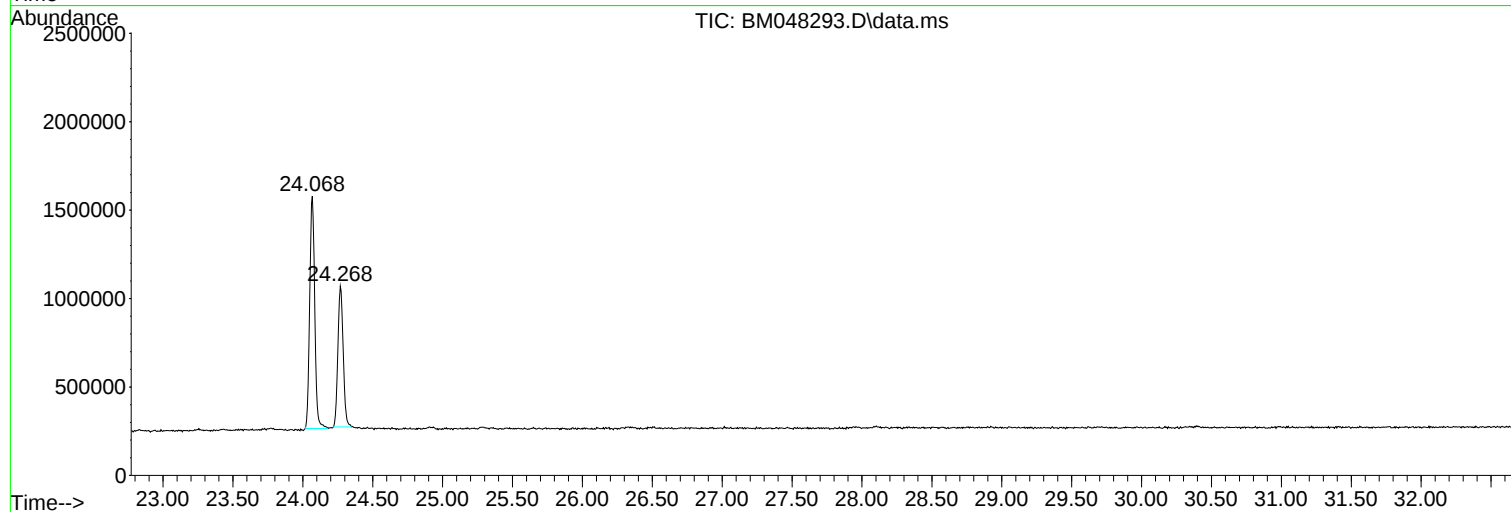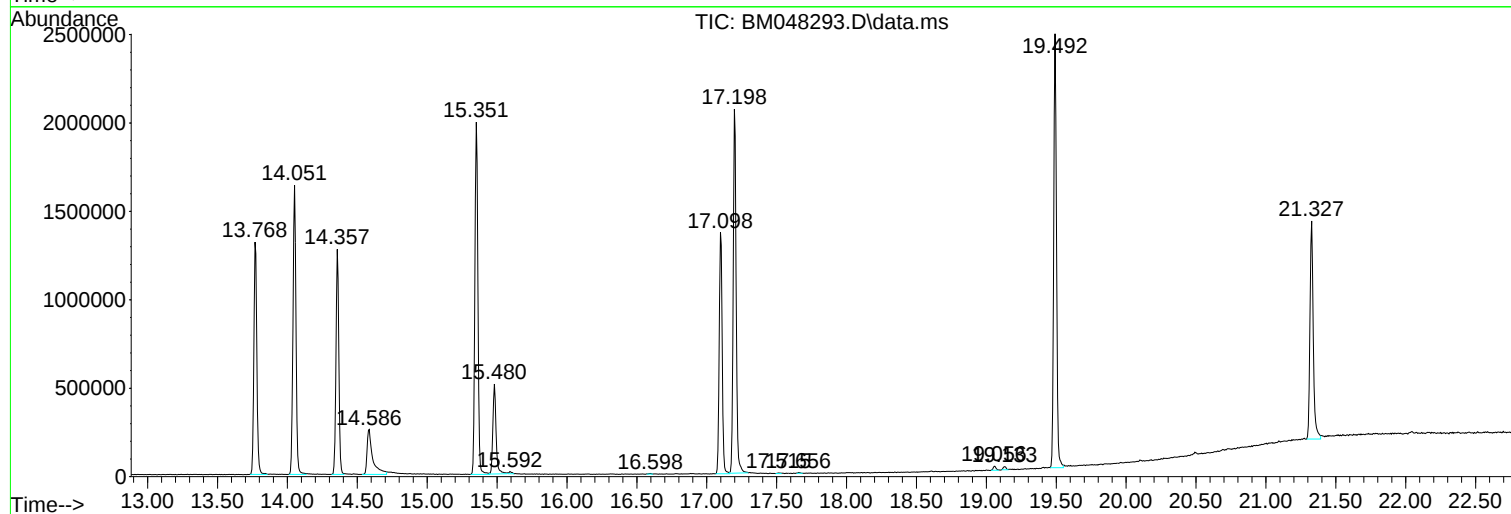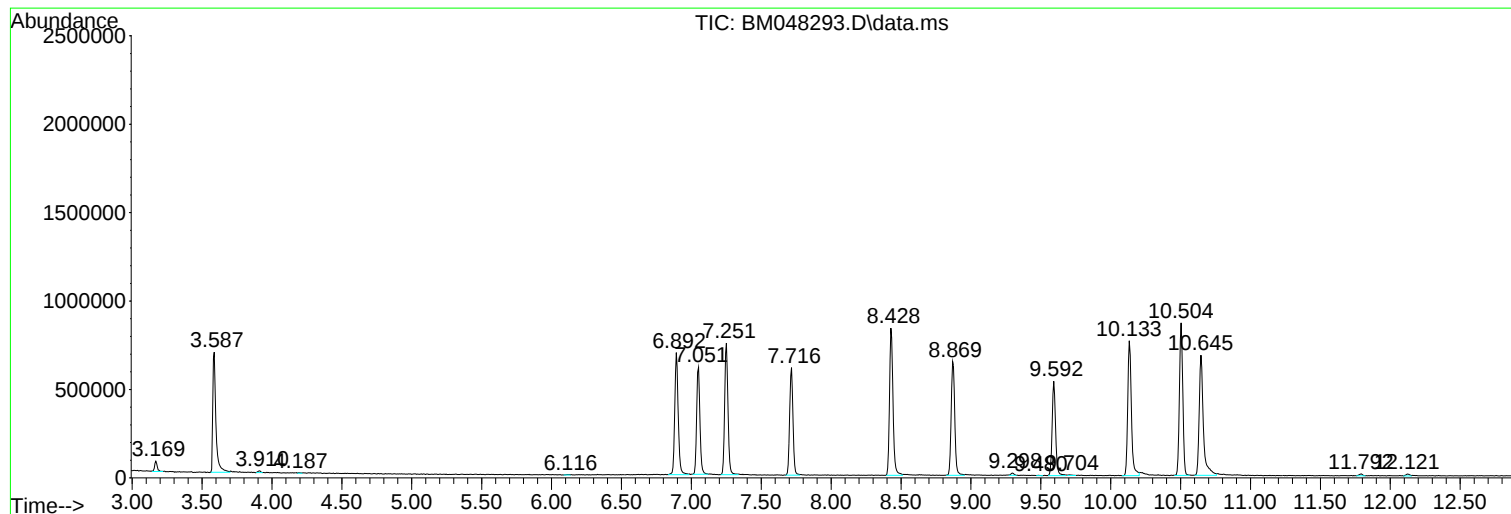

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048293.D
Acq On : 29 Oct 2024 18:43
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048293.D
Acq On : 29 Oct 2024 18:43
Operator : RC/JU
Sample : PB164419BL
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK419

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc