

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048294.D
 Acq On : 29 Oct 2024 19:23
 Operator : RC/JU
 Sample : P4562-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048294.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.911	154	157	162	rVB	10589	11608	0.58%	0.117%
2	5.069	351	354	355	rBV2	1818	2005	0.10%	0.020%
3	5.140	365	366	369	rBV3	2627	3260	0.16%	0.033%
4	5.422	411	414	419	rVB5	4317	6015	0.30%	0.061%
5	5.669	453	456	459	rBV5	2581	4426	0.22%	0.045%
6	5.775	471	474	475	rBV3	2824	2287	0.11%	0.023%
7	6.199	543	546	549	rBV6	1781	2341	0.12%	0.024%
8	6.334	566	569	571	rBV3	2487	2932	0.15%	0.030%
9	6.840	652	655	656	rBV3	2699	3110	0.16%	0.031%
10	6.857	656	658	665	rVB4	5733	8309	0.42%	0.084%
11	7.716	797	804	816	rBV	494084	899881	45.14%	9.059%
12	7.957	843	845	849	rVB5	1649	2131	0.11%	0.021%
13	8.063	861	863	866	rBV3	2744	3239	0.16%	0.033%
14	8.310	902	905	908	rBV5	2669	2959	0.15%	0.030%
15	8.404	914	921	923	rBV6	2622	4844	0.24%	0.049%
16	8.575	946	950	951	rBV3	2589	2167	0.11%	0.022%
17	8.657	957	964	966	rVB8	2373	3515	0.18%	0.035%
18	8.793	983	987	990	rBV4	1354	2511	0.13%	0.025%
19	8.946	1009	1013	1015	rVB4	2799	2636	0.13%	0.027%
20	9.028	1025	1027	1031	rBV5	1600	2053	0.10%	0.021%
21	9.298	1065	1073	1079	rVV4	9570	17145	0.86%	0.173%
22	9.598	1122	1124	1127	rBV3	1655	2275	0.11%	0.023%
23	9.763	1150	1152	1155	rBV4	1951	2385	0.12%	0.024%
24	9.834	1161	1164	1169	rVB5	2610	3542	0.18%	0.036%
25	9.893	1169	1174	1175	rBV4	1686	2493	0.13%	0.025%
26	10.251	1232	1235	1241	rBV5	1338	2466	0.12%	0.025%
27	10.404	1259	1261	1265	rVB5	1716	2471	0.12%	0.025%
28	10.504	1271	1278	1292	rBV	662654	1259808	63.19%	12.682%
29	10.598	1292	1294	1302	rVB2	14826	28413	1.43%	0.286%
30	10.910	1346	1347	1351	rBV2	2472	2209	0.11%	0.022%
31	11.092	1374	1378	1379	rVB4	2486	2352	0.12%	0.024%
32	11.110	1379	1381	1384	rBV4	2126	2383	0.12%	0.024%
33	11.357	1420	1423	1427	rBV5	1442	2182	0.11%	0.022%
34	11.387	1427	1428	1433	rVV5	1898	2047	0.10%	0.021%
35	11.704	1479	1482	1485	rBV4	2275	3079	0.15%	0.031%
36	11.792	1491	1497	1502	rVB4	6815	10971	0.55%	0.110%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048294.D
 Acq On : 29 Oct 2024 19:23
 Operator : RC/JU
 Sample : P4562-05
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

37	11.863	1507	1509	1513	rVB5	1488	2260	0.11%	0.023%
38	12.063	1542	1543	1549	rBV4	2552	3079	0.15%	0.031%
39	12.204	1561	1567	1568	rBV4	2154	3320	0.17%	0.033%
40	12.269	1576	1578	1581	rBV4	1855	2370	0.12%	0.024%
41	12.569	1625	1629	1631	rBV5	2025	2105	0.11%	0.021%
42	12.598	1633	1634	1639	rBV3	2077	2527	0.13%	0.025%
43	13.098	1716	1719	1723	rVB4	1768	2254	0.11%	0.023%
44	13.151	1725	1728	1731	rVB4	1686	2024	0.10%	0.020%
45	13.469	1779	1782	1787	rBV6	1276	2216	0.11%	0.022%
46	13.792	1832	1837	1841	rBV6	5550	9940	0.50%	0.100%
47	14.057	1879	1882	1886	rVB6	2107	3180	0.16%	0.032%
48	14.292	1920	1922	1926	rVB4	2233	2235	0.11%	0.022%
49	14.357	1926	1933	1951	rBV	1051420	1718008	86.18%	17.295%
50	14.492	1955	1956	1961	rVV5	3150	4471	0.22%	0.045%
51	14.557	1963	1967	1970	rVB6	1560	2293	0.12%	0.023%
52	14.739	1996	1998	2001	rVB3	2071	2108	0.11%	0.021%
53	14.780	2001	2005	2006	rVB3	2586	2372	0.12%	0.024%
54	15.339	2097	2100	2101	rBV3	1977	2244	0.11%	0.023%
55	15.351	2101	2102	2107	rVB3	4179	4299	0.22%	0.043%
56	15.757	2170	2171	2174	rVB3	2245	2137	0.11%	0.022%
57	15.969	2204	2207	2210	rVB3	1720	2189	0.11%	0.022%
58	16.092	2227	2228	2231	rBV3	1701	2058	0.10%	0.021%
59	16.592	2310	2313	2317	rVB5	3761	5494	0.28%	0.055%
60	16.904	2362	2366	2368	rVB5	2454	3274	0.16%	0.033%
61	17.021	2383	2386	2388	rBV2	2932	3242	0.16%	0.033%
62	17.104	2393	2400	2430	rVV	1026562	1867189	93.66%	18.797%
63	17.657	2492	2494	2498	rVB5	2559	2206	0.11%	0.022%
64	17.968	2544	2547	2548	rBV3	1741	2163	0.11%	0.022%
65	18.251	2594	2595	2597	rBV2	2554	2012	0.10%	0.020%
66	21.327	3112	3118	3128	rBV	1126208	1956218	98.12%	19.693%
67	24.268	3610	3618	3637	rVB	739218	1993607	100.00%	20.069%




Sum of corrected areas: 9933544

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048294.D
Acq On : 29 Oct 2024 19:23
Operator : RC/JU
Sample : P4562-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

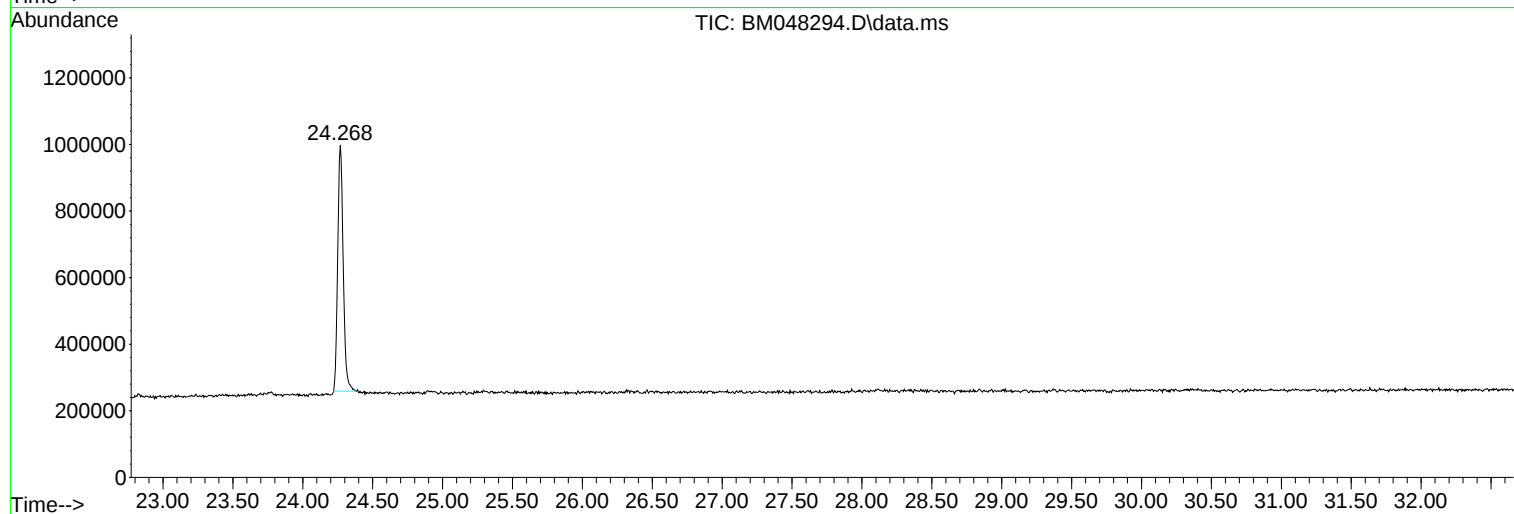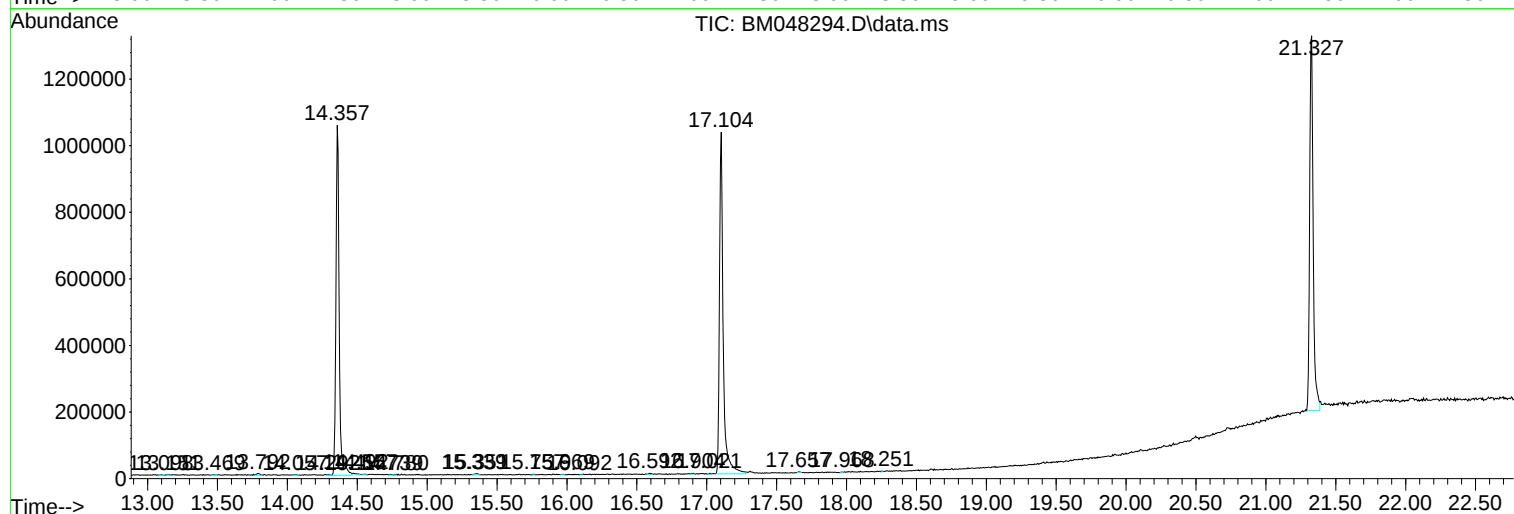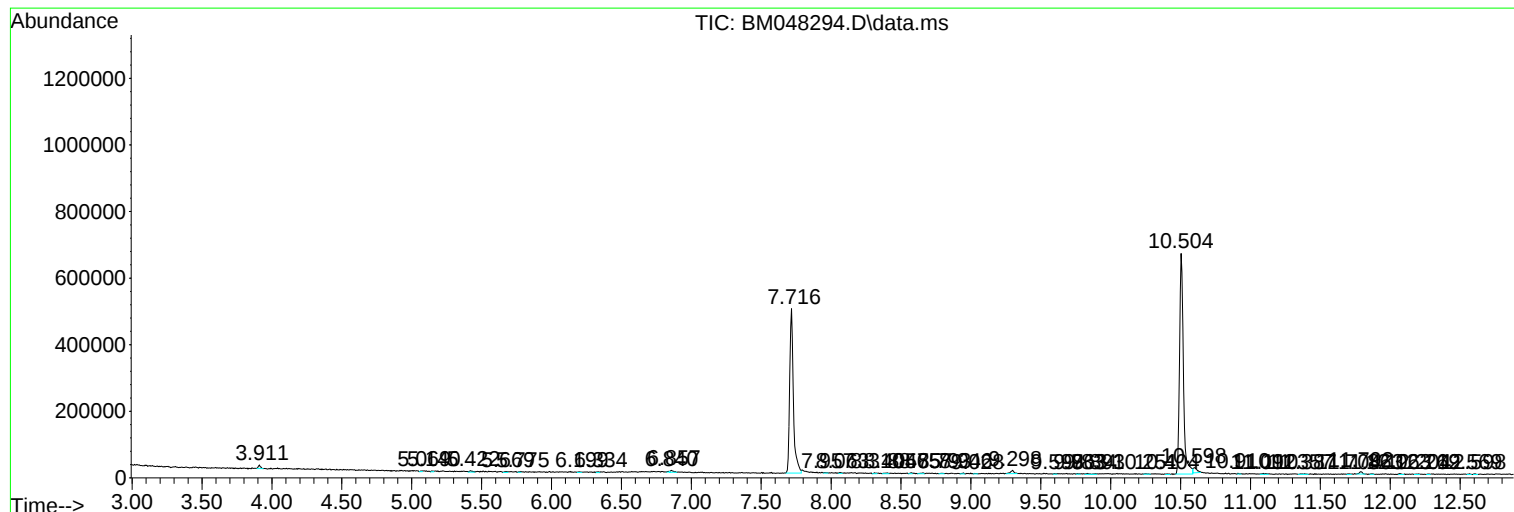

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048294.D
Acq On : 29 Oct 2024 19:23
Operator : RC/JU
Sample : P4562-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048294.D
Acq On : 29 Oct 2024 19:23
Operator : RC/JU
Sample : P4562-05
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc