

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048295.D
 Acq On : 29 Oct 2024 20:02
 Operator : RC/JU
 Sample : P4562-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM048295.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.910	154	157	164	rVB4	9246	16883	0.84%	0.167%
2	4.769	301	303	305	rBV3	3167	2393	0.12%	0.024%
3	4.822	310	312	314	rBV3	2331	2269	0.11%	0.022%
4	5.193	374	375	378	rBV3	2719	2482	0.12%	0.025%
5	5.269	384	388	389	rBV3	1885	2690	0.13%	0.027%
6	5.422	412	414	418	rVB5	2631	2670	0.13%	0.026%
7	5.563	436	438	441	rVB4	2571	2273	0.11%	0.023%
8	6.693	629	630	633	rVB3	3074	2641	0.13%	0.026%
9	6.863	655	659	662	rVB4	4475	5862	0.29%	0.058%
10	6.987	676	680	683	rBV6	3409	4155	0.21%	0.041%
11	7.028	683	687	688	rVV4	2369	2673	0.13%	0.026%
12	7.051	688	691	692	rVB3	2881	2314	0.11%	0.023%
13	7.540	772	774	776	rBV3	2894	2244	0.11%	0.022%
14	7.640	788	791	795	rVB6	1991	2456	0.12%	0.024%
15	7.716	797	804	820	rBV	512336	935606	46.32%	9.265%
16	8.134	871	875	877	rBV5	2349	2562	0.13%	0.025%
17	9.304	1067	1074	1078	rVB4	7100	12146	0.60%	0.120%
18	9.663	1131	1135	1138	rVB5	1836	3190	0.16%	0.032%
19	9.698	1138	1141	1142	rBV2	2011	2229	0.11%	0.022%
20	9.716	1142	1144	1148	rVB3	2442	2083	0.10%	0.021%
21	9.951	1178	1184	1185	rBV5	1615	2239	0.11%	0.022%
22	10.504	1271	1278	1291	rBV	678974	1280826	63.40%	12.684%
23	10.839	1331	1335	1340	rBV6	3298	4617	0.23%	0.046%
24	10.886	1342	1343	1346	rBV3	2511	2615	0.13%	0.026%
25	10.986	1358	1360	1365	rVB5	1679	2275	0.11%	0.023%
26	11.404	1427	1431	1435	rBV6	2053	3532	0.17%	0.035%
27	11.481	1441	1444	1446	rBV3	2256	2787	0.14%	0.028%
28	11.539	1448	1454	1456	rVV6	2210	3088	0.15%	0.031%
29	11.569	1456	1459	1462	rVB5	1677	2334	0.12%	0.023%
30	11.792	1491	1497	1504	rVB4	6852	13339	0.66%	0.132%
31	12.163	1559	1560	1564	rVB3	2592	2404	0.12%	0.024%
32	12.316	1583	1586	1587	rVB2	2676	2269	0.11%	0.022%
33	12.451	1606	1609	1612	rBV4	2768	2908	0.14%	0.029%
34	12.645	1638	1642	1646	rVB6	1867	3158	0.16%	0.031%
35	13.175	1731	1732	1736	rVB3	2293	2698	0.13%	0.027%
36	13.751	1827	1830	1833	rVB5	1388	2067	0.10%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
 Data File : BM048295.D
 Acq On : 29 Oct 2024 20:02
 Operator : RC/JU
 Sample : P4562-10
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SVOC-GPC2-BLANK

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
 Title : SVOA CALIBRATION

37	13.786	1833	1836	1841	rBV4	4944	7767	0.38%	0.077%
38	14.063	1882	1883	1886	rVB3	2866	2266	0.11%	0.022%
39	14.092	1886	1888	1890	rBV2	2438	2442	0.12%	0.024%
40	14.274	1916	1919	1921	rBV4	2530	2692	0.13%	0.027%
41	14.357	1927	1933	1950	rBV	1094106	1740302	86.15%	17.234%
42	14.586	1971	1972	1975	rBV2	2984	2453	0.12%	0.024%
43	15.163	2068	2070	2073	rVB3	1679	2136	0.11%	0.021%
44	15.351	2100	2102	2106	rVB4	4204	5141	0.25%	0.051%
45	15.698	2159	2161	2164	rVB3	1695	2112	0.10%	0.021%
46	15.810	2176	2180	2182	rBV4	2941	3474	0.17%	0.034%
47	15.845	2182	2186	2189	rVB6	1502	2253	0.11%	0.022%
48	16.410	2279	2282	2284	rBV4	2183	3024	0.15%	0.030%
49	16.516	2295	2300	2305	rBV7	1573	2804	0.14%	0.028%
50	16.568	2305	2309	2310	rVV4	1828	2167	0.11%	0.021%
51	16.598	2310	2314	2318	rVB5	3448	5857	0.29%	0.058%
52	16.880	2359	2362	2363	rBV3	2015	2352	0.12%	0.023%
53	16.892	2363	2364	2370	rVB5	3078	2996	0.15%	0.030%
54	17.104	2393	2400	2427	rVV	1040754	1891678	93.64%	18.733%
55	17.310	2432	2435	2436	rVV3	3353	4594	0.23%	0.045%
56	17.504	2467	2468	2471	rBV2	3365	2986	0.15%	0.030%
57	17.533	2471	2473	2475	rVB3	3079	2076	0.10%	0.021%
58	17.621	2485	2488	2490	rVB3	2331	2553	0.13%	0.025%
59	17.645	2490	2492	2493	rBV2	3046	2577	0.13%	0.026%
60	17.668	2493	2496	2499	rVB5	2990	4267	0.21%	0.042%
61	17.751	2508	2510	2514	rBV4	2180	2223	0.11%	0.022%
62	17.998	2551	2552	2556	rBV4	2543	2917	0.14%	0.029%
63	18.121	2571	2573	2578	rBV6	2397	3447	0.17%	0.034%
64	18.221	2587	2590	2593	rBV5	2428	2704	0.13%	0.027%
65	18.251	2593	2595	2597	rBV3	2086	2027	0.10%	0.020%
66	18.604	2653	2655	2658	rVB4	3386	3037	0.15%	0.030%
67	21.327	3112	3118	3130	rBV	1214253	2020087	100.00%	20.005%
68	24.268	3610	3618	3632	rBV	761140	2013731	99.69%	19.942%




Sum of corrected areas: 10098119

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048295.D
Acq On : 29 Oct 2024 20:02
Operator : RC/JU
Sample : P4562-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

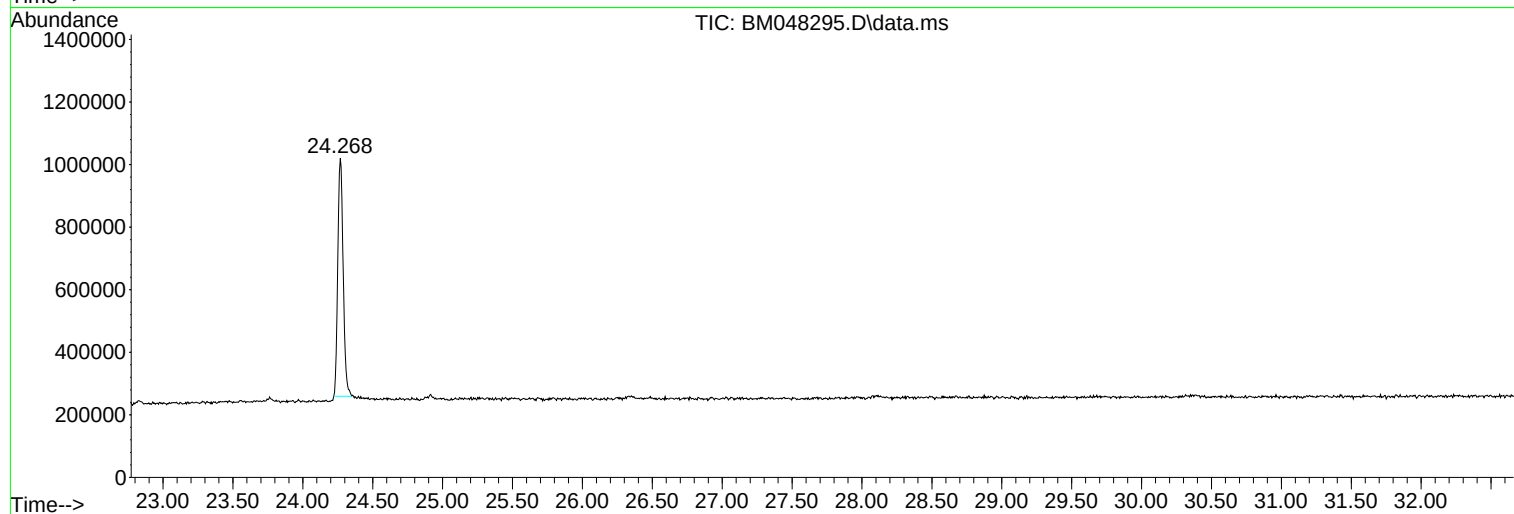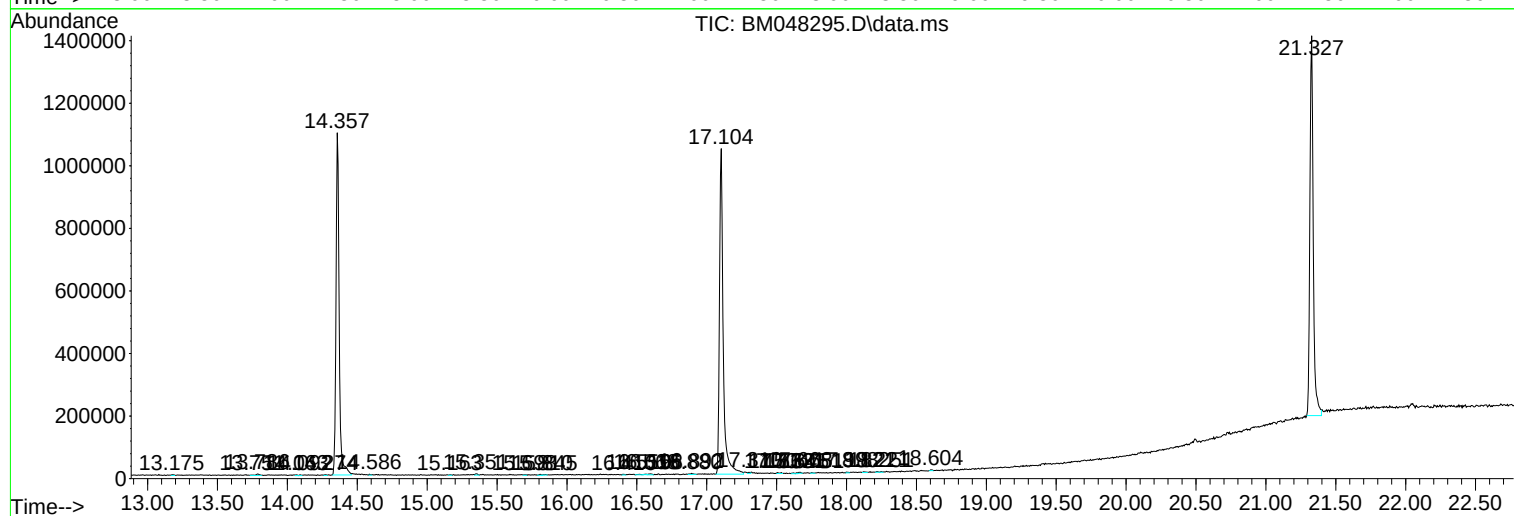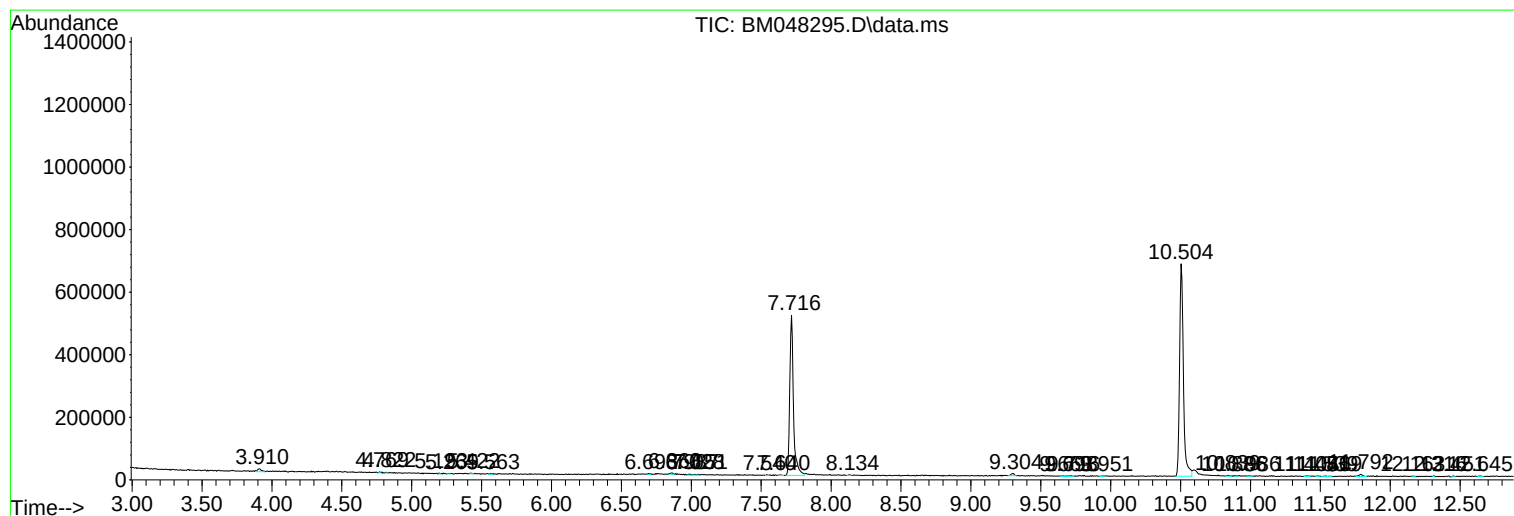

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048295.D
Acq On : 29 Oct 2024 20:02
Operator : RC/JU
Sample : P4562-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM102824\
Data File : BM048295.D
Acq On : 29 Oct 2024 20:02
Operator : RC/JU
Sample : P4562-10
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SVOC-GPC2-BLANK

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM102624.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc